




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052846.D
Acq On : 26 Mar 2022 2:27
Operator : CG/JU
Sample : N2079-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW5Z4

Manual IntegrationsAPPROVED

Quant Time: Mar 26 05:02:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

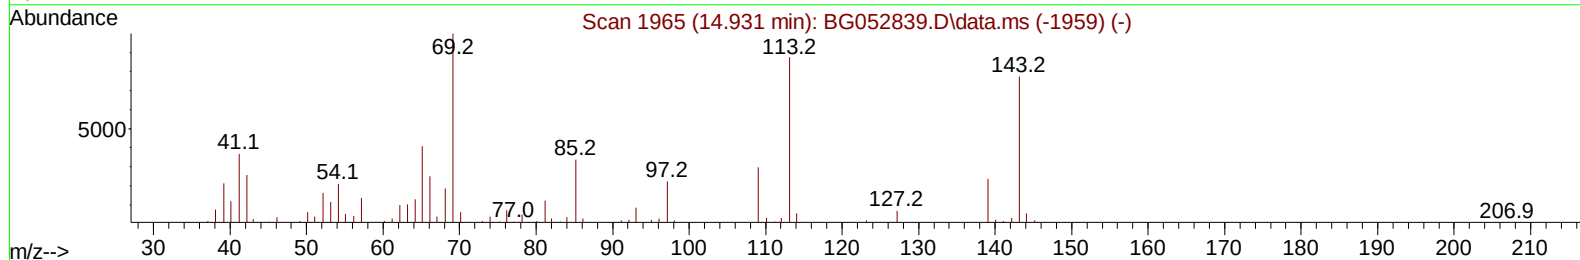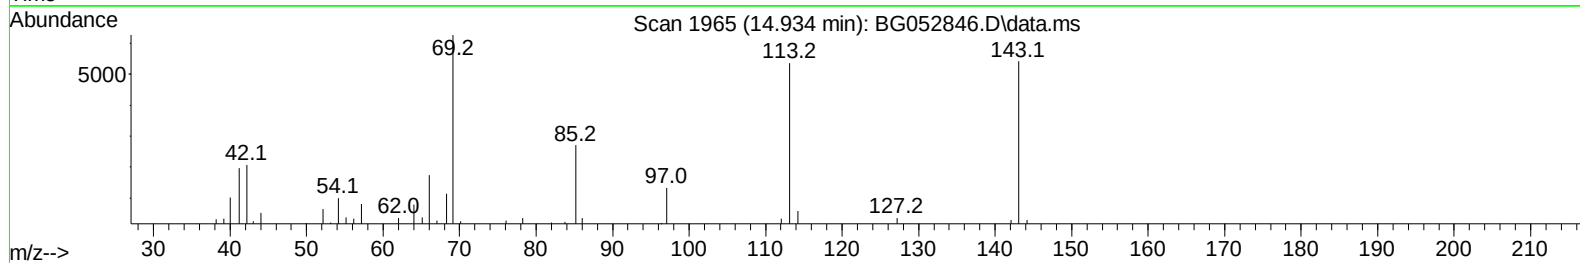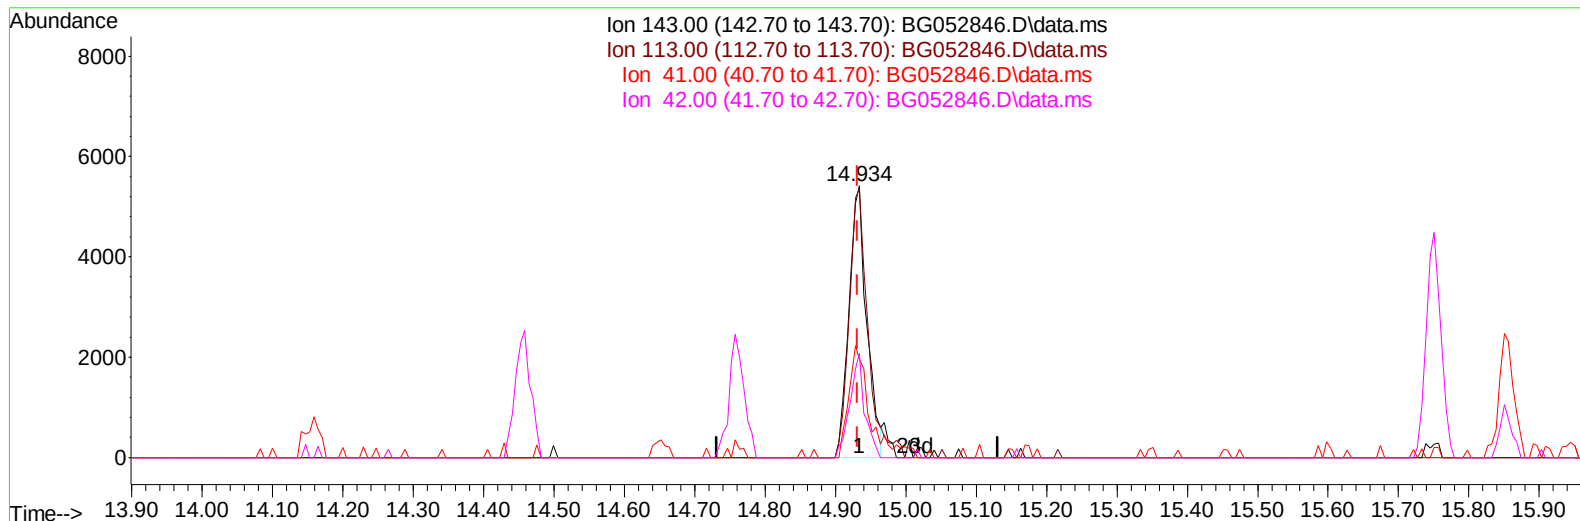

TIC: BG052846.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.934min (+ 0.003) 7.19 ng/ul

response 9427

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	99.02
41.00	47.20	36.19#
42.00	29.40	38.22#

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052846.D
 Acq On : 26 Mar 2022 2:27
 Operator : CG/JU
 Sample : N2079-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW5Z4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 26 05:02:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.143	152	26541	20.000	ng/ul	0.00
20) Naphthalene-d8	10.957	136	124350	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.764	164	101493	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.507	188	253218	20.000	ng/ul	0.00
79) Chrysene-d12	21.789	240	274756	20.000	ng/ul	0.00
88) Perylene-d12	25.108	264	271466	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.549	96	3098	4.123	ng/uL	0.00
4) Pyridine-d5	3.978	84	11075	5.904	ng/ul	0.00
7) Phenol-d5	7.280	99	16258	6.839	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.456	67	50419	34.727	ng/ul	0.00
11) 2-Chlorophenol-d4	7.667	132	41168	25.505	ng/ul	0.00
15) 4-Methylphenol-d8	8.831	113	29944	17.389	ng/ul	0.00
21) Nitrobenzene-d5	9.300	128	29792	33.283	ng/ul	0.00
24) 2-Nitrophenol-d4	10.023	143	33104	35.063	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.563	165	57601	28.044	ng/ul	0.00
31) 4-Chloroaniline-d4	11.080	131	69182	25.485	ng/ul	0.00
46) Dimethylphthalate-d6	14.159	166	262973	33.727	ng/ul	0.00
49) Acenaphthylene-d8	14.452	160	301065	31.776	ng/ul	0.00
54) 4-Nitrophenol-d4	14.934	143	9893m	7.546	ng/ul	0.00
60) Fluorene-d10	15.751	176	234300	34.223	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.856	200	47480	36.845	ng/ul	0.00
73) Anthracene-d10	17.601	188	419349	35.564	ng/ul	0.00
81) Pyrene-d10	19.886	212	520486	33.863	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.879	264	511018	36.432	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052846.D
Acq On : 26 Mar 2022 2:27
Operator : CG/JU
Sample : N2079-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW5Z4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 26 05:02:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

