




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052863.D
 Acq On : 26 Mar 2022 14:06
 Operator : CG/JU
 Sample : N2068-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAYW8

Manual IntegrationsAPPROVED

Quant Time: Mar 28 00:59:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

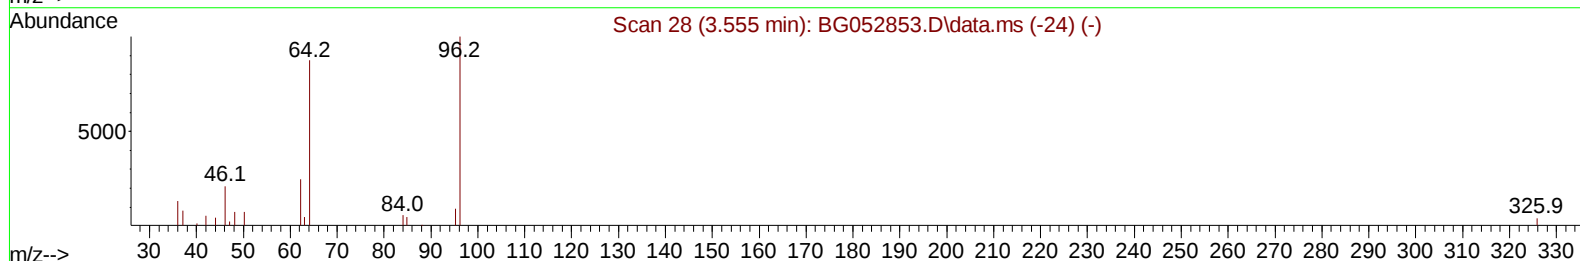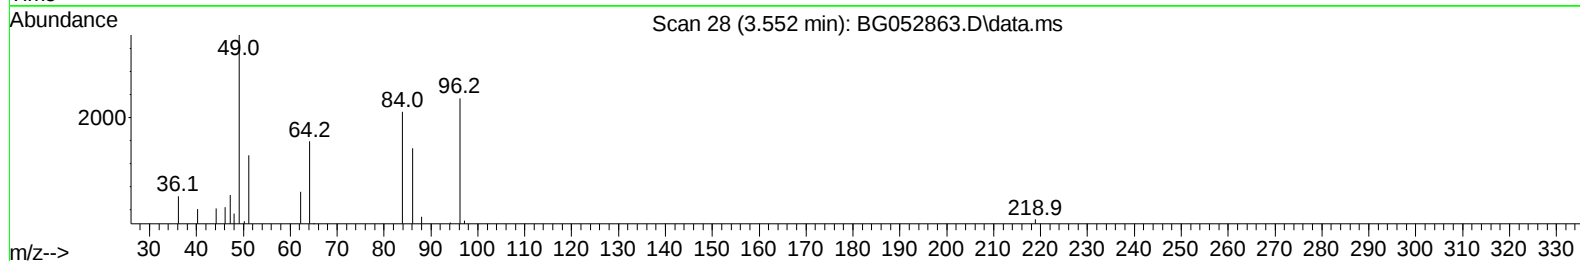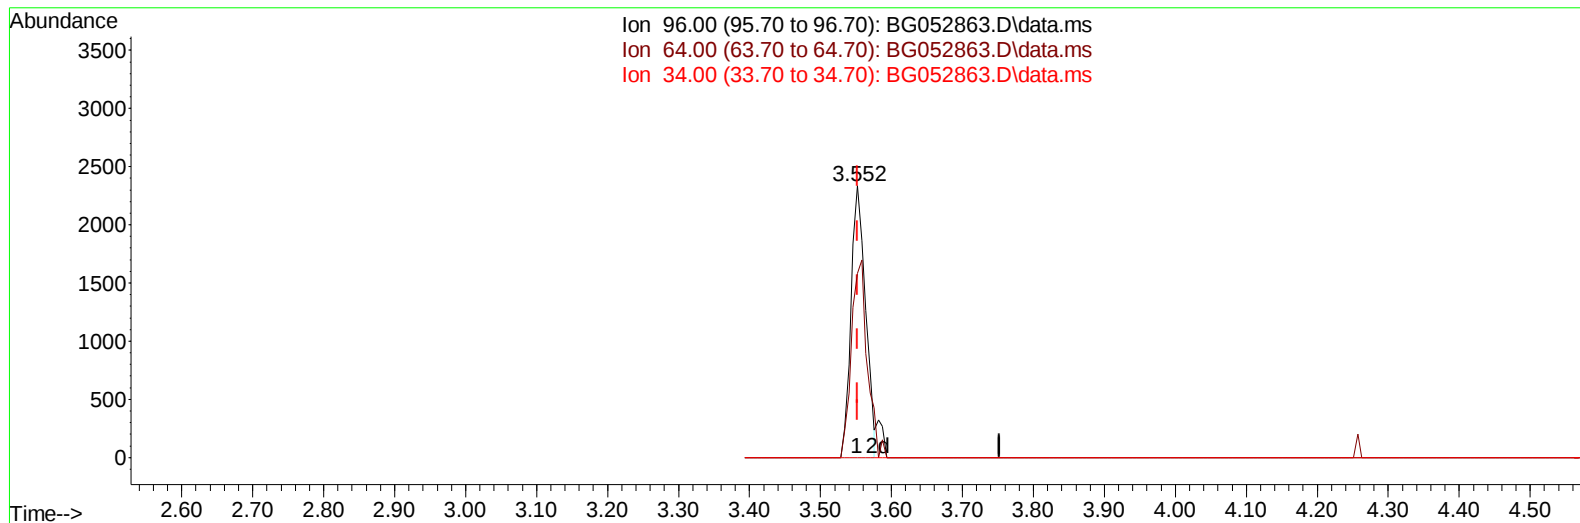

TIC: BG052863.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.552min (-0.000) 3.85 ng/uL

response 3285

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.40	67.91
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052863.D
 Acq On : 26 Mar 2022 14:06
 Operator : CG/JU
 Sample : N2068-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAYW8

Manual IntegrationsAPPROVED

Quant Time: Mar 28 00:59:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

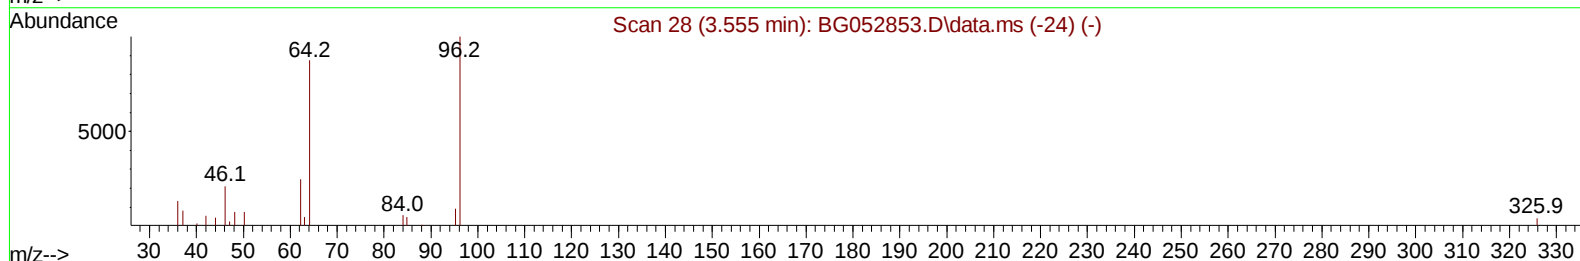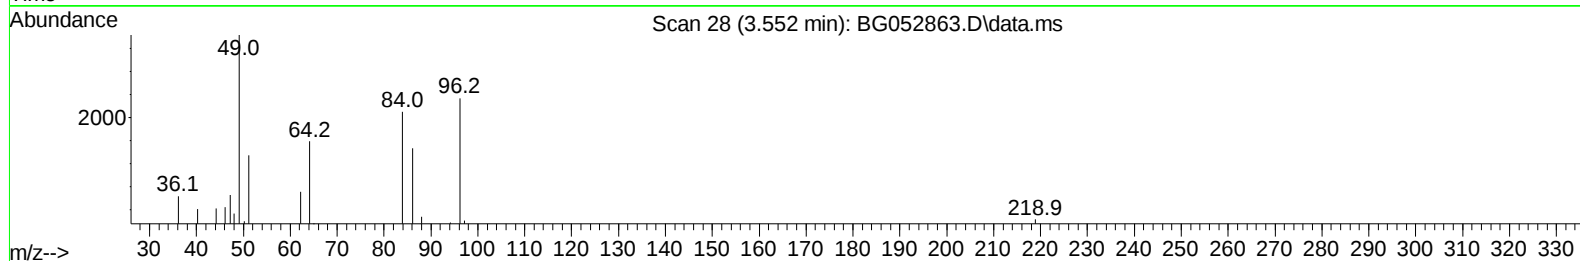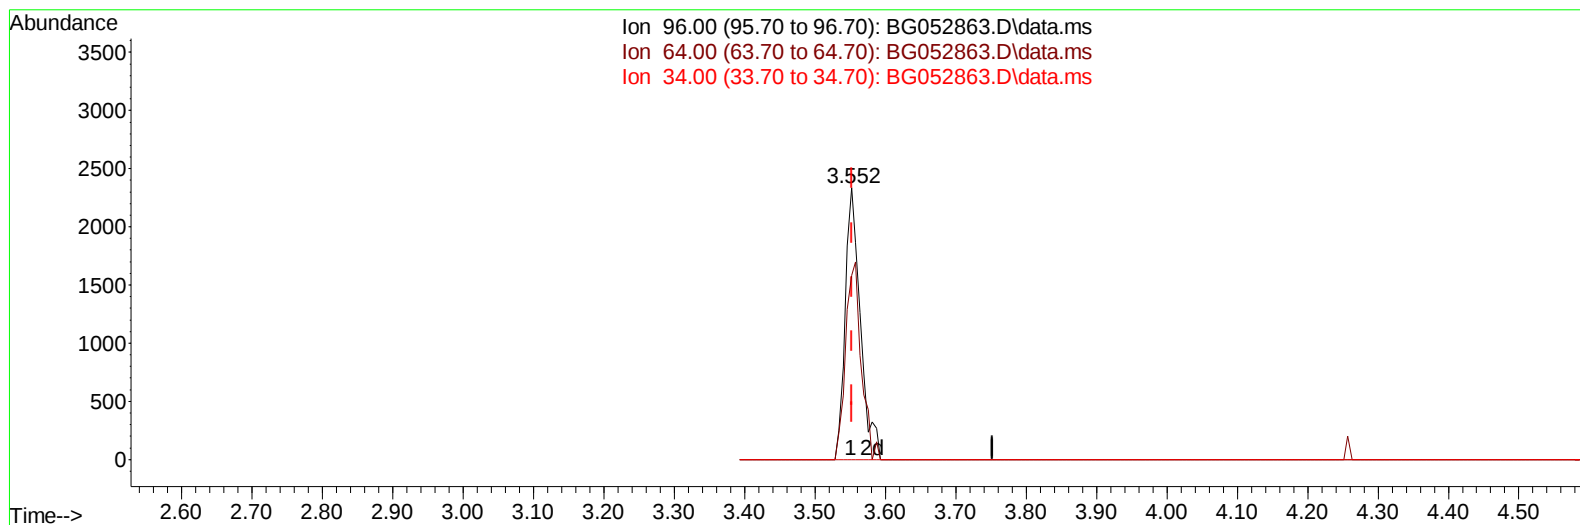

TIC: BG052863.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.552min (-0.000) 4.10 ng/uL m

response 3493

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.40	67.91
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052863.D
Acq On : 26 Mar 2022 14:06
Operator : CG/JU
Sample : N2068-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAYW8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 28 00:59:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

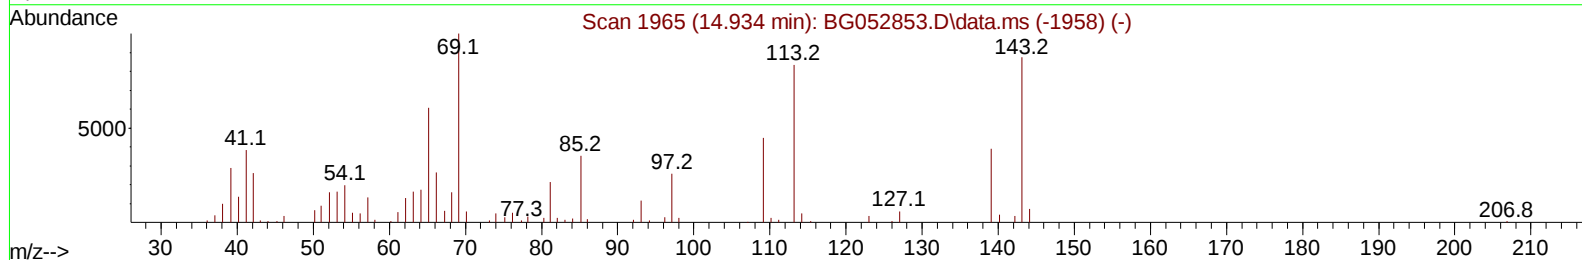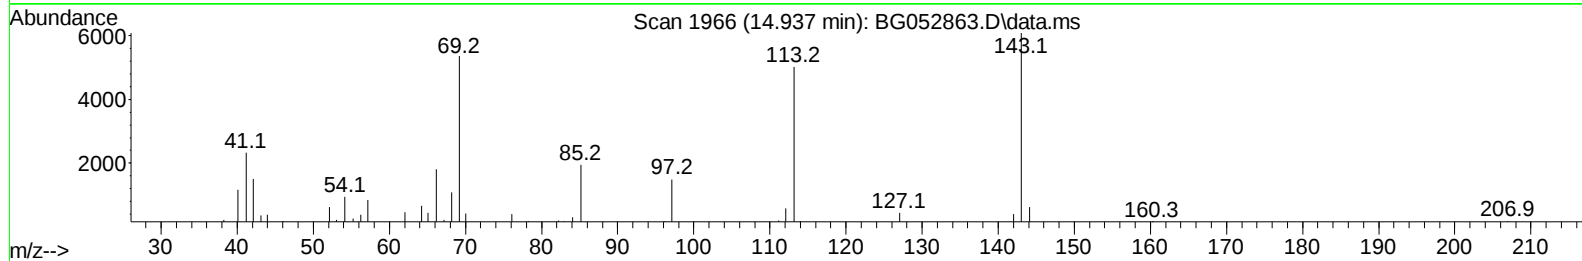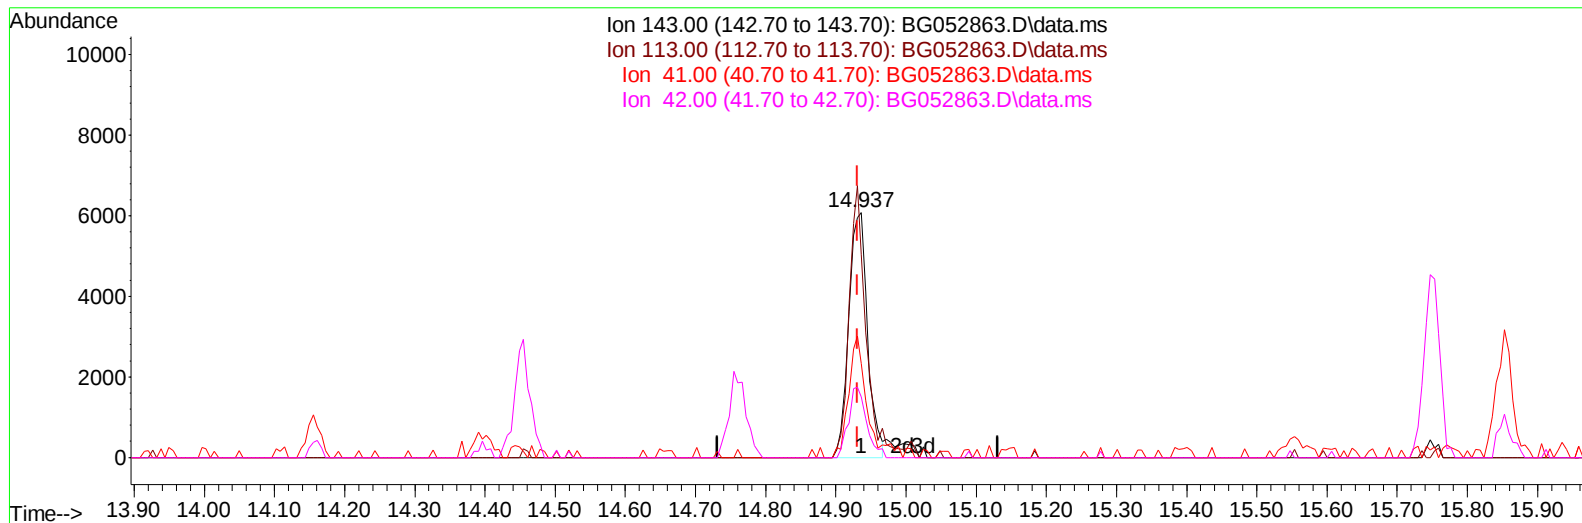

TIC: BG052863.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.937min (+ 0.005) 8.32 ng/u1

response 11343

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	82.64#
41.00	47.20	38.36
42.00	29.40	24.70




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052863.D
Acq On : 26 Mar 2022 14:06
Operator : CG/JU
Sample : N2068-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAYW8

Manual IntegrationsAPPROVED

Quant Time: Mar 28 00:59:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

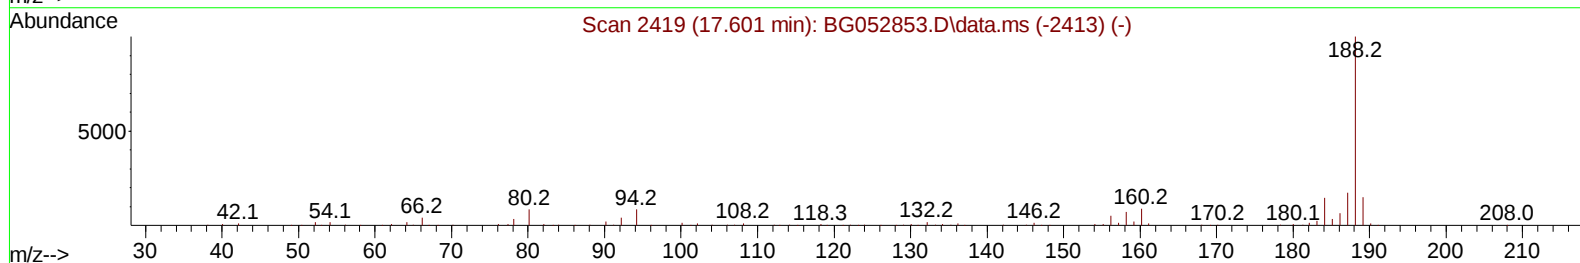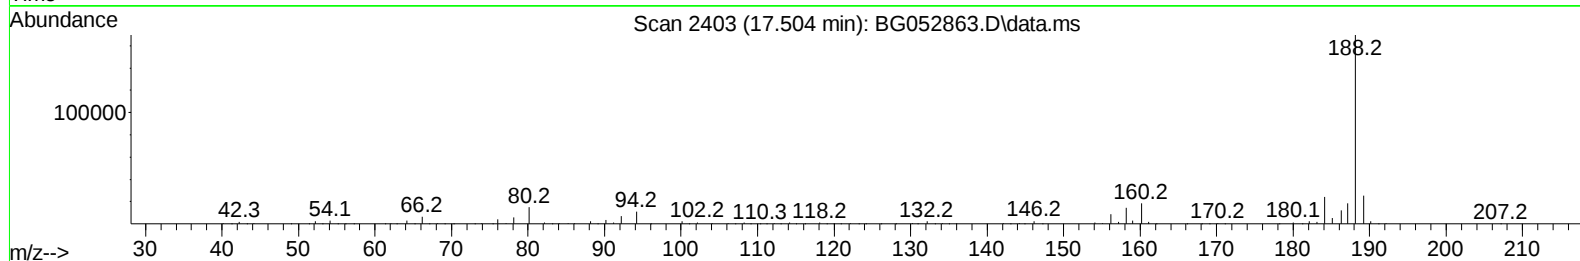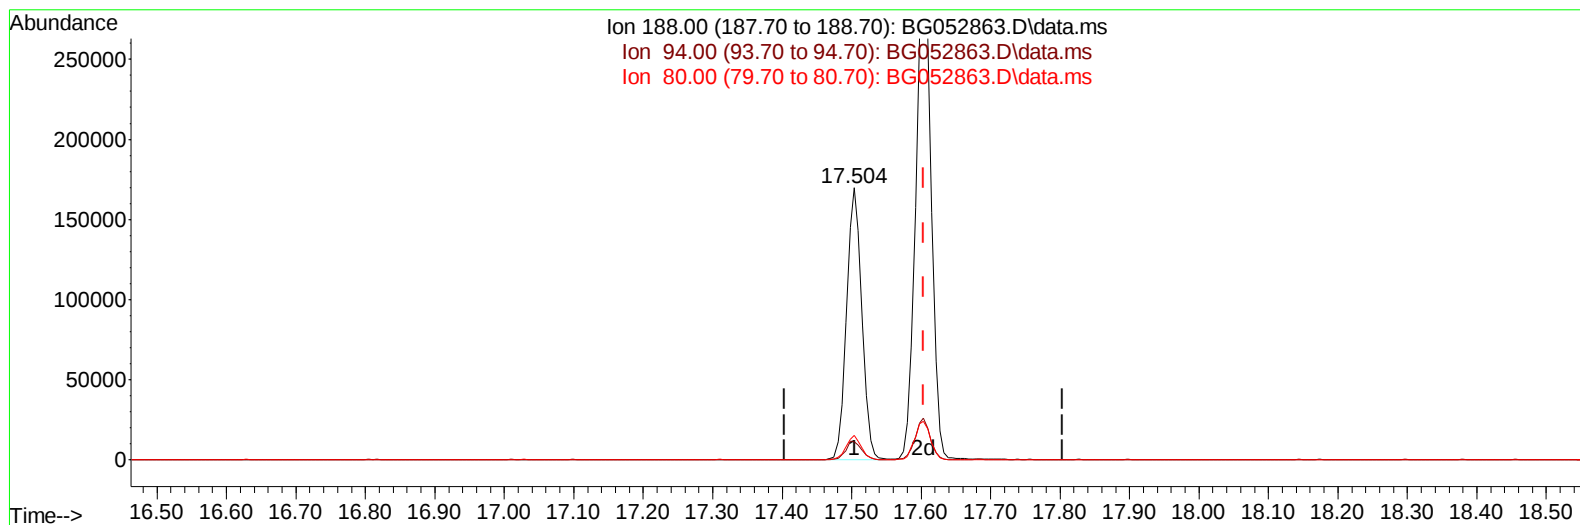

TIC: BG052863.D\data.ms

(73) Anthracene-d10 (S)

17.504min (-0.100) 21.47 ng/u1

response 257429

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.90	6.59
80.00	9.50	8.78
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052863.D
Acq On : 26 Mar 2022 14:06
Operator : CG/JU
Sample : N2068-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAYW8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 28 00:59:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

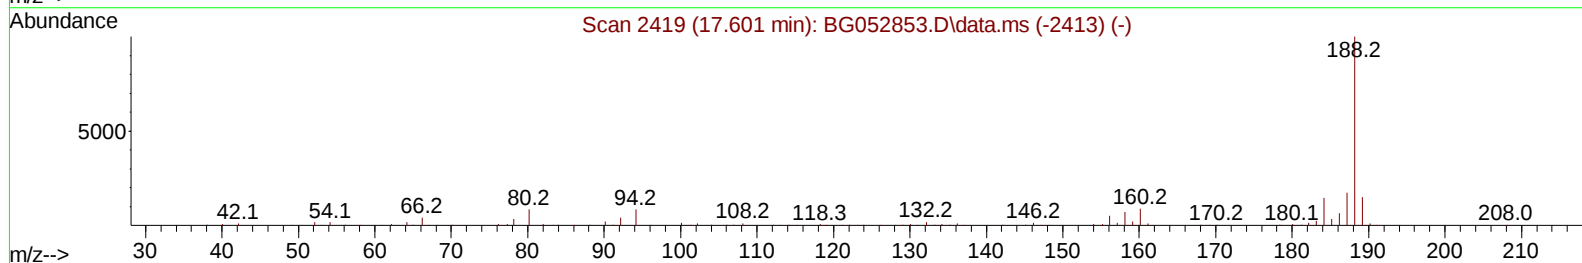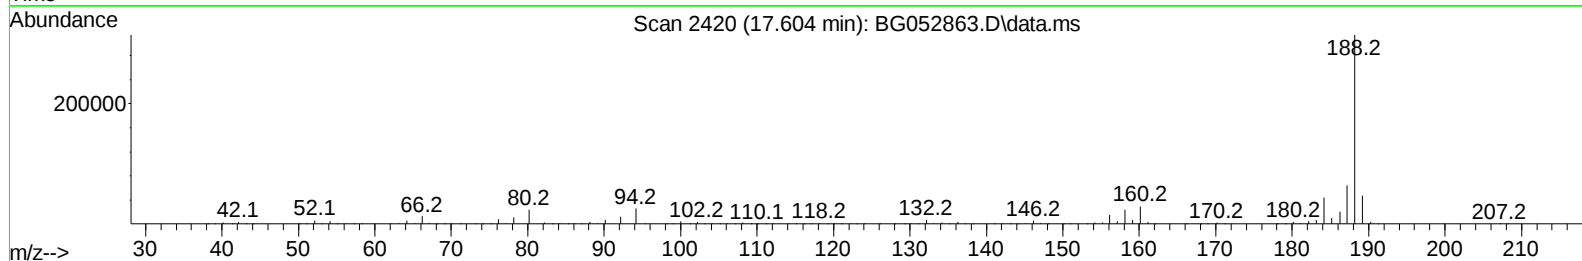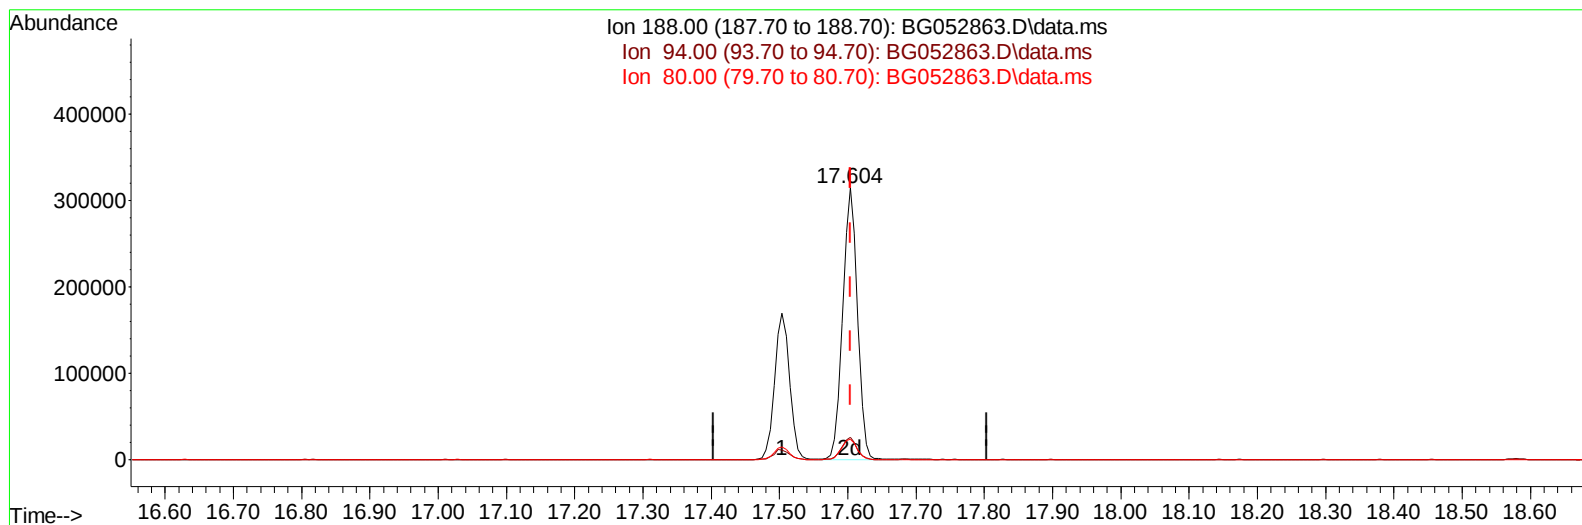

TIC: BG052863.D\data.ms

(73) Anthracene-d10 (S)

17.604min (-0.000) 39.38 ng/ul m

response 472119

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.90	8.18
80.00	9.50	7.52#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052863.D
 Acq On : 26 Mar 2022 14:06
 Operator : CG/JU
 Sample : N2068-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAYW8

Manual IntegrationsAPPROVED

Quant Time: Mar 28 00:59:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.140	152	30103	20.000	ng/ul	0.00
20) Naphthalene-d8	10.954	136	129817	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.760	164	105574	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.504	188	257429	20.000	ng/ul	0.00
79) Chrysene-d12	21.792	240	282964	20.000	ng/ul	0.00
88) Perylene-d12	25.111	264	292387	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.552	96	3493m	4.099	ng/uL	0.00
4) Pyridine-d5	3.975	84	18651	8.766	ng/ul	0.00
7) Phenol-d5	7.288	99	22752	8.439	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.458	67	57962	35.199	ng/ul	0.00
11) 2-Chlorophenol-d4	7.670	132	47539	25.967	ng/ul	0.00
15) 4-Methylphenol-d8	8.833	113	39466	20.207	ng/ul	0.00
21) Nitrobenzene-d5	9.297	128	35530	38.021	ng/ul	0.00
24) 2-Nitrophenol-d4	10.026	143	38590	39.152	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.566	165	68513	31.952	ng/ul	0.00
31) 4-Chloroaniline-d4	11.077	131	88708	31.301	ng/ul	0.00
46) Dimethylphthalate-d6	14.155	166	302770	37.330	ng/ul	0.00
49) Acenaphthylene-d8	14.455	160	336661	34.159	ng/ul	0.00
54) 4-Nitrophenol-d4	14.937	143	11732m	8.603	ng/ul	0.00
60) Fluorene-d10	15.753	176	261273	36.688	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.853	200	54264	41.421	ng/ul	0.00
73) Anthracene-d10	17.604	188	472119m	39.384	ng/ul	0.00
81) Pyrene-d10	19.883	212	575459	36.353	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.882	264	601907	39.841	ng/ul	0.00
Target Compounds						
					Qvalue	
78) Di-n-butylphthalate	18.455	149	18035	1.270	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052863.D
Acq On : 26 Mar 2022 14:06
Operator : CG/JU
Sample : N2068-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAYW8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 28 00:59:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

