




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052873.D
 Acq On : 26 Mar 2022 21:13
 Operator : CG/JU
 Sample : N2068-08
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAZ44

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 28 01:03:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

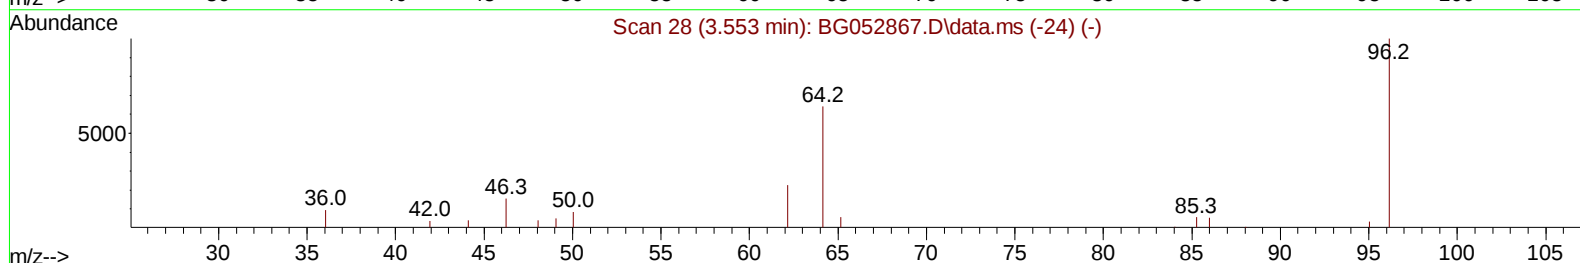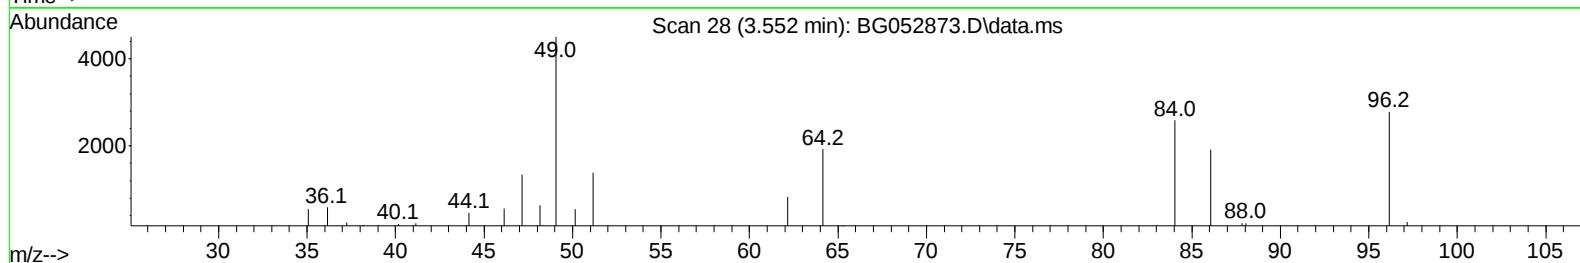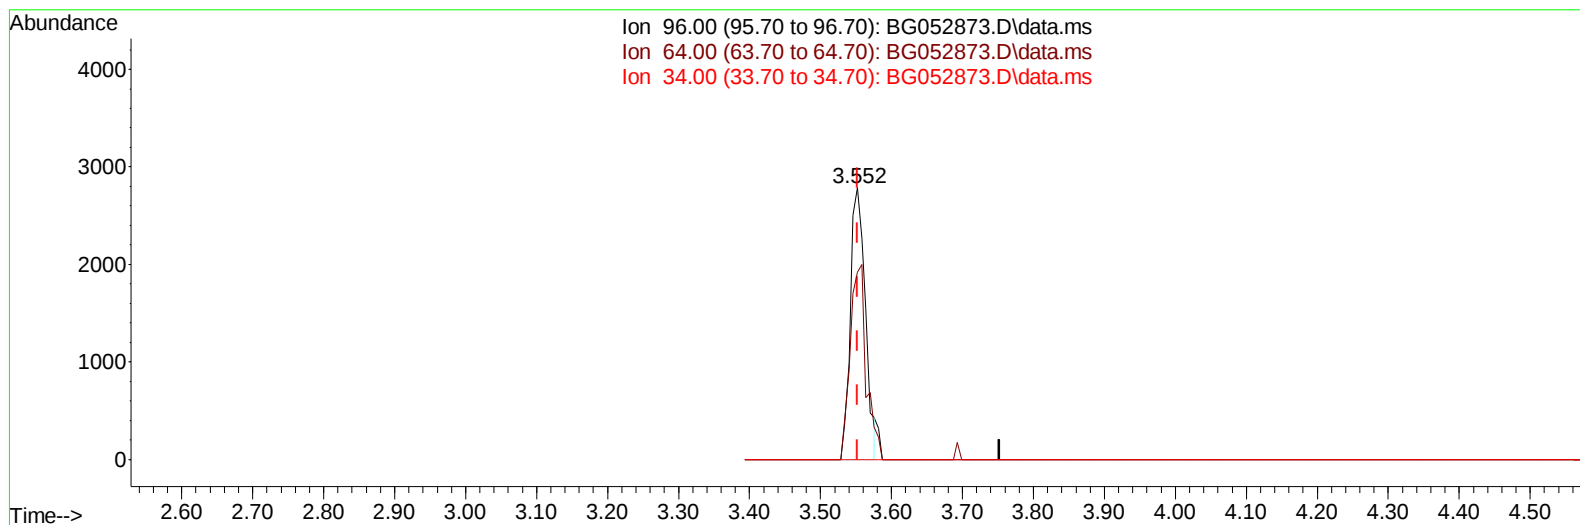

TIC: BG052873.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.552min (-0.000) 5.12 ng/uL

response 4005

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.40	69.07
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052873.D
 Acq On : 26 Mar 2022 21:13
 Operator : CG/JU
 Sample : N2068-08
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAZ44

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 28 01:03:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

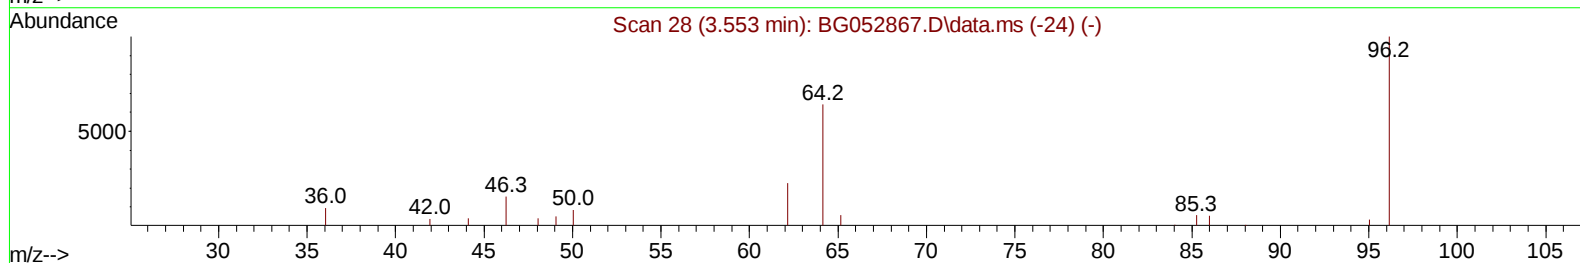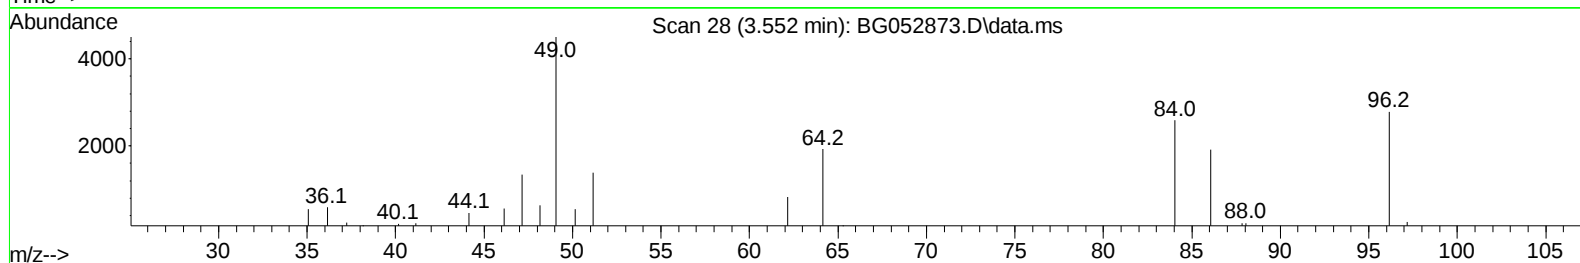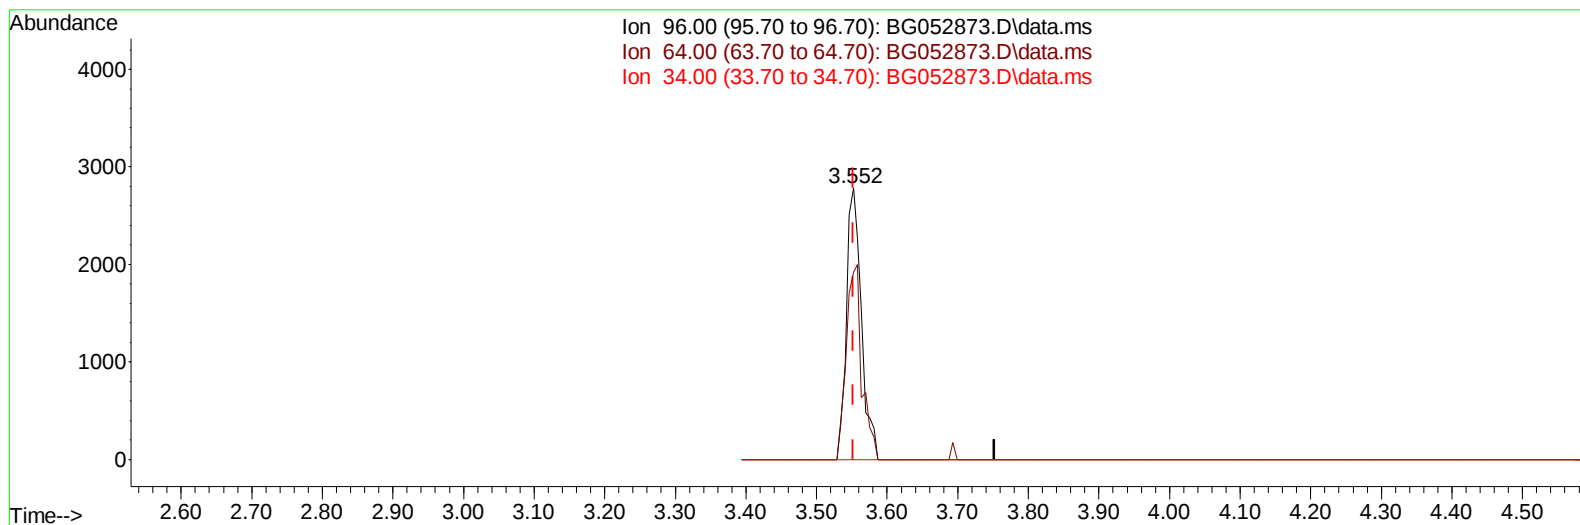

TIC: BG052873.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.552min (-0.000) 5.26 ng/uL m

response 4118

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	83.40	69.07
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052873.D
 Acq On : 26 Mar 2022 21:13
 Operator : CG/JU
 Sample : N2068-08
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAZ44

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 28 01:03:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.140	152	27650	20.000	ng/ul	0.00
20) Naphthalene-d8	10.954	136	125281	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.760	164	105016	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.504	188	256003	20.000	ng/ul	0.00
79) Chrysene-d12	21.792	240	283666	20.000	ng/ul	# 0.00
88) Perylene-d12	25.105	264	289410	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.552	96	4118m	5.261	ng/uL	0.00
4) Pyridine-d5	3.969	84	27523	14.084	ng/ul	0.00
7) Phenol-d5	7.288	99	34947	14.112	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.458	67	58759	38.848	ng/ul	0.00
11) 2-Chlorophenol-d4	7.670	132	52588	31.273	ng/ul	0.00
15) 4-Methylphenol-d8	8.833	113	45140	25.163	ng/ul	0.00
21) Nitrobenzene-d5	9.297	128	35328	39.174	ng/ul	0.00
24) 2-Nitrophenol-d4	10.026	143	39143	41.151	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.566	165	72345	34.961	ng/ul	0.00
31) 4-Chloroaniline-d4	11.077	131	83258	30.442	ng/ul	0.00
46) Dimethylphthalate-d6	14.155	166	320296	39.701	ng/ul	0.00
49) Acenaphthylene-d8	14.455	160	351643	35.869	ng/ul	0.00
54) 4-Nitrophenol-d4	14.925	143	22508	16.593	ng/ul	0.00
60) Fluorene-d10	15.747	176	277928	39.234	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.853	200	61750	47.398	ng/ul	0.00
73) Anthracene-d10	17.604	188	498552	41.821	ng/ul	0.00
81) Pyrene-d10	19.883	212	646603	40.747	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.882	264	690925	46.204	ng/ul	0.00
Target Compounds						
					Qvalue	
78) Di-n-butylphthalate	18.455	149	17150	1.215	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052873.D
Acq On : 26 Mar 2022 21:13
Operator : CG/JU
Sample : N2068-08
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAZ44

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 28 01:03:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

