




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG032522\  
 Data File : BG052882.D  
 Acq On : 27 Mar 2022 3:06  
 Operator : CG/JU  
 Sample : SSTDCCC020EC  
 Misc :  
 ALS Vial : 61 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 LabSampleId :  
 SSTDCCC020EC

Manual IntegrationsAPPROVED

Quant Time: Mar 28 01:05:47 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG031822.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Mar 23 13:16:32 2022  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022  
 Supervised By :mohammad ahmed 03/29/2022

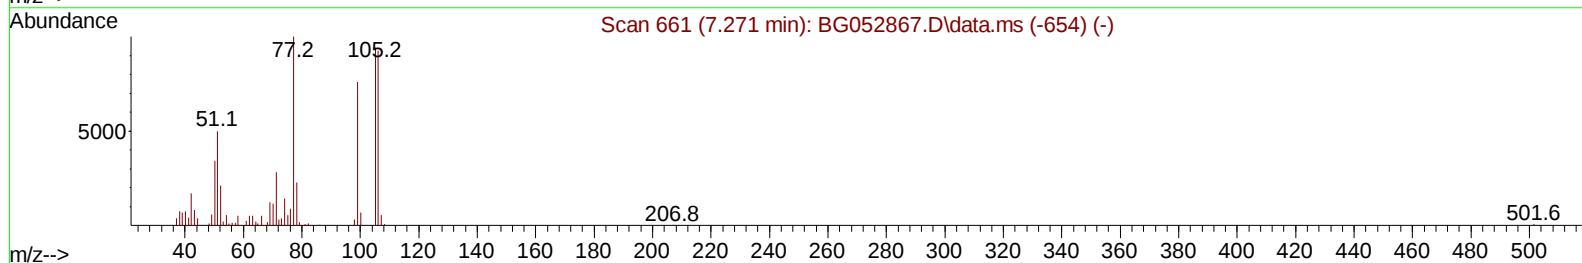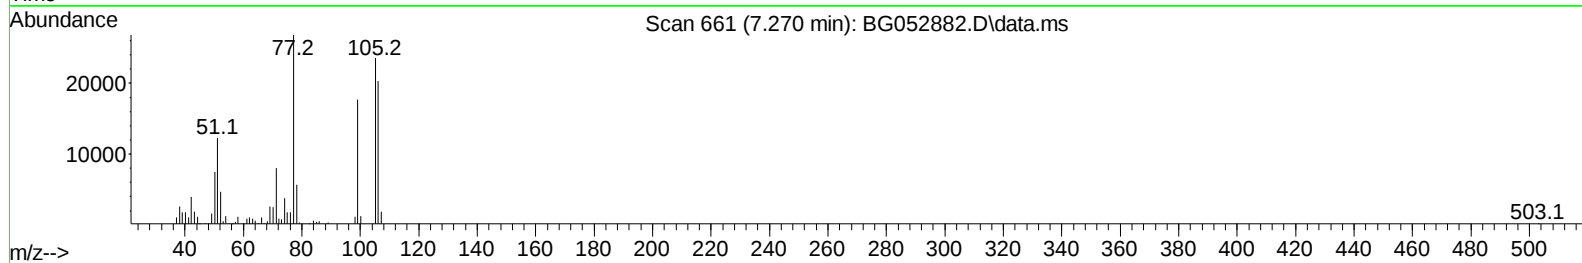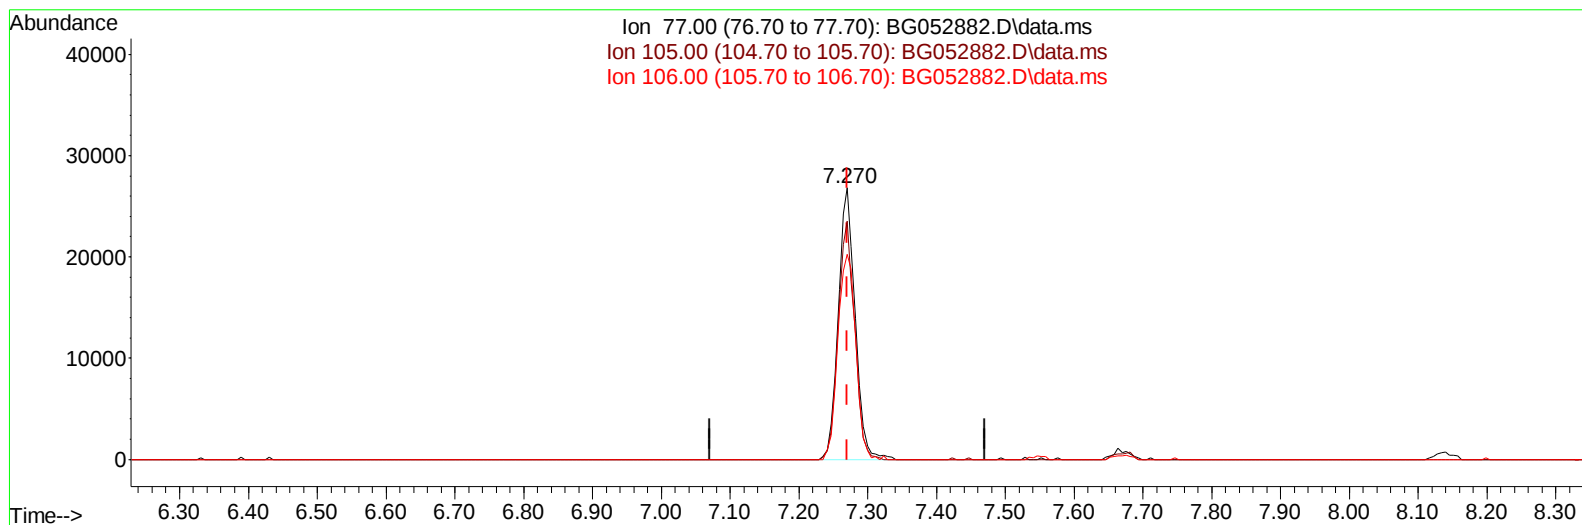

TIC: BG052882.D\data.ms

#### (6) Benzaldehyde

7.270min (-0.000) 22.44 ng/u1

response 45857

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 77.00  | 100.00 | 100.00 |
| 105.00 | 91.10  | 87.94  |
| 106.00 | 83.10  | 75.62  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG032522\  
 Data File : BG052882.D  
 Acq On : 27 Mar 2022 3:06  
 Operator : CG/JU  
 Sample : SSTDCCC020EC  
 Misc :  
 ALS Vial : 61 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 LabSampleId :  
 SSTDCCC020EC

Manual IntegrationsAPPROVED

Quant Time: Mar 28 01:05:47 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG031822.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Mar 23 13:16:32 2022  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022  
 Supervised By :mohammad ahmed 03/29/2022

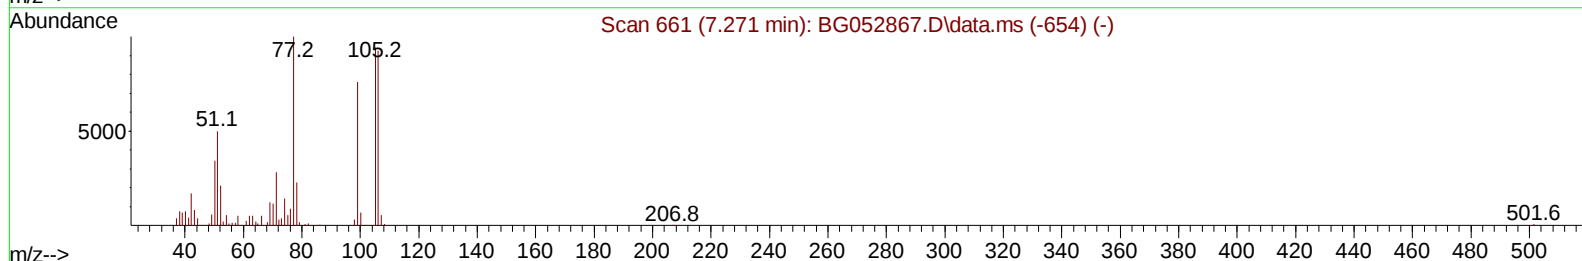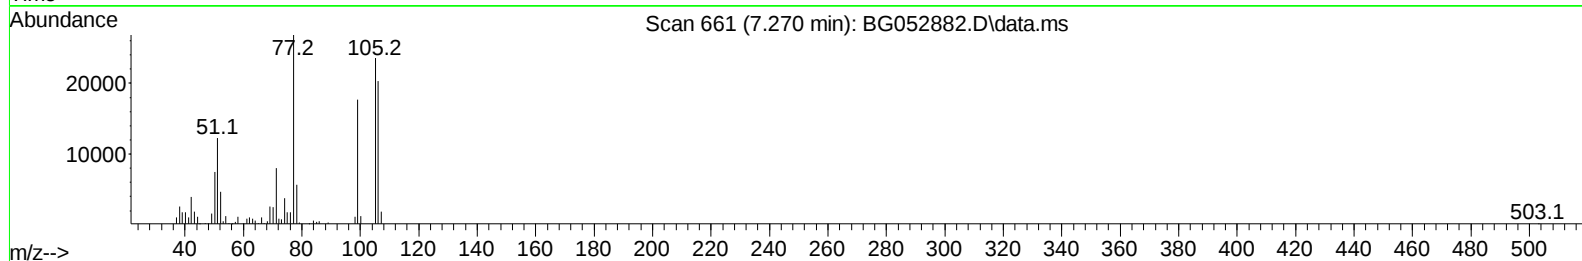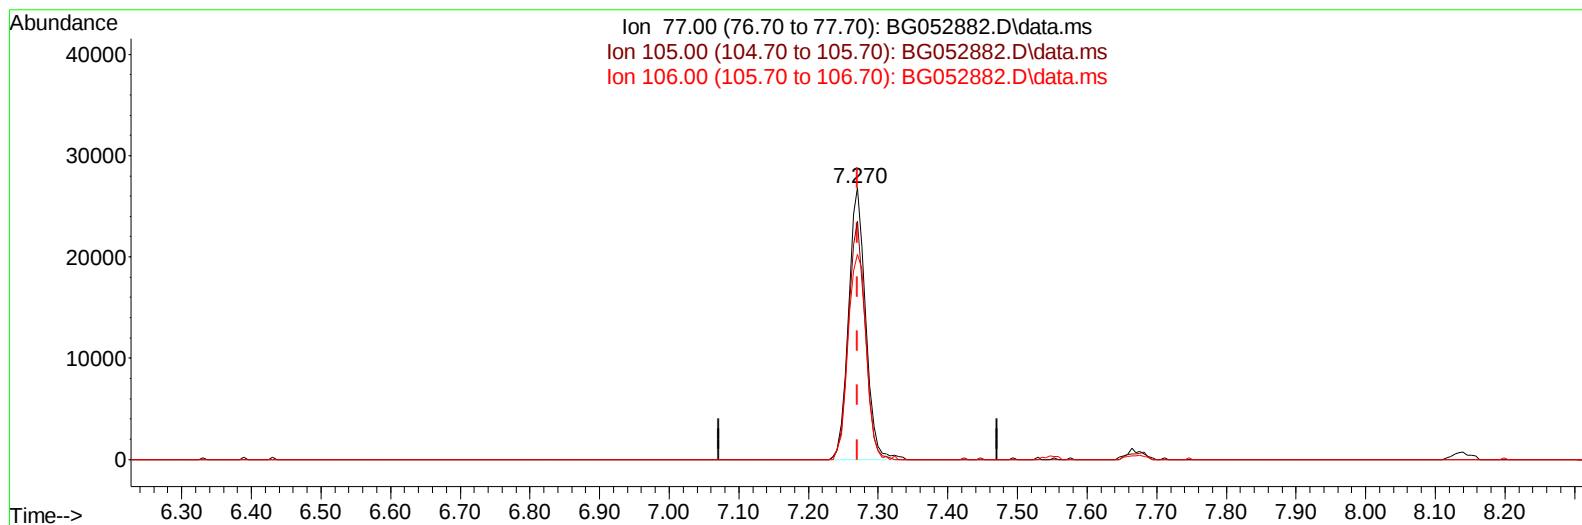

TIC: BG052882.D\data.ms

#### (6) Benzaldehyde

7.270min (-0.000) 22.21 ng/ul m

response 45381

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 77.00  | 100.00 | 100.00 |
| 105.00 | 91.10  | 87.94  |
| 106.00 | 83.10  | 75.62  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG032522\  
Data File : BG052882.D  
Acq On : 27 Mar 2022 3:06  
Operator : CG/JU  
Sample : SSTDCCC020EC  
Misc :  
ALS Vial : 61 Sample Multiplier: 1

Instrument :  
BNA\_G  
LabSampleId :  
SSTDCCC020EC

Manual IntegrationsAPPROVED

Quant Time: Mar 28 01:05:47 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG031822.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Mar 23 13:16:32 2022  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022  
Supervised By :mohammad ahmed 03/29/2022

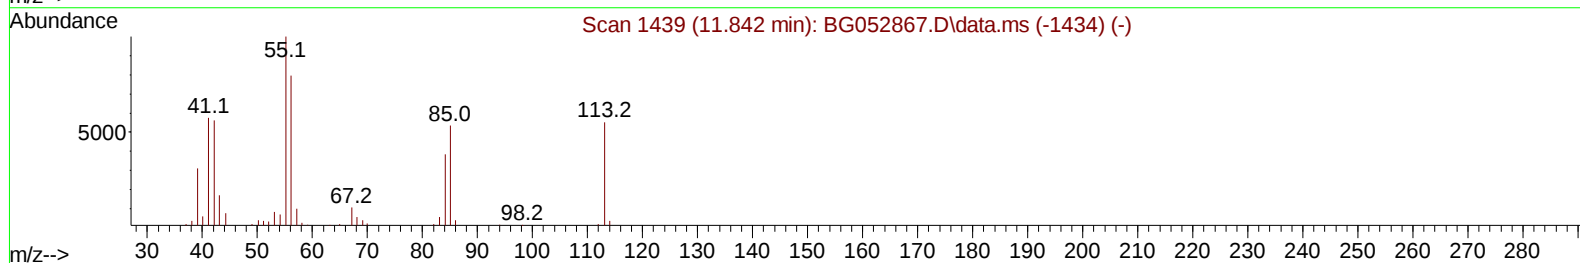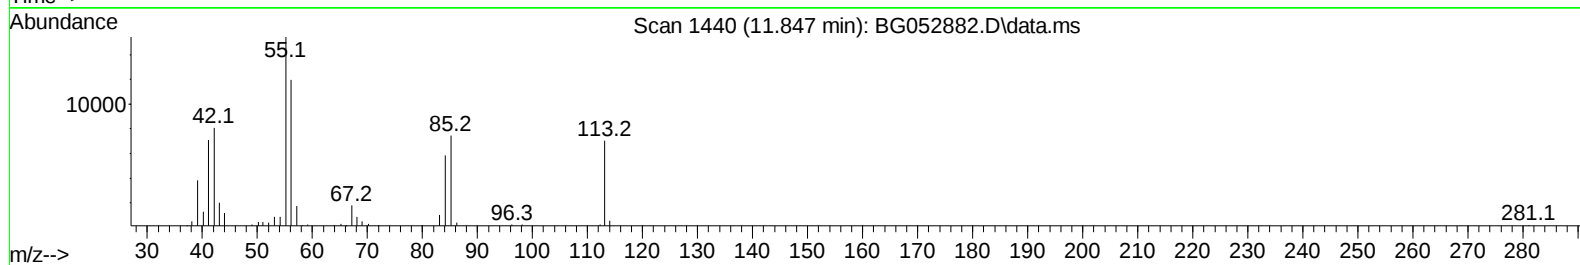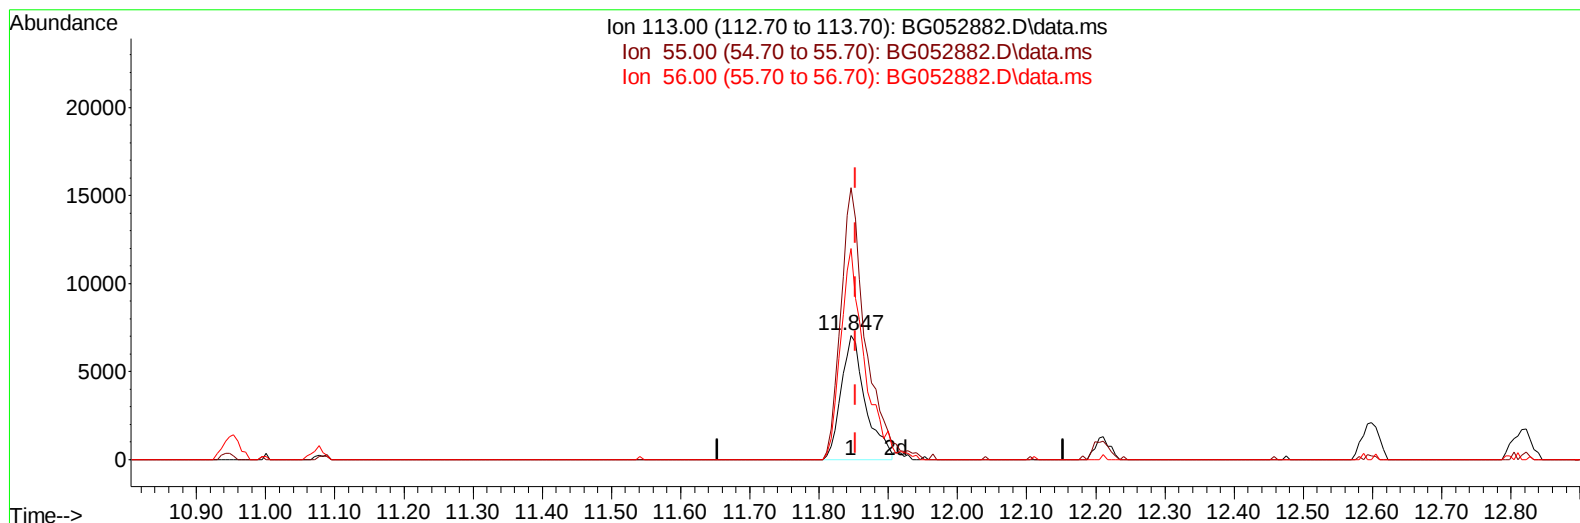

TIC: BG052882.D\data.ms

(34) Caprolactam

11.847min (-0.006) 23.52 ng/ul

response 17093

| Ion    | Exp%   | Act%    |
|--------|--------|---------|
| 113.00 | 100.00 | 100.00  |
| 55.00  | 177.50 | 218.96# |
| 56.00  | 120.10 | 169.98# |
| 0.00   | 0.00   | 0.00    |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG032522\  
Data File : BG052882.D  
Acq On : 27 Mar 2022 3:06  
Operator : CG/JU  
Sample : SSTDCCC020EC  
Misc :  
ALS Vial : 61 Sample Multiplier: 1

Instrument :  
BNA\_G  
LabSampleId :  
SSTDCCC020EC

Manual IntegrationsAPPROVED

Quant Time: Mar 28 01:05:47 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG031822.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Mar 23 13:16:32 2022  
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022  
Supervised By :mohammad ahmed 03/29/2022

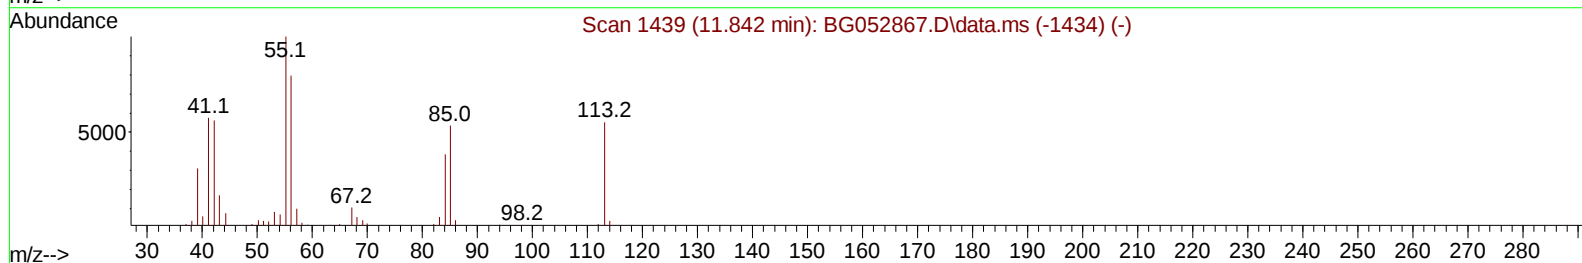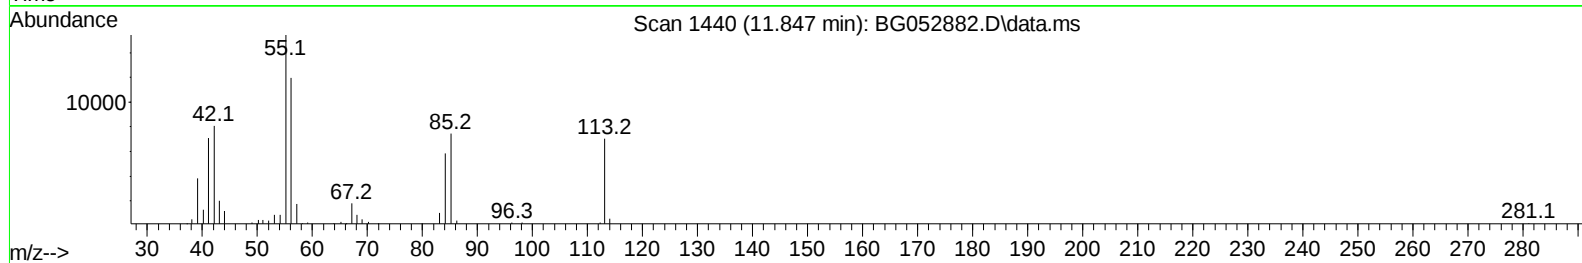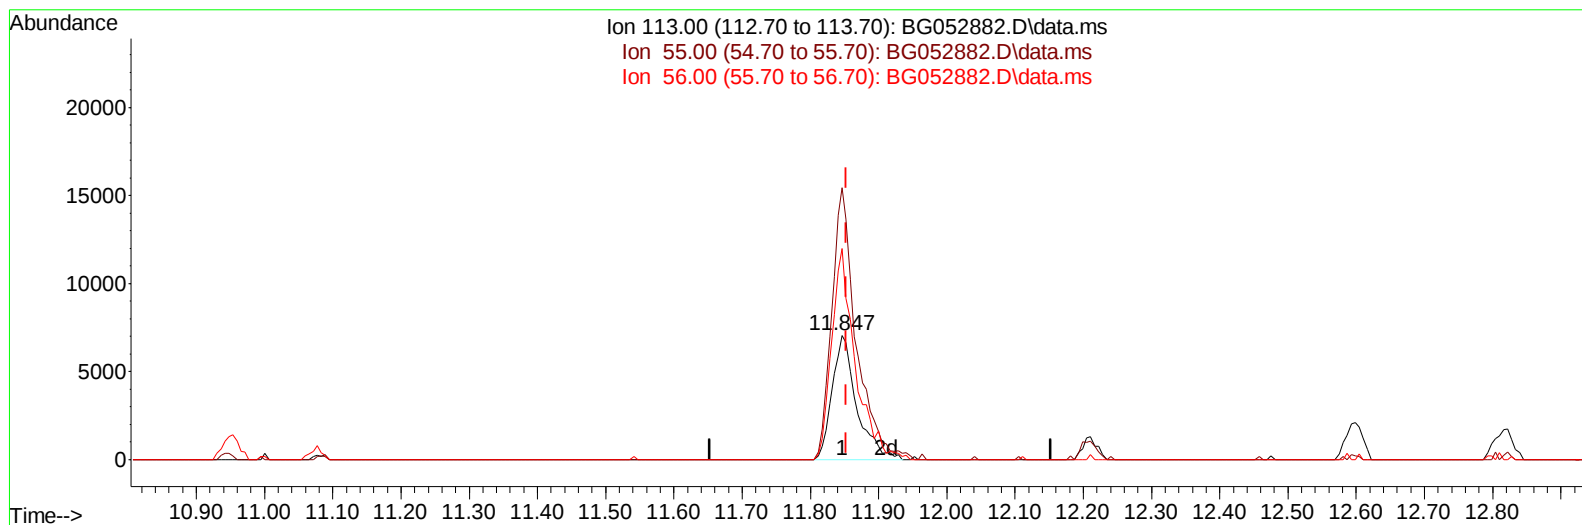

TIC: BG052882.D\data.ms

(34) Caprolactam

11.847min (-0.006) 24.12 ng/ul m

response 17533

| Ion    | Exp%   | Act%    |
|--------|--------|---------|
| 113.00 | 100.00 | 100.00  |
| 55.00  | 177.50 | 218.96# |
| 56.00  | 120.10 | 169.98# |
| 0.00   | 0.00   | 0.00    |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG032522\  
 Data File : BG052882.D  
 Acq On : 27 Mar 2022 3:06  
 Operator : CG/JU  
 Sample : SSTDCCC020EC  
 Misc :  
 ALS Vial : 61 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 LabSampleId :  
 SSTDCCC020EC

Manual IntegrationsAPPROVED

Quant Time: Mar 28 01:05:47 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG031822.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Mar 23 13:16:32 2022  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022  
 Supervised By :mohammad ahmed 03/29/2022

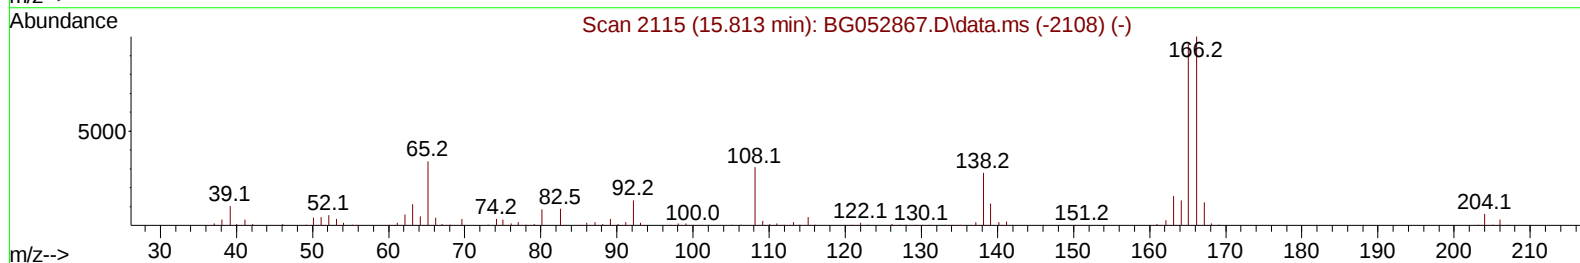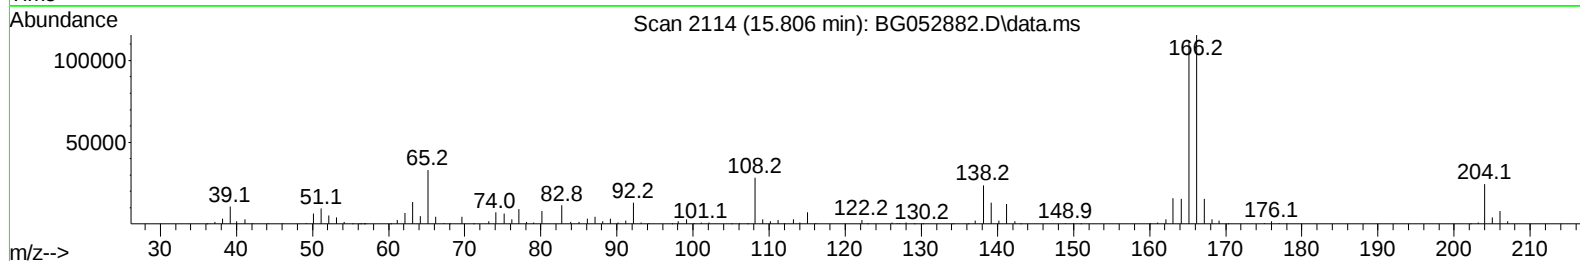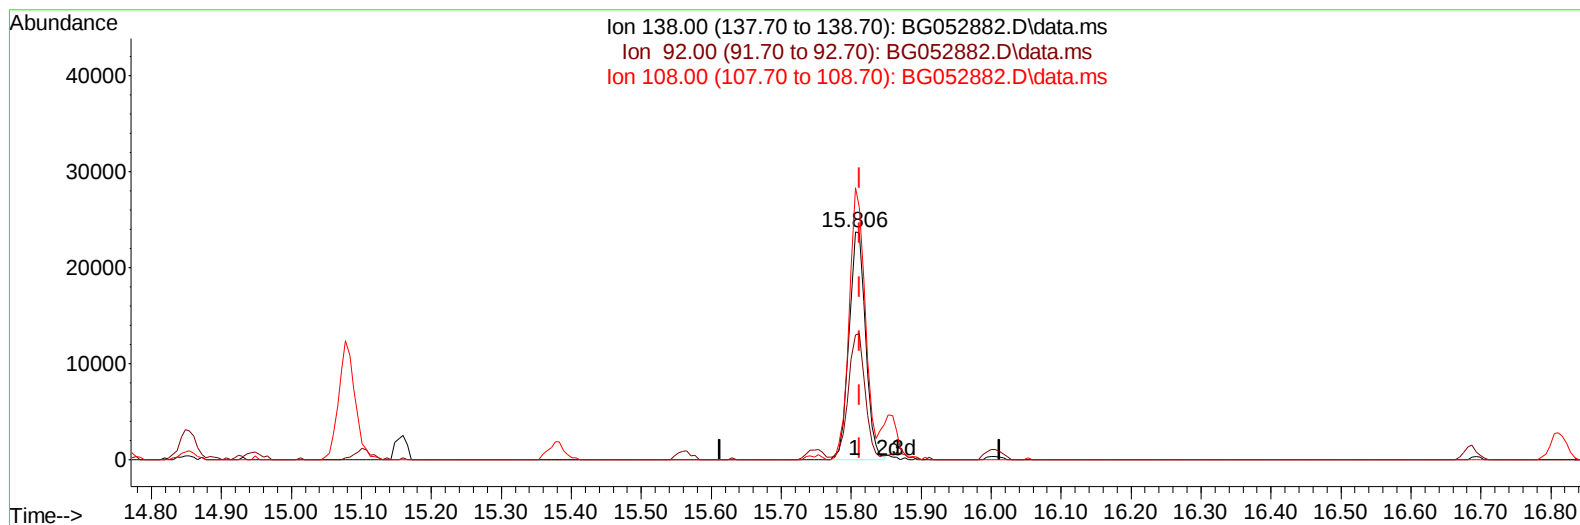

TIC: BG052882.D\data.ms

**(63) 4-Nitroaniline**

**15.806min (-0.006) 23.98 ng/ul**

**response 38736**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 138.00 | 100.00 | 100.00 |
| 92.00  | 53.80  | 54.84  |
| 108.00 | 105.70 | 119.40 |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG032522\  
 Data File : BG052882.D  
 Acq On : 27 Mar 2022 3:06  
 Operator : CG/JU  
 Sample : SSTDCCC020EC  
 Misc :  
 ALS Vial : 61 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 LabSampleId :  
 SSTDCCC020EC

Manual IntegrationsAPPROVED

Quant Time: Mar 28 01:05:47 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG031822.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Mar 23 13:16:32 2022  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022  
 Supervised By :mohammad ahmed 03/29/2022

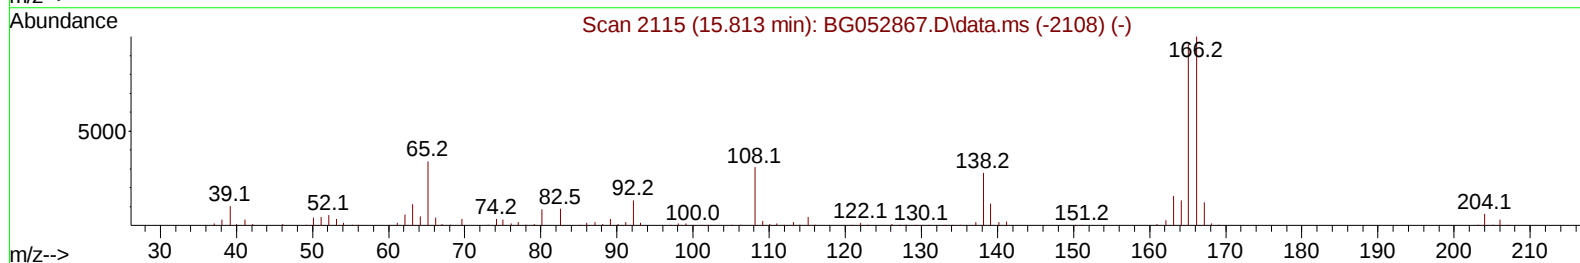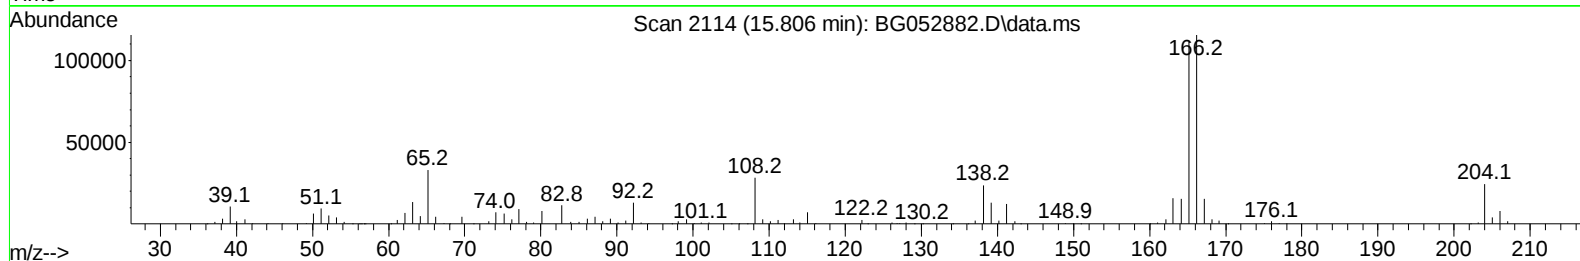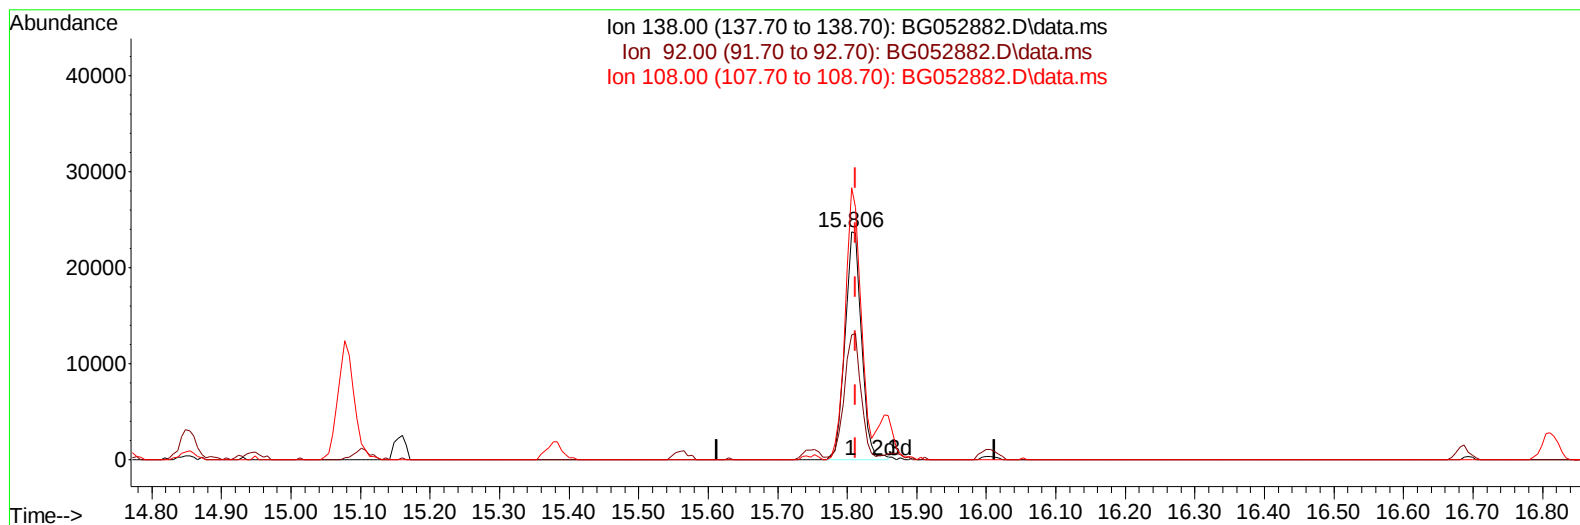

TIC: BG052882.D\data.ms

**(63) 4-Nitroaniline**

**15.806min (-0.006) 24.13 ng/ul m**

**response 38972**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 138.00 | 100.00 | 100.00 |
| 92.00  | 53.80  | 54.84  |
| 108.00 | 105.70 | 119.40 |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG032522\  
 Data File : BG052882.D  
 Acq On : 27 Mar 2022 3:06  
 Operator : CG/JU  
 Sample : SSTDCCC020EC  
 Misc :  
 ALS Vial : 61 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 LabSampleId :  
 SSTDCCC020EC

Manual IntegrationsAPPROVED

Quant Time: Mar 28 01:05:47 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG031822.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Mar 23 13:16:32 2022  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022  
 Supervised By :mohammad ahmed 03/29/2022

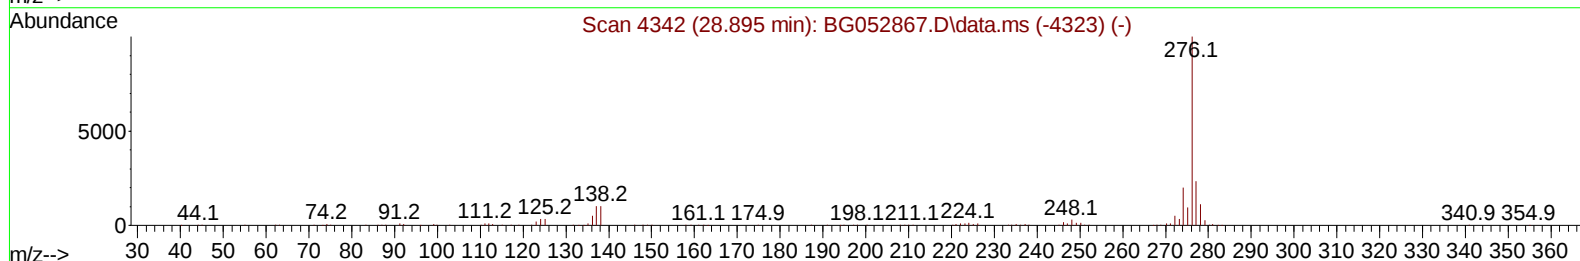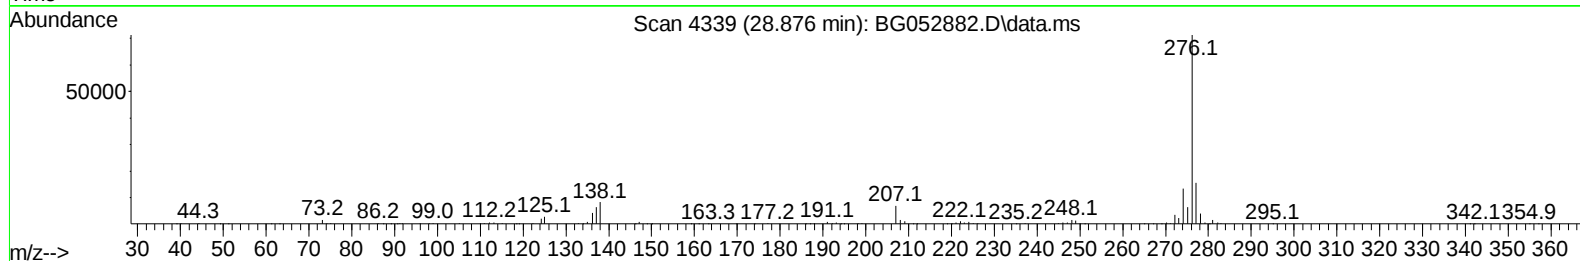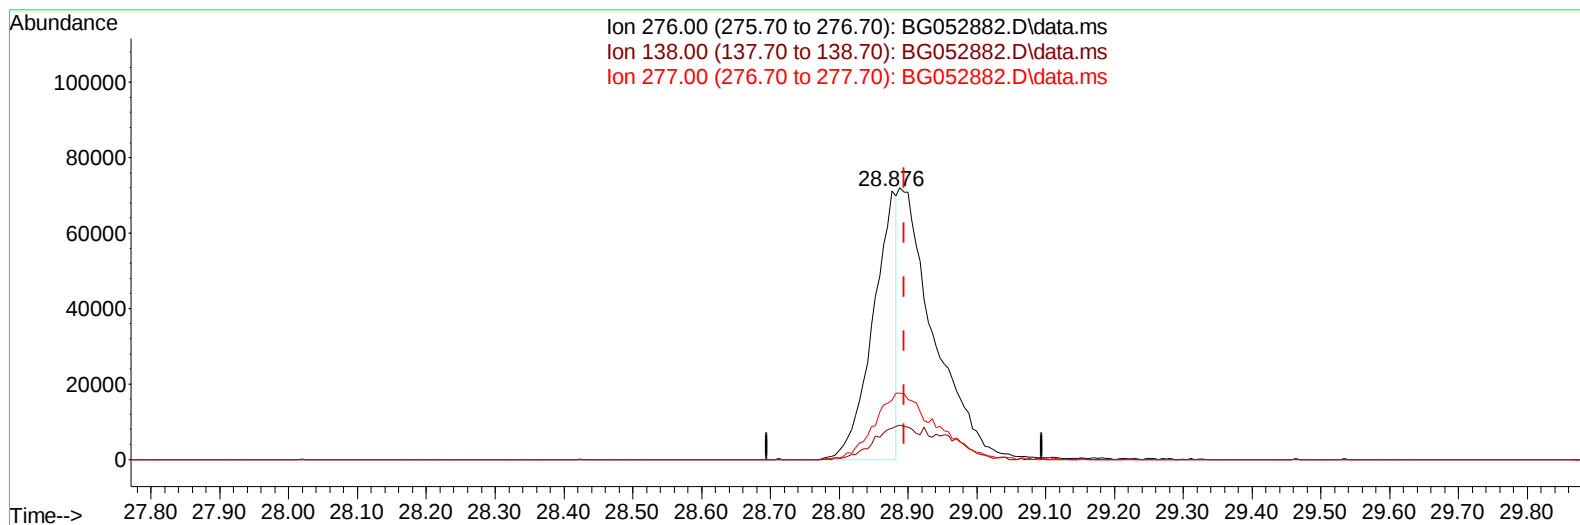

TIC: BG052882.D\data.ms

**(94) Indeno(1,2,3-cd)pyrene**

28.876min (-0.018) 7.83 ng/u1

response 169926

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 276.00 | 100.00 | 100.00 |
| 138.00 | 11.60  | 11.60  |
| 277.00 | 24.30  | 21.99  |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG032522\  
 Data File : BG052882.D  
 Acq On : 27 Mar 2022 3:06  
 Operator : CG/JU  
 Sample : SSTDCCC020EC  
 Misc :  
 ALS Vial : 61 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 LabSampleId :  
 SSTDCCC020EC

Manual IntegrationsAPPROVED

Quant Time: Mar 28 01:05:47 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG031822.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Mar 23 13:16:32 2022  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022  
 Supervised By :mohammad ahmed 03/29/2022

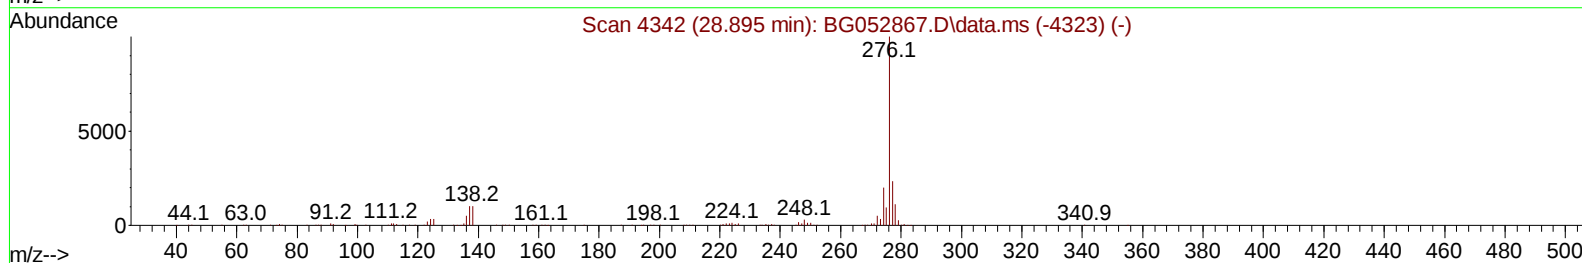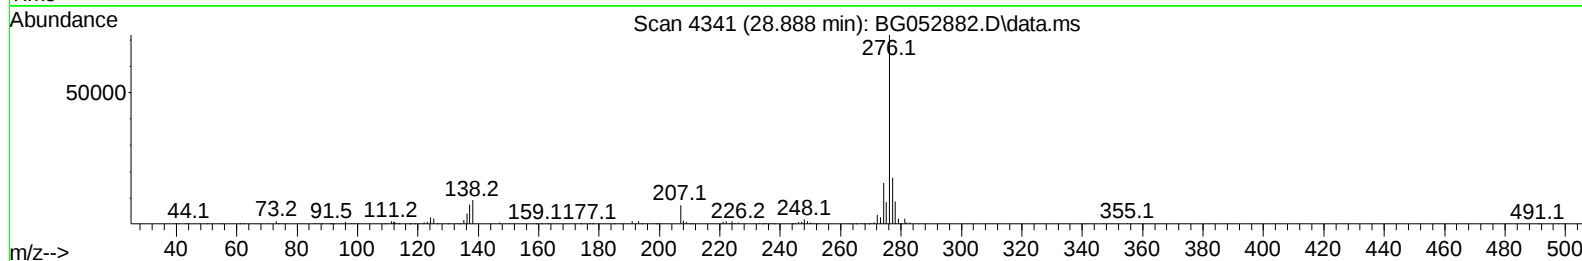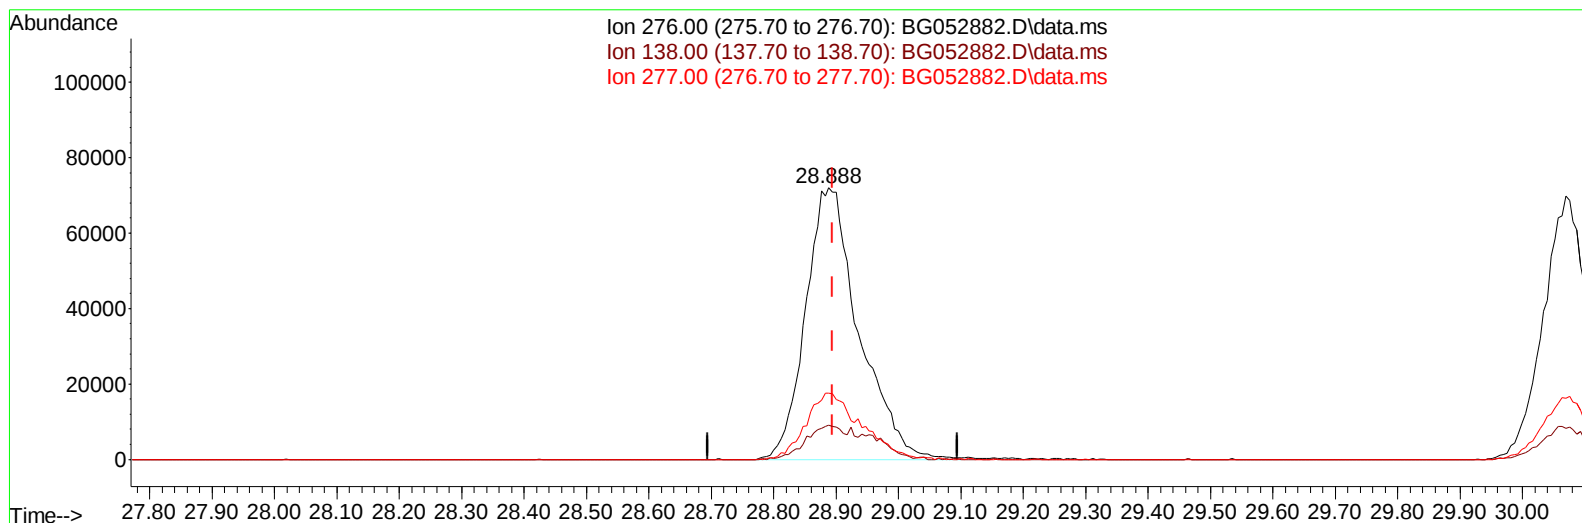

TIC: BG052882.D\data.ms

**(94) Indeno(1,2,3-cd)pyrene**

**28.888min (-0.006) 19.69 ng/ul m**

**response 427320**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 276.00 | 100.00 | 100.00 |
| 138.00 | 11.60  | 12.72  |
| 277.00 | 24.30  | 24.41  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG032522\  
 Data File : BG052882.D  
 Acq On : 27 Mar 2022 3:06  
 Operator : CG/JU  
 Sample : SSTDCCC020EC  
 Misc :  
 ALS Vial : 61 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 LabSampleId :  
 SSTDCCC020EC

Manual IntegrationsAPPROVED

Quant Time: Mar 28 01:05:47 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG031822.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Mar 23 13:16:32 2022  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022  
 Supervised By :mohammad ahmed 03/29/2022

| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| -----                         |        |      |          |        |        |          |
| Internal Standards            |        |      |          |        |        |          |
| 1) 1,4-Dichlorobenzene-d4     | 8.140  | 152  | 34317    | 20.000 | ng/ul  | 0.00     |
| 20) Naphthalene-d8            | 10.954 | 136  | 150268   | 20.000 | ng/ul  | 0.00     |
| 38) Acenaphthene-d10          | 14.760 | 164  | 122528   | 20.000 | ng/ul  | 0.00     |
| 64) Phenanthrene-d10          | 17.504 | 188  | 294247   | 20.000 | ng/ul  | 0.00     |
| 79) Chrysene-d12              | 21.792 | 240  | 300689   | 20.000 | ng/ul  | 0.00     |
| 88) Perylene-d12              | 25.105 | 264  | 314759   | 20.000 | ng/ul  | 0.00     |
| System Monitoring Compounds   |        |      |          |        |        |          |
| 3) 1,4-Dioxane-d8             | 3.552  | 96   | 6401     | 6.589  | ng/uL  | 0.00     |
| 4) Pyridine-d5                | 3.969  | 84   | 42881    | 17.680 | ng/ul  | 0.00     |
| 7) Phenol-d5                  | 7.288  | 99   | 63265    | 20.583 | ng/ul  | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.453  | 67   | 37511    | 19.982 | ng/ul  | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.670  | 132  | 41014    | 19.652 | ng/ul  | 0.00     |
| 15) 4-Methylphenol-d8         | 8.833  | 113  | 49726    | 22.334 | ng/ul  | 0.00     |
| 21) Nitrobenzene-d5           | 9.297  | 128  | 22838    | 21.113 | ng/ul  | 0.00     |
| 24) 2-Nitrophenol-d4          | 10.026 | 143  | 27433    | 24.045 | ng/ul  | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.566 | 165  | 53613    | 21.600 | ng/ul  | 0.00     |
| 31) 4-Chloroaniline-d4        | 11.077 | 131  | 68067    | 20.749 | ng/ul  | 0.00     |
| 46) Dimethylphthalate-d6      | 14.155 | 166  | 185086   | 19.663 | ng/ul  | 0.00     |
| 49) Acenaphthylene-d8         | 14.455 | 160  | 217690   | 19.032 | ng/ul  | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.931 | 143  | 31899    | 20.155 | ng/ul  | 0.00     |
| 60) Fluorene-d10              | 15.747 | 176  | 160337   | 19.399 | ng/ul  | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.853 | 200  | 32474    | 21.687 | ng/ul  | 0.00     |
| 73) Anthracene-d10            | 17.604 | 188  | 264512   | 19.305 | ng/ul  | 0.00     |
| 81) Pyrene-d10                | 19.883 | 212  | 323052   | 19.205 | ng/ul  | 0.00     |
| 92) Benzo(a)pyrene-d12        | 24.876 | 264  | 315766   | 19.415 | ng/ul  | 0.00     |
| Target Compounds              |        |      |          |        |        |          |
|                               |        |      |          |        | Qvalue |          |
| 2) 1,4-Dioxane                | 3.587  | 88   | 7106     | 5.970  | ng/uL  | 94       |
| 5) Pyridine                   | 3.987  | 79   | 47511    | 18.129 | ng/ul# | 85       |
| 6) Benzaldehyde               | 7.270  | 77   | 45381m   | 22.209 | ng/ul  |          |
| 8) Phenol                     | 7.312  | 94   | 64379    | 21.733 | ng/ul  | 97       |
| 10) Bis(2-Chloroethyl)ether   | 7.547  | 93   | 44084    | 19.727 | ng/ul  | 99       |
| 12) 2-Chlorophenol            | 7.699  | 128  | 42081    | 19.735 | ng/ul  | 92       |
| 13) 2-Methylphenol            | 8.569  | 108  | 46706    | 20.287 | ng/ul  | 98       |
| 14) 2,2'-oxybis(1-Chloropr... | 8.663  | 45   | 75850    | 20.881 | ng/ul  | 96       |
| 16) Acetophenone              | 8.956  | 105  | 77192    | 22.223 | ng/ul  | 98       |
| 17) N-Nitroso-di-n-propyla... | 8.939  | 70   | 45808    | 22.622 | ng/ul  | 96       |
| 18) 4-Methylphenol            | 8.898  | 108  | 52629    | 21.941 | ng/ul  | 92       |
| 19) Hexachloroethane          | 9.232  | 117  | 18521    | 19.576 | ng/ul  | 91       |
| 22) Nitrobenzene              | 9.344  | 77   | 67497    | 21.356 | ng/ul  | 98       |
| 23) Isophorone                | 9.861  | 82   | 127131   | 21.044 | ng/ul  | 98       |
| 25) 2-Nitrophenol             | 10.061 | 139  | 26918    | 22.752 | ng/ul# | 94       |
| 26) 2,4-Dimethylphenol        | 10.108 | 107  | 61916    | 21.120 | ng/ul  | 98       |
| 27) Bis(2-Chloroethoxy)met... | 10.343 | 93   | 68295    | 20.328 | ng/ul  | 98       |
| 29) 2,4-Dichlorophenol        | 10.589 | 162  | 51409    | 21.303 | ng/ul  | 95       |
| 30) Naphthalene               | 11.001 | 128  | 152711   | 19.638 | ng/ul  | 98       |
| 32) 4-Chloroaniline           | 11.101 | 127  | 67021    | 20.792 | ng/ul  | 98       |
| 33) Hexachlorobutadiene       | 11.294 | 225  | 38429    | 19.499 | ng/ul  | 95       |
| 34) Caprolactam               | 11.847 | 113  | 17533m   | 24.123 | ng/ul  |          |
| 35) 4-Chloro-3-methylphenol   | 12.211 | 107  | 61368    | 23.443 | ng/ul  | 88       |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG032522\  
 Data File : BG052882.D  
 Acq On : 27 Mar 2022 3:06  
 Operator : CG/JU  
 Sample : SSTDCCC020EC  
 Misc :  
 ALS Vial : 61 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 LabSampleId :  
 SSTDCCC020EC

Manual IntegrationsAPPROVED

Quant Time: Mar 28 01:05:47 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG031822.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Mar 23 13:16:32 2022  
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/28/2022  
 Supervised By :mohammad ahmed 03/29/2022

| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| 36) 2-Methylnaphthalene       | 12.599 | 142  | 112515   | 20.502 | ng/ul  | 96       |
| 37) 1-Methylnaphthalene       | 12.816 | 142  | 116289   | 20.931 | ng/ul# | 92       |
| 39) 1,2,4,5-Tetrachloroben... | 12.963 | 216  | 75925    | 18.747 | ng/ul  | 96       |
| 40) Hexachlorocyclopentadiene | 12.951 | 237  | 48876    | 17.432 | ng/ul  | 94       |
| 41) 2,4,6-Trichlorophenol     | 13.192 | 196  | 49423    | 19.971 | ng/ul  | 99       |
| 42) 2,4,5-Trichlorophenol     | 13.262 | 196  | 54738    | 20.482 | ng/ul  | 96       |
| 43) 1,1'-Biphenyl             | 13.597 | 154  | 162460   | 18.555 | ng/ul  | 99       |
| 44) 2-Chloronaphthalene       | 13.638 | 162  | 129145   | 18.420 | ng/ul  | 96       |
| 45) 2-Nitroaniline            | 13.832 | 65   | 47431    | 23.079 | ng/ul  | 97       |
| 47) Dimethylphthalate         | 14.202 | 163  | 173862   | 19.355 | ng/ul  | 97       |
| 48) 2,6-Dinitrotoluene        | 14.320 | 165  | 35843    | 22.027 | ng/ul  | 94       |
| 50) Acenaphthylene            | 14.484 | 152  | 212493   | 19.235 | ng/ul  | 98       |
| 51) 3-Nitroaniline            | 14.649 | 138  | 38368    | 23.359 | ng/ul  | 95       |
| 52) Acenaphthene              | 14.825 | 153  | 137775   | 19.091 | ng/ul  | 96       |
| 53) 2,4-Dinitrophenol         | 14.854 | 184  | 22903    | 22.656 | ng/ul# | 65       |
| 55) 4-Nitrophenol             | 14.942 | 109  | 36375    | 21.839 | ng/ul  | 94       |
| 56) Dibenzofuran              | 15.154 | 168  | 211431   | 19.762 | ng/ul  | 98       |
| 57) 2,4-Dinitrotoluene        | 15.107 | 165  | 53228    | 23.054 | ng/ul# | 95       |
| 58) 2,3,4,6-Tetrachlorophenol | 15.377 | 232  | 52148    | 21.647 | ng/ul# | 95       |
| 59) Diethylphthalate          | 15.565 | 149  | 183658   | 20.187 | ng/ul  | 99       |
| 61) Fluorene                  | 15.806 | 166  | 172435   | 19.444 | ng/ul  | 98       |
| 62) 4-Chlorophenyl-phenyle... | 15.794 | 204  | 92360    | 19.572 | ng/ul  | 96       |
| 63) 4-Nitroaniline            | 15.806 | 138  | 38972m   | 24.128 | ng/ul  |          |
| 66) 4,6-Dinitro-2-methylph... | 15.871 | 198  | 31424    | 21.448 | ng/ul# | 95       |
| 67) N-Nitrosodiphenylamine    | 16.000 | 169  | 154269   | 19.391 | ng/ul  | 97       |
| 68) 4-Bromophenyl-phenylether | 16.687 | 248  | 64416    | 22.110 | ng/ul  | 97       |
| 69) Hexachlorobenzene         | 16.810 | 284  | 75235    | 19.991 | ng/ul# | 93       |
| 70) Atrazine                  | 16.946 | 200  | 66969    | 20.540 | ng/ul  | 99       |
| 71) Pentachlorophenol         | 17.151 | 266  | 43228    | 18.889 | ng/ul  | 91       |
| 72) Phenanthrene              | 17.545 | 178  | 298144   | 19.306 | ng/ul  | 99       |
| 74) Anthracene                | 17.639 | 178  | 299519   | 19.400 | ng/ul  | 97       |
| 75) 1,2,3,4-Tetrachloroben... | 13.568 | 216  | 83551    | 19.065 | ng/uL  | 97       |
| 76) Pentachlorobenzene        | 15.078 | 250  | 82122    | 19.532 | ng/uL  | 97       |
| 77) Carbazole                 | 17.897 | 167  | 270536   | 19.827 | ng/ul  | 96       |
| 78) Di-n-butylphthalate       | 18.455 | 149  | 311358   | 19.189 | ng/ul  | 99       |
| 80) Fluoranthene              | 19.548 | 202  | 389259   | 19.637 | ng/ul  | 100      |
| 82) Pyrene                    | 19.912 | 202  | 384358   | 19.508 | ng/ul  | 97       |
| 83) Butylbenzylphthalate      | 20.793 | 149  | 137279   | 20.040 | ng/ul  | 97       |
| 84) 3,3'-Dichlorobenzidine    | 21.680 | 252  | 140743   | 20.884 | ng/ul  | 98       |
| 85) Benzo(a)anthracene        | 21.768 | 228  | 374450   | 19.295 | ng/ul  | 99       |
| 86) Bis(2-ethylhexyl)phtha... | 21.669 | 149  | 192338   | 20.272 | ng/ul  | 99       |
| 87) Chrysene                  | 21.839 | 228  | 355617   | 19.211 | ng/ul  | 100      |
| 89) Di-n-octyl phthalate      | 22.914 | 149  | 322272   | 19.657 | ng/ul  | 100      |
| 90) Benzo(b)fluoranthene      | 24.048 | 252  | 391539   | 19.264 | ng/ul  | 99       |
| 91) Benzo(k)fluoranthene      | 24.118 | 252  | 358150   | 19.093 | ng/ul  | 97       |
| 93) Benzo(a)pyrene            | 24.952 | 252  | 369629   | 19.263 | ng/ul# | 98       |
| 94) Indeno(1,2,3-cd)pyrene    | 28.888 | 276  | 427320m  | 19.691 | ng/ul  |          |
| 95) Dibenzo(a,h)anthracene    | 28.953 | 278  | 359175   | 19.473 | ng/ul  | 97       |
| 96) Benzo(g,h,i)perylene      | 30.069 | 276  | 349234   | 19.037 | ng/ul  | 98       |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

**Instrument :**

BNA\_G

**LabSampleId :**

SSTDCCC020EC

**Manual IntegrationsAPPROVED**

Reviewed By :Jagrut Upadhyay 03/28/2022  
Supervised By :mohammad ahmed 03/29/2022

## Manual IntegrationsAPPROVED

Quant Time: Mar 28 01:05:47 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG031822.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Mar 23 13:16:32 2022  
Response via : Initial Calibration

