

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052862.D
 Acq On : 26 Mar 2022 13:28
 Operator : CG/JU
 Sample : N2068-05
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAZ10

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
 Supervised By :mohammad ahmed 03/29/2022

Quant Time: Mar 28 00:59:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.139	152	28794	20.000	ng/u1	0.00
20) Naphthalene-d8	10.953	136	131781	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.760	164	107494	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.503	188	268217	20.000	ng/u1	0.00
79) Chrysene-d12	21.791	240	299893	20.000	ng/u1	0.00
88) Perylene-d12	25.104	264	292561	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.551	96	4227m	5.185	ng/uL	0.00
4) Pyridine-d5	3.974	84	27447	13.487	ng/u1	0.00
7) Phenol-d5	7.287	99	36605	14.194	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.452	67	68166	43.277	ng/u1	0.00
11) 2-Chlorophenol-d4	7.669	132	59856	34.181	ng/u1	0.00
15) 4-Methylphenol-d8	8.832	113	49023	26.241	ng/u1	0.00
21) Nitrobenzene-d5	9.296	128	40869	43.083	ng/u1	0.00
24) 2-Nitrophenol-d4	10.025	143	47968	47.942	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.565	165	79986	36.747	ng/u1	0.00
31) 4-Chloroaniline-d4	11.076	131	102820	35.740	ng/u1	0.00
46) Dimethylphthalate-d6	14.160	166	355243	43.017	ng/u1	0.00
49) Acenaphthylene-d8	14.454	160	398357	39.697	ng/u1	0.00
54) 4-Nitrophenol-d4	14.930	143	21975m	15.827	ng/u1	0.00
60) Fluorene-d10	15.752	176	316431	43.639	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.852	200	67387	49.369	ng/u1	0.00
73) Anthracene-d10	17.603	188	578516	46.319	ng/u1	0.00
81) Pyrene-d10	19.888	212	708908	42.256	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.881	264	731175	48.369	ng/u1	0.00
Target Compounds						
78) Di-n-butylphthalate	18.455	149	18444	1.247	ng/u1	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052862.D
Acq On : 26 Mar 2022 13:28
Operator : CG/JU
Sample : N2068-05
Misc :
ALS Vial : 40 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
YAZ10

Quant Time: Mar 28 00:59:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022
Supervised By :mohammad ahmed 03/29/2022

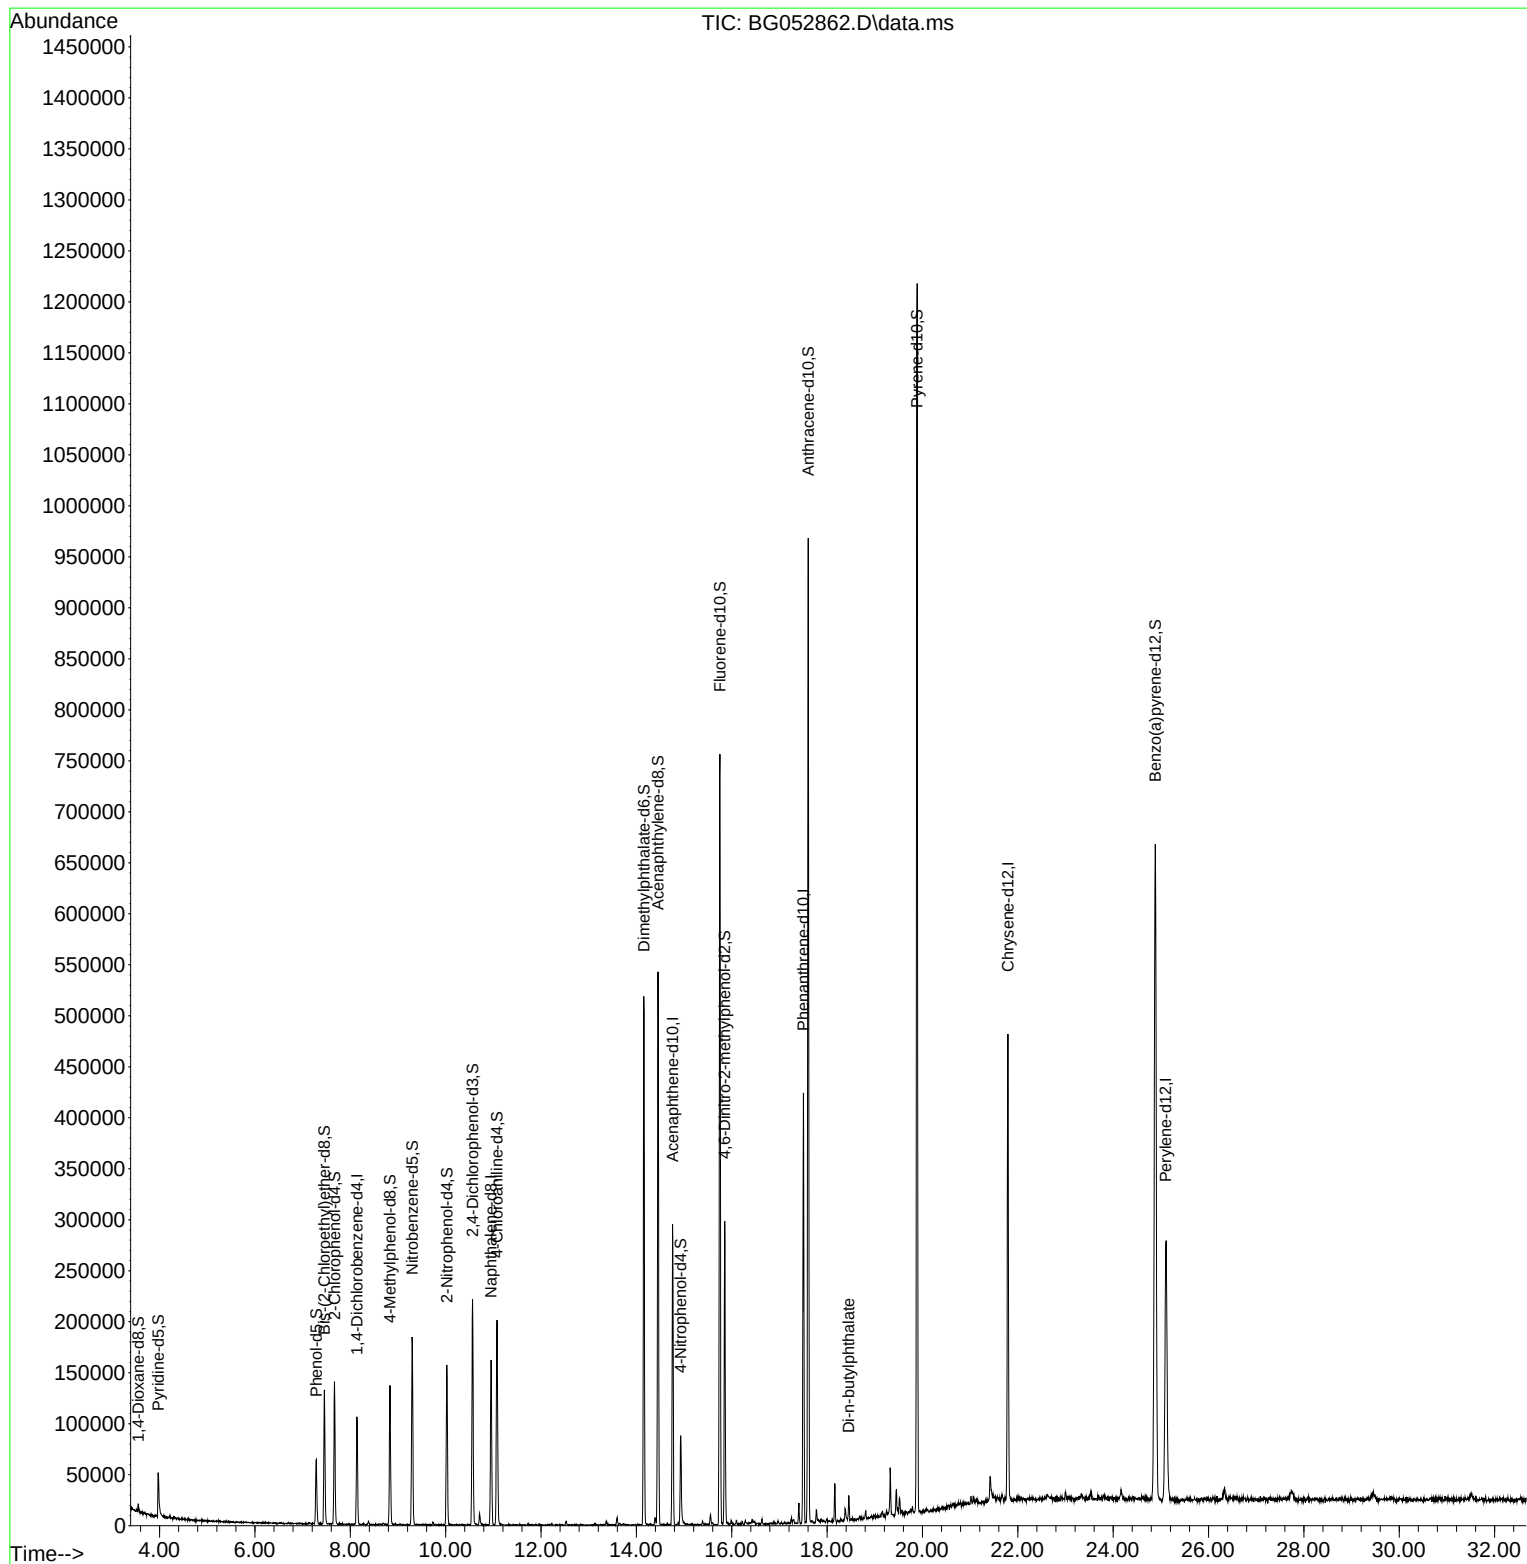

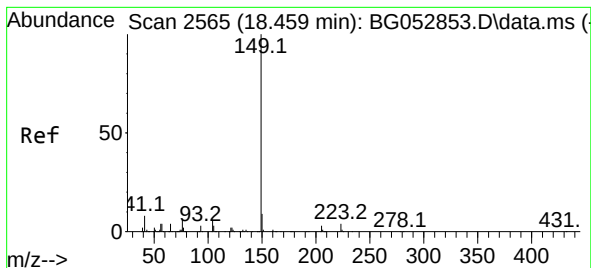

#78

Di-n-butylphthalate

Concen: 1.247 ng/ul

RT: 18.455 min Scan# 2

Delta R.T. -0.007 min

Lab File: BG052862.D


Acq: 26 Mar 2022 13:28

Instrument :

BNA_G

ClientSampleId :

YAZ10

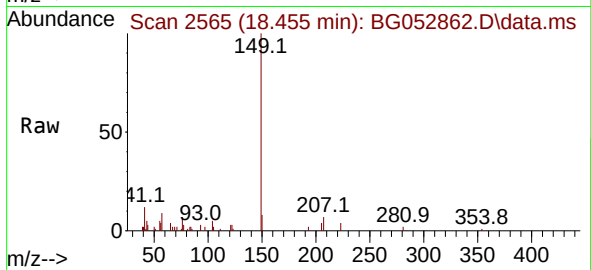

Tgt Ion:149 Resp: 1844

Ion Ratio Lower Upper

149 100

150 8.3 7.5 11.3

104 5.3 4.6 6.8

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 03/28/2022

Supervised By :mohammad ahmed 03/29/2022

