

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052864.D
 Acq On : 26 Mar 2022 14:45
 Operator : CG/JU
 Sample : N2068-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAZ12

Quant Time: Mar 28 00:59:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 23 13:16:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.139	152	26529	20.000	ng/ul	0.00
20) Naphthalene-d8	10.953	136	120826	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.760	164	97885	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.503	188	241326	20.000	ng/ul	0.00
79) Chrysene-d12	21.792	240	272224	20.000	ng/ul	# 0.00
88) Perylene-d12	25.111	264	274199	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.557	96	3935	5.239	ng/uL	0.00
4) Pyridine-d5	3.969	84	18683	9.964	ng/ul	0.00
7) Phenol-d5	7.282	99	37196	15.654	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.452	67	63881	44.019	ng/ul	0.00
11) 2-Chlorophenol-d4	7.670	132	55286	34.267	ng/ul	0.00
15) 4-Methylphenol-d8	8.833	113	46586	27.066	ng/ul	0.00
21) Nitrobenzene-d5	9.297	128	39915	45.892	ng/ul	0.00
24) 2-Nitrophenol-d4	10.025	143	44857	48.897	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.566	165	77949	39.058	ng/ul	0.00
31) 4-Chloroaniline-d4	11.077	131	81986	31.082	ng/ul	0.00
46) Dimethylphthalate-d6	14.155	166	338040	44.952	ng/ul	0.00
49) Acenaphthylene-d8	14.454	160	385118	42.145	ng/ul	0.00
54) 4-Nitrophenol-d4	14.924	143	21268	16.821	ng/ul	0.00
60) Fluorene-d10	15.753	176	290505	43.997	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.853	200	63950	52.072	ng/ul	0.00
73) Anthracene-d10	17.603	188	545990	48.586	ng/ul	0.00
81) Pyrene-d10	19.888	212	686604	45.086	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.881	264	714671	50.443	ng/ul	0.00
Target Compounds						
78) Di-n-butylphthalate	18.455	149	16065	1.207	ng/ul#	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052864.D
Acq On : 26 Mar 2022 14:45
Operator : CG/JU
Sample : N2068-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAZ12

Quant Time: Mar 28 00:59:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 23 13:16:32 2022
Response via : Initial Calibration

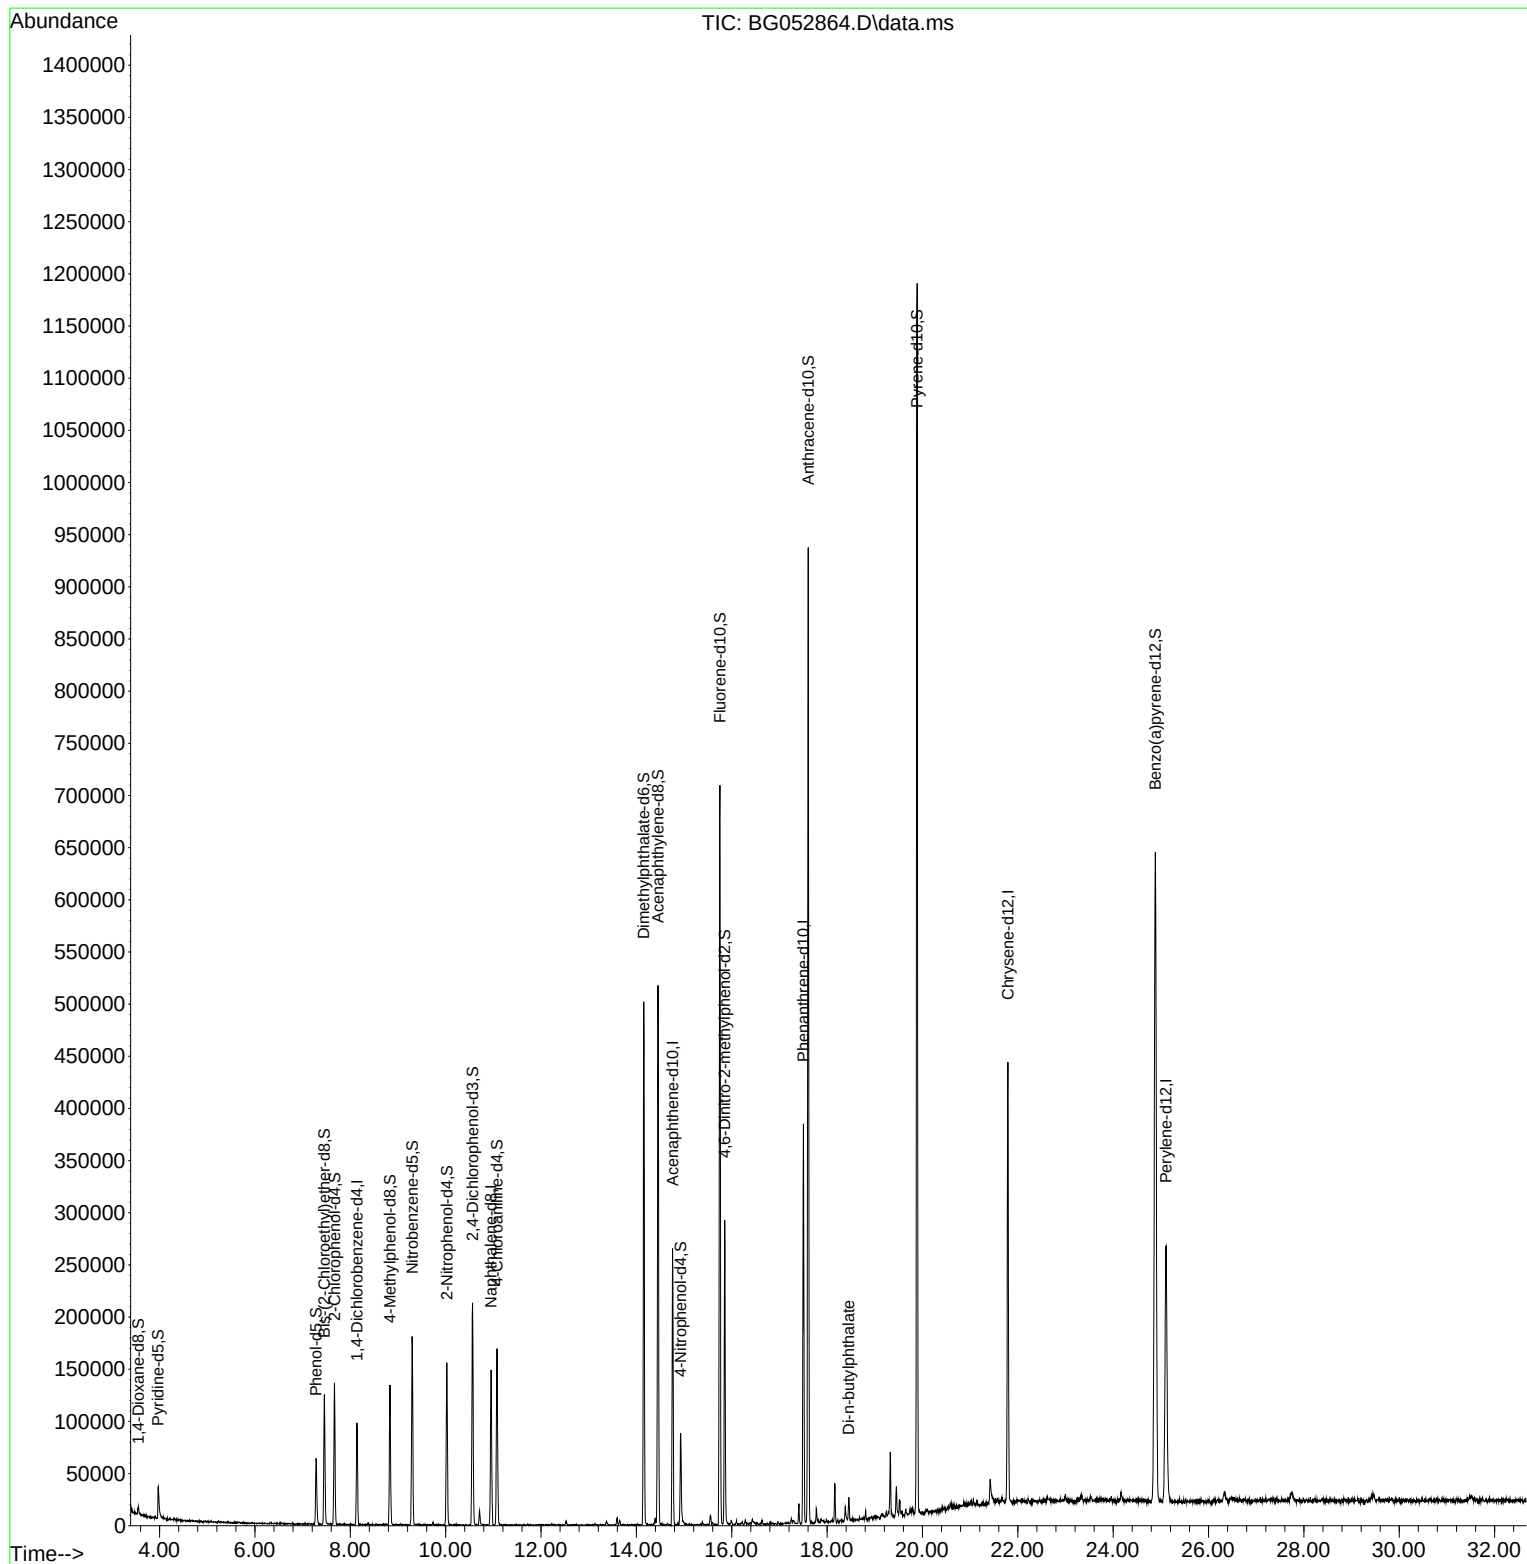

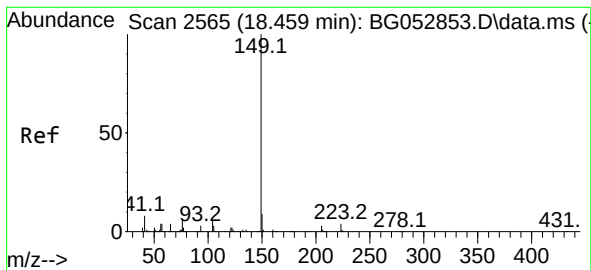

#78

Di-n-butylphthalate

Concen: 1.207 ng/ul

RT: 18.455 min Scan# 2

Delta R.T. -0.007 min

Lab File: BG052864.D


Acq: 26 Mar 2022 14:45

Instrument :

BNA_G

ClientSampleId :

YAZ12

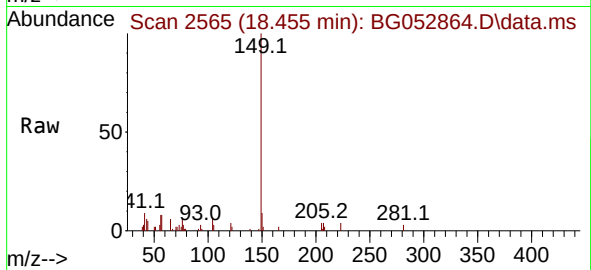

Tgt Ion:149 Resp: 16065

Ion Ratio Lower Upper

149 100

150 9.4 7.5 11.3

104 7.0 4.6 6.8#

