

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052826.D
 Acq On : 25 Mar 2022 12:50
 Operator : CG/JU
 Sample : PB143573BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK573

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052826.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.487	16	17	19	rBV2	2099	1873	0.18%	0.019%
2	3.528	22	24	25	rVV2	2497	1387	0.13%	0.014%
3	3.552	25	28	35	rVB5	10560	13569	1.27%	0.139%
4	3.628	39	41	44	rBV4	1676	1954	0.18%	0.020%
5	3.716	54	56	60	rBV3	1662	1696	0.16%	0.017%
6	3.969	95	99	110	rBV	93407	156063	14.61%	1.597%
7	4.357	164	165	167	rBV	2101	1306	0.12%	0.013%
8	4.421	172	176	178	rVB3	1327	1306	0.12%	0.013%
9	4.509	189	191	193	rBV3	2281	1166	0.11%	0.012%
10	4.921	259	261	264	rVB3	1103	1207	0.11%	0.012%
11	5.091	286	290	294	rVB5	1720	2732	0.26%	0.028%
12	5.138	294	298	301	rBV2	925	1534	0.14%	0.016%
13	5.226	310	313	314	rVB3	1886	1574	0.15%	0.016%
14	5.250	316	317	321	rVB4	1268	1410	0.13%	0.014%
15	5.285	321	323	326	rBV3	1016	1458	0.14%	0.015%
16	5.438	346	349	350	rBV3	1130	1237	0.12%	0.013%
17	5.661	386	387	391	rVB4	1612	1230	0.12%	0.013%
18	6.066	453	456	462	rVB4	1371	2120	0.20%	0.022%
19	6.160	470	472	476	rVB3	1246	1367	0.13%	0.014%
20	6.377	506	509	512	rBV4	826	1214	0.11%	0.012%
21	6.477	523	526	528	rVB2	1716	1729	0.16%	0.018%
22	6.542	534	537	540	rBV2	1771	1664	0.16%	0.017%
23	6.612	546	549	550	rVB3	1579	1342	0.13%	0.014%
24	6.894	596	597	601	rVB3	1261	1270	0.12%	0.013%
25	7.288	657	664	674	rBV	127499	221374	20.73%	2.265%
26	7.364	674	677	680	rVB3	884	1230	0.12%	0.013%
27	7.458	686	693	700	rBV	87077	150982	14.14%	1.545%
28	7.670	722	729	736	rVB	110259	191518	17.93%	1.960%
29	7.987	780	783	787	rBV2	861	1177	0.11%	0.012%
30	8.140	803	809	817	rBV	78127	135752	12.71%	1.389%
31	8.833	921	927	935	rBV	145285	256795	24.04%	2.628%
32	9.303	1000	1007	1020	rVB	118115	219423	20.54%	2.245%
33	9.426	1024	1028	1030	rBV2	1255	1490	0.14%	0.015%
34	10.025	1123	1130	1138	rVV2	102233	182526	17.09%	1.868%
35	10.566	1215	1222	1236	rVV	150860	270082	25.29%	2.764%
36	10.954	1280	1288	1296	rBV	118477	210749	19.73%	2.156%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052826.D
 Acq On : 25 Mar 2022 12:50
 Operator : CG/JU
 Sample : PB143573BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK573

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	11.077	1302	1309	1318	rBV	150989	279060	26.13%	2.855%
38	11.136	1318	1319	1323	rVV	1350	1140	0.11%	0.012%
39	11.165	1323	1324	1330	rVB2	958	1171	0.11%	0.012%
40	11.694	1411	1414	1417	rVB	951	1240	0.12%	0.013%
41	11.788	1426	1430	1434	rBV	720	1144	0.11%	0.012%
42	12.534	1553	1557	1562	rVB3	3507	4954	0.46%	0.051%
43	12.657	1577	1578	1583	rBV2	1021	1300	0.12%	0.013%
44	14.038	1807	1813	1814	rVB2	902	1466	0.14%	0.015%
45	14.161	1827	1834	1840	rBV	339421	494020	46.25%	5.055%
46	14.455	1877	1884	1893	rBV	346336	554079	51.88%	5.670%
47	14.760	1930	1936	1945	rVB	217463	349871	32.76%	3.580%
48	14.931	1959	1965	1980	rBV	160864	294550	27.58%	3.014%
49	15.030	1980	1982	1985	rVV3	1840	2464	0.23%	0.025%
50	15.101	1992	1994	1998	rVV2	1488	1267	0.12%	0.013%
51	15.753	2098	2105	2113	rBV	480311	726545	68.02%	7.434%
52	15.853	2115	2122	2133	rBV	145459	225275	21.09%	2.305%
53	15.994	2142	2146	2149	rVB4	2346	3228	0.30%	0.033%
54	16.282	2191	2195	2199	rBV2	976	1251	0.12%	0.013%
55	16.317	2199	2201	2205	rVB3	1205	1275	0.12%	0.013%
56	16.481	2228	2229	2233	rVV3	1095	1372	0.13%	0.014%
57	16.523	2235	2236	2241	rVB2	954	1286	0.12%	0.013%
58	16.757	2273	2276	2279	rBV2	1366	1458	0.14%	0.015%
59	16.945	2305	2308	2310	rBV3	1074	1293	0.12%	0.013%
60	17.163	2342	2345	2347	rVB3	1142	1179	0.11%	0.012%
61	17.292	2362	2367	2371	rBV2	2127	3106	0.29%	0.032%
62	17.451	2390	2394	2396	rVB3	1023	1254	0.12%	0.013%
63	17.504	2396	2403	2411	rBV	306018	495175	46.36%	5.067%
64	17.603	2414	2420	2429	rVV	568073	877960	82.20%	8.984%
65	17.662	2429	2430	2433	rVV2	1368	1177	0.11%	0.012%
66	17.692	2433	2435	2437	rVV2	1298	1156	0.11%	0.012%
67	17.909	2470	2472	2476	rBV4	1053	1434	0.13%	0.015%
68	17.979	2481	2484	2486	rVB3	977	1222	0.11%	0.013%
69	18.167	2512	2516	2517	rVV2	1433	1304	0.12%	0.013%
70	18.203	2520	2522	2526	rVB2	1186	1283	0.12%	0.013%
71	18.244	2528	2529	2534	rVV4	1254	1306	0.12%	0.013%
72	18.373	2546	2551	2552	rBV4	1382	2174	0.20%	0.022%
73	18.449	2561	2564	2571	rVB5	2056	3898	0.36%	0.040%
74	18.673	2599	2602	2603	rBV3	1599	1831	0.17%	0.019%
75	18.743	2613	2614	2616	rBV	2130	1601	0.15%	0.016%
76	18.778	2618	2620	2622	rBV4	1249	1127	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052826.D
 Acq On : 25 Mar 2022 12:50
 Operator : CG/JU
 Sample : PB143573BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK573

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	18.814	2624	2626	2628	rBV2	1229	1454	0.14%	0.015%
78	18.878	2635	2637	2640	rBV3	1379	1579	0.15%	0.016%
79	19.125	2675	2679	2680	rBV4	1078	1247	0.12%	0.013%
80	19.242	2697	2699	2702	rBV3	1375	1423	0.13%	0.015%
81	19.383	2720	2723	2725	rBV4	2064	1875	0.18%	0.019%
82	19.454	2731	2735	2741	rVB7	10738	13989	1.31%	0.143%
83	19.524	2743	2747	2751	rVV3	9161	12677	1.19%	0.130%
84	19.560	2751	2753	2754	rVB	2288	1337	0.13%	0.014%
85	19.736	2781	2783	2786	rBV3	1840	2285	0.21%	0.023%
86	19.889	2802	2809	2820	rVB	739893	1068064	100.00%	10.929%
87	20.006	2828	2829	2831	rBV2	3730	2839	0.27%	0.029%
88	20.335	2884	2885	2886	rBV	2951	1359	0.13%	0.014%
89	20.376	2890	2892	2894	rVB2	3480	1909	0.18%	0.020%
90	20.687	2943	2945	2946	rVB2	6053	3369	0.32%	0.034%
91	20.699	2946	2947	2949	rBV2	4499	3670	0.34%	0.038%
92	20.840	2969	2971	2973	rBV2	4162	3189	0.30%	0.033%
93	21.351	3055	3058	3060	rBV4	5611	7488	0.70%	0.077%
94	21.792	3127	3133	3144	rVB	339131	574988	53.83%	5.884%
95	23.331	3393	3395	3396	rBV2	6734	4096	0.38%	0.042%
96	24.177	3534	3539	3545	rBV8	10614	20454	1.92%	0.209%
97	24.882	3649	3659	3673	rVB2	362243	1047464	98.07%	10.718%
98	25.111	3689	3698	3715	rVB2	191534	593017	55.52%	6.068%
99	27.155	4044	4046	4047	rBV2	6150	4480	0.42%	0.046%
100	30.462	4607	4609	4610	rBV2	6230	3114	0.29%	0.032%




Sum of corrected areas: 9772768

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052826.D
Acq On : 25 Mar 2022 12:50
Operator : CG/JU
Sample : PB143573BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK573

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

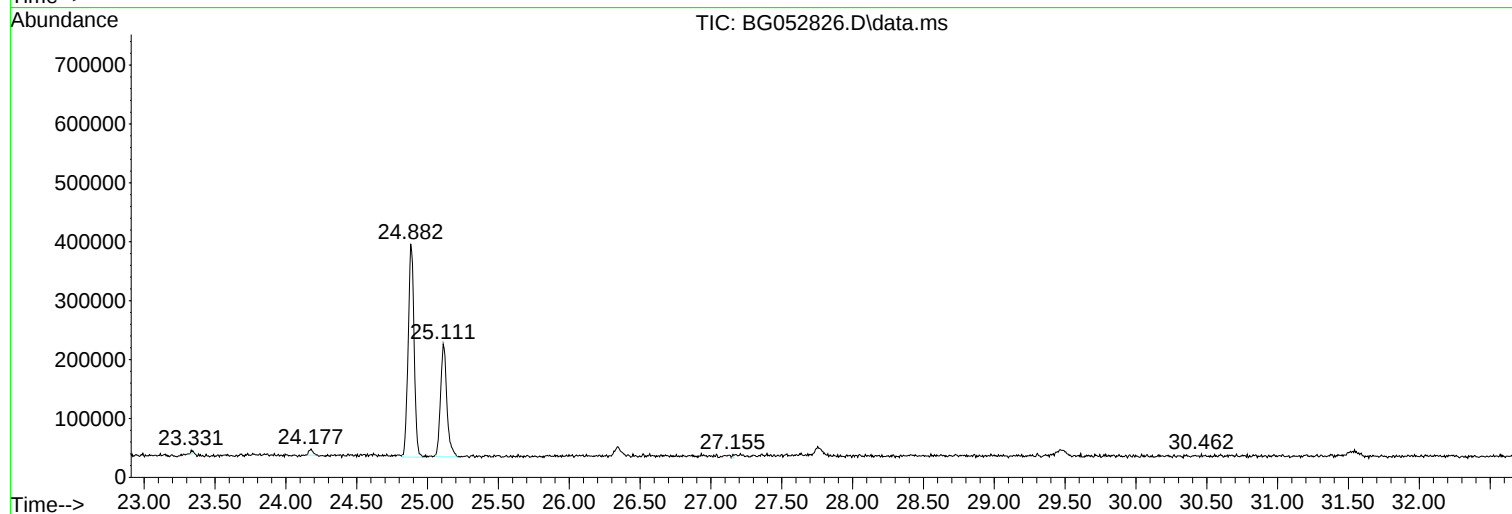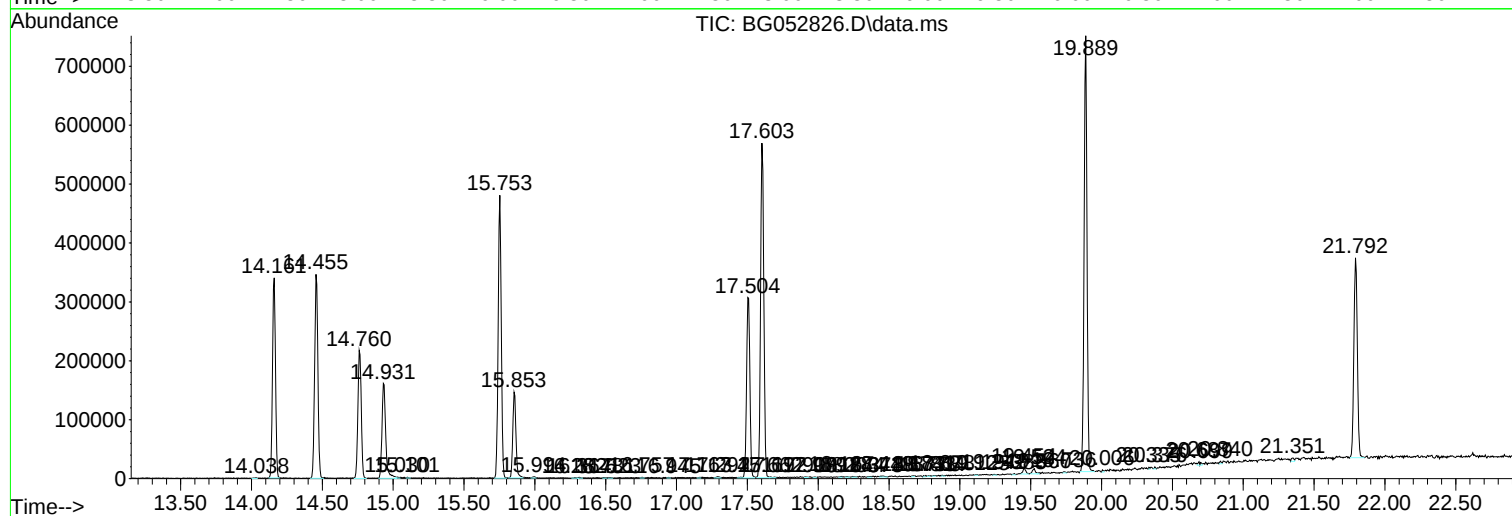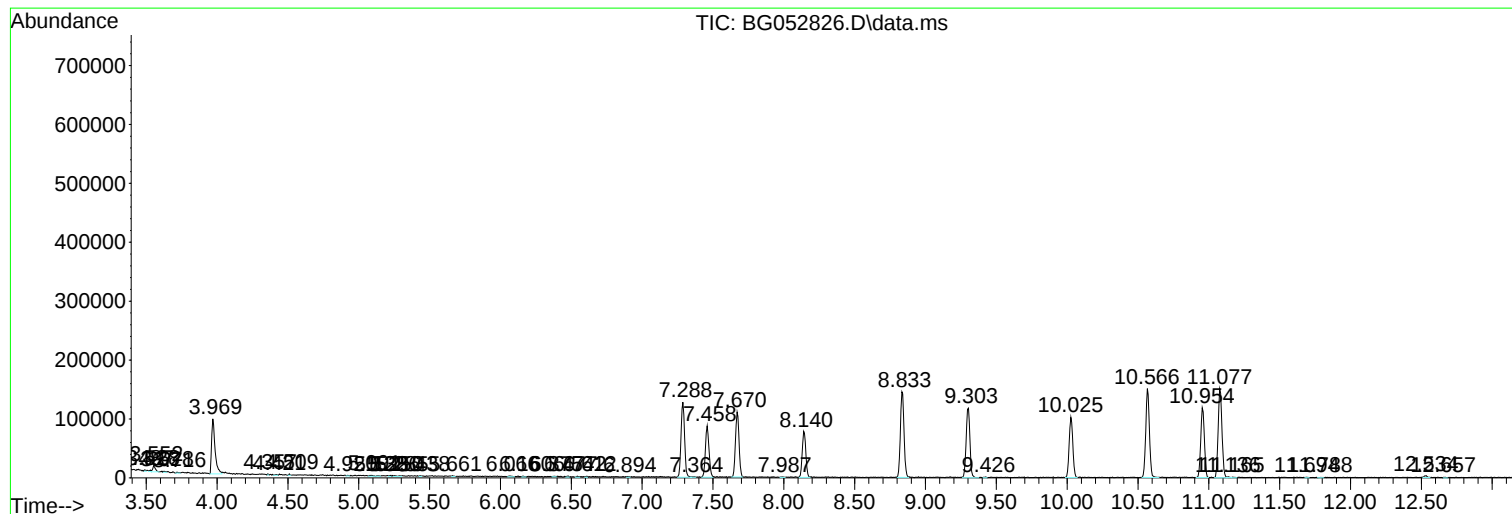

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052826.D
Acq On : 25 Mar 2022 12:50
Operator : CG/JU
Sample : PB143573BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK573

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052826.D
Acq On : 25 Mar 2022 12:50
Operator : CG/JU
Sample : PB143573BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK573

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------