

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052841.D
 Acq On : 25 Mar 2022 23:12
 Operator : CG/JU
 Sample : PB143571BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK571

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052841.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.467	11	13	15	rBV3	2319	1173	0.10%	0.011%
2	3.561	24	29	33	rVB5	7767	11846	1.05%	0.112%
3	3.678	47	49	51	rVB2	2336	1420	0.13%	0.013%
4	3.754	60	62	63	rBV2	1702	1386	0.12%	0.013%
5	3.901	85	87	89	rBV2	1857	1357	0.12%	0.013%
6	3.942	92	94	95	rBV	1660	1370	0.12%	0.013%
7	3.972	95	99	111	rVV	89990	154258	13.68%	1.465%
8	4.177	132	134	137	rVB3	2744	1880	0.17%	0.018%
9	4.260	147	148	150	rBV2	1754	1278	0.11%	0.012%
10	4.301	153	155	156	rVV	2242	1566	0.14%	0.015%
11	4.318	156	158	160	rVB3	2990	2116	0.19%	0.020%
12	4.489	185	187	190	rVB2	1754	1562	0.14%	0.015%
13	4.518	190	192	194	rBV2	1616	1389	0.12%	0.013%
14	4.724	225	227	231	rVB4	1415	1659	0.15%	0.016%
15	4.753	231	232	235	rBV2	1140	1138	0.10%	0.011%
16	4.841	244	247	251	rBV4	1472	2051	0.18%	0.019%
17	5.117	292	294	297	rVB4	1784	1721	0.15%	0.016%
18	5.452	349	351	353	rVB2	1606	1405	0.12%	0.013%
19	5.529	362	364	368	rBV3	1043	1326	0.12%	0.013%
20	5.587	370	374	375	rBV3	1359	1579	0.14%	0.015%
21	5.640	380	383	386	rVV4	1206	1452	0.13%	0.014%
22	5.822	411	414	416	rBV2	1113	1245	0.11%	0.012%
23	6.768	572	575	578	rVB2	1020	1351	0.12%	0.013%
24	6.821	580	584	587	rVB3	1277	1470	0.13%	0.014%
25	6.868	587	592	594	rBV2	1120	2122	0.19%	0.020%
26	6.950	604	606	610	rBV2	1213	1167	0.10%	0.011%
27	7.285	656	663	671	rVV	126291	214517	19.03%	2.037%
28	7.461	685	693	700	rVV	83166	148312	13.15%	1.408%
29	7.673	722	729	737	rVB	112633	192754	17.10%	1.830%
30	8.143	802	809	816	rVB	95844	161671	14.34%	1.535%
31	8.836	919	927	936	rBV	147359	263151	23.34%	2.499%
32	9.000	954	955	962	rVB2	939	1319	0.12%	0.013%
33	9.071	962	967	969	rBV2	933	1266	0.11%	0.012%
34	9.300	998	1006	1014	rVV	123226	220952	19.60%	2.098%
35	10.028	1121	1130	1138	rVB	105749	187989	16.67%	1.785%
36	10.563	1214	1221	1230	rBV	150843	276845	24.55%	2.629%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052841.D
 Acq On : 25 Mar 2022 23:12
 Operator : CG/JU
 Sample : PB143571BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK571

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	10.686	1236	1242	1244	rBV2	1072	1544	0.14%	0.015%
38	10.851	1267	1270	1272	rBV	960	1182	0.10%	0.011%
39	10.956	1279	1288	1295	rBV	143749	262903	23.32%	2.496%
40	11.080	1301	1309	1316	rBV	157924	290400	25.76%	2.757%
41	11.591	1391	1396	1399	rVB2	966	1386	0.12%	0.013%
42	12.531	1549	1556	1561	rVB3	2843	4813	0.43%	0.046%
43	13.488	1714	1719	1721	rVB	1045	1377	0.12%	0.013%
44	14.158	1826	1833	1839	rBV	369840	534029	47.36%	5.071%
45	14.452	1877	1883	1892	rVB	358128	577516	51.22%	5.484%
46	14.681	1919	1922	1926	rBV2	792	1176	0.10%	0.011%
47	14.763	1928	1936	1943	rVB	262094	423887	37.60%	4.025%
48	14.933	1958	1965	1979	rBV	172824	306784	27.21%	2.913%
49	15.750	2096	2104	2116	rBV	499924	768805	68.19%	7.300%
50	15.856	2116	2122	2130	rBV	156463	241863	21.45%	2.297%
51	15.991	2142	2145	2148	rVB2	2472	2848	0.25%	0.027%
52	16.455	2222	2224	2226	rBV	1281	1225	0.11%	0.012%
53	16.608	2246	2250	2254	rBV3	881	1683	0.15%	0.016%
54	17.289	2363	2366	2374	rVB4	2046	3524	0.31%	0.033%
55	17.506	2393	2403	2411	rBV	381308	590202	52.35%	5.604%
56	17.600	2413	2419	2427	rVB	584859	911650	80.86%	8.657%
57	17.847	2459	2461	2463	rBV2	1240	1258	0.11%	0.012%
58	17.965	2479	2481	2484	rVB3	1488	1646	0.15%	0.016%
59	18.082	2498	2501	2504	rBV3	1451	1572	0.14%	0.015%
60	18.205	2519	2522	2525	rBV3	1696	2242	0.20%	0.021%
61	18.505	2571	2573	2575	rBV3	1206	1147	0.10%	0.011%
62	18.875	2635	2636	2638	rBV2	1373	1263	0.11%	0.012%
63	18.975	2651	2653	2656	rVB2	1084	1163	0.10%	0.011%
64	19.051	2663	2666	2669	rBV2	1617	2416	0.21%	0.023%
65	19.151	2681	2683	2687	rVB4	1618	1941	0.17%	0.018%
66	19.245	2696	2699	2701	rBV4	1778	1900	0.17%	0.018%
67	19.292	2705	2707	2708	rBV2	1870	1597	0.14%	0.015%
68	19.374	2717	2721	2725	rBV5	1620	2345	0.21%	0.022%
69	19.451	2730	2734	2740	rBV5	9089	13746	1.22%	0.131%
70	19.521	2742	2746	2751	rVB	8761	11886	1.05%	0.113%
71	19.780	2788	2790	2792	rVB3	2526	1406	0.12%	0.013%
72	19.803	2792	2794	2795	rBV2	2316	1197	0.11%	0.011%
73	19.886	2801	2808	2814	rBV	762017	1127489	100.00%	10.706%
74	20.132	2848	2850	2851	rBV2	2052	1711	0.15%	0.016%
75	20.173	2855	2857	2859	rVB3	2805	1909	0.17%	0.018%
76	20.320	2879	2882	2884	rBV4	2611	2848	0.25%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052841.D
 Acq On : 25 Mar 2022 23:12
 Operator : CG/JU
 Sample : PB143571BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK571

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	20.502	2911	2913	2915	rBV3	2587	2055	0.18%	0.020%
78	20.596	2927	2929	2931	rBV3	3161	3461	0.31%	0.033%
79	21.789	3126	3132	3143	rVB2	413965	704586	62.49%	6.690%
80	22.929	3324	3326	3328	rBV3	4870	3740	0.33%	0.036%
81	24.045	3514	3516	3518	rBV3	4896	5305	0.47%	0.050%
82	24.879	3647	3658	3669	rBV2	380803	1104715	97.98%	10.490%
83	25.108	3687	3697	3713	rVB	239928	705845	62.60%	6.702%
84	26.394	3914	3916	3917	rBV2	4421	3298	0.29%	0.031%
85	28.445	4263	4265	4269	rBV5	4691	4559	0.40%	0.043%
86	30.266	4573	4575	4578	rBV4	4615	6567	0.58%	0.062%
87	30.912	4683	4685	4687	rBV3	4645	4606	0.41%	0.044%




Sum of corrected areas: 10531279

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052841.D
Acq On : 25 Mar 2022 23:12
Operator : CG/JU
Sample : PB143571BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

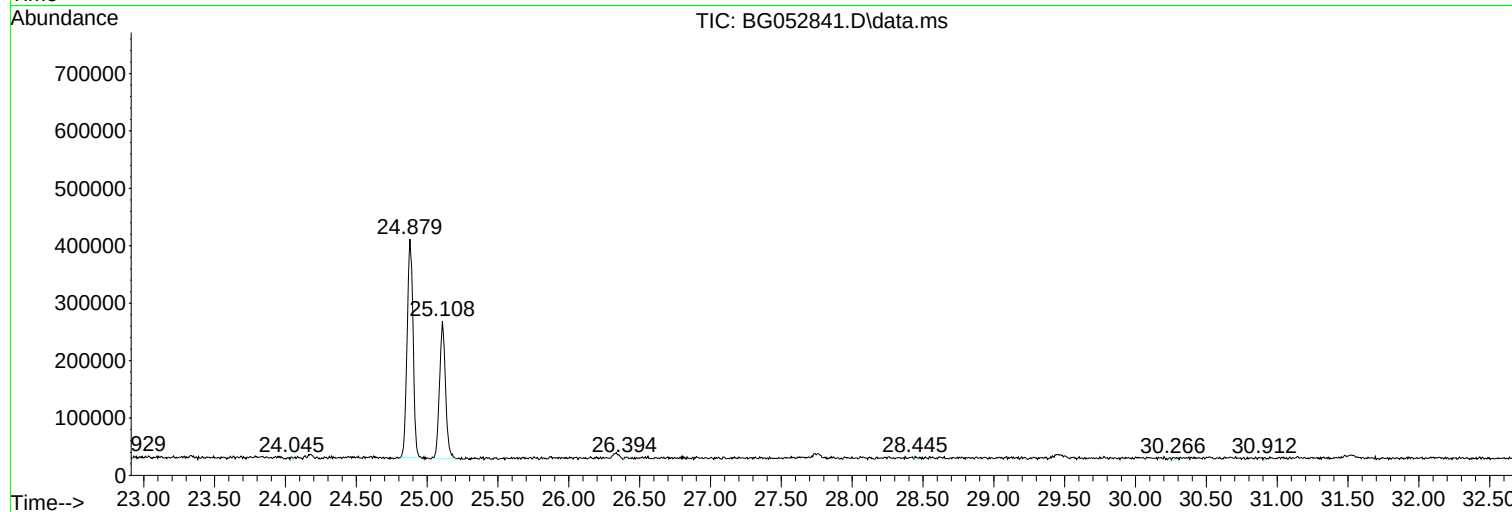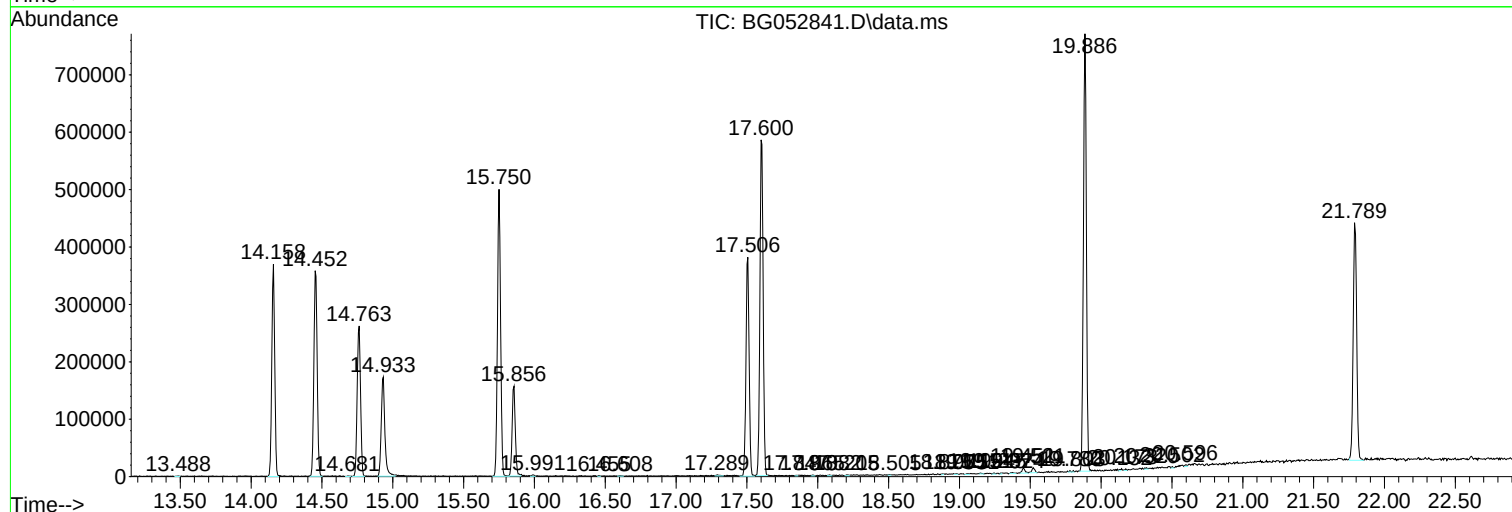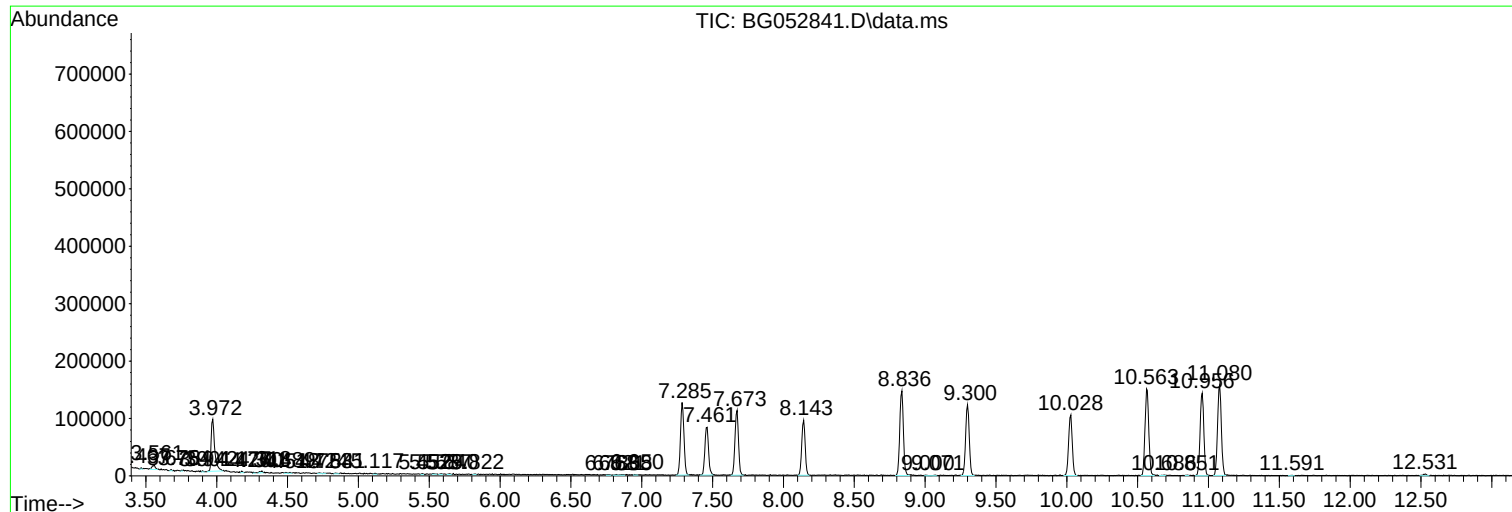

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052841.D
Acq On : 25 Mar 2022 23:12
Operator : CG/JU
Sample : PB143571BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052841.D
Acq On : 25 Mar 2022 23:12
Operator : CG/JU
Sample : PB143571BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc