

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052842.D
 Acq On : 25 Mar 2022 23:51
 Operator : CG/JU
 Sample : PB143563BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK563

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052842.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.482	14	16	21	rBV5	2594	4043	0.38%	0.041%
2	3.552	25	28	37	rVB5	12645	24406	2.31%	0.247%
3	3.711	53	55	56	rVB2	3205	1710	0.16%	0.017%
4	3.729	56	58	60	rBV3	2025	1789	0.17%	0.018%
5	3.969	96	99	108	rBV	87068	141559	13.40%	1.435%
6	4.081	117	118	121	rVB2	3326	1655	0.16%	0.017%
7	4.181	134	135	138	rVB3	2266	1236	0.12%	0.013%
8	4.310	155	157	160	rVB4	2664	2776	0.26%	0.028%
9	4.645	213	214	216	rVB2	1938	1313	0.12%	0.013%
10	4.716	225	226	229	rVB2	2742	2021	0.19%	0.020%
11	4.921	259	261	262	rBV	1640	1110	0.11%	0.011%
12	4.998	272	274	279	rVB4	1491	1870	0.18%	0.019%
13	5.050	281	283	285	rVV3	1502	1238	0.12%	0.013%
14	5.091	289	290	294	rVV3	1545	1261	0.12%	0.013%
15	5.121	294	295	299	rVB3	1188	1295	0.12%	0.013%
16	5.444	348	350	351	rBV2	1489	1134	0.11%	0.011%
17	5.479	353	356	359	rVB3	1042	1359	0.13%	0.014%
18	5.685	387	391	395	rBV4	995	1371	0.13%	0.014%
19	5.738	396	400	404	rVB4	881	1318	0.12%	0.013%
20	5.826	413	415	419	rBV3	1425	1787	0.17%	0.018%
21	6.020	446	448	451	rVB2	1365	1119	0.11%	0.011%
22	6.266	487	490	492	rBV3	1237	1109	0.10%	0.011%
23	6.360	505	506	513	rVB5	898	1432	0.14%	0.015%
24	6.848	588	589	593	rVB2	1839	1613	0.15%	0.016%
25	7.101	629	632	634	rVB2	1169	1288	0.12%	0.013%
26	7.148	638	640	643	rBV3	1028	1156	0.11%	0.012%
27	7.283	656	663	671	rBV2	117852	205546	19.45%	2.084%
28	7.453	686	692	701	rVB	79405	142130	13.45%	1.441%
29	7.670	723	729	737	rVV2	104831	179907	17.02%	1.824%
30	8.140	803	809	816	rVV2	92416	156118	14.77%	1.583%
31	8.581	882	884	889	rVV	798	1136	0.11%	0.012%
32	8.833	919	927	937	rBV	141345	243860	23.08%	2.472%
33	9.298	999	1006	1014	rBV	113772	208504	19.73%	2.114%
34	10.026	1122	1130	1137	rBV2	100186	177830	16.83%	1.803%
35	10.179	1154	1156	1159	rBV2	1574	1584	0.15%	0.016%
36	10.326	1178	1181	1185	rVV	1105	2014	0.19%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052842.D
 Acq On : 25 Mar 2022 23:51
 Operator : CG/JU
 Sample : PB143563BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK563

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	10.431	1197	1199	1202	rVB2	1449	1302	0.12%	0.013%
38	10.566	1214	1222	1229	rBV	141008	254669	24.10%	2.582%
39	10.954	1281	1288	1296	rVB	135203	247838	23.45%	2.513%
40	11.078	1300	1309	1319	rBV	147831	271003	25.64%	2.747%
41	12.534	1550	1557	1560	rBV2	3734	5052	0.48%	0.051%
42	14.026	1808	1811	1813	rBV	892	1197	0.11%	0.012%
43	14.156	1826	1833	1842	rBV	327999	477689	45.20%	4.843%
44	14.455	1877	1884	1894	rBV	346026	534576	50.59%	5.419%
45	14.614	1906	1911	1914	rVB3	823	1265	0.12%	0.013%
46	14.761	1929	1936	1945	rBV	255668	403355	38.17%	4.089%
47	14.931	1958	1965	1974	rBV	156526	268284	25.39%	2.720%
48	15.090	1989	1992	1996	rVB2	1380	1735	0.16%	0.018%
49	15.748	2097	2104	2115	rBV	445300	695177	65.78%	7.048%
50	15.853	2116	2122	2129	rVV	139414	211711	20.03%	2.146%
51	15.989	2141	2145	2148	rBV4	2116	2661	0.25%	0.027%
52	16.529	2233	2237	2240	rBV2	831	1293	0.12%	0.013%
53	17.293	2366	2367	2370	rVB2	1554	1284	0.12%	0.013%
54	17.445	2390	2393	2396	rBV3	1115	1792	0.17%	0.018%
55	17.504	2396	2403	2411	rVV	371607	562970	53.27%	5.707%
56	17.604	2413	2420	2430	rVB	554566	828485	78.40%	8.399%
57	18.244	2527	2529	2531	rVV2	1638	1317	0.12%	0.013%
58	18.344	2543	2546	2547	rBV2	994	1186	0.11%	0.012%
59	18.462	2564	2566	2569	rVB2	2035	2064	0.20%	0.021%
60	18.491	2569	2571	2572	rBV2	1305	1215	0.11%	0.012%
61	18.515	2572	2575	2579	rVB4	1473	1977	0.19%	0.020%
62	18.550	2579	2581	2582	rBV3	1923	1513	0.14%	0.015%
63	18.614	2589	2592	2593	rVB3	1752	1669	0.16%	0.017%
64	18.638	2593	2596	2598	rBV3	2599	2809	0.27%	0.028%
65	18.761	2615	2617	2621	rVB4	1045	1123	0.11%	0.011%
66	18.867	2629	2635	2636	rBV4	1342	1355	0.13%	0.014%
67	18.896	2638	2640	2642	rVV	1029	1172	0.11%	0.012%
68	19.008	2655	2659	2660	rBV2	1049	1144	0.11%	0.012%
69	19.202	2690	2692	2694	rVV3	2438	1926	0.18%	0.020%
70	19.231	2694	2697	2701	rVB4	1825	2237	0.21%	0.023%
71	19.272	2701	2704	2706	rBV3	1940	2807	0.27%	0.028%
72	19.325	2710	2713	2714	rVB3	1596	1248	0.12%	0.013%
73	19.349	2714	2717	2719	rBV4	1988	2033	0.19%	0.021%
74	19.449	2731	2734	2740	rBV4	8589	13116	1.24%	0.133%
75	19.525	2742	2747	2751	rBV3	8527	14707	1.39%	0.149%
76	19.631	2762	2765	2766	rBV3	1553	1711	0.16%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052842.D
 Acq On : 25 Mar 2022 23:51
 Operator : CG/JU
 Sample : PB143563BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK563

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	19.648	2766	2768	2770	rVB2	2006	1429	0.14%	0.014%
78	19.672	2770	2772	2776	rBV4	2841	2741	0.26%	0.028%
79	19.766	2786	2788	2789	rBV2	1955	1247	0.12%	0.013%
80	19.795	2791	2793	2794	rVV2	2127	1349	0.13%	0.014%
81	19.830	2797	2799	2802	rVV4	1582	1430	0.14%	0.014%
82	19.883	2802	2808	2817	rVV	714621	1056785	100.00%	10.713%
83	20.330	2882	2884	2887	rBV3	2645	1945	0.18%	0.020%
84	20.359	2887	2889	2891	rVB3	2381	1949	0.18%	0.020%
85	20.524	2916	2917	2920	rBV3	3503	4327	0.41%	0.044%
86	20.641	2935	2937	2939	rBV2	3617	3047	0.29%	0.031%
87	20.847	2969	2972	2974	rBV4	3719	4249	0.40%	0.043%
88	21.158	3023	3025	3026	rBV2	4394	2789	0.26%	0.028%
89	21.792	3126	3133	3139	rVB	400751	672920	63.68%	6.822%
90	22.820	3306	3308	3309	rBV	4546	2307	0.22%	0.023%
91	23.120	3357	3359	3362	rBV4	4794	4559	0.43%	0.046%
92	24.876	3648	3658	3671	rVB2	365481	1039531	98.37%	10.539%
93	25.106	3687	3697	3713	rVB2	226487	680896	64.43%	6.903%
94	26.210	3883	3885	3888	rBV4	5284	4934	0.47%	0.050%
95	26.474	3928	3930	3931	rBV2	4428	2084	0.20%	0.021%
96	26.510	3934	3936	3938	rVB3	6475	4321	0.41%	0.044%
97	30.240	4569	4571	4572	rBV2	4781	3264	0.31%	0.033%
98	31.027	4703	4705	4707	rBV3	6087	4764	0.45%	0.048%
99	31.473	4778	4781	4782	rBV3	5568	4559	0.43%	0.046%
100	32.026	4873	4875	4876	rVB	4944	2430	0.23%	0.025%


Sum of corrected areas: 9864120

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052842.D
Acq On : 25 Mar 2022 23:51
Operator : CG/JU
Sample : PB143563BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK563

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

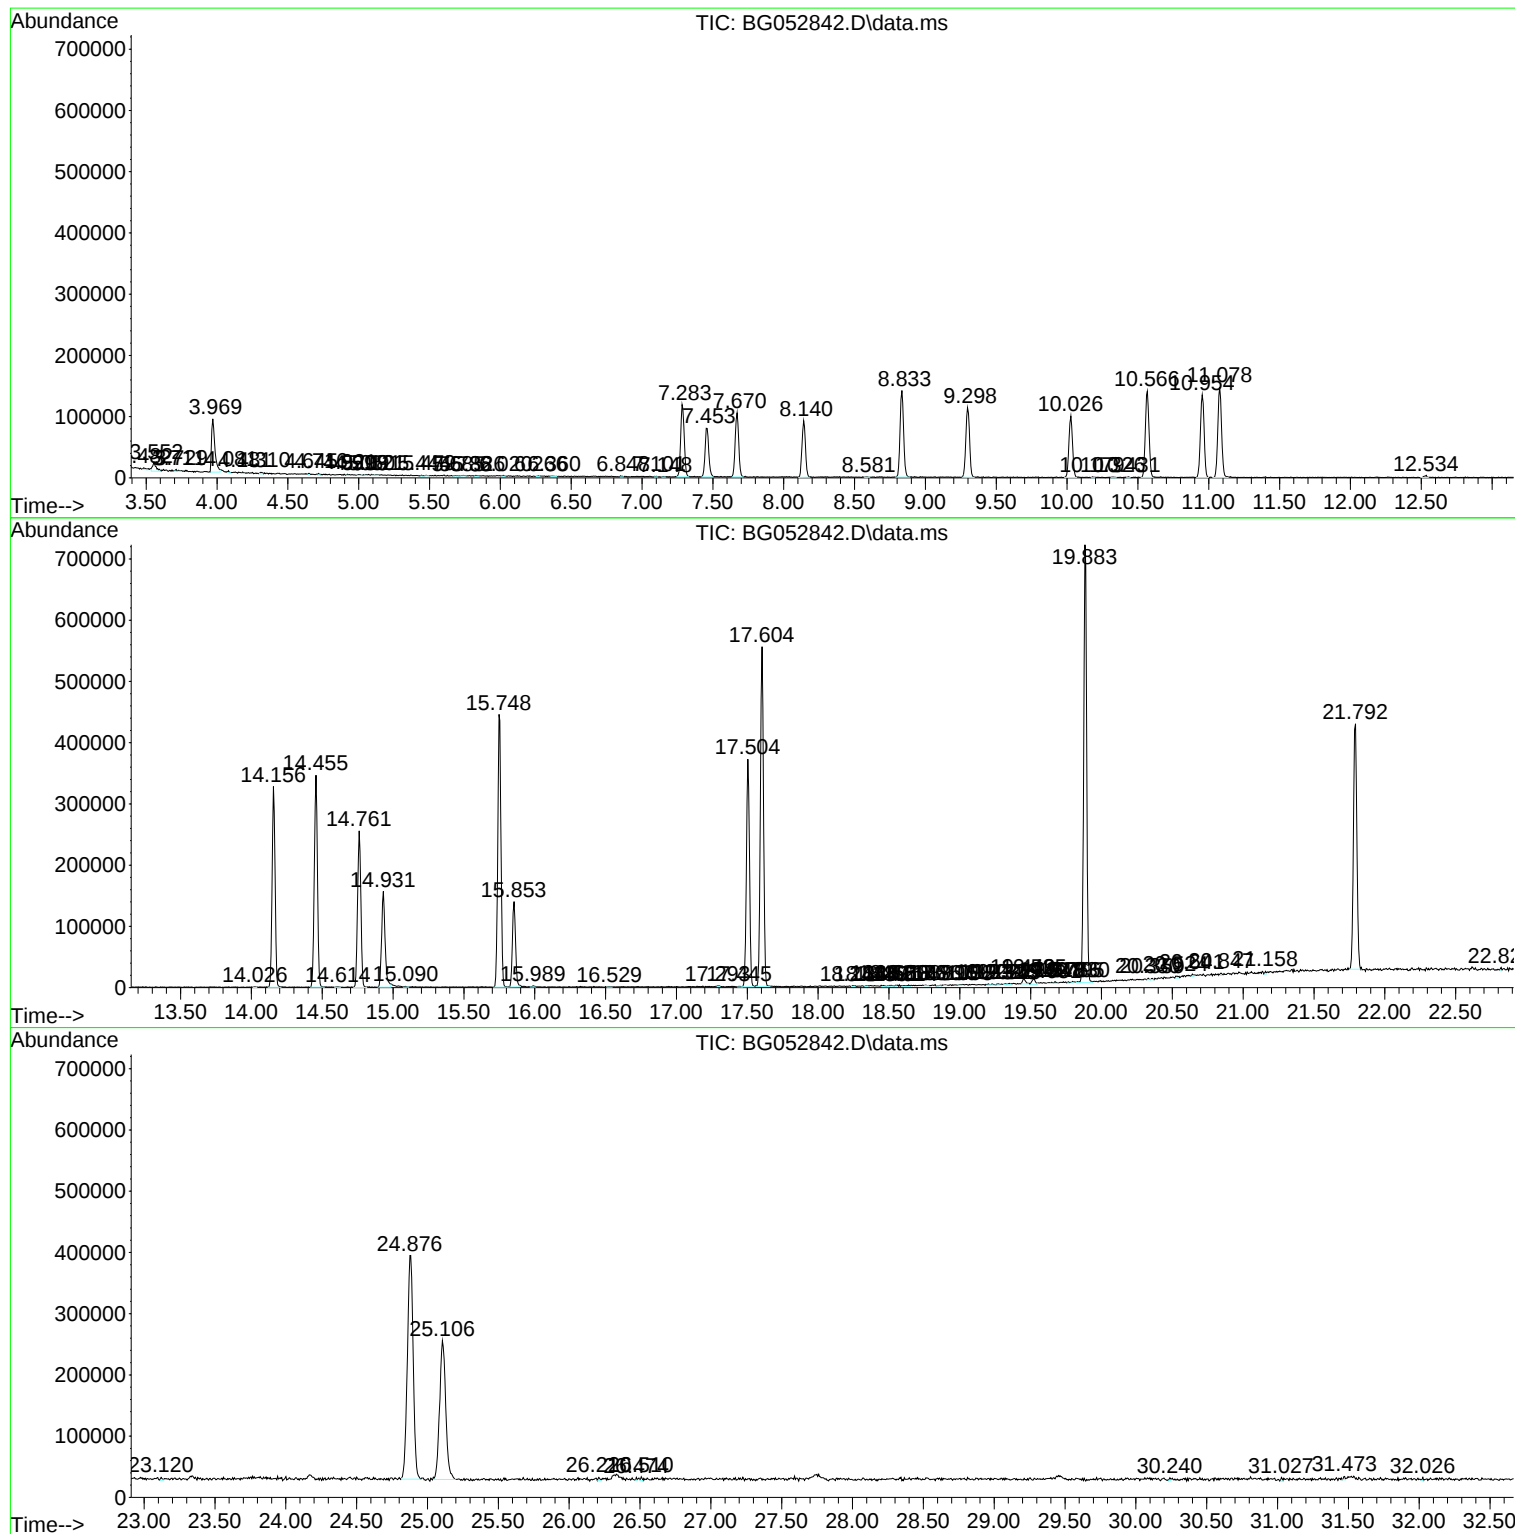

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052842.D
Acq On : 25 Mar 2022 23:51
Operator : CG/JU
Sample : PB143563BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK563

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052842.D
Acq On : 25 Mar 2022 23:51
Operator : CG/JU
Sample : PB143563BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK563

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc