

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052855.D
 Acq On : 26 Mar 2022 8:56
 Operator : CG/JU
 Sample : PB143594BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK594

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052855.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.558	25	29	31	rBV4	8652	12723	0.95%	0.108%
2	3.969	95	99	114	rBV	101273	181031	13.55%	1.540%
3	4.069	114	116	122	rVV6	3984	5413	0.41%	0.046%
4	4.116	122	124	126	rVB2	2473	1971	0.15%	0.017%
5	4.145	127	129	132	rBV3	1980	1795	0.13%	0.015%
6	4.527	192	194	198	rVB4	1982	2039	0.15%	0.017%
7	4.644	211	214	216	rBV4	2123	2968	0.22%	0.025%
8	4.920	260	261	264	rBV2	1493	1396	0.10%	0.012%
9	5.126	294	296	299	rVB3	2394	1525	0.11%	0.013%
10	5.238	314	315	317	rBV2	2153	1518	0.11%	0.013%
11	5.314	326	328	331	rBV4	1272	1771	0.13%	0.015%
12	5.432	345	348	352	rBV4	1362	2425	0.18%	0.021%
13	5.520	360	363	365	rBV2	1414	2026	0.15%	0.017%
14	6.084	456	459	461	rBV3	1116	1364	0.10%	0.012%
15	6.489	525	528	532	rBV4	1269	1680	0.13%	0.014%
16	6.742	568	571	574	rBV4	1451	1372	0.10%	0.012%
17	6.906	597	599	602	rVB2	1309	1364	0.10%	0.012%
18	7.094	627	631	635	rBV3	1551	1713	0.13%	0.015%
19	7.282	657	663	672	rBV	143676	245371	18.36%	2.088%
20	7.458	685	693	700	rBV	97169	171965	12.87%	1.463%
21	7.670	721	729	739	rBV	129278	225032	16.84%	1.915%
22	8.140	801	809	818	rBV	92402	155535	11.64%	1.323%
23	8.833	920	927	937	rBV2	168044	293441	21.96%	2.497%
24	9.297	997	1006	1015	rBV	140190	251789	18.84%	2.143%
25	10.025	1123	1130	1140	rBV2	123377	216238	16.18%	1.840%
26	10.566	1215	1222	1229	rBV	177075	315232	23.59%	2.682%
27	10.953	1281	1288	1296	rVB	132133	241660	18.08%	2.056%
28	11.024	1296	1300	1301	rVB	1398	1381	0.10%	0.012%
29	11.077	1301	1309	1318	rBV2	186437	340116	25.45%	2.894%
30	12.522	1550	1555	1560	rVB4	3482	6616	0.50%	0.056%
31	13.080	1646	1650	1652	rVB	1148	1413	0.11%	0.012%
32	13.949	1794	1798	1801	rBV2	975	1505	0.11%	0.013%
33	14.155	1826	1833	1840	rBV	433387	619665	46.37%	5.273%
34	14.455	1876	1884	1894	rBV	430001	674374	50.46%	5.738%
35	14.760	1930	1936	1944	rVB	261886	412018	30.83%	3.506%
36	14.930	1958	1965	1980	rBV	215889	363735	27.22%	3.095%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052855.D
 Acq On : 26 Mar 2022 8:56
 Operator : CG/JU
 Sample : PB143594BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK594

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	15.753	2098	2105	2112	rBV	572043	905177	67.73%	7.702%
38	15.853	2116	2122	2131	rVV	190019	285737	21.38%	2.431%
39	15.917	2131	2133	2135	rVV2	2161	1965	0.15%	0.017%
40	15.970	2139	2142	2143	rVV2	1322	1395	0.10%	0.012%
41	15.982	2143	2144	2148	rVB3	2361	2736	0.20%	0.023%
42	16.534	2233	2238	2241	rBV2	3636	5020	0.38%	0.043%
43	17.186	2345	2349	2352	rVB3	1372	2081	0.16%	0.018%
44	17.503	2396	2403	2413	rBV	387779	585382	43.80%	4.981%
45	17.603	2413	2420	2430	rBV	719018	1087997	81.41%	9.258%
46	17.874	2464	2466	2470	rVB3	1397	1737	0.13%	0.015%
47	18.449	2559	2564	2565	rBV3	1567	2411	0.18%	0.021%
48	18.590	2586	2588	2591	rVB2	1808	1436	0.11%	0.012%
49	18.702	2605	2607	2611	rBV3	1990	1951	0.15%	0.017%
50	18.802	2622	2624	2627	rBV2	1620	1346	0.10%	0.011%
51	18.937	2645	2647	2650	rBV2	1828	2174	0.16%	0.018%
52	19.084	2671	2672	2674	rBV	1729	1341	0.10%	0.011%
53	19.184	2688	2689	2692	rBV3	1587	1384	0.10%	0.012%
54	19.266	2701	2703	2705	rBV3	1983	1923	0.14%	0.016%
55	19.301	2705	2709	2710	rVV2	1565	1851	0.14%	0.016%
56	19.448	2730	2734	2741	rVB5	11606	17149	1.28%	0.146%
57	19.518	2741	2746	2753	rBV3	10479	17761	1.33%	0.151%
58	19.583	2755	2757	2759	rBV3	1309	1389	0.10%	0.012%
59	19.818	2794	2797	2798	rBV3	1639	1591	0.12%	0.014%
60	19.836	2798	2800	2802	rVV2	1292	1702	0.13%	0.014%
61	19.883	2802	2808	2815	rVV	896671	1336376	100.00%	11.372%
62	19.953	2817	2820	2823	rBV4	2335	2823	0.21%	0.024%
63	19.994	2823	2827	2828	rBV4	2844	2875	0.22%	0.024%
64	20.341	2884	2886	2887	rBV2	2178	1816	0.14%	0.015%
65	20.376	2890	2892	2893	rBV2	1935	1532	0.11%	0.013%
66	20.558	2922	2923	2925	rBV2	3535	2528	0.19%	0.022%
67	20.717	2948	2950	2952	rBV2	2902	2313	0.17%	0.020%
68	21.792	3126	3133	3141	rBV	400435	677272	50.68%	5.763%
69	22.273	3213	3215	3216	rBV	4566	3772	0.28%	0.032%
70	22.855	3313	3314	3317	rVB3	4444	2999	0.22%	0.026%
71	23.149	3362	3364	3365	rBV2	3757	2590	0.19%	0.022%
72	23.924	3494	3496	3497	rBV2	3955	2620	0.20%	0.022%
73	24.882	3648	3659	3671	rVB2	450474	1299665	97.25%	11.059%
74	25.105	3686	3697	3713	rVB2	224725	691936	51.78%	5.888%
75	25.457	3755	3757	3758	rBV2	4088	2493	0.19%	0.021%
76	28.113	4208	4209	4210	rBV	4237	2117	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052855.D
Acq On : 26 Mar 2022 8:56
Operator : CG/JU
Sample : PB143594BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK594

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Title : SVOA CALIBRATION

77	28.571	4285	4287	4288	rBV2	3904	2553	0.19%	0.022%
78	29.423	4430	4432	4434	rBV3	5361	6007	0.45%	0.051%
79	31.414	4769	4771	4772	rBV2	4676	3055	0.23%	0.026%
80	31.831	4839	4842	4845	rBV4	4464	6818	0.51%	0.058%




Sum of corrected areas: 11751976

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052855.D
Acq On : 26 Mar 2022 8:56
Operator : CG/JU
Sample : PB143594BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK594

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

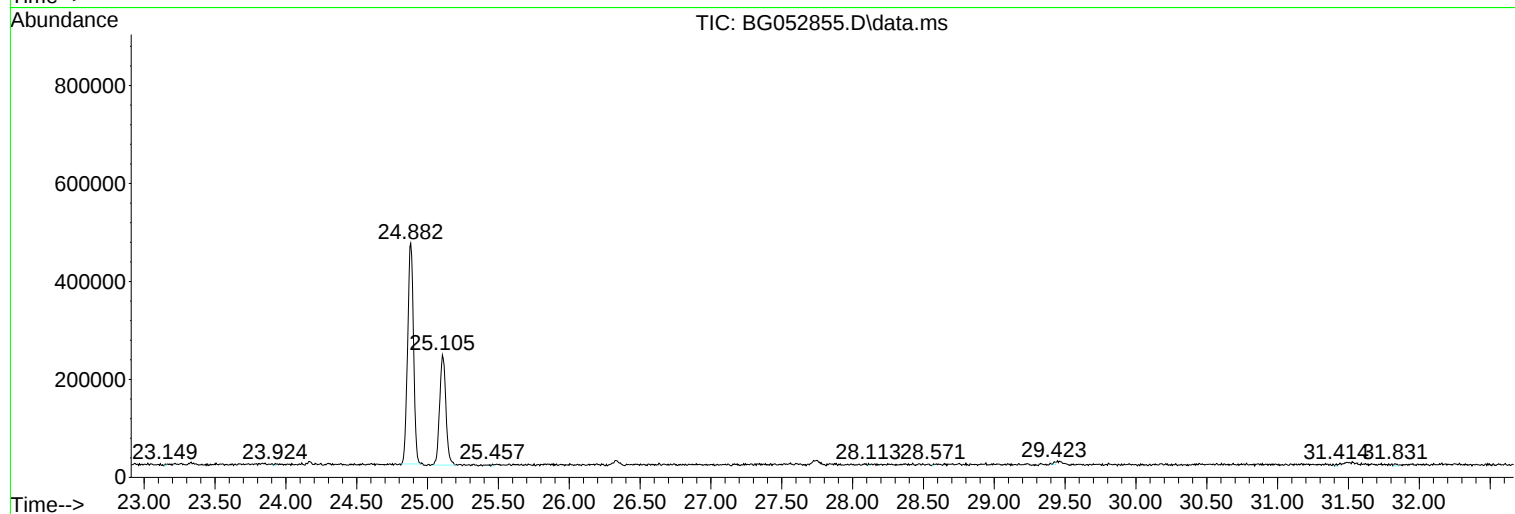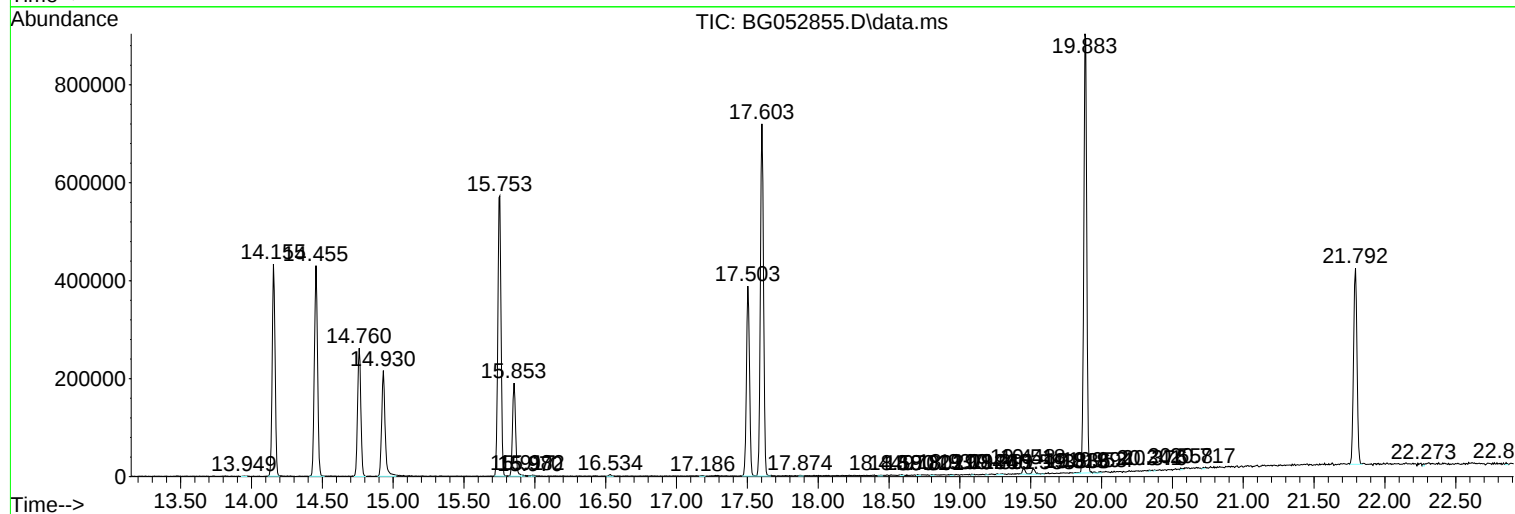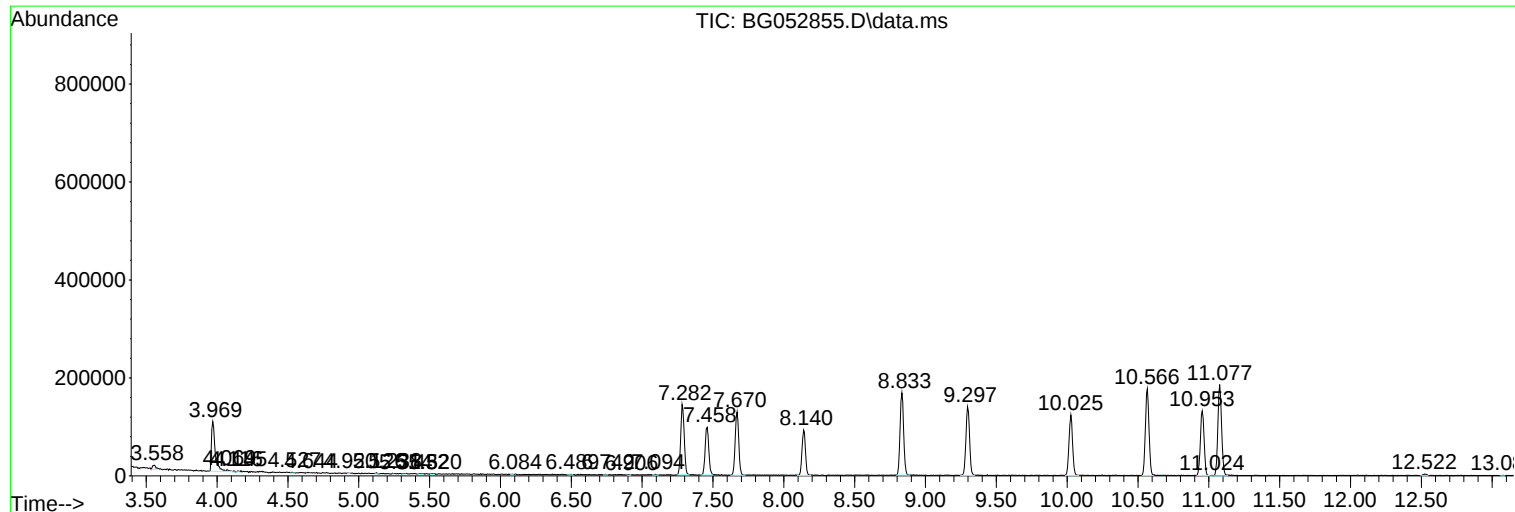

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052855.D
Acq On : 26 Mar 2022 8:56
Operator : CG/JU
Sample : PB143594BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK594

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052855.D
Acq On : 26 Mar 2022 8:56
Operator : CG/JU
Sample : PB143594BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK594

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc