

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052856.D
 Acq On : 26 Mar 2022 9:35
 Operator : CG/JU
 Sample : N2079-16
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW5Z3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052856.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.449	9	10	13	rBV2	3475	2318	0.19%	0.024%
2	3.972	96	99	111	rVV	30040	50884	4.13%	0.537%
3	4.101	118	121	123	rBV2	2444	2525	0.20%	0.027%
4	4.137	126	127	129	rBV2	1807	1487	0.12%	0.016%
5	4.301	151	155	156	rBV3	4321	4085	0.33%	0.043%
6	4.519	189	192	195	rBV4	2115	3233	0.26%	0.034%
7	4.677	217	219	221	rVB3	2244	1823	0.15%	0.019%
8	4.706	221	224	227	rBV4	1512	1546	0.13%	0.016%
9	4.924	257	261	262	rBV2	1997	1708	0.14%	0.018%
10	4.941	262	264	267	rBV3	1671	1787	0.14%	0.019%
11	6.146	466	469	471	rVV4	1211	1477	0.12%	0.016%
12	6.428	514	517	523	rVB3	1204	1608	0.13%	0.017%
13	7.279	657	662	670	rBV2	10903	22173	1.80%	0.234%
14	7.456	684	692	699	rBV	88402	153637	12.47%	1.622%
15	7.667	722	728	736	rVB2	30880	55113	4.47%	0.582%
16	8.143	802	809	816	rVV	94814	160771	13.04%	1.697%
17	8.196	816	818	824	rVB4	1898	2231	0.18%	0.024%
18	8.830	920	926	936	rVV3	40634	72753	5.90%	0.768%
19	9.300	998	1006	1014	rBV	123701	224615	18.22%	2.371%
20	9.459	1030	1033	1038	rBV3	1291	2059	0.17%	0.022%
21	9.729	1077	1079	1080	rBV	1813	1444	0.12%	0.015%
22	10.029	1124	1130	1136	rBV3	18752	33238	2.70%	0.351%
23	10.563	1215	1221	1228	rVV	40831	74318	6.03%	0.784%
24	10.951	1278	1287	1295	rVB	136034	250931	20.36%	2.648%
25	11.074	1301	1308	1320	rBV	138071	257326	20.88%	2.716%
26	11.215	1329	1332	1336	rBV2	824	1384	0.11%	0.015%
27	11.850	1438	1440	1442	rBV	1214	1381	0.11%	0.015%
28	12.361	1523	1527	1531	rBV2	3020	3529	0.29%	0.037%
29	12.531	1552	1556	1557	rBV3	2461	2993	0.24%	0.032%
30	13.166	1662	1664	1669	rBV2	1520	1784	0.14%	0.019%
31	13.589	1731	1736	1740	rBV2	5363	8636	0.70%	0.091%
32	14.158	1826	1833	1839	rBV	360664	520135	42.20%	5.490%
33	14.458	1877	1884	1893	rBV	363361	590184	47.89%	6.229%
34	14.581	1901	1905	1909	rBV	1765	2380	0.19%	0.025%
35	14.652	1915	1917	1920	rVB2	2027	2023	0.16%	0.021%
36	14.758	1929	1935	1945	rBV	251357	418725	33.97%	4.419%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052856.D
 Acq On : 26 Mar 2022 9:35
 Operator : CG/JU
 Sample : N2079-16
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW5Z3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	15.322	2026	2031	2033	rBV4	1900	2911	0.24%	0.031%
38	15.486	2055	2059	2063	rBV4	4872	6423	0.52%	0.068%
39	15.562	2066	2072	2077	rVV	36885	50894	4.13%	0.537%
40	15.750	2097	2104	2113	rVV	520208	803522	65.19%	8.480%

41	15.985	2141	2144	2147	rBV	2135	2401	0.19%	0.025%
42	16.244	2185	2188	2197	rVB5	3906	5189	0.42%	0.055%
43	16.438	2216	2221	2222	rBV2	1567	1524	0.12%	0.016%
44	16.755	2271	2275	2278	rBV3	2011	3305	0.27%	0.035%
45	16.896	2297	2299	2304	rVB5	1056	1421	0.12%	0.015%

46	17.319	2369	2371	2375	rVB2	1630	1460	0.12%	0.015%
47	17.507	2396	2403	2412	rVB	367879	580055	47.06%	6.122%
48	17.601	2412	2419	2429	rBV	639485	1012207	82.13%	10.683%
49	17.677	2429	2432	2436	rVB4	6610	6312	0.51%	0.067%
50	17.865	2462	2464	2467	rVB3	1589	1650	0.13%	0.017%

51	18.159	2512	2514	2518	rVV4	1696	2172	0.18%	0.023%
52	18.364	2544	2549	2550	rBV3	2895	2521	0.20%	0.027%
53	18.500	2570	2572	2575	rBV2	1695	1721	0.14%	0.018%
54	18.635	2593	2595	2598	rVV3	2135	1839	0.15%	0.019%
55	18.764	2615	2617	2618	rBV2	1770	1401	0.11%	0.015%

56	18.964	2650	2651	2654	rVB2	2436	1956	0.16%	0.021%
57	19.017	2654	2660	2661	rBV5	1791	3172	0.26%	0.033%
58	19.075	2668	2670	2672	rVV2	1279	1562	0.13%	0.016%
59	19.152	2681	2683	2685	rVB3	2919	1881	0.15%	0.020%
60	19.363	2718	2719	2721	rBV2	2425	1561	0.13%	0.016%

61	19.457	2731	2735	2740	rVB3	10346	15013	1.22%	0.158%
62	19.522	2742	2746	2751	rVV3	9558	13623	1.11%	0.144%
63	19.645	2765	2767	2769	rBV3	1924	1396	0.11%	0.015%
64	19.721	2779	2780	2782	rBV2	2852	1955	0.16%	0.021%
65	19.786	2789	2791	2792	rBV2	2436	2332	0.19%	0.025%

66	19.827	2796	2798	2801	rVV3	2823	2286	0.19%	0.024%
67	19.886	2801	2808	2816	rVB	869654	1232492	100.00%	13.008%
68	20.050	2835	2836	2839	rVB3	3289	2136	0.17%	0.023%
69	20.561	2921	2923	2924	rBV2	3003	2465	0.20%	0.026%
70	20.708	2946	2948	2950	rBV3	3224	2488	0.20%	0.026%

71	20.896	2978	2980	2981	rBV2	3380	2172	0.18%	0.023%
72	21.090	3011	3013	3014	rBV2	3177	2051	0.17%	0.022%
73	21.261	3040	3042	3043	rVB2	4295	2118	0.17%	0.022%
74	21.419	3064	3069	3082	rBV2	59943	129375	10.50%	1.365%
75	21.672	3108	3112	3117	rVB7	8298	11992	0.97%	0.127%

76	21.789	3125	3132	3139	rVB	401882	664182	53.89%	7.010%
----	--------	------	------	------	-----	--------	--------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052856.D
 Acq On : 26 Mar 2022 9:35
 Operator : CG/JU
 Sample : N2079-16
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW5Z3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	22.330	3223	3224	3225	rBV	4200	2039	0.17%	0.022%
78	22.988	3333	3336	3338	rBV4	5142	7469	0.61%	0.079%
79	23.187	3368	3370	3372	rBV3	4117	3578	0.29%	0.038%
80	23.322	3391	3393	3394	rBV2	3965	2182	0.18%	0.023%
81	23.734	3461	3463	3464	rBV2	4202	3128	0.25%	0.033%
82	24.568	3604	3605	3607	rBV2	4737	4394	0.36%	0.046%
83	24.879	3647	3658	3671	rBV2	422159	1218816	98.89%	12.864%
84	25.108	3685	3697	3710	rBV	221733	665314	53.98%	7.022%
85	25.320	3731	3733	3735	rVB2	3843	2307	0.19%	0.024%
86	27.393	4085	4086	4089	rBV3	4683	2968	0.24%	0.031%
87	27.581	4116	4118	4120	rVB3	3921	2454	0.20%	0.026%
88	27.963	4181	4183	4184	rBV	3963	2661	0.22%	0.028%
89	27.998	4187	4189	4191	rBV3	3758	2984	0.24%	0.031%
90	28.357	4249	4250	4251	rBV	4095	1675	0.14%	0.018%
91	30.107	4546	4548	4551	rBV5	3787	2887	0.23%	0.030%
92	30.489	4612	4613	4614	rVB	5567	1962	0.16%	0.021%
93	30.953	4690	4692	4695	rVB3	5192	2746	0.22%	0.029%
94	31.071	4710	4712	4714	rVB3	3951	2194	0.18%	0.023%
95	31.253	4741	4743	4744	rBV2	4085	2977	0.24%	0.031%
96	31.553	4792	4794	4795	rVB2	4862	3020	0.25%	0.032%
97	32.410	4938	4940	4941	rBV2	3593	1837	0.15%	0.019%
98	32.528	4958	4960	4961	rVB2	6608	3198	0.26%	0.034%
99	32.545	4961	4963	4964	rBV2	3920	2337	0.19%	0.025%
100	32.628	4974	4977	4978	rBV2	4781	4464	0.36%	0.047%




Sum of corrected areas: 9474971

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052856.D
Acq On : 26 Mar 2022 9:35
Operator : CG/JU
Sample : N2079-16
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW5Z3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

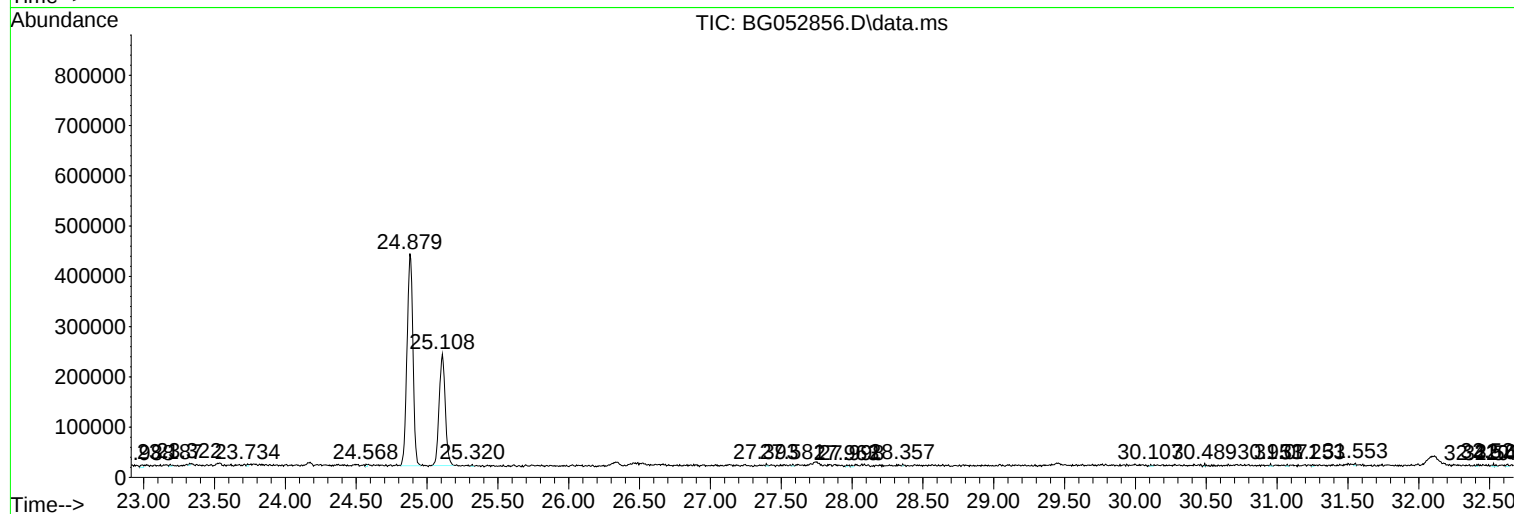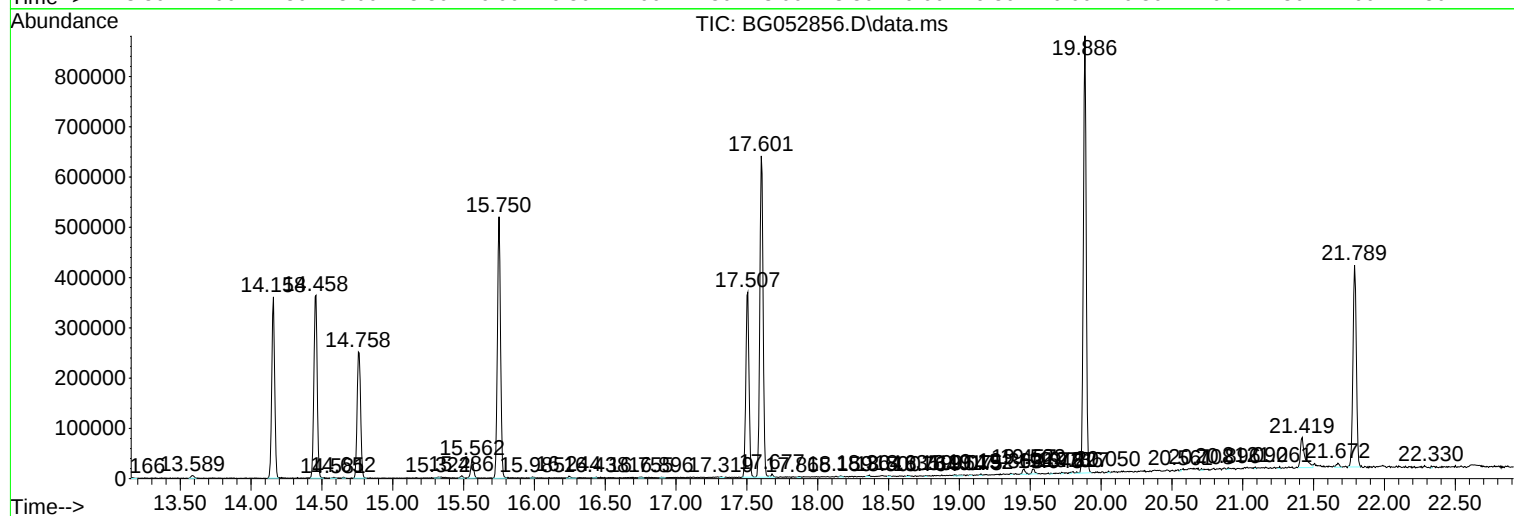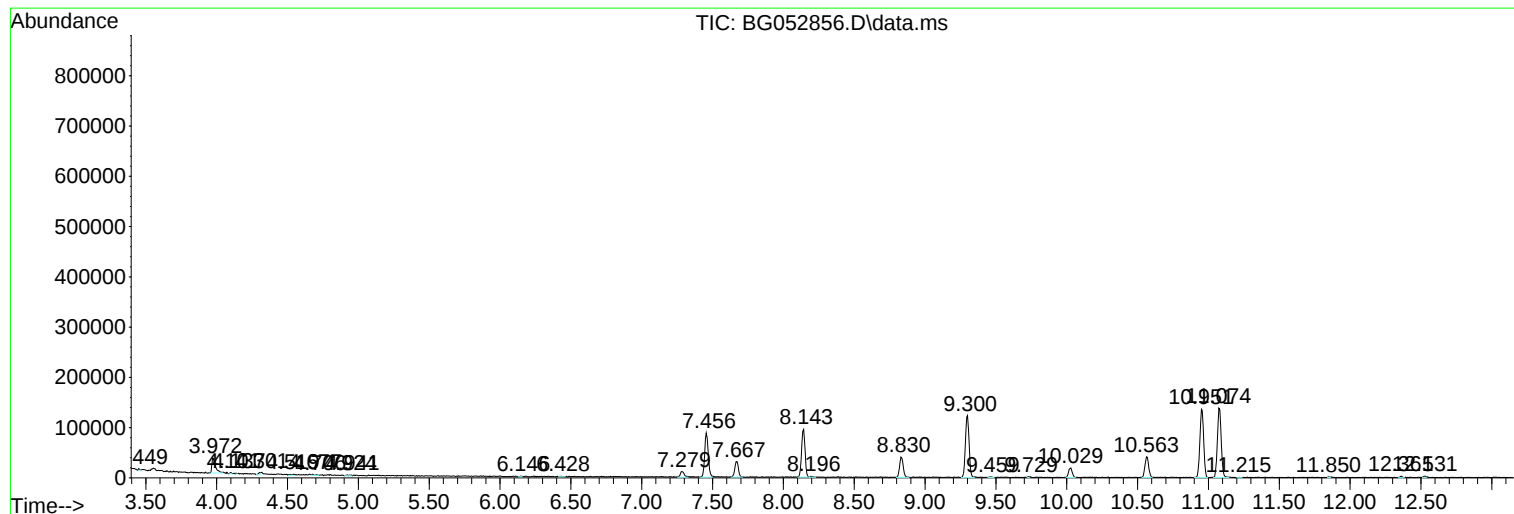

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052856.D
Acq On : 26 Mar 2022 9:35
Operator : CG/JU
Sample : N2079-16
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW5Z3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Diethyl Phthalate Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.562	2.43 ng/ul	50894	Acenaphthene-d10	14.758

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diethyl Phthalate	222	C12H14O4	000084-66-2	91
2			Diethyl Phthalate	222	C12H14O4	000084-66-2	91
3			Diethyl Phthalate	222	C12H14O4	000084-66-2	90
4			Diethyl Phthalate	222	C12H14O4	000084-66-2	86
5			Phthalic acid, 2-ethoxyethyl eth...	266	C14H18O5	1000322-86-9	78

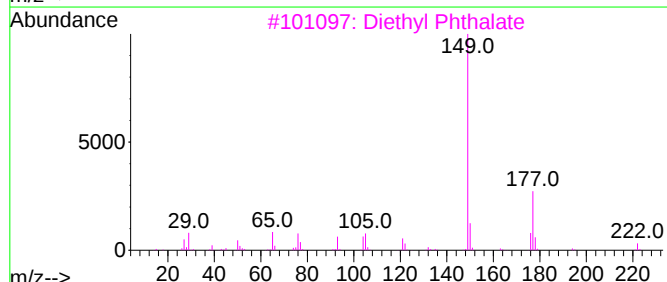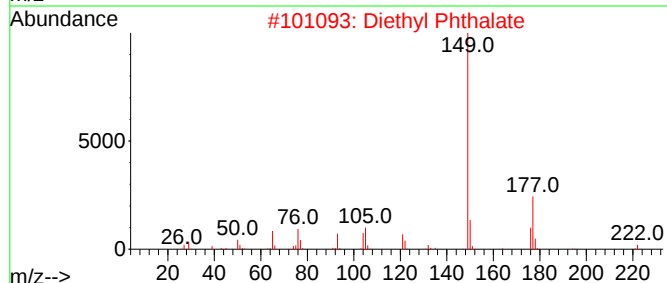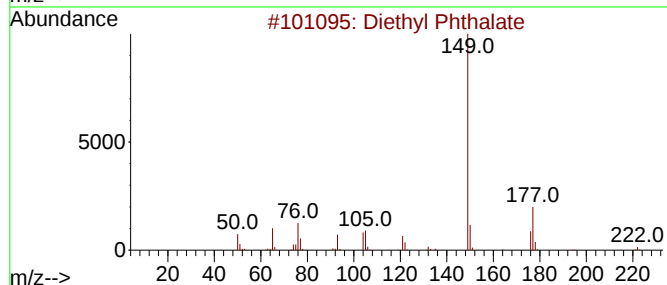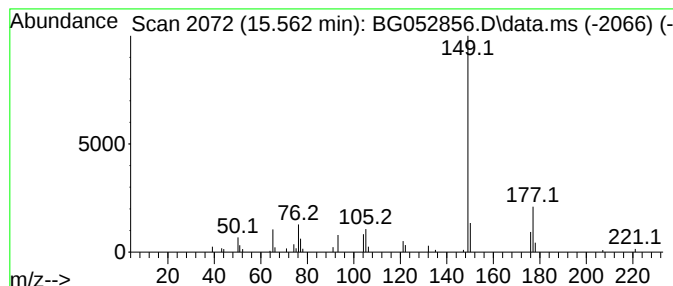

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052856.D
Acq On : 26 Mar 2022 9:35
Operator : CG/JU
Sample : N2079-16
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW5Z3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.419	3.90 ng/ul	129375	Chrysene-d12	21.789

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Nonadecene			266	C19H38	018435-45-5	95
2	Trichloroacetic acid, hexadecyl ...			386	C18H33Cl3O2	074339-54-1	93
3	1-Nonadecene			266	C19H38	018435-45-5	91
4	Bromoacetic acid, octadecyl ester			390	C20H39BrO2	018992-03-5	91
5	1-Octadecanol			270	C18H38O	000112-92-5	90

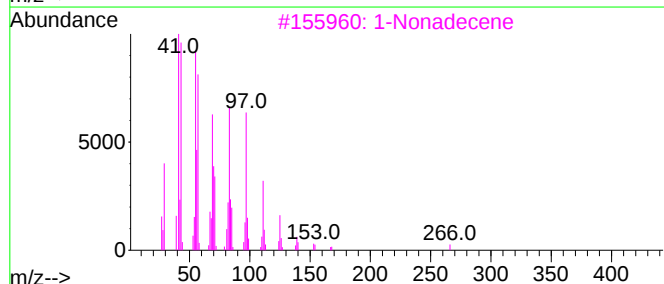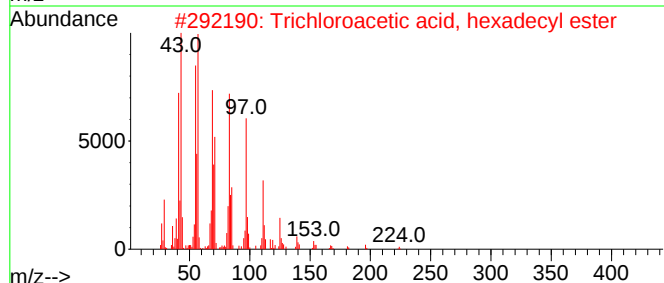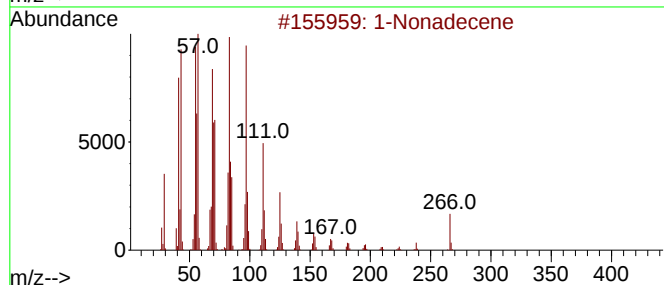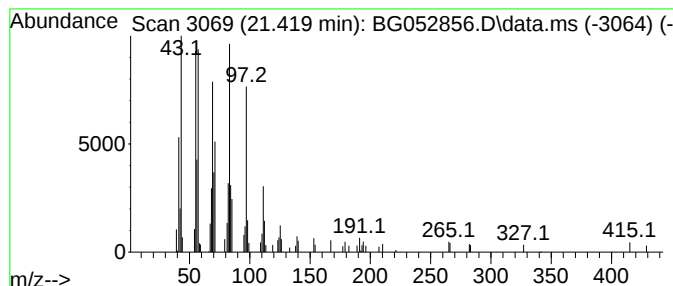

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052856.D
Acq On : 26 Mar 2022 9:35
Operator : CG/JU
Sample : N2079-16
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW5Z3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diethyl Phthalate	15.562	2.4	ng/u1	50894	3	14.758	418725	20.0
(DEL) Alkane: S...	21.419	3.9	ng/u1	129375	5	21.789	664182	20.0