

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052868.D
 Acq On : 26 Mar 2022 17:59
 Operator : CG/JU
 Sample : PB143606BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK606

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.555	24	28	34	rVB4	8976	13463	1.06%	0.115%
2	3.802	69	70	72	rBV	2587	1703	0.13%	0.015%
3	3.901	86	87	90	rBV2	2008	1710	0.13%	0.015%
4	3.966	95	98	108	rBV	98220	167258	13.12%	1.428%
5	4.172	131	133	136	rVB3	2423	2838	0.22%	0.024%
6	4.230	141	143	147	rBV3	1662	2284	0.18%	0.019%
7	4.430	176	177	180	rBV3	1751	1628	0.13%	0.014%
8	4.618	207	209	212	rBV3	1439	1894	0.15%	0.016%
9	4.648	212	214	217	rVB2	1782	1838	0.14%	0.016%
10	4.800	236	240	242	rBV3	1469	1848	0.15%	0.016%
11	4.841	245	247	249	rBV2	1372	1510	0.12%	0.013%
12	4.982	268	271	272	rBV3	1213	1436	0.11%	0.012%
13	5.070	283	286	287	rBV2	1311	1376	0.11%	0.012%
14	5.347	329	333	334	rBV4	1404	1616	0.13%	0.014%
15	5.623	378	380	385	rVB3	976	1374	0.11%	0.012%
16	6.439	518	519	524	rVB3	1507	1492	0.12%	0.013%
17	6.615	546	549	554	rBV4	774	1482	0.12%	0.013%
18	7.285	654	663	671	rBV	143141	249300	19.56%	2.128%
19	7.455	686	692	702	rBV	98873	170570	13.38%	1.456%
20	7.526	702	704	708	rVB2	900	1302	0.10%	0.011%
21	7.667	720	728	736	rBV	124483	223601	17.54%	1.909%
22	8.143	802	809	815	rVB	98702	168233	13.20%	1.436%
23	8.830	920	926	938	rBV	174071	306686	24.06%	2.618%
24	9.300	998	1006	1015	rVB	136758	253618	19.90%	2.165%
25	10.023	1123	1129	1137	rBV	117244	215625	16.92%	1.841%
26	10.563	1213	1221	1230	rBV	181433	328299	25.76%	2.802%
27	10.669	1237	1239	1244	rVB3	1184	1815	0.14%	0.015%
28	10.951	1280	1287	1297	rVB	148724	267943	21.02%	2.287%
29	11.074	1301	1308	1317	rBV	177239	337004	26.44%	2.877%
30	12.525	1551	1555	1560	rBV3	2689	5241	0.41%	0.045%
31	13.394	1698	1703	1707	rBV2	754	1557	0.12%	0.013%
32	14.158	1826	1833	1840	rBV	412850	603663	47.37%	5.153%
33	14.452	1876	1883	1892	rBV	409795	672217	52.74%	5.738%
34	14.757	1928	1935	1944	rBV	275196	449397	35.26%	3.836%
35	14.928	1957	1964	1984	rBV	193604	339651	26.65%	2.899%
36	15.580	2071	2075	2079	rVB2	1350	1884	0.15%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
 Data File : BG052868.D
 Acq On : 26 Mar 2022 17:59
 Operator : CG/JU
 Sample : PB143606BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK606

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	15.750	2097	2104	2111	rVV	576273	882531	69.25%	7.534%
38	15.856	2115	2122	2131	rBV	167478	264463	20.75%	2.258%
39	15.932	2133	2135	2137	rVV3	2159	1744	0.14%	0.015%
40	15.985	2141	2144	2150	rVB4	2824	3570	0.28%	0.030%
41	16.443	2220	2222	2228	rVB2	976	1455	0.11%	0.012%
42	16.526	2234	2236	2241	rVB3	3271	4064	0.32%	0.035%
43	17.283	2362	2365	2368	rBV2	2040	2603	0.20%	0.022%
44	17.501	2396	2402	2410	rVB	395694	613083	48.10%	5.234%
45	17.601	2412	2419	2430	rVV2	674543	1023879	80.34%	8.740%
46	18.082	2497	2501	2505	rBV3	1080	1721	0.14%	0.015%
47	18.323	2540	2542	2546	rVB2	1251	1569	0.12%	0.013%
48	18.458	2562	2565	2566	rBV2	1409	1435	0.11%	0.012%
49	18.582	2582	2586	2587	rVB3	1833	1670	0.13%	0.014%
50	18.752	2614	2615	2619	rBV3	1243	1563	0.12%	0.013%
51	18.881	2633	2637	2639	rBV2	1326	1923	0.15%	0.016%
52	18.958	2648	2650	2653	rBV3	1168	1279	0.10%	0.011%
53	19.257	2698	2701	2703	rBV3	1708	2419	0.19%	0.021%
54	19.451	2729	2734	2740	rBV5	11050	17242	1.35%	0.147%
55	19.521	2740	2746	2753	rBV3	10458	17705	1.39%	0.151%
56	19.798	2790	2793	2796	rBV4	1946	2348	0.18%	0.020%
57	19.886	2802	2808	2816	rVB	872987	1268135	99.50%	10.825%
58	20.138	2849	2851	2852	rBV2	2337	1279	0.10%	0.011%
59	20.156	2852	2854	2855	rBV2	2692	1417	0.11%	0.012%
60	20.279	2871	2875	2877	rBV5	2679	3588	0.28%	0.031%
61	20.332	2882	2884	2888	rBV4	2041	2646	0.21%	0.023%
62	20.397	2893	2895	2896	rBV2	2141	1748	0.14%	0.015%
63	20.456	2903	2905	2906	rBV2	2284	1870	0.15%	0.016%
64	20.473	2906	2908	2909	rVV	2438	1410	0.11%	0.012%
65	20.555	2921	2922	2924	rBV2	2601	2604	0.20%	0.022%
66	21.249	3038	3040	3041	rVB2	4769	2409	0.19%	0.021%
67	21.789	3125	3132	3141	rVB2	430807	748381	58.72%	6.388%
68	22.817	3305	3307	3308	rBV2	3934	2421	0.19%	0.021%
69	24.885	3647	3659	3671	rVB2	446517	1274469	100.00%	10.879%
70	25.108	3687	3697	3711	rVB2	242940	732893	57.51%	6.256%
71	26.776	3979	3981	3982	rBV2	3733	1957	0.15%	0.017%
72	29.067	4369	4371	4372	rVB2	4797	2283	0.18%	0.019%
73	30.395	4596	4597	4600	rBV2	4097	3388	0.27%	0.029%
74	31.452	4775	4777	4778	rBV2	4308	2120	0.17%	0.018%
75	31.635	4806	4808	4809	rBV	3513	2440	0.19%	0.021%
76	31.799	4835	4836	4840	rBV4	4180	2715	0.21%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052868.D
Acq On : 26 Mar 2022 17:59
Operator : CG/JU
Sample : PB143606BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK606

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Title : SVOA CALIBRATION

77	31.911	4854	4855	4856	rVB	5063	1785	0.14%	0.015%
----	--------	------	------	------	-----	------	------	-------	--------




Sum of corrected areas: 11714580

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052868.D
Acq On : 26 Mar 2022 17:59
Operator : CG/JU
Sample : PB143606BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK606

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

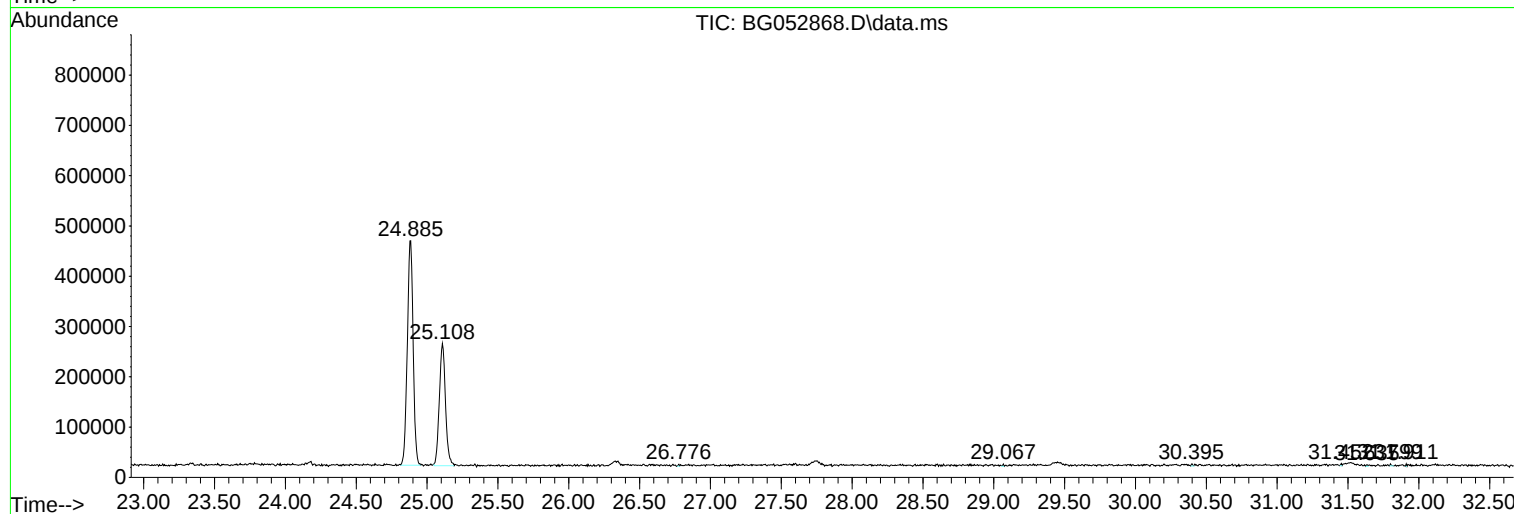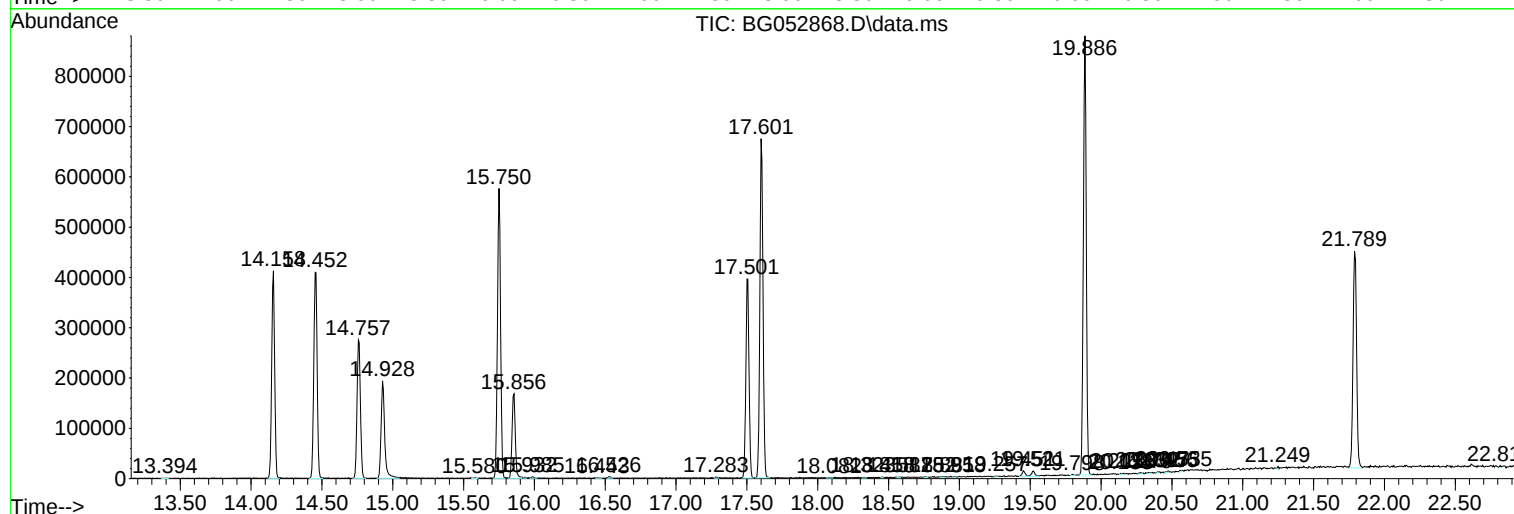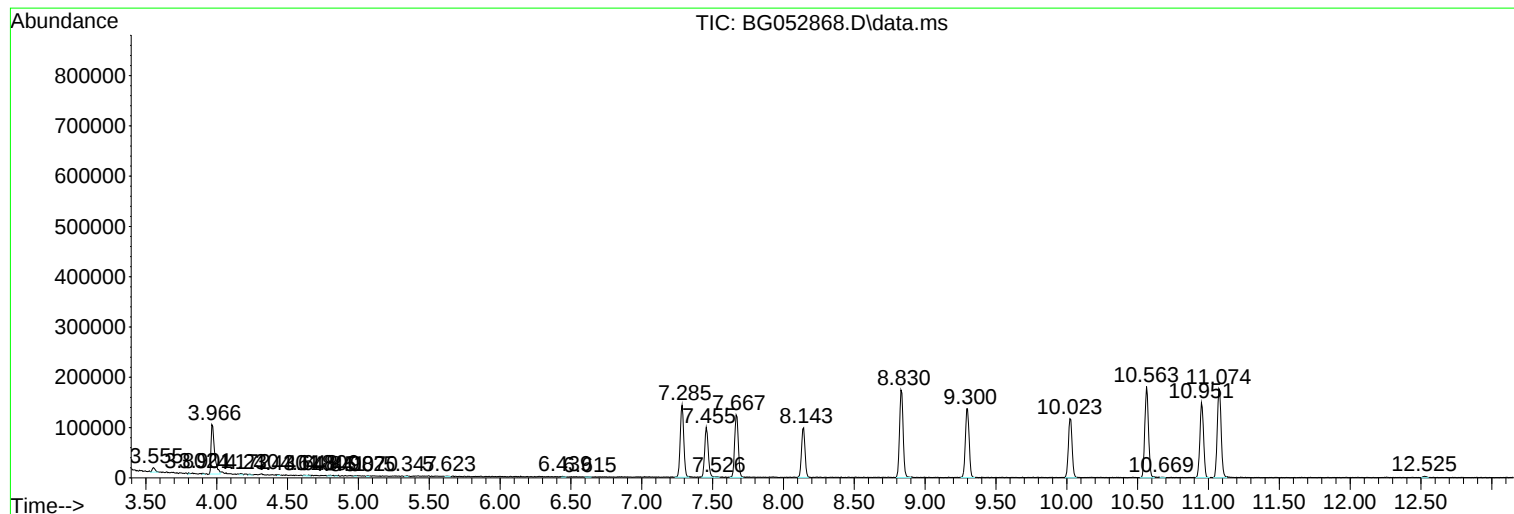

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052868.D
Acq On : 26 Mar 2022 17:59
Operator : CG/JU
Sample : PB143606BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK606

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032522\
Data File : BG052868.D
Acq On : 26 Mar 2022 17:59
Operator : CG/JU
Sample : PB143606BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK606

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc