

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032619\
 Data File : BG040160.D
 Acq On : 26 Mar 2019 23:38
 Operator : JU/SJ
 Sample : K2099-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MH-C02-SETTLED-1H-A

Quant Time: Mar 27 02:49:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 14:38:15 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.14	152	45859	20.00	ng	-0.03
21) Naphthalene-d8	10.96	136	226055	20.00	ng	-0.03
39) Acenaphthene-d10	14.76	164	121441	20.00	ng	-0.03
64) Phenanthrene-d10	17.51	188	281753	20.00	ng	-0.03
76) Chrysene-d12	21.79	240	281042	20.00	ng	-0.03
87) Perylene-d12	25.15	264	289889	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	128182	47.69	ng	-0.02
7) Phenol-d6	7.28	99	118466	29.56	ng	-0.03
23) Nitrobenzene-d5	9.32	82	338056	80.88	ng	-0.03
42) 2,4,6-Tribromophenol	16.25	330	139093	98.27	ng	-0.03
45) 2-Fluorobiphenyl	13.39	172	773697	90.71	ng	-0.03
79) Terphenyl-d14	20.10	244	1015768	79.58	ng	-0.02
Target Compounds						
15) Benzyl Alcohol	8.38	79	17240	5.422	ng	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032619\
Data File : BG040160.D
Acq On : 26 Mar 2019 23:38
Operator : JU/SJ
Sample : K2099-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MH-C02-SETTLED-1H-A

Quant Time: Mar 27 02:49:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 14:38:15 2019
Response via : Initial Calibration

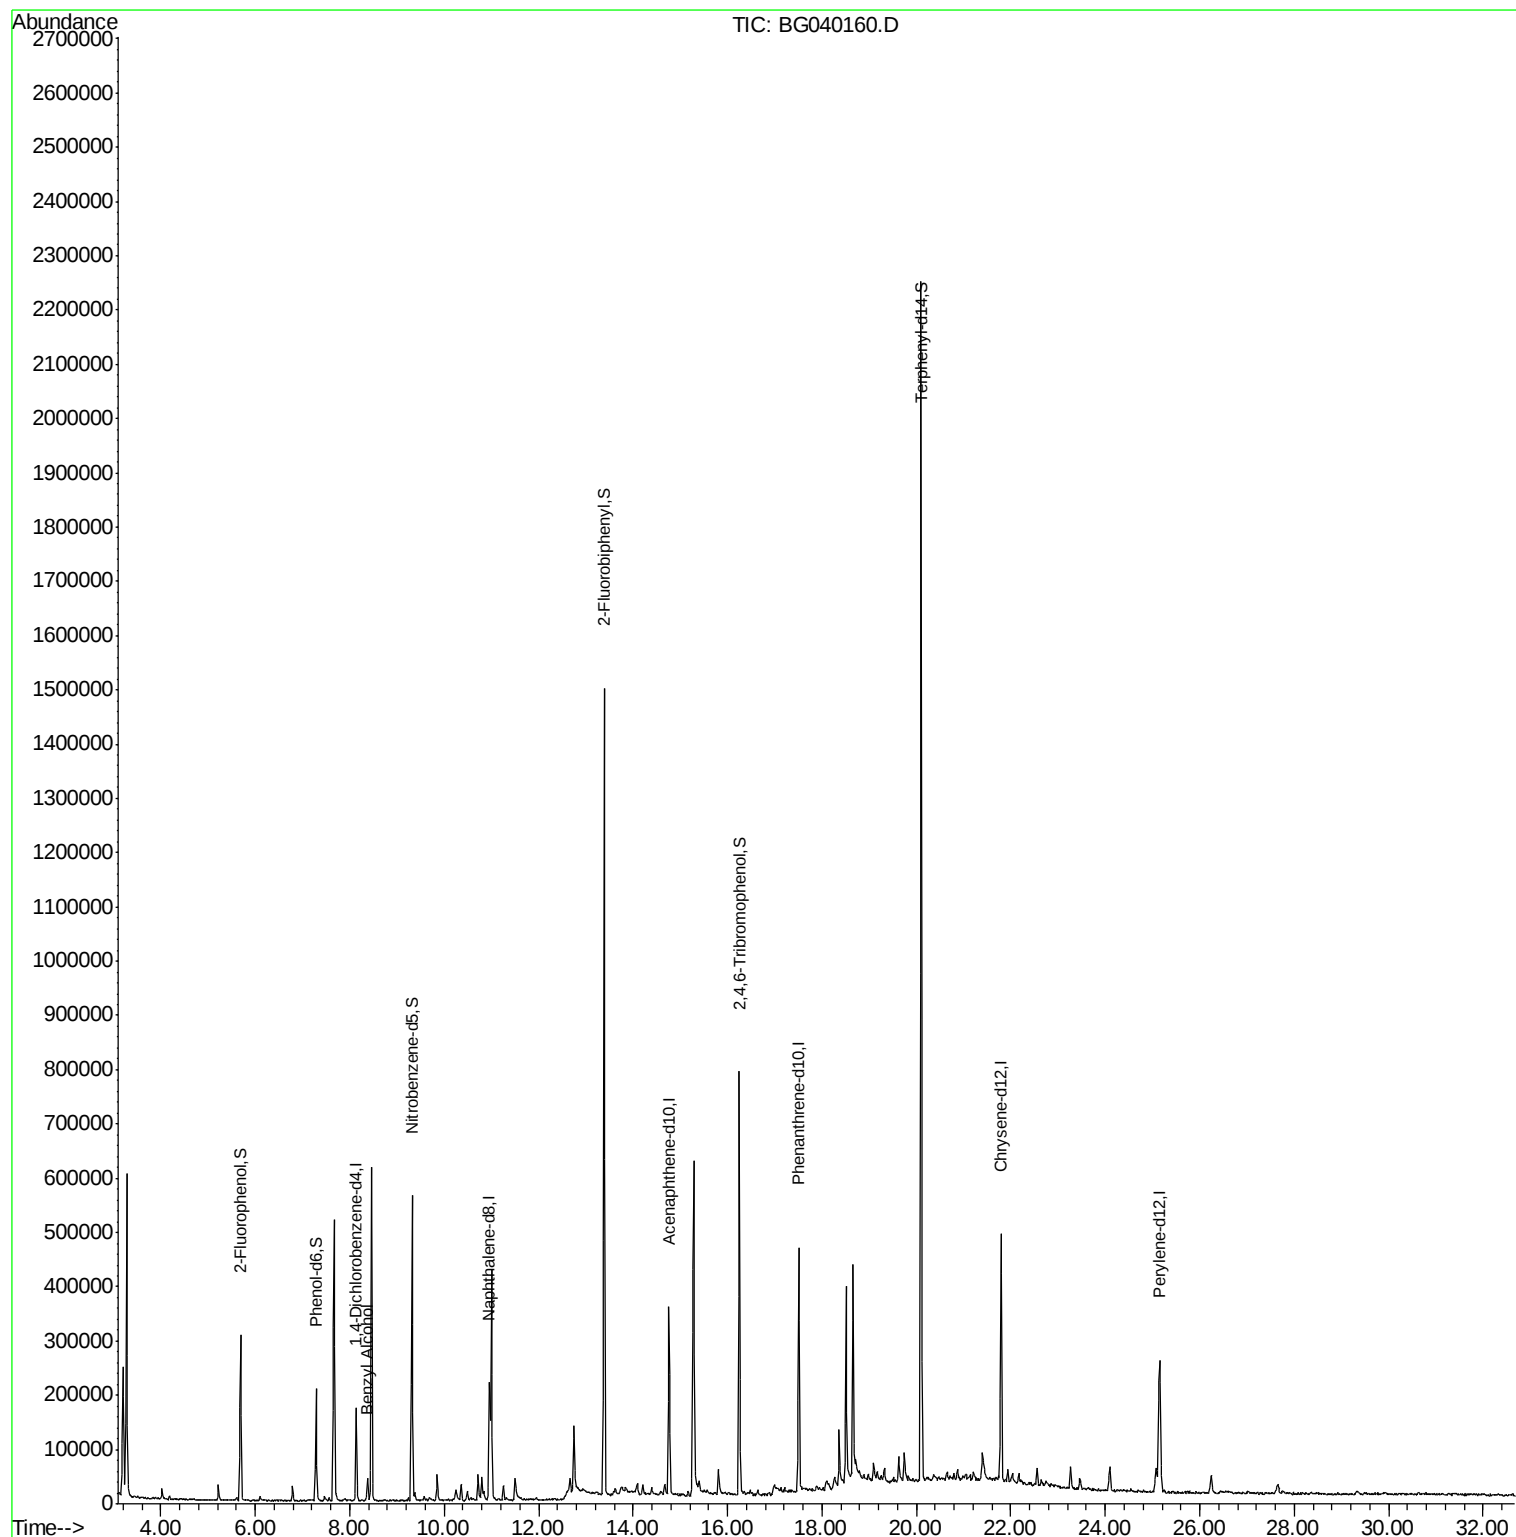



#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.14 min Scan# 859

Delta R.T. -0.03 min

Lab File: BG040160.D

Acq: 26 Mar 2019 23:38

Instrument :

BNA_G

ClientSampleId :

MH-C02-SETTLED-1H-A


Tot Ion:152 Resp: 45859

Ion Ratio Lower Upper

152 100

150 154.1 123.7 185.5




115 63.7 45.9 68.9

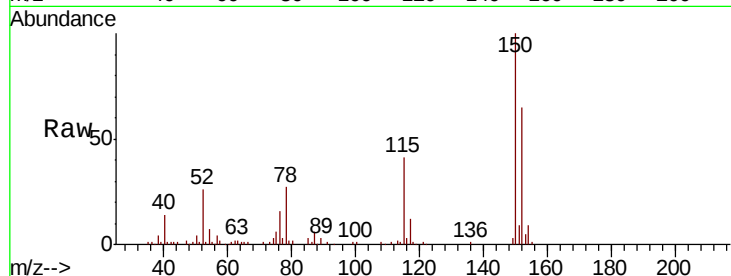

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

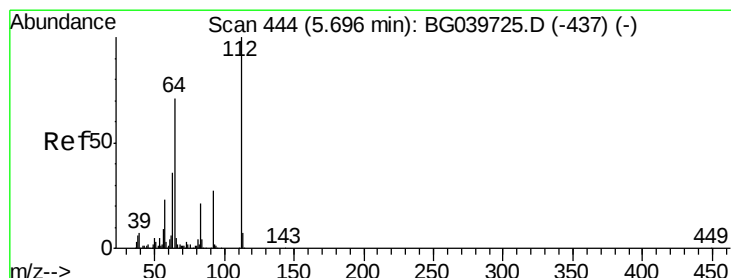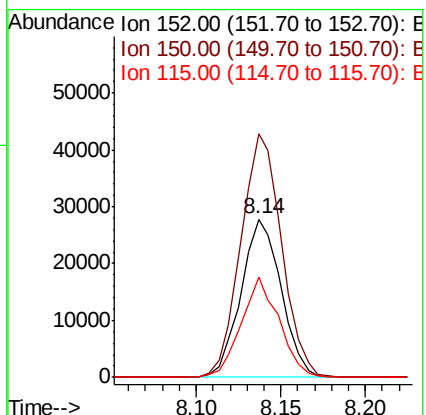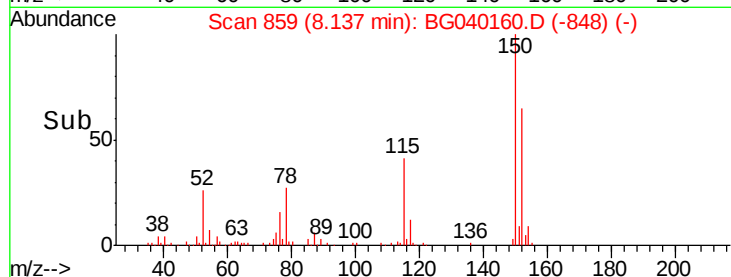

#5

2-Fluorophenol

Concen: 47.685 ng

RT: 5.69 min Scan# 442

Delta R.T. -0.02 min

Lab File: BG040160.D

Acq: 26 Mar 2019 23:38


Tgt Ion:112 Resp: 128182

Ion Ratio Lower Upper

112 100

64 65.0 57.8 86.8



63 35.8 29.8 44.6



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

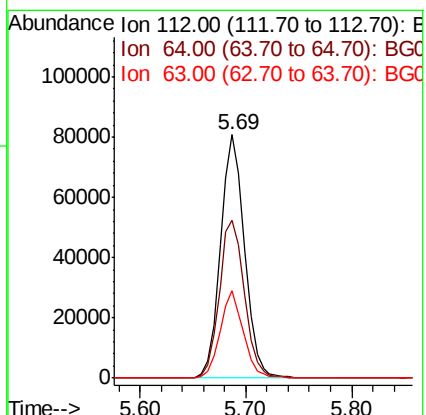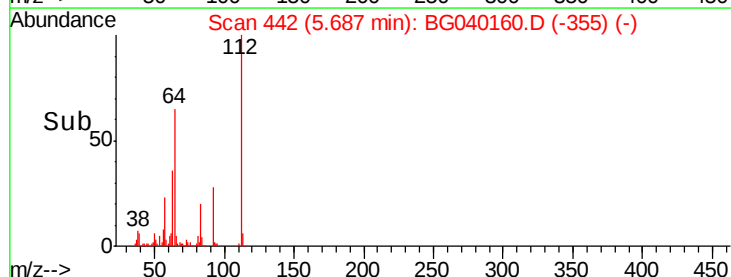



#7

Phenol-d6

Concen: 29.557 ng

RT: 7.28 min Scan# 714

Delta R.T. -0.03 min

Lab File: BG040160.D

Acq: 26 Mar 2019 23:38

Instrument :

BNA_G

ClientSampleId :

MH-C02-SETTLED-1H-A


Tot Ion: 99 Resp: 118466

Ion Ratio Lower Upper




99 100

42 17.7 18.2 27.2#

71 35.7 28.0 42.0

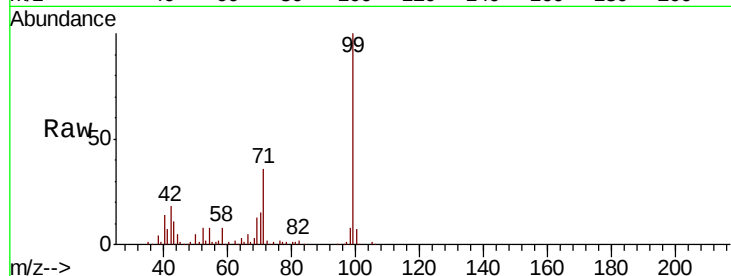

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

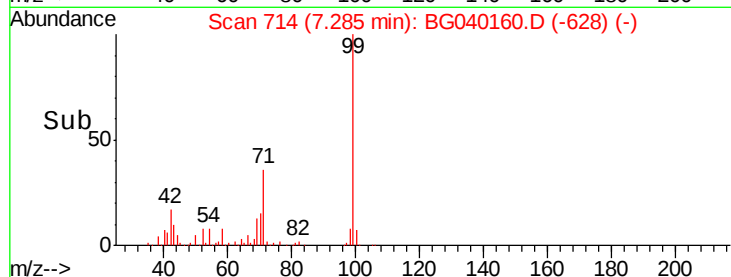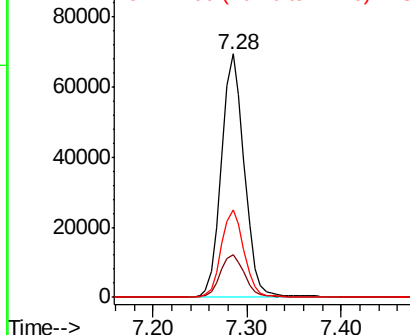

#15

Benzyl Alcohol

Concen: 5.422 ng

RT: 8.38 min Scan# 900

Delta R.T. -0.03 min

Lab File: BG040160.D

Acq: 26 Mar 2019 23:38


Tgt Ion: 79 Resp: 17240

Ion Ratio Lower Upper



79 100

108 77.7 57.8 86.6

77 62.4 51.1 76.7



Abundance Ion 79.00 (78.70 to 79.70): BGC
Ion 108.00 (107.70 to 108.70): BGC
Ion 77.00 (76.70 to 77.70): BGC

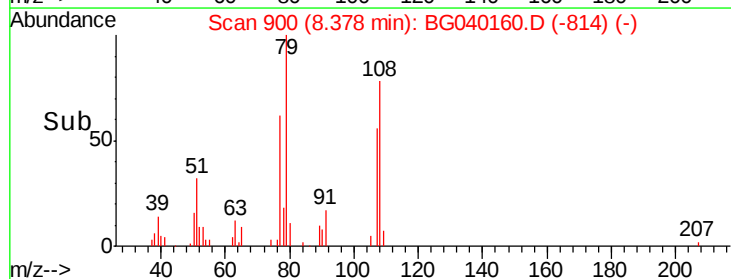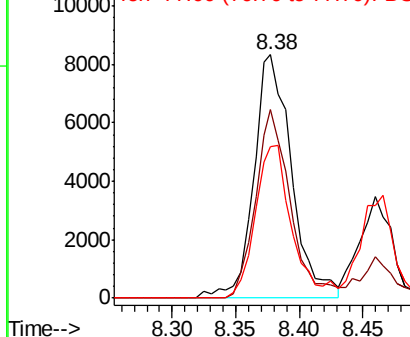







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.96 min Scan# 1339
Delta R.T. -0.03 min
Lab File: BG040160.D
Acq: 26 Mar 2019 23:38

Instrument :
BNA_G
ClientSampleId :
MH-C02-SETTLED-1H-A

Tot Ion:136	Resp:	226055
Ion	Ratio	Lower Upper
136	100	
137	11.6	9.1 13.7
54	11.0	9.4 14.2
68	6.0	4.2 6.4




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

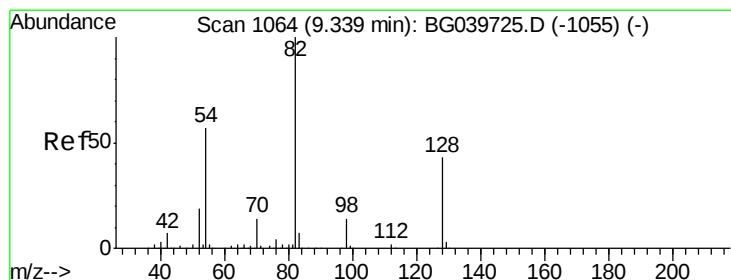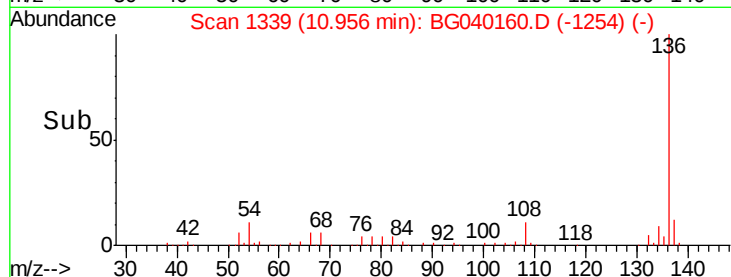
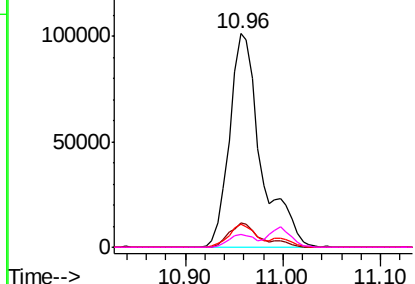



#23
Nitrobenzene-d5
Concen: 80.880 ng
RT: 9.32 min Scan# 1060
Delta R.T. -0.03 min
Lab File: BG040160.D
Acq: 26 Mar 2019 23:38

Tgt Ion: 82	Resp:	338056
Ion	Ratio	Lower Upper
82	100	
128	44.5	31.3 46.9
54	57.9	50.9 76.3



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

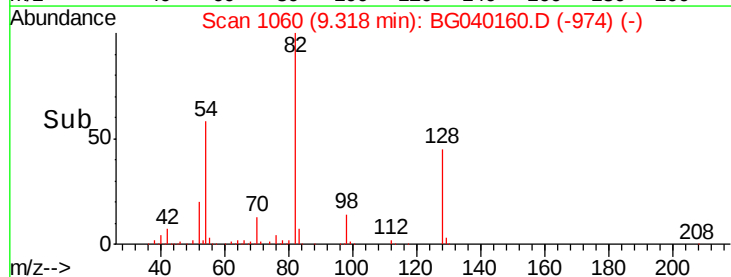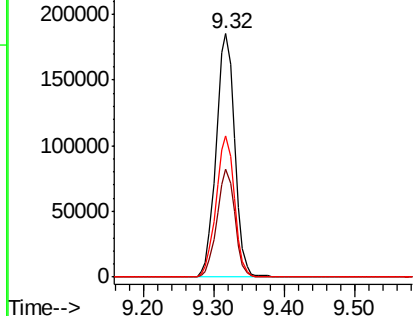

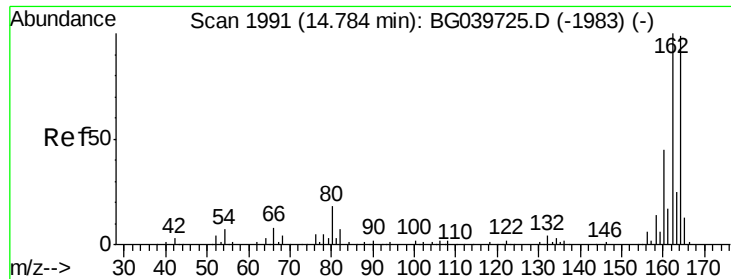

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.76 min Scan# 1987

Delta R.T. -0.03 min

Lab File: BG040160.D

Acq: 26 Mar 2019 23:38

Instrument :

BNA_G

ClientSampleId :

MH-C02-SETTLED-1H-A


Tot Ion:164 Resp: 121441

Ion Ratio Lower Upper

164 100

162 107.6 81.6 122.4




160 45.4 34.2 51.2



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

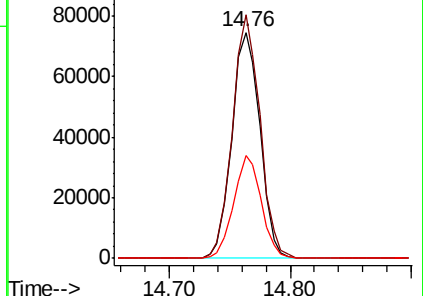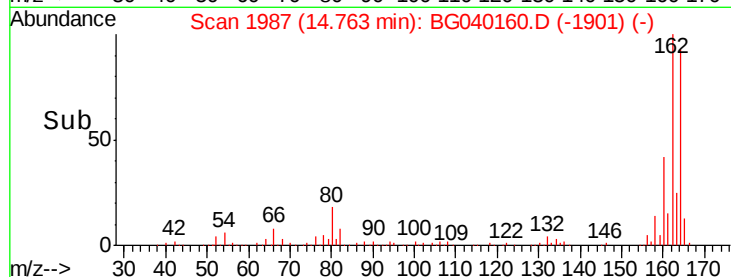

#42

2,4,6-Tribromophenol

Concen: 98.265 ng

RT: 16.25 min Scan# 2240

Delta R.T. -0.03 min

Lab File: BG040160.D

Acq: 26 Mar 2019 23:38


Tgt Ion:330 Resp: 139093

Ion Ratio Lower Upper

330 100

332 96.5 75.7 113.5



141 41.3 35.6 53.4



Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



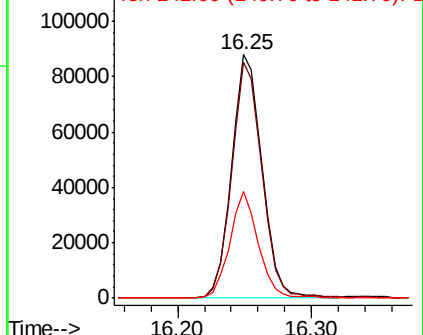
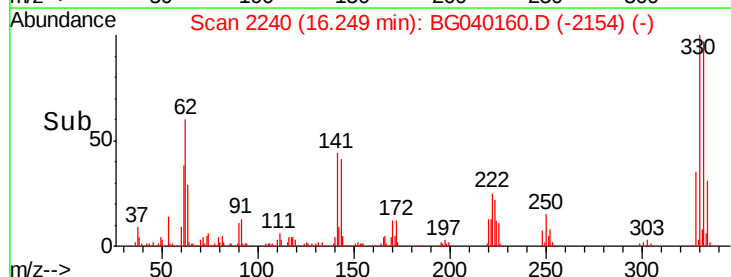




#45
 2-Fluorobiphenyl
 Concen: 90.712 ng
 RT: 13.39 min Scan# 1753
 Delta R.T. -0.03 min
 Lab File: BG040160.D
 Acq: 26 Mar 2019 23:38




Instrument :
 BNA_G
 ClientSampleId :
 MH-C02-SETTLED-1H-A


Tot Ion	Ratio	Lower	Upper
172	100		
171	37.1	30.8	46.2
170	25.0	20.2	30.4

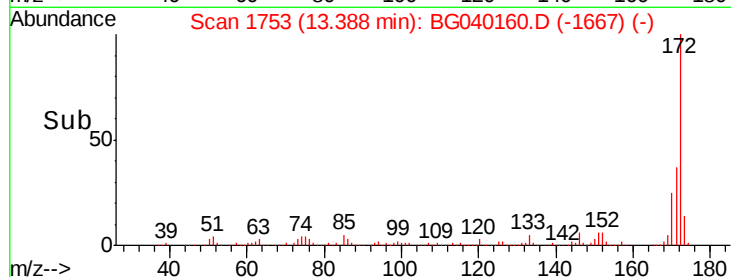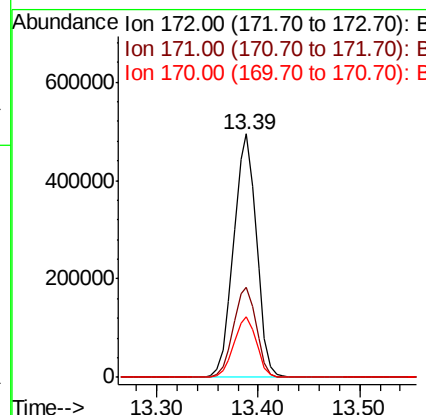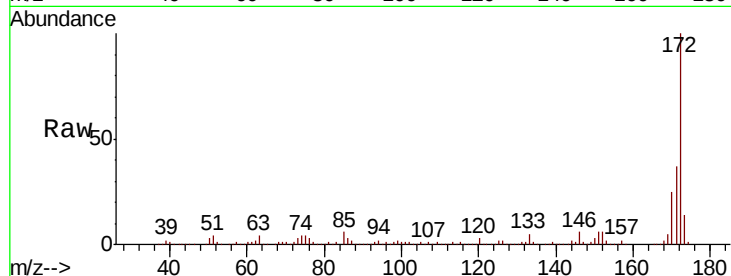

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.51 min Scan# 2454
 Delta R.T. -0.03 min
 Lab File: BG040160.D
 Acq: 26 Mar 2019 23:38

Tgt Ion	Ratio	Lower	Upper
188	100		
94	7.7	6.9	10.3
80	8.7	8.1	12.1


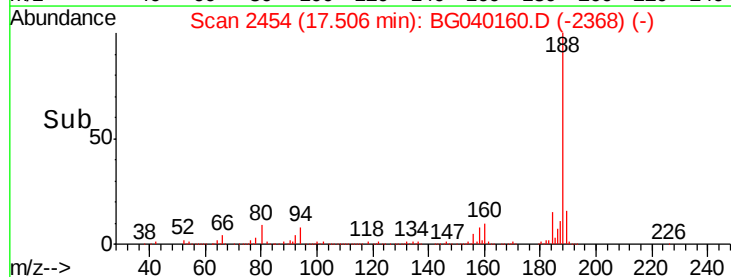
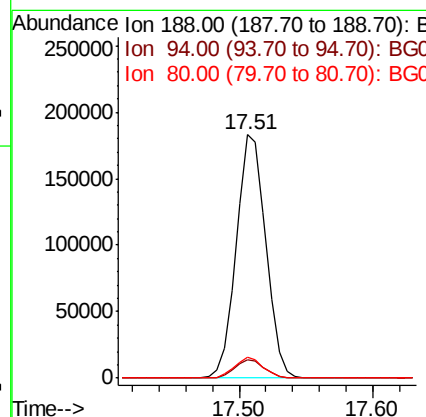



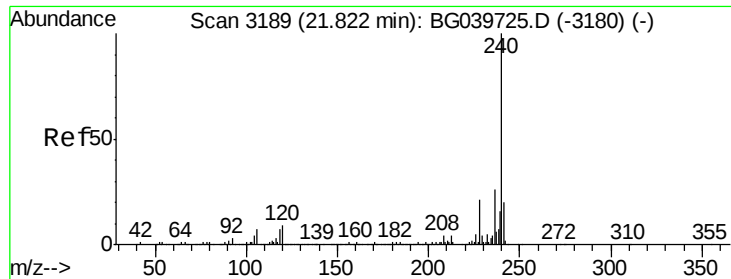

#76
 Chrvsene-d12
 Concen: 20.000 ng
 RT: 21.79 min Scan# 3184
 Delta R.T. -0.03 min
 Lab File: BG040160.D
 Acq: 26 Mar 2019 23:38




Instrument :
 BNA_G
 ClientSampleId :
 MH-C02-SETTLED-1H-A


Tot Ion:240 Resp: 281042
 Ion Ratio Lower Upper
 240 100
 120 8.1 7.0 10.6
 236 27.5 21.0 31.4

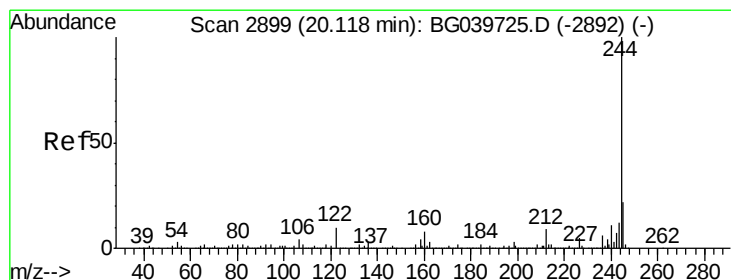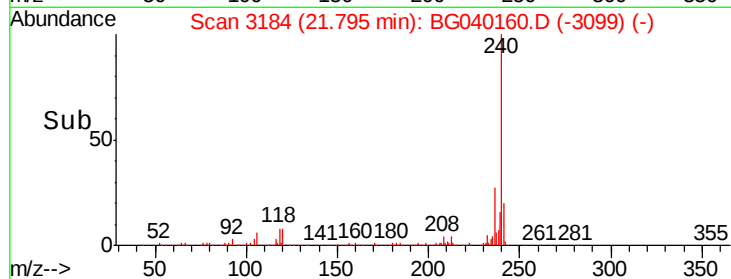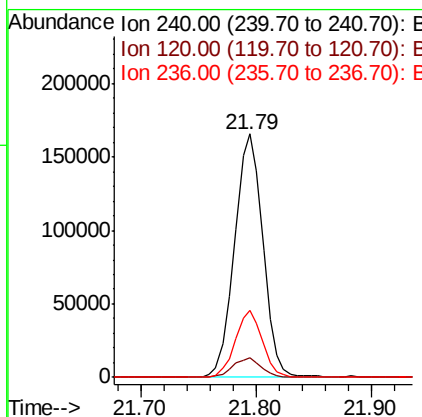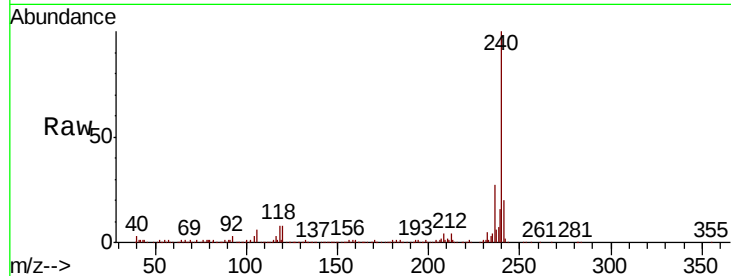

#79
 Terphenyl-d14
 Concen: 79.580 ng
 RT: 20.10 min Scan# 2896
 Delta R.T. -0.02 min
 Lab File: BG040160.D
 Acq: 26 Mar 2019 23:38

Tgt Ion:244 Resp: 1015768
 Ion Ratio Lower Upper
 244 100
 212 9.0 7.3 10.9
 122 9.0 8.4 12.6

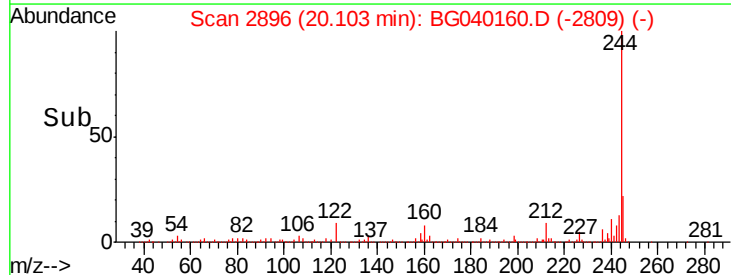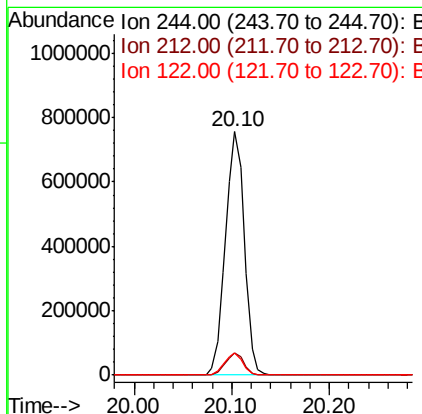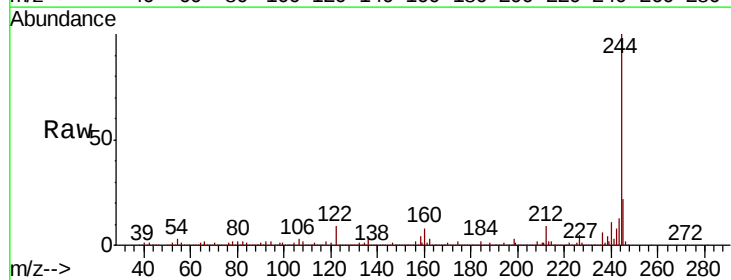

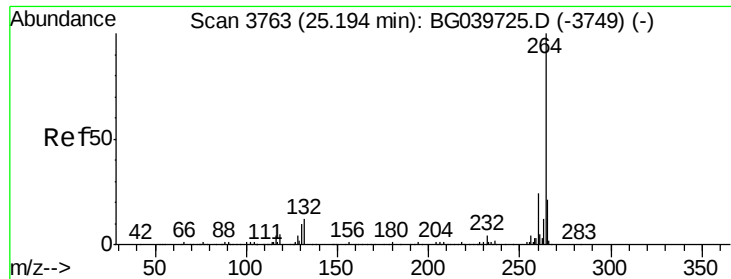

#87
Pervlene-d12
Concen: 20.000 ng
RT: 25.15 min Scan# 3755
Delta R.T. -0.05 min
Lab File: BG040160.D
Acq: 26 Mar 2019 23:38

Instrument :
BNA_G
ClientSampleId :
MH-C02-SETTLED-1H-A

Tot Ion: 264 Resp: 289889

Ion	Ratio	Lower	Upper
264	100		
260	23.8	18.2	27.4
265	21.3	18.5	27.7

