


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032619\
 Data File : BG040147.D
 Acq On : 26 Mar 2019 14:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

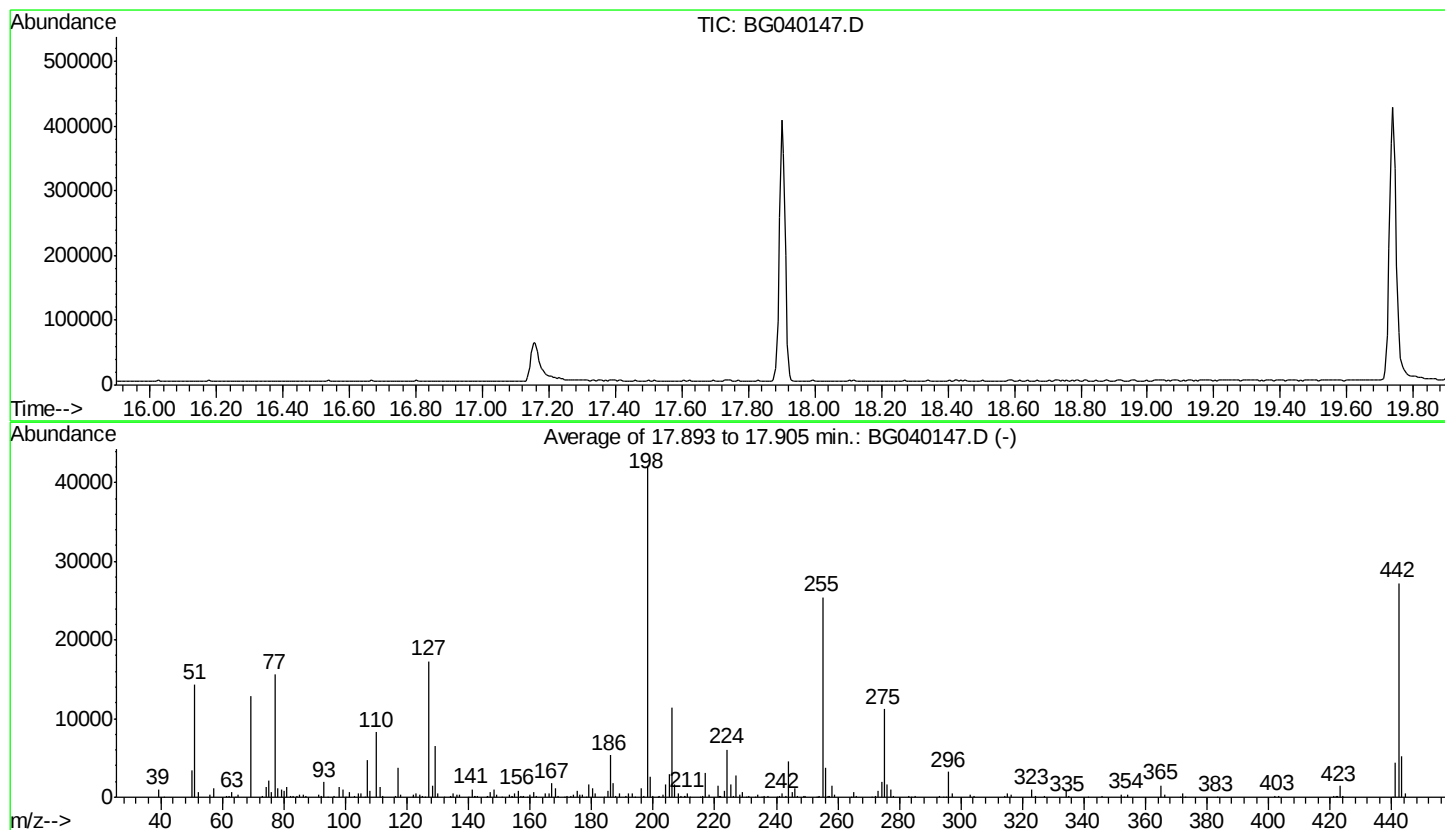

AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	14277	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.3	12787	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.0	17288	PASS
197	198	0.00	2	0.5	222	PASS
198	198	100	100	100.0	42160	PASS
199	198	5	9	6.1	2581	PASS
275	198	10	60	26.6	11217	PASS
365	198	1	100	3.5	1480	PASS
441	198	0.01	100	10.5	4442	PASS
442	198	50	100	64.6	27249	PASS
443	442	15	24	19.2	5223	PASS