


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032619\
 Data File : BG040166.D
 Acq On : 27 Mar 2019 3:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 04 14:38:15 2019

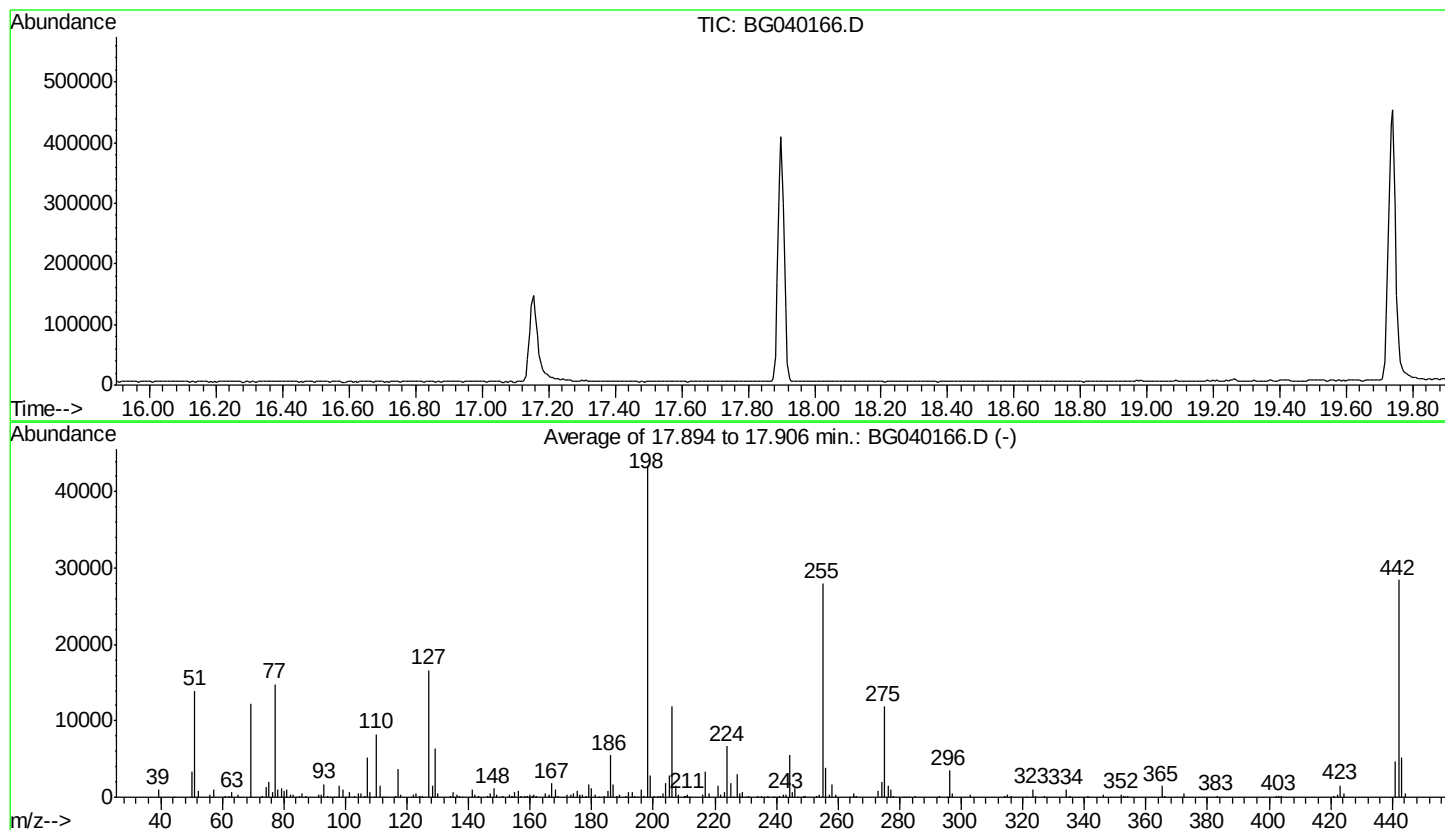

AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	13915	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.0	12179	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.4	16664	PASS
197	198	0.00	2	0.3	123	PASS
198	198	100	100	100.0	43426	PASS
199	198	5	9	6.4	2773	PASS
275	198	10	60	27.3	11845	PASS
365	198	1	100	3.4	1466	PASS
441	198	0.01	100	10.8	4698	PASS
442	198	50	100	65.6	28477	PASS
443	442	15	24	18.5	5262	PASS