

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032819\
 Data File : BG040227.D
 Acq On : 29 Mar 2019 9:41
 Operator : JU/SJ
 Sample : K2107-18
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-9

Quant Time: Mar 29 13:26:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 28 05:47:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	57992	20.00	ng	0.00
21) Naphthalene-d8	10.89	136	236419	20.00	ng	0.00
39) Acenaphthene-d10	14.70	164	143935	20.00	ng	0.00
64) Phenanthrene-d10	17.44	188	372747	20.00	ng	0.00
76) Chrysene-d12	21.72	240	409765	20.00	ng	-0.01
87) Perylene-d12	25.02	264	401089	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	456985	131.00	ng	0.00
7) Phenol-d6	7.22	99	582283	120.78	ng	0.00
23) Nitrobenzene-d5	9.25	82	411742	92.57	ng	0.00
42) 2,4,6-Tribromophenol	16.19	330	224233	144.15	ng	0.00
45) 2-Fluorobiphenyl	13.32	172	923135	95.03	ng	0.00
79) Terphenyl-d14	20.05	244	1552363	85.23	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032819\
Data File : BG040227.D
Acq On : 29 Mar 2019 9:41
Operator : JU/SJ
Sample : K2107-18
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-9

Quant Time: Mar 29 13:26:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 28 05:47:00 2019
Response via : Initial Calibration

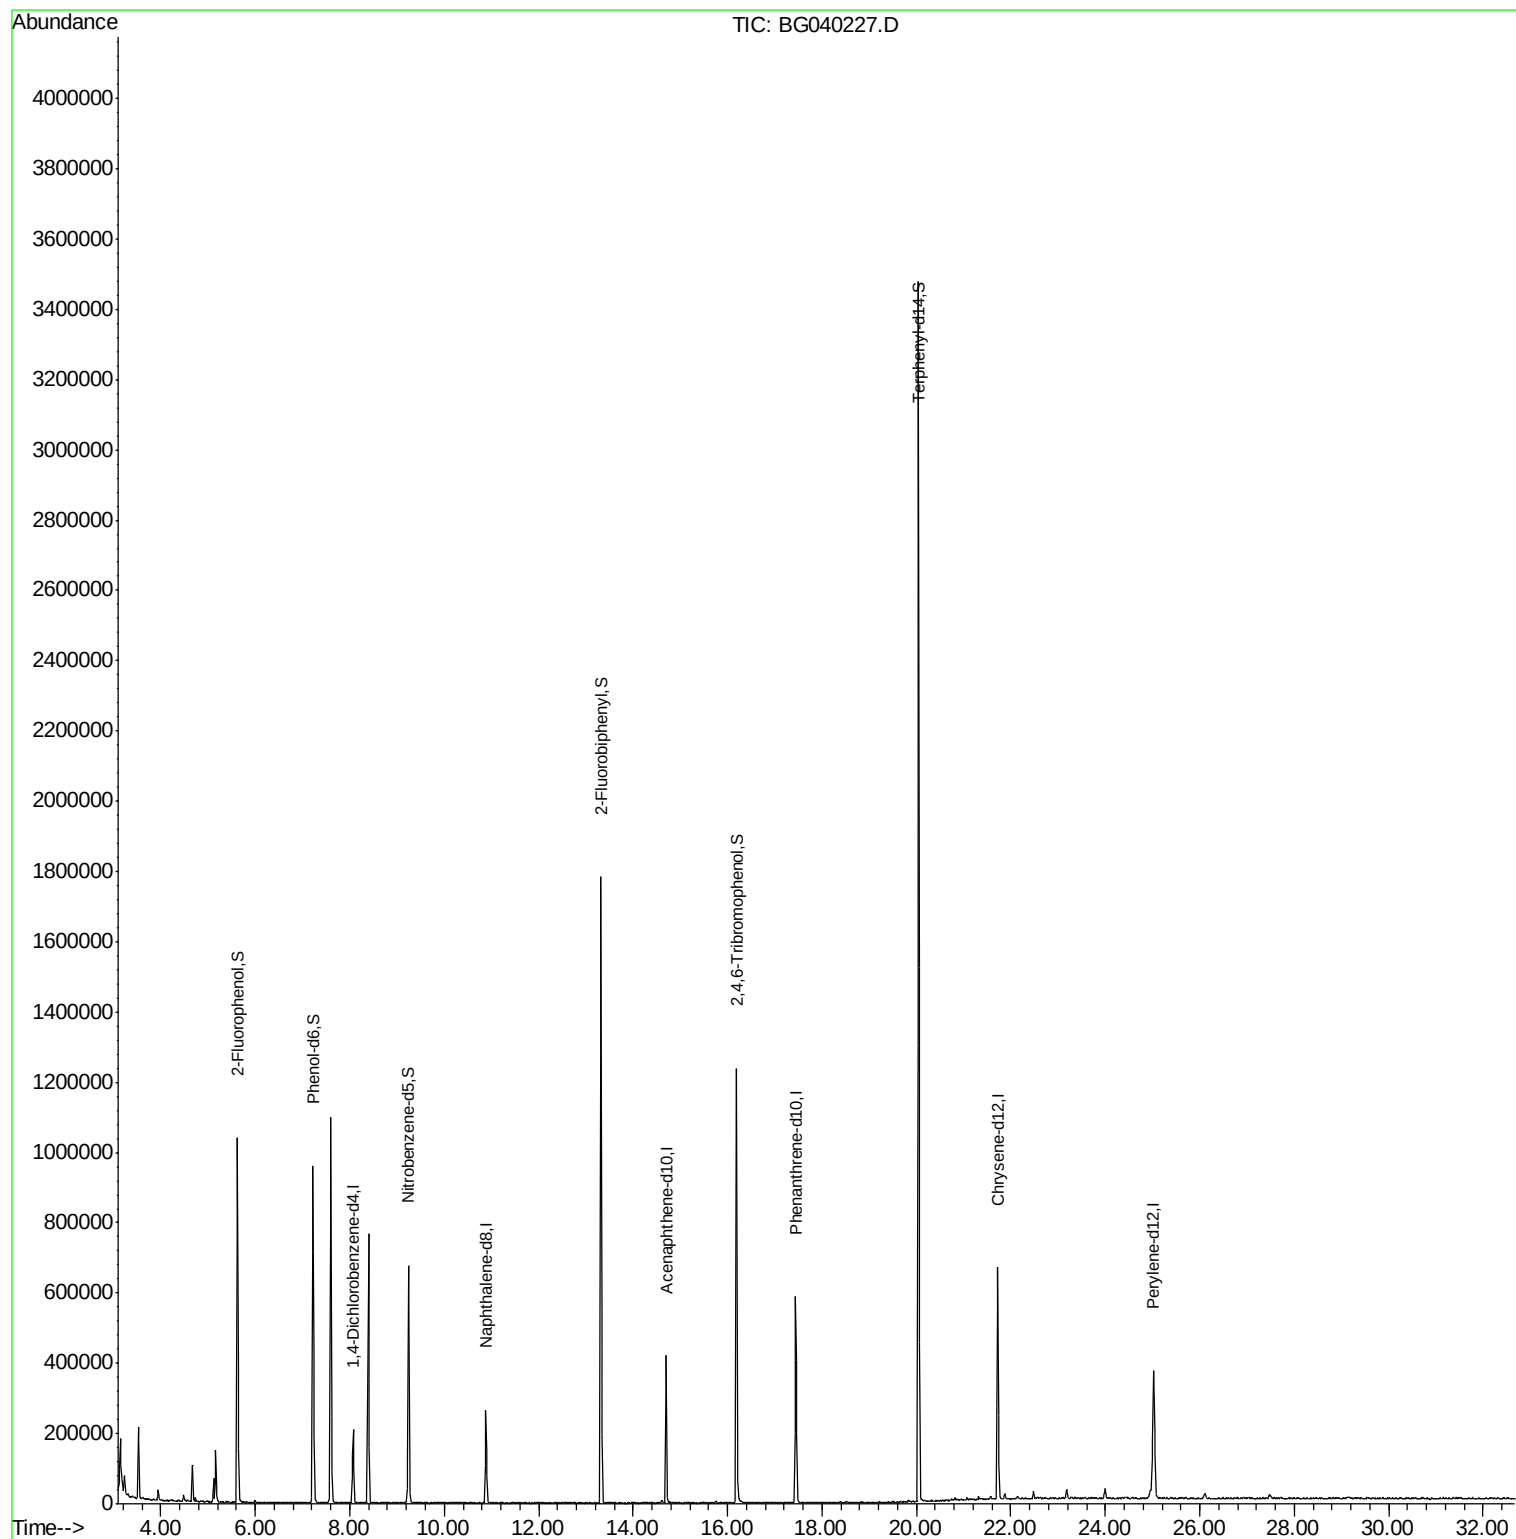




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.07 min Scan# 848
Delta R.T. 0.00 min
Lab File: BG040227.D
Acq: 29 Mar 2019 9:41

Instrument :
BNA_G
ClientSampleId :
TP-9

Tot Ion	Ratio	Lower	Upper
152	100		
150	168.2	123.7	185.5
115	64.2	46.9	70.3






Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

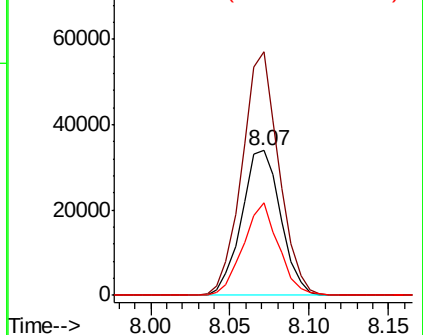

#5

2-Fluorophenol
Concen: 131.000 ng
RT: 5.63 min Scan# 432
Delta R.T. 0.01 min
Lab File: BG040227.D
Acq: 29 Mar 2019 9:41

Tgt Ion	Ratio	Lower	Upper
112	100		
64	67.0	54.2	81.2
63	33.1	26.4	39.6






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG0

Ion 63.00 (62.70 to 63.70): BG0

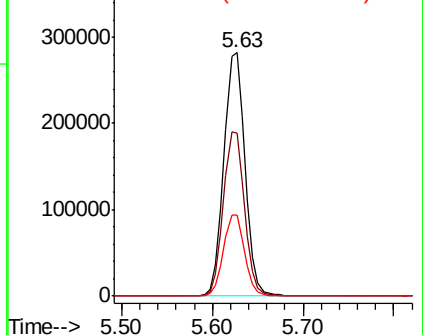



#7

Phenol-d6

Concen: 120.779 ng

RT: 7.22 min Scan# 704

Delta R.T. 0.00 min

Lab File: BG040227.D

Acq: 29 Mar 2019 9:41

Instrument :

BNA_G

ClientSampled :

TP-9


Tot Ion: 99 Resp: 582283

Ion Ratio Lower Upper




99 100

42 18.5 16.2 24.2

71 33.4 26.8 40.2

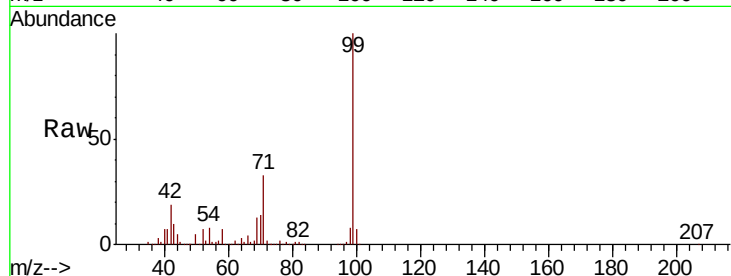

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

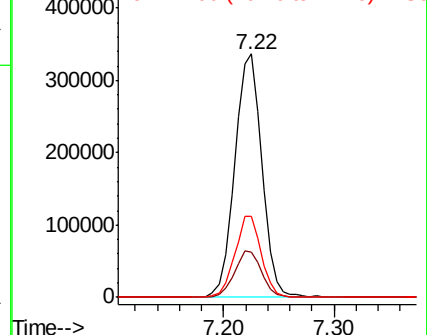

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.89 min Scan# 1327

Delta R.T. 0.00 min

Lab File: BG040227.D

Acq: 29 Mar 2019 9:41

Tgt Ion: 136 Resp: 236419


Ion Ratio Lower Upper

136 100



137 10.3 8.9 13.3


54 10.1 9.6 14.4

68 6.1 5.1 7.7



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

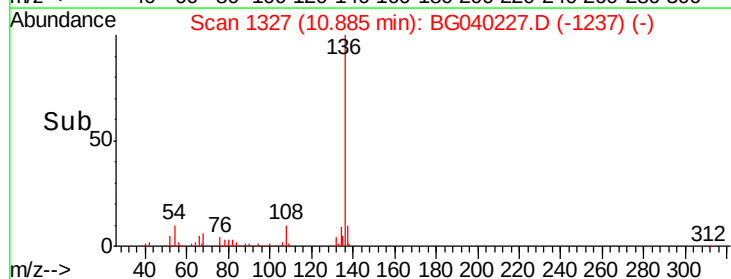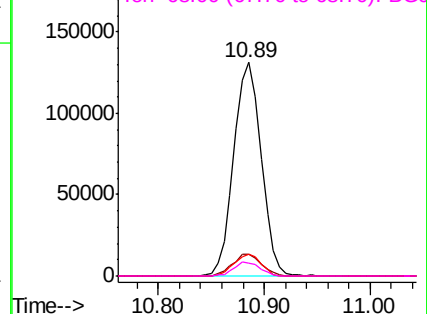







#23
 Nitrobenzene-d5
 Concen: 92.571 ng
 RT: 9.25 min Scan# 1048
 Delta R.T. 0.00 min
 Lab File: BG040227.D
 Acq: 29 Mar 2019 9:41

Instrument :
 BNA_G
 ClientSampled :
 TP-9

Tot Ion: 82 Resp: 411742
 Ion Ratio Lower Upper
 82 100
 128 43.6 35.8 53.8
 54 54.9 46.2 69.2

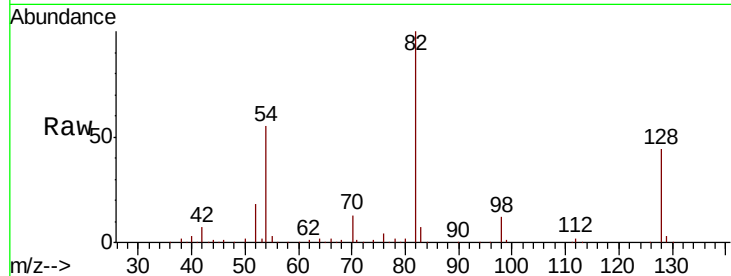


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC


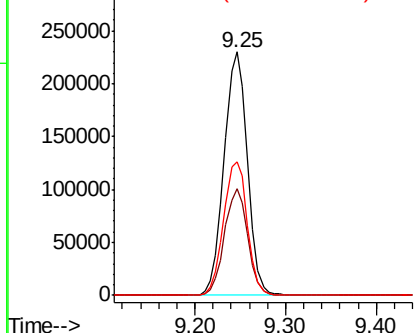



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.70 min Scan# 1976
 Delta R.T. -0.00 min
 Lab File: BG040227.D
 Acq: 29 Mar 2019 9:41

Tgt Ion:164 Resp: 143935
 Ion Ratio Lower Upper
 164 100
 162 104.0 77.4 116.2
 160 44.4 35.3 52.9

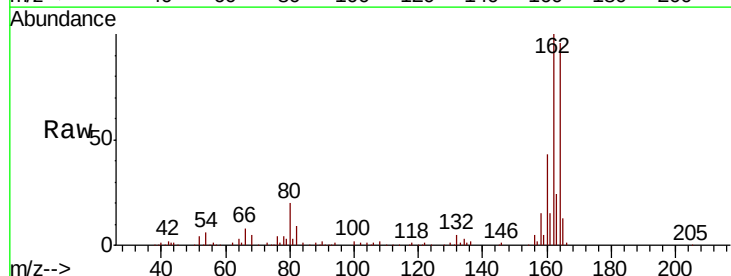

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

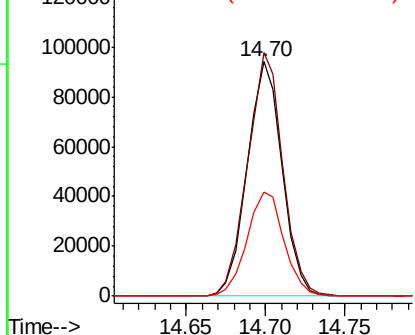


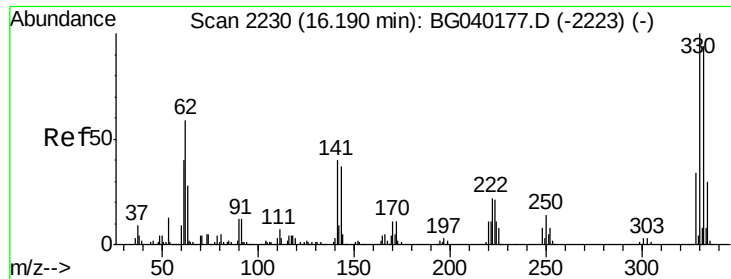

#42
 2,4,6-Tribromophenol
 Concen: 144.149 ng
 RT: 16.19 min Scan# 2230
 Delta R.T. 0.00 min
 Lab File: BG040227.D
 Acq: 29 Mar 2019 9:41

Instrument :
 BNA_G
 ClientSampled :
 TP-9

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.7	76.6	115.0
141	40.2	32.6	48.8



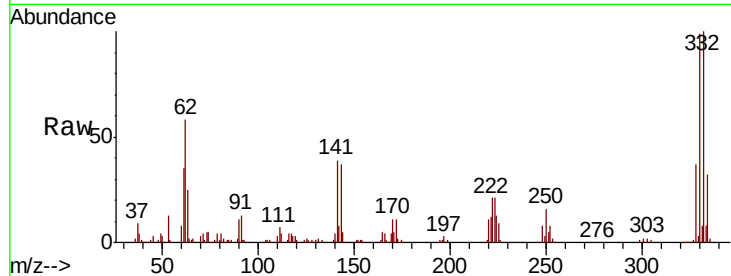


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

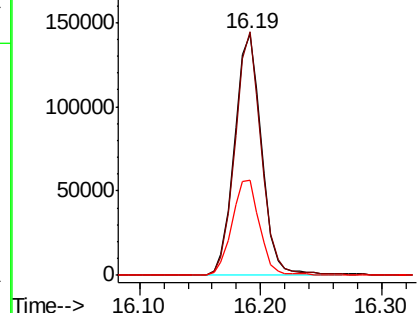

#45
 2-Fluorobiphenyl
 Concen: 95.034 ng
 RT: 13.32 min Scan# 1741
 Delta R.T. -0.00 min
 Lab File: BG040227.D
 Acq: 29 Mar 2019 9:41

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.5	30.5	45.7
170	24.6	20.1	30.1






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

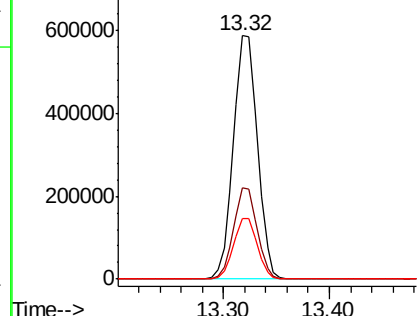

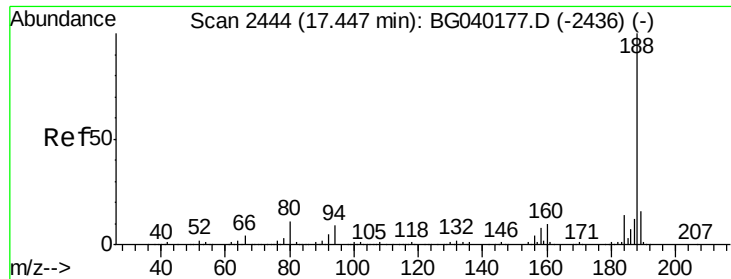

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.44 min Scan# 2443

Delta R.T. -0.00 min

Lab File: BG040227.D

Acq: 29 Mar 2019 9:41

Instrument :

BNA_G

ClientSampleId :

TP-9


Tot Ion:188 Resp: 372747

Ion Ratio Lower Upper

188 100

94 9.1 7.0 10.4




80 9.4 8.6 13.0

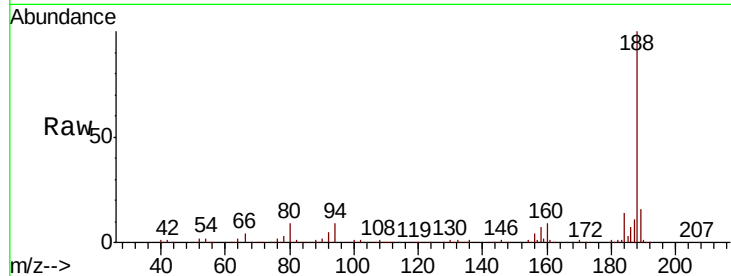

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

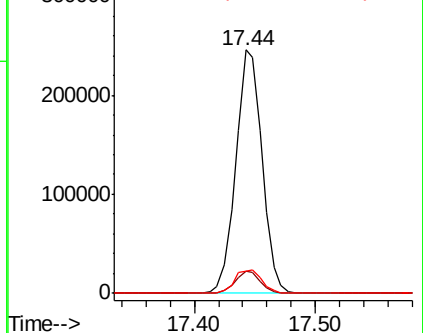

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.72 min Scan# 3171

Delta R.T. -0.01 min

Lab File: BG040227.D

Acq: 29 Mar 2019 9:41


Tgt Ion:240 Resp: 409765

Ion Ratio Lower Upper

240 100

120 10.7 8.4 12.6



236 26.3 20.8 31.2




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

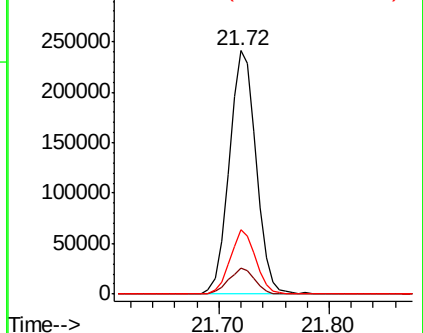



#79

Terphenyl-d14

Concen: 85.226 ng

RT: 20.05 min Scan# 2886

Delta R.T. -0.00 min

Lab File: BG040227.D

Acq: 29 Mar 2019 9:41

Instrument :

BNA_G

ClientSampleId :

TP-9


Tot Ion:244 Resp: 1552363

Ion Ratio Lower Upper




244 100

212 8.9 7.0 10.6

122 11.9 8.5 12.7



Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

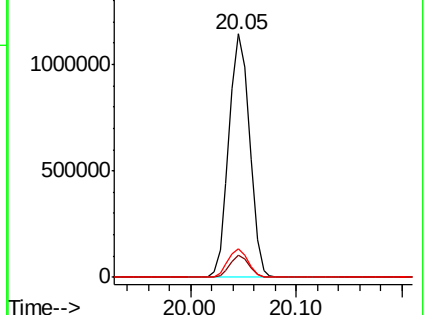

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.02 min Scan# 3733

Delta R.T. -0.01 min

Lab File: BG040227.D

Acq: 29 Mar 2019 9:41


Tgt Ion:264 Resp: 401089

Ion Ratio Lower Upper

264 100

260 23.3 17.9 26.9

265 21.6 16.8 25.2



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

