


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032819\
 Data File : BG040192.D
 Acq On : 28 Mar 2019 9:43
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 28 05:47:00 2019

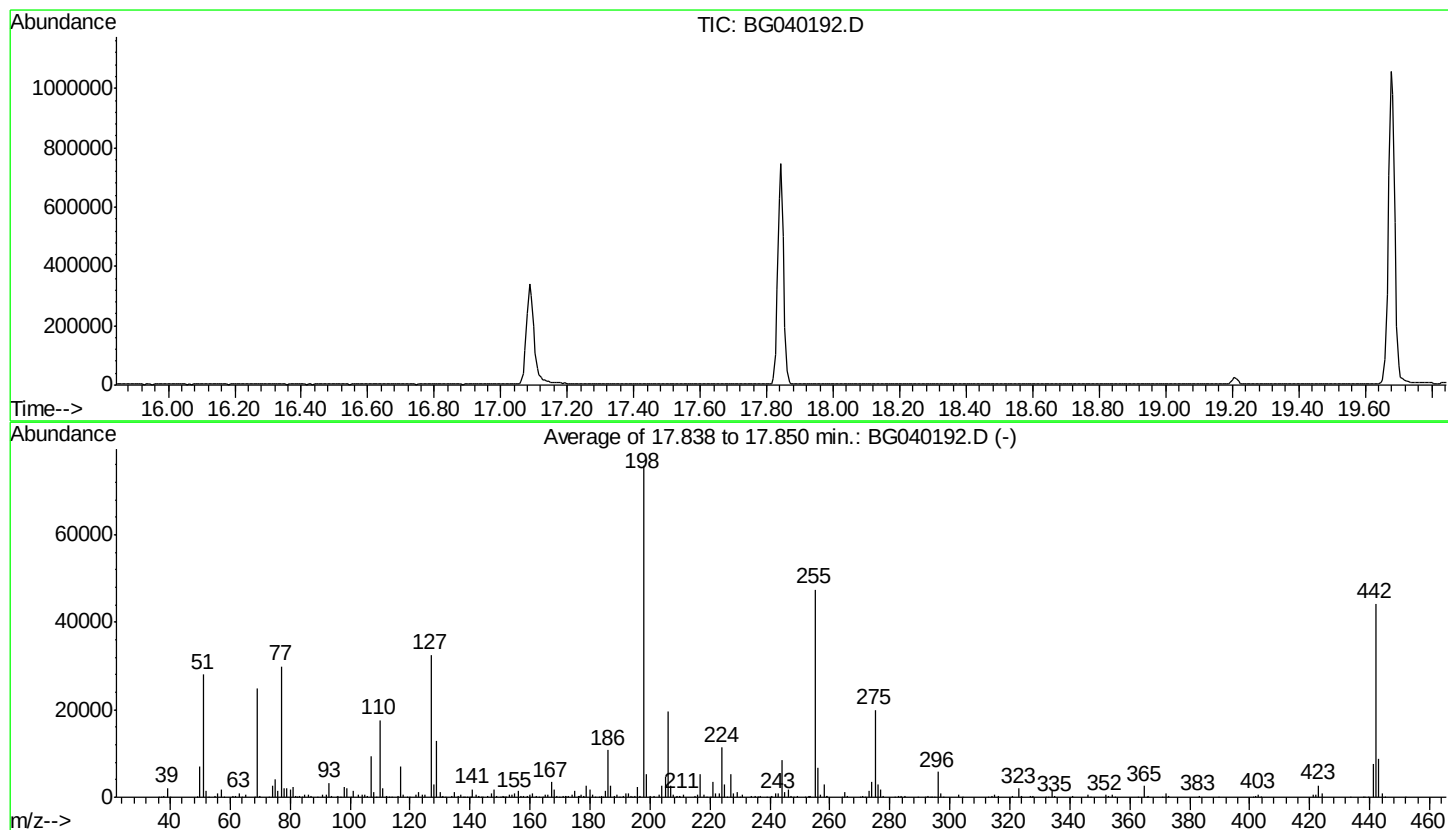

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	28056	PASS
68	69	0.00	2	0.3	85	PASS
69	198	0.00	100	33.0	25021	PASS
70	69	0.00	2	0.8	208	PASS
127	198	10	80	42.9	32570	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75840	PASS
199	198	5	9	6.9	5252	PASS
275	198	10	60	26.3	19978	PASS
365	198	1	100	3.4	2588	PASS
441	198	0.01	100	10.0	7587	PASS
442	198	50	100	58.4	44325	PASS
443	442	15	24	19.8	8796	PASS