


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG032819\
 Data File : BG040210.D
 Acq On : 28 Mar 2019 22:24
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 28 05:47:00 2019

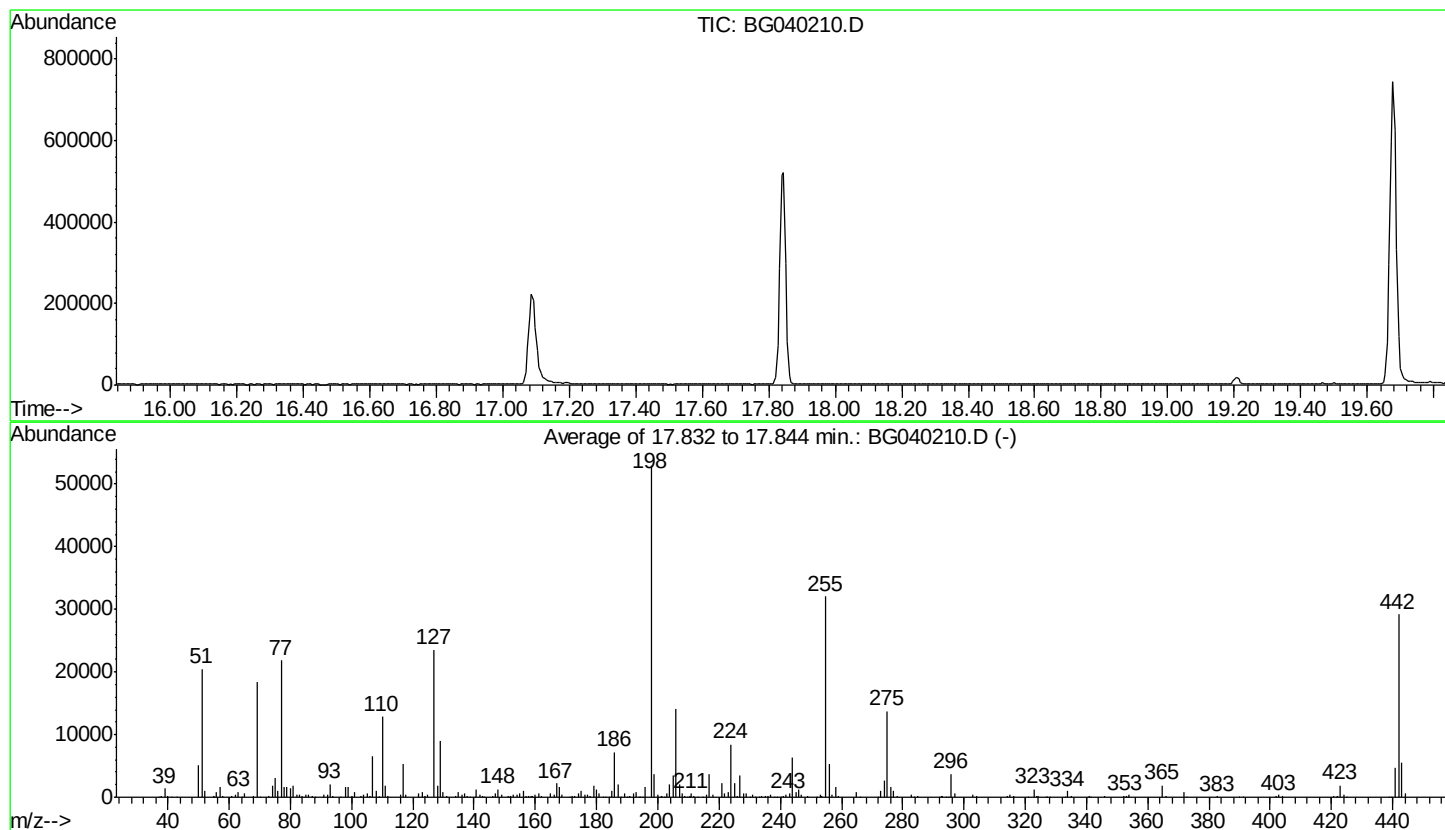

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	20512	PASS
68	69	0.00	2	1.5	282	PASS
69	198	0.00	100	34.6	18342	PASS
70	69	0.00	2	0.3	56	PASS
127	198	10	80	44.5	23570	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52938	PASS
199	198	5	9	7.1	3753	PASS
275	198	10	60	25.9	13711	PASS
365	198	1	100	3.5	1877	PASS
441	198	0.01	100	8.9	4715	PASS
442	198	50	100	55.1	29178	PASS
443	442	15	24	19.2	5611	PASS