
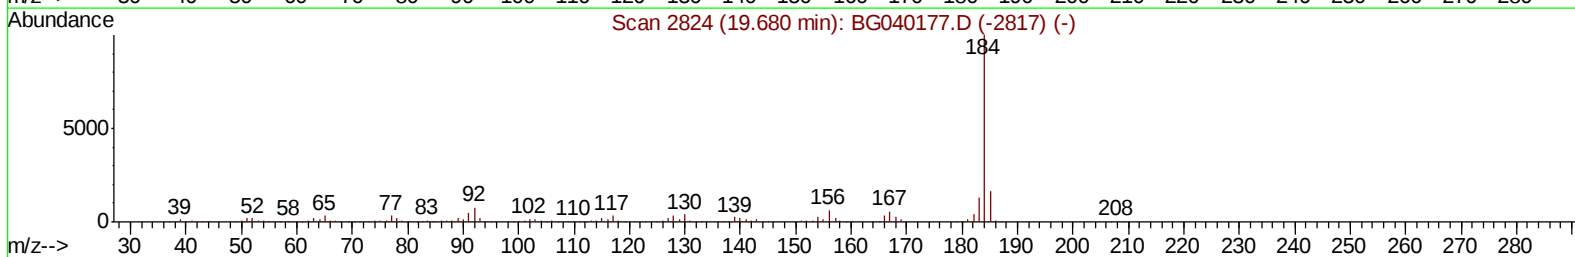
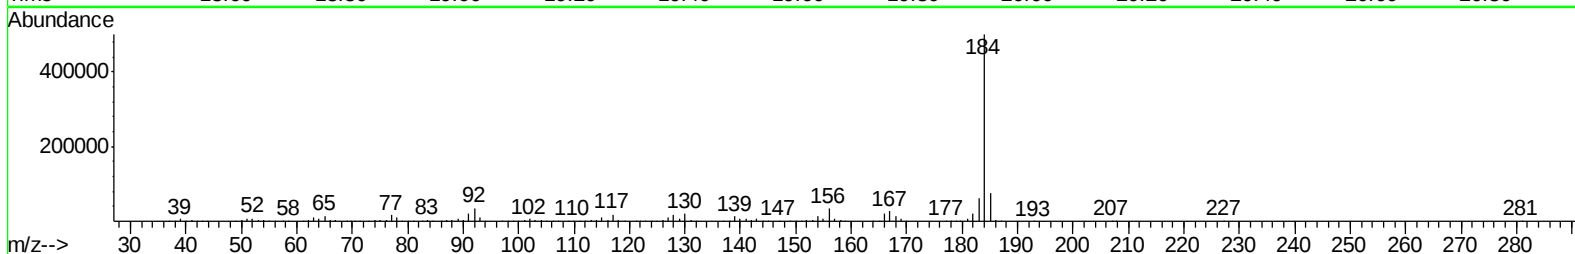


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG032919\
 Data File : BG040228.D
 Acq On : 29 Mar 2019 15:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 05:49:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 28 05:47:00 2019
 Response via : Initial Calibration

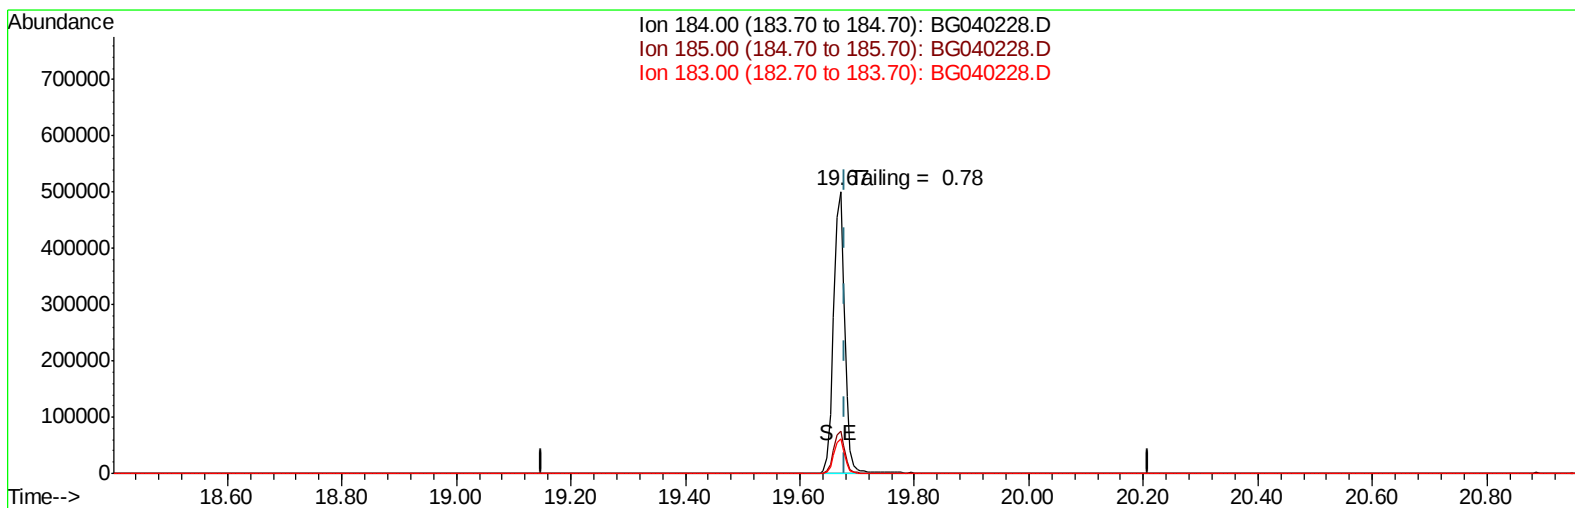

TIC: BG040228.D

(77) Benzidine




19.671min (-0.009) 22513.09ng

response 680458

Ion	Exp%	Act%
184.00	100	100
185.00	16.60	14.89
183.00	12.90	12.32
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG032919\
Data File : BG040228.D
Acq On : 29 Mar 2019 15:57
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 05:49:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 28 05:47:00 2019
Response via : Initial Calibration

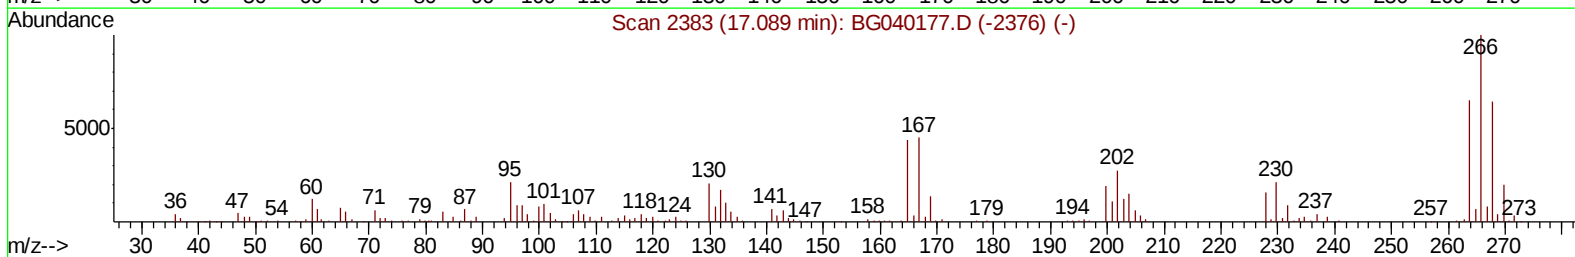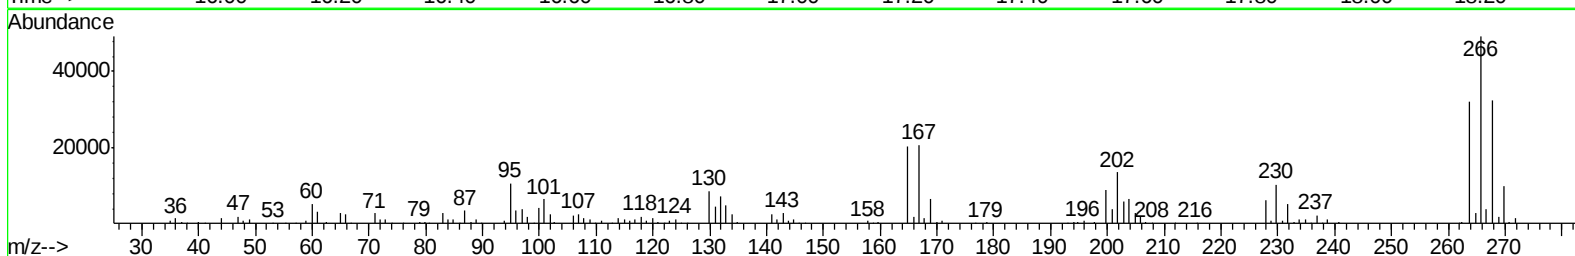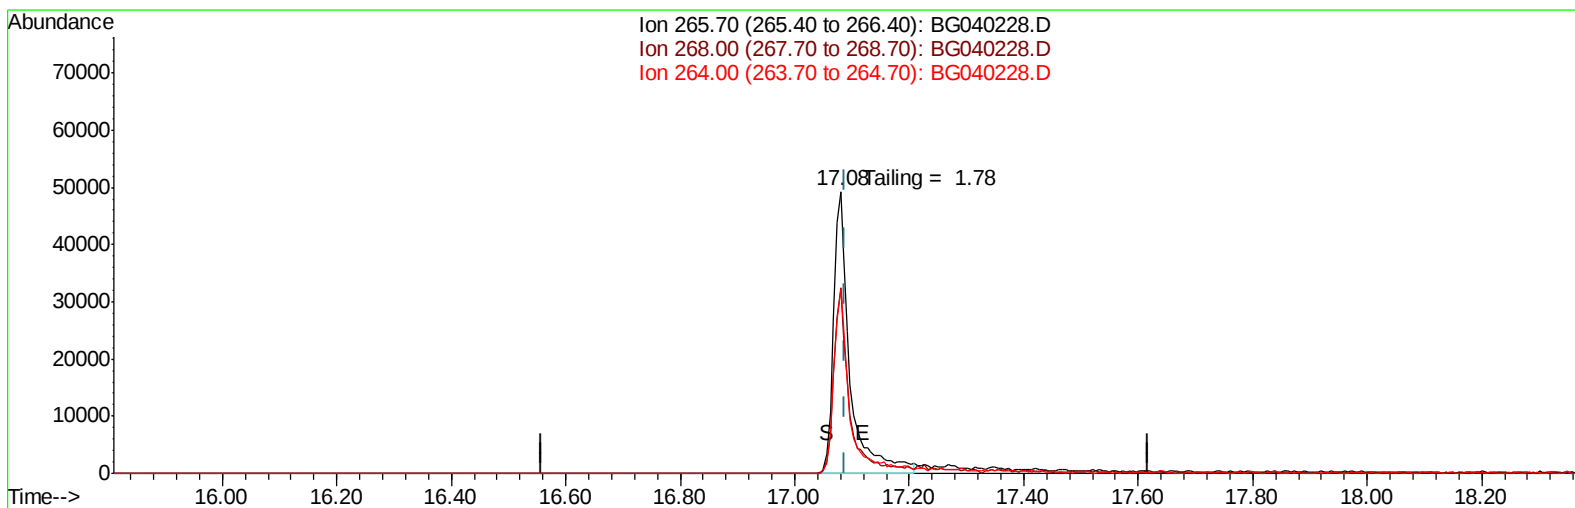

TIC: BG040228.D

(70) Pentachlorophenol (C)

17.080min (-0.009) 37634.25ng

response 94536

Ion	Exp%	Act%
265.70	100	100
268.00	68.70	66.10
264.00	64.80	65.31
0.00	0.00	0.00