

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG032919\
 Data File : BG040261.D
 Acq On : 30 Mar 2019 14:36
 Operator : JU/SJ
 Sample : K1685-10
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 AU-06-032819-A

Quant Time: Apr 01 02:48:31 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 28 05:47:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	64970	20.00	ng	-0.01
21) Naphthalene-d8	10.87	136	281886	20.00	ng	-0.01
39) Acenaphthene-d10	14.68	164	182733	20.00	ng	-0.02
64) Phenanthrene-d10	17.43	188	480945	20.00	ng	-0.01
76) Chrysene-d12	21.71	240	503889	20.00	ng	-0.02
87) Perylene-d12	25.02	264	499952	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	448487	114.76	ng	0.00
7) Phenol-d6	7.21	99	560655	103.80	ng	-0.01
23) Nitrobenzene-d5	9.23	82	452436	85.31	ng	-0.01
42) 2,4,6-Tribromophenol	16.18	330	287739	145.70	ng	-0.01
45) 2-Fluorobiphenyl	13.31	172	1066247	86.46	ng	-0.01
79) Terphenyl-d14	20.04	244	1788300	79.84	ng	-0.01


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG032919\
Data File : BG040261.D
Acq On : 30 Mar 2019 14:36
Operator : JU/SJ
Sample : K1685-10
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
AU-06-032819-A

Quant Time: Apr 01 02:48:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 28 05:47:00 2019
Response via : Initial Calibration

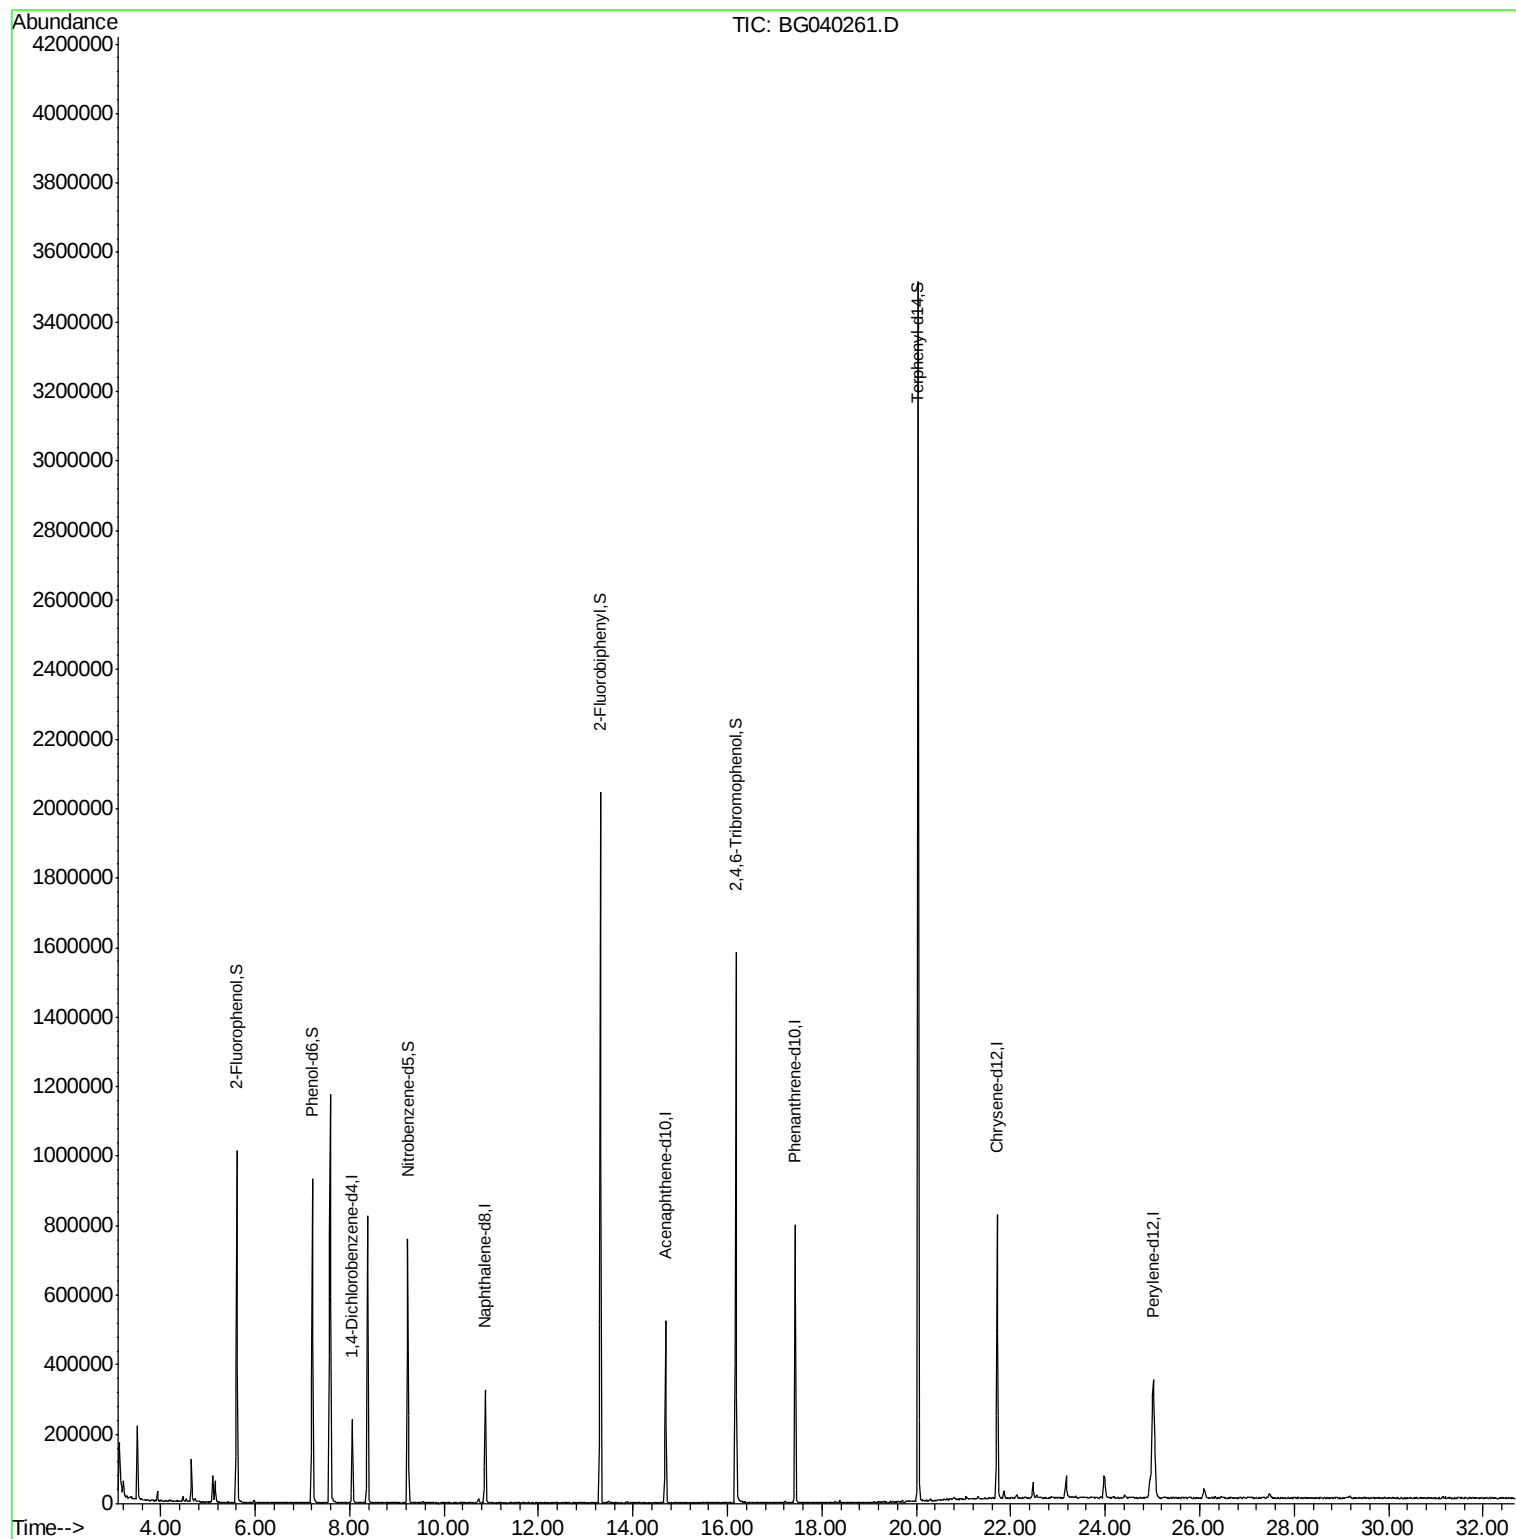

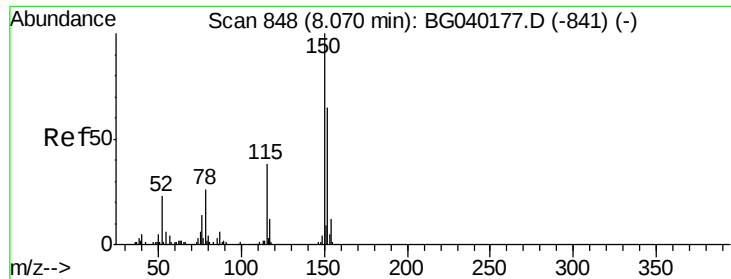


#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.06 min Scan# 845
 Delta R.T. -0.01 min
 Lab File: BG040261.D
 Acq: 30 Mar 2019 14:36

Instrument :
 BNA_G
 ClientSampleId :
 AU-06-032819-A

Tgt Ion:152 Resp: 64970
 Ion Ratio Lower Upper
 152 100
 150 162.7 123.7 185.5
 115 58.1 46.9 70.3

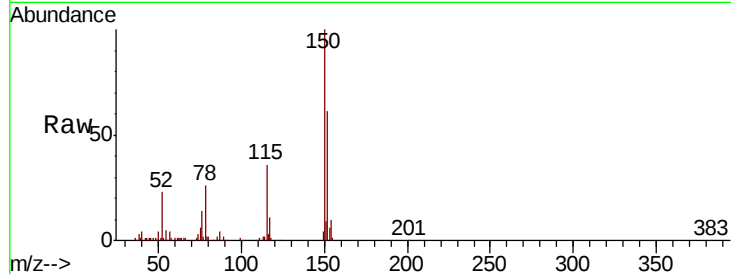


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

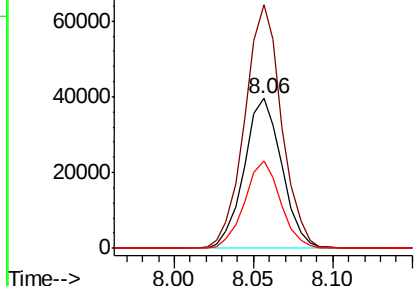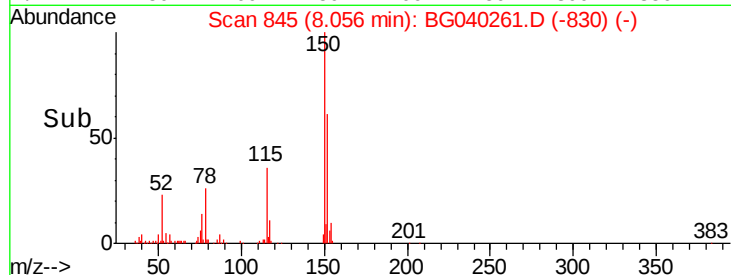



#5

2-Fluorophenol
 Concen: 114.756 ng
 RT: 5.61 min Scan# 429
 Delta R.T. -0.01 min
 Lab File: BG040261.D
 Acq: 30 Mar 2019 14:36

Tgt Ion:112 Resp: 448487
 Ion Ratio Lower Upper
 112 100
 64 67.0 54.2 81.2
 63 33.2 26.4 39.6

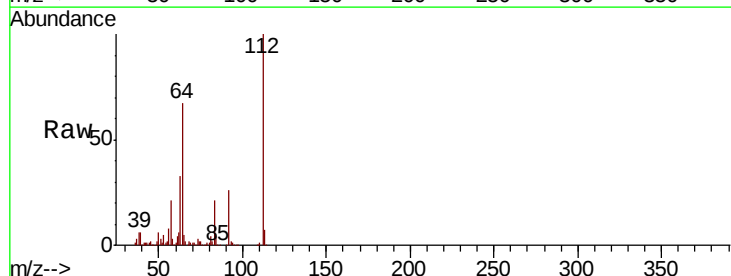

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BG
 Ion 63.00 (62.70 to 63.70): BG

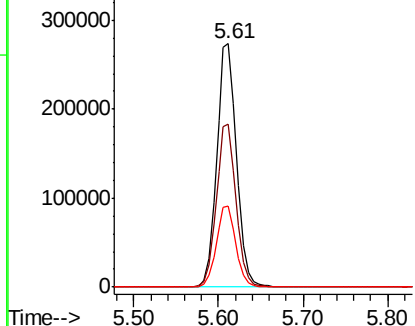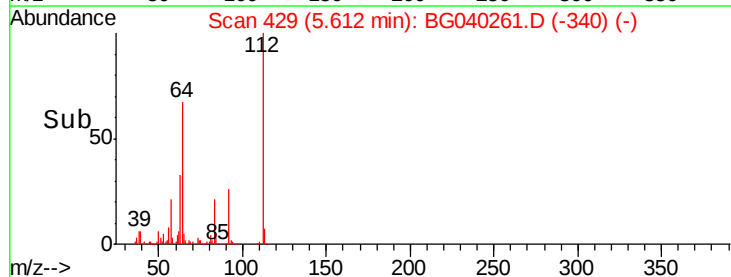



#7

Phenol-d6

Concen: 103.803 ng

RT: 7.21 min Scan# 701

Delta R.T. -0.01 min

Lab File: BG040261.D

Acq: 30 Mar 2019 14:36

Instrument :

BNA_G

ClientSampleId :

AU-06-032819-A


Tgt Ion: 99 Resp: 560655

Ion Ratio Lower Upper



99 100

42 18.7 16.2 24.2

71 32.1 26.8 40.2

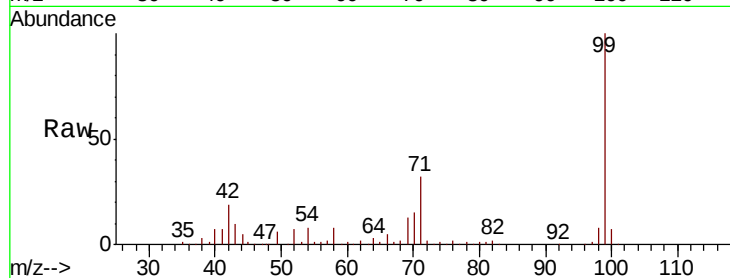

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

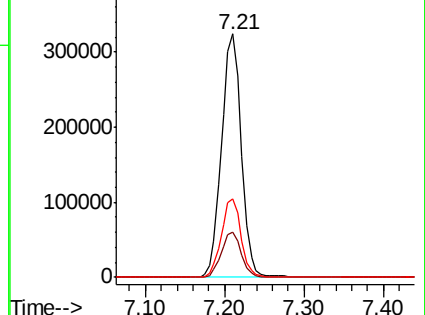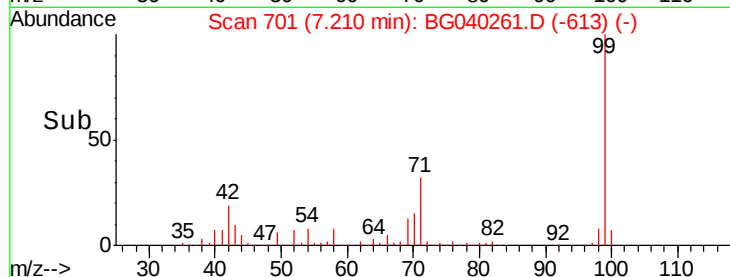

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.87 min Scan# 1324

Delta R.T. -0.01 min

Lab File: BG040261.D

Acq: 30 Mar 2019 14:36

Tgt Ion: 136 Resp: 281886


Ion Ratio Lower Upper

136 100



137 10.3 8.9 13.3


54 10.4 9.6 14.4

68 6.3 5.1 7.7

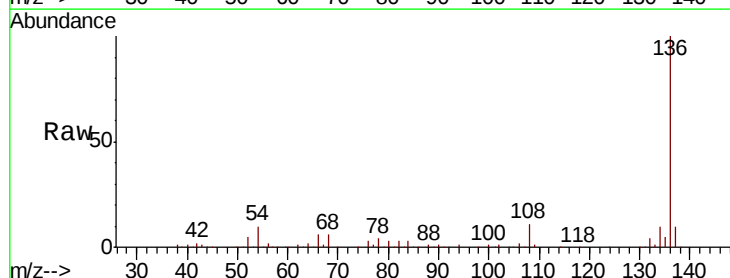

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



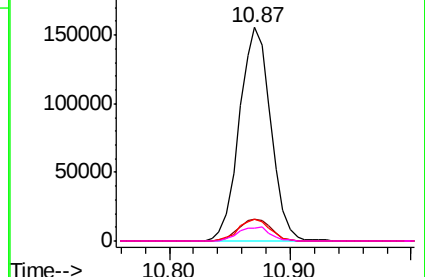
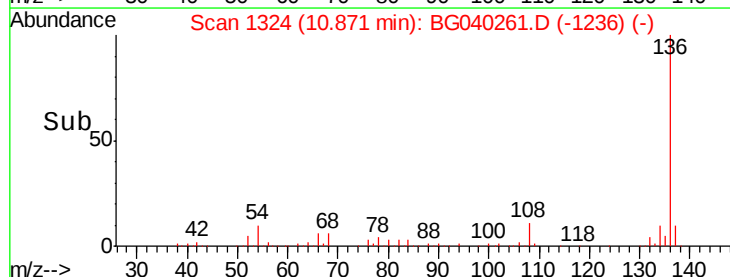


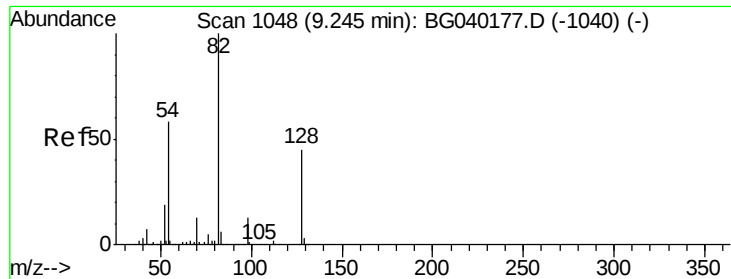

#23
Nitrobenzene-d5
Concen: 85.313 ng
RT: 9.23 min Scan# 1045
Delta R.T. -0.01 min
Lab File: BG040261.D
Acq: 30 Mar 2019 14:36




Instrument :
BNA_G
ClientSampleId :
AU-06-032819-A


Tgt Ion: 82 Resp: 452436
Ion Ratio Lower Upper
82 100
128 43.0 35.8 53.8
54 53.6 46.2 69.2

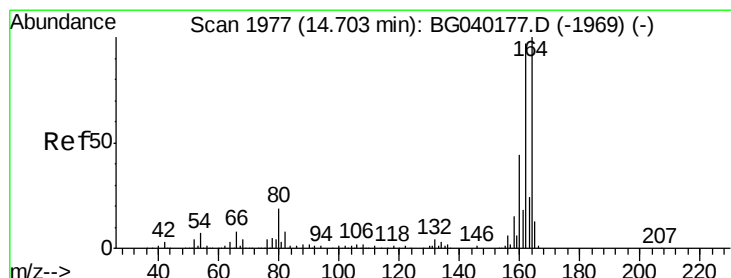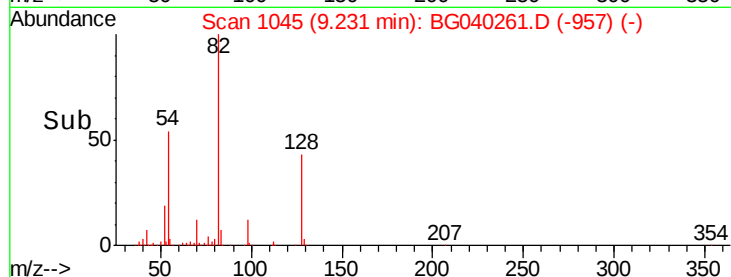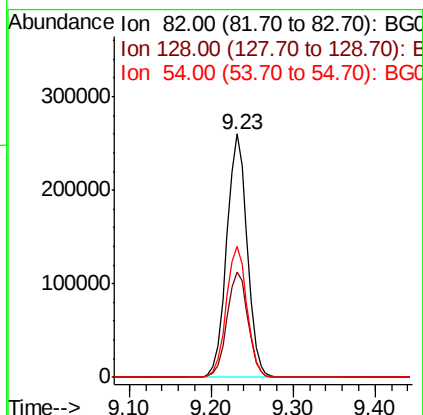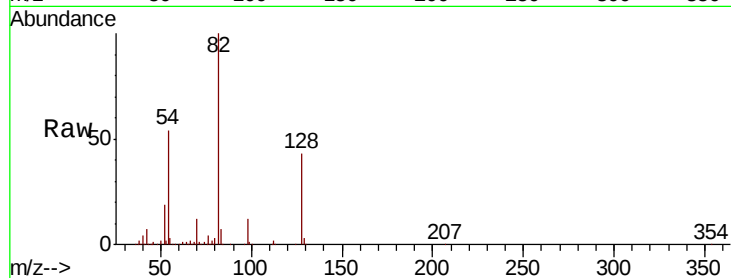

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.68 min Scan# 1973
Delta R.T. -0.02 min
Lab File: BG040261.D
Acq: 30 Mar 2019 14:36

Tgt Ion: 164 Resp: 182733
Ion Ratio Lower Upper
164 100
162 102.2 77.4 116.2
160 44.0 35.3 52.9

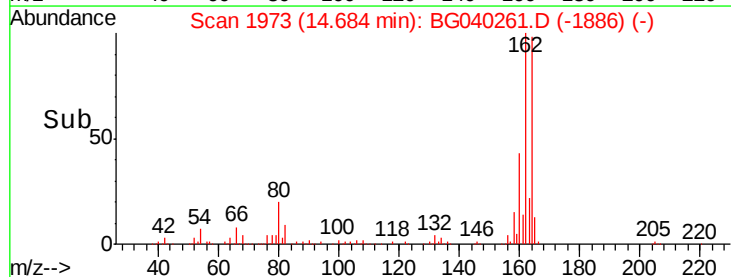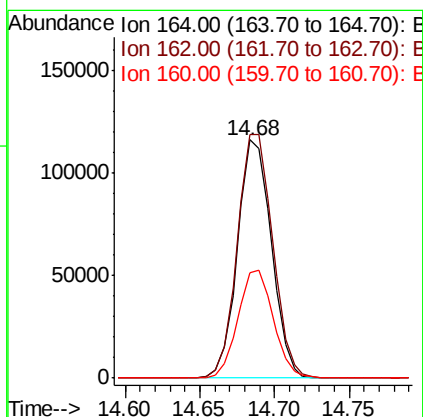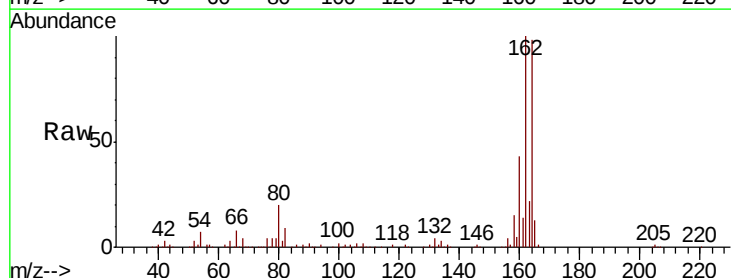


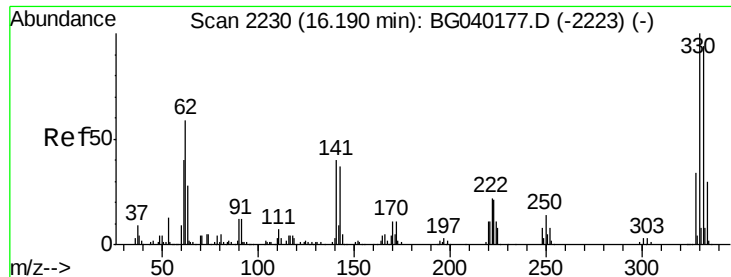




#42
 2,4,6-Tribromophenol
 Concen: 145.700 ng
 RT: 16.18 min Scan# 2227
 Delta R.T. -0.01 min
 Lab File: BG040261.D
 Acq: 30 Mar 2019 14:36

Instrument :
 BNA_G
 ClientSampleId :
 AU-06-032819-A

Tgt Ion:330 Resp: 287739
 Ion Ratio Lower Upper
 330 100
 332 97.1 76.6 115.0
 141 38.9 32.6 48.8

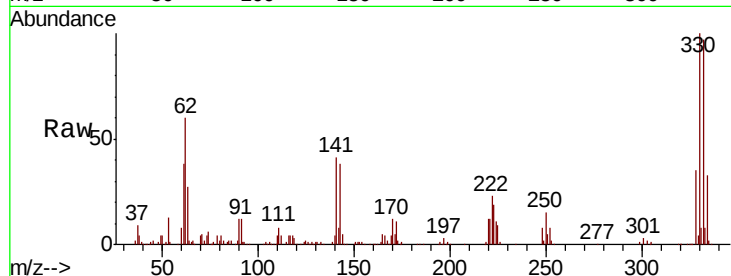


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

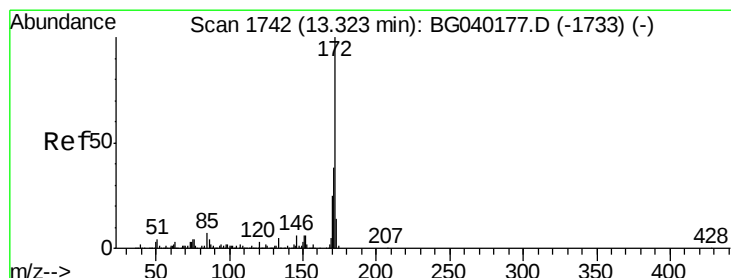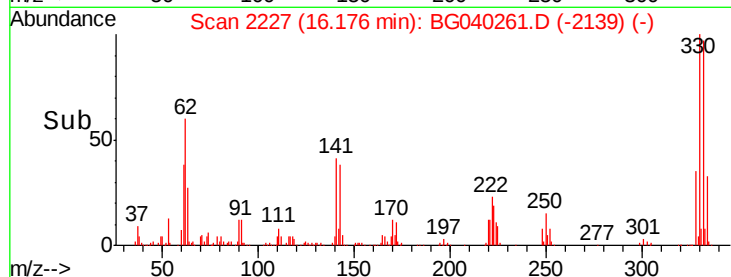
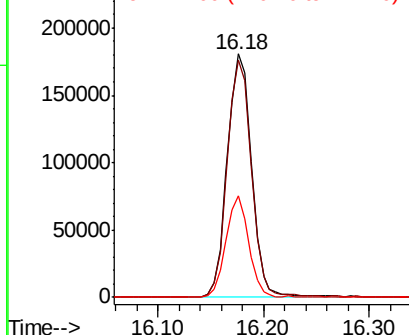



#45
 2-Fluorobiphenyl
 Concen: 86.461 ng
 RT: 13.31 min Scan# 1739
 Delta R.T. -0.01 min
 Lab File: BG040261.D
 Acq: 30 Mar 2019 14:36

Tgt Ion:172 Resp: 1066247
 Ion Ratio Lower Upper
 172 100
 171 37.8 30.5 45.7
 170 25.5 20.1 30.1

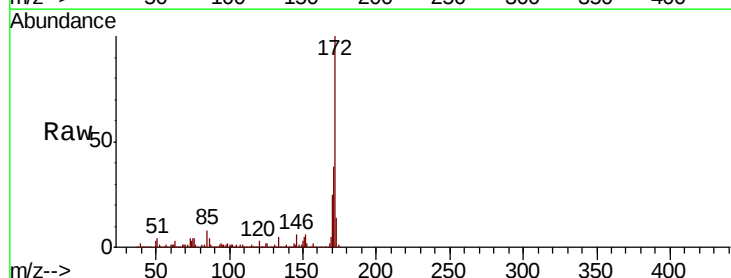

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

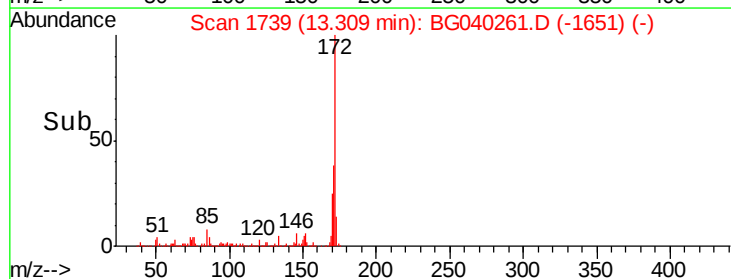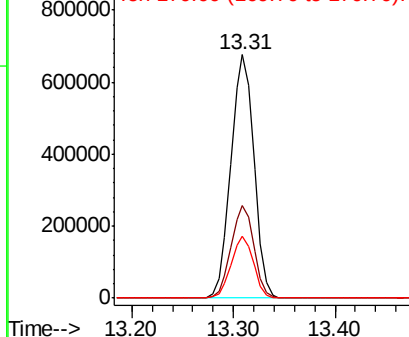


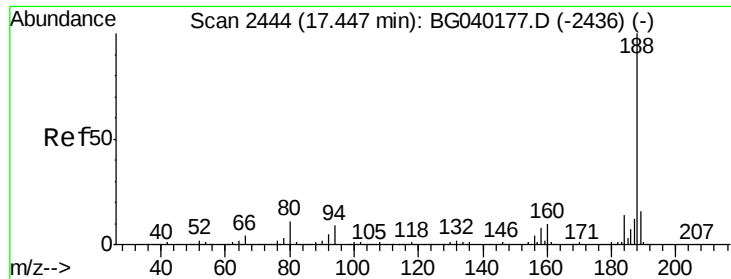




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.43 min Scan# 2441
Delta R.T. -0.01 min
Lab File: BG040261.D
Acq: 30 Mar 2019 14:36

Instrument :
BNA_G
ClientSampleId :
AU-06-032819-A

Tgt Ion:188 Resp: 480945
Ion Ratio Lower Upper
188 100
94 9.3 7.0 10.4
80 10.1 8.6 13.0

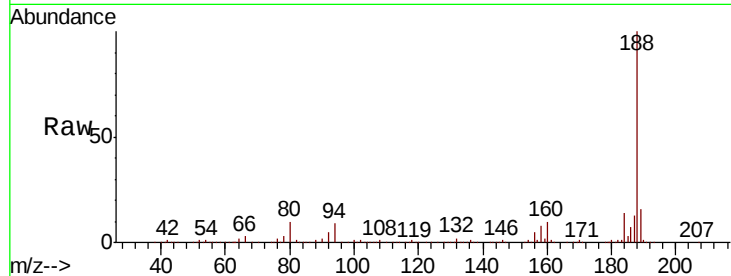


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BG
Ion 80.00 (79.70 to 80.70): BG

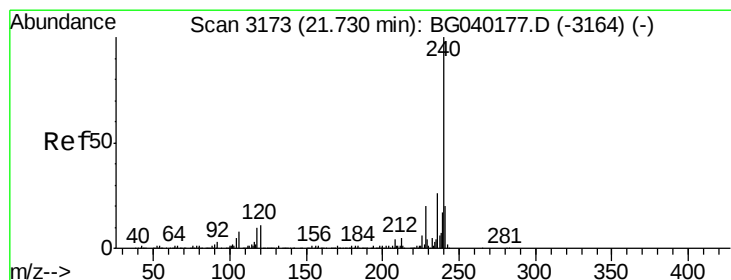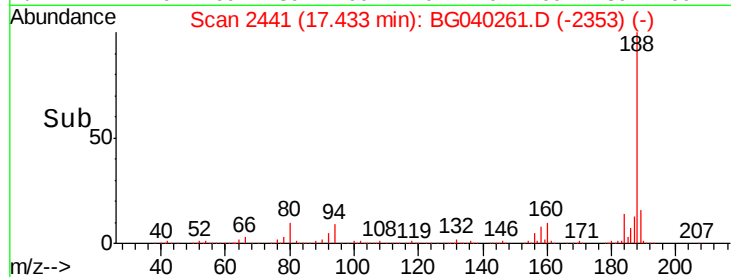
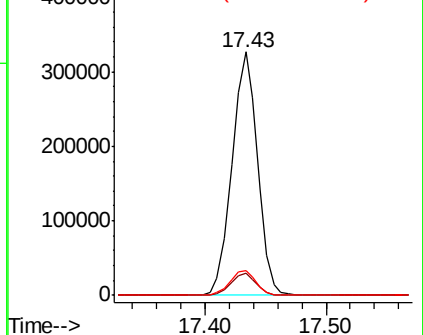


#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.71 min Scan# 3169
Delta R.T. -0.02 min
Lab File: BG040261.D
Acq: 30 Mar 2019 14:36

Tgt Ion:240 Resp: 503889
Ion Ratio Lower Upper
240 100
120 9.8 8.4 12.6
236 25.7 20.8 31.2

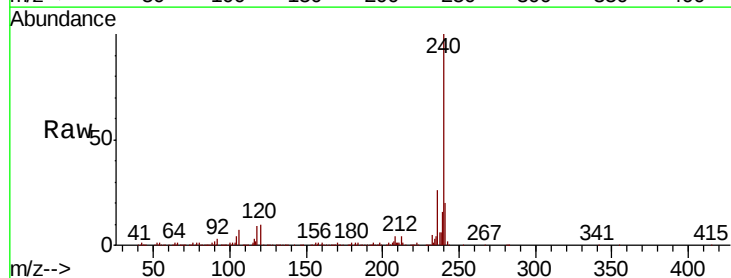

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

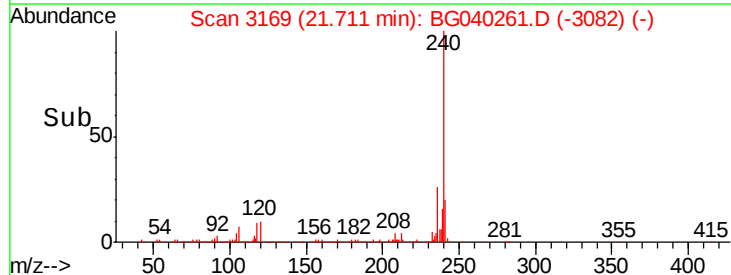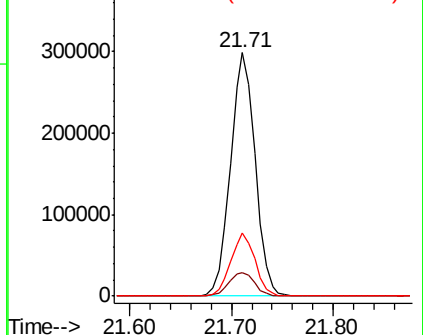



#79

Terphenyl-d14

Concen: 79.840 ng

RT: 20.04 min Scan# 2884

Delta R.T. -0.01 min

Lab File: BG040261.D

Acq: 30 Mar 2019 14:36

Instrument :

BNA_G

ClientSampleId :

AU-06-032819-A


Tgt Ion:244 Resp: 1788300

Ion Ratio Lower Upper

244 100

212 9.1 7.0 10.6




122 11.6 8.5 12.7

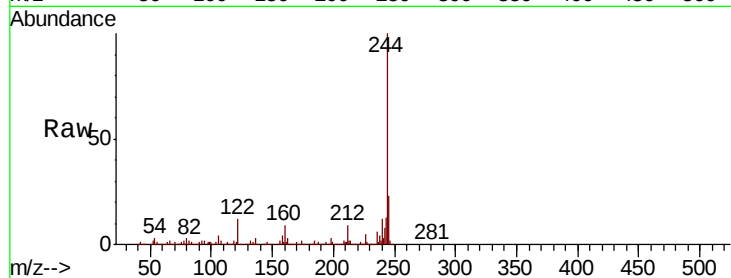

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

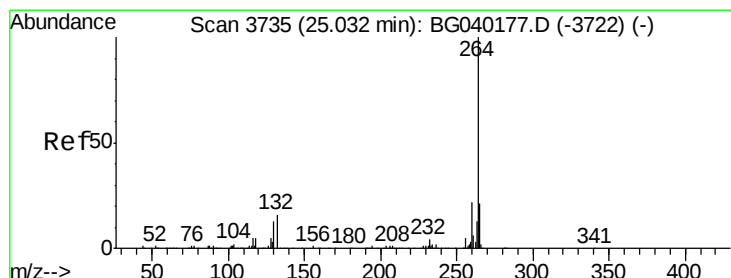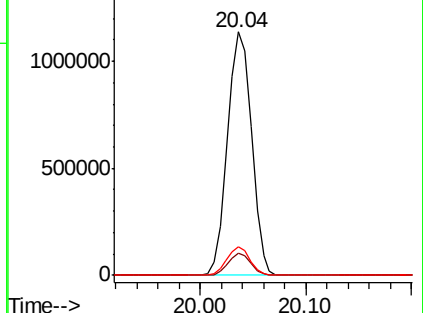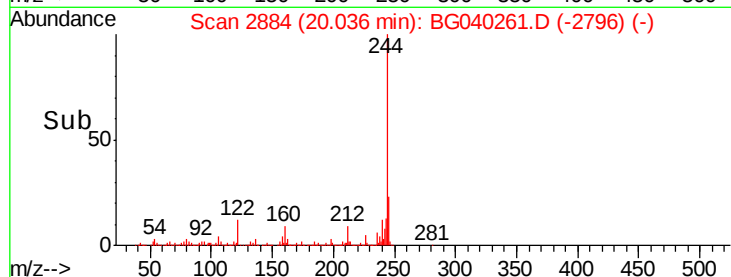

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.02 min Scan# 3732

Delta R.T. -0.01 min

Lab File: BG040261.D

Acq: 30 Mar 2019 14:36


Tgt Ion:264 Resp: 499952

Ion Ratio Lower Upper

264 100

260 22.6 17.9 26.9

265 20.4 16.8 25.2

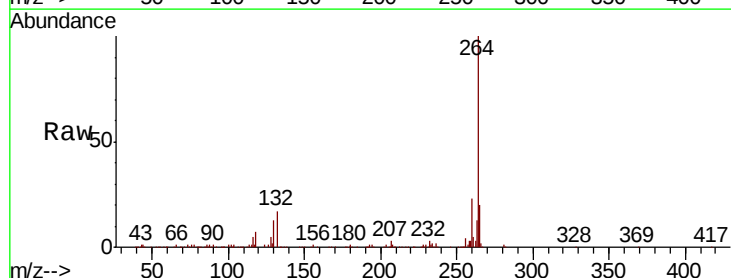

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

