


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032919\
 Data File : BG040228.D
 Acq On : 29 Mar 2019 15:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 28 05:47:00 2019

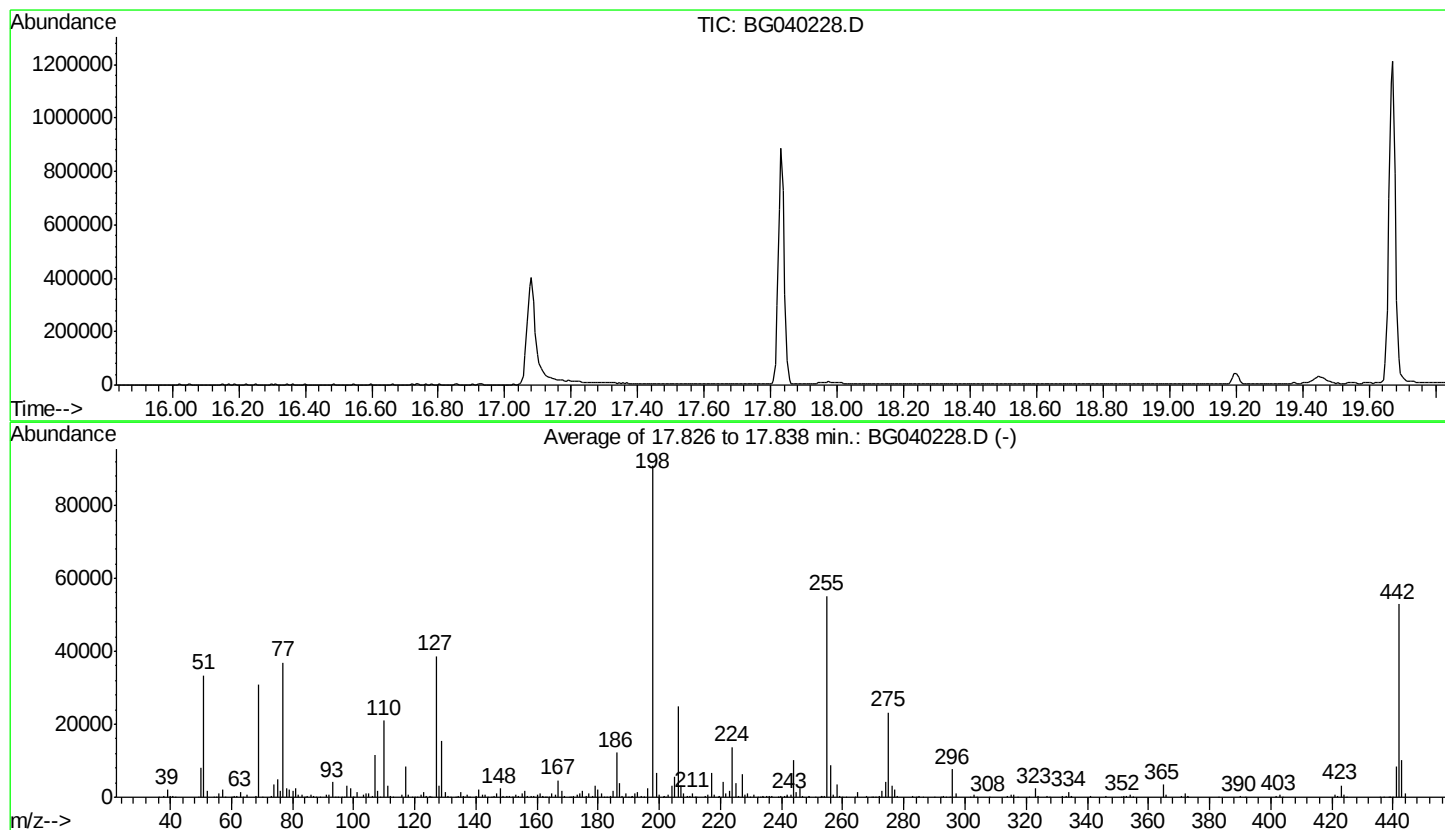

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	33443	PASS
68	69	0.00	2	0.7	202	PASS
69	198	0.00	100	33.8	30749	PASS
70	69	0.00	2	0.3	78	PASS
127	198	10	80	42.6	38773	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	90930	PASS
199	198	5	9	7.4	6755	PASS
275	198	10	60	25.5	23192	PASS
365	198	1	100	3.8	3435	PASS
441	198	0.01	100	9.2	8328	PASS
442	198	50	100	58.2	52893	PASS
443	442	15	24	19.1	10120	PASS