


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032919\
 Data File : BG040245.D
 Acq On : 30 Mar 2019 3:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 28 05:47:00 2019

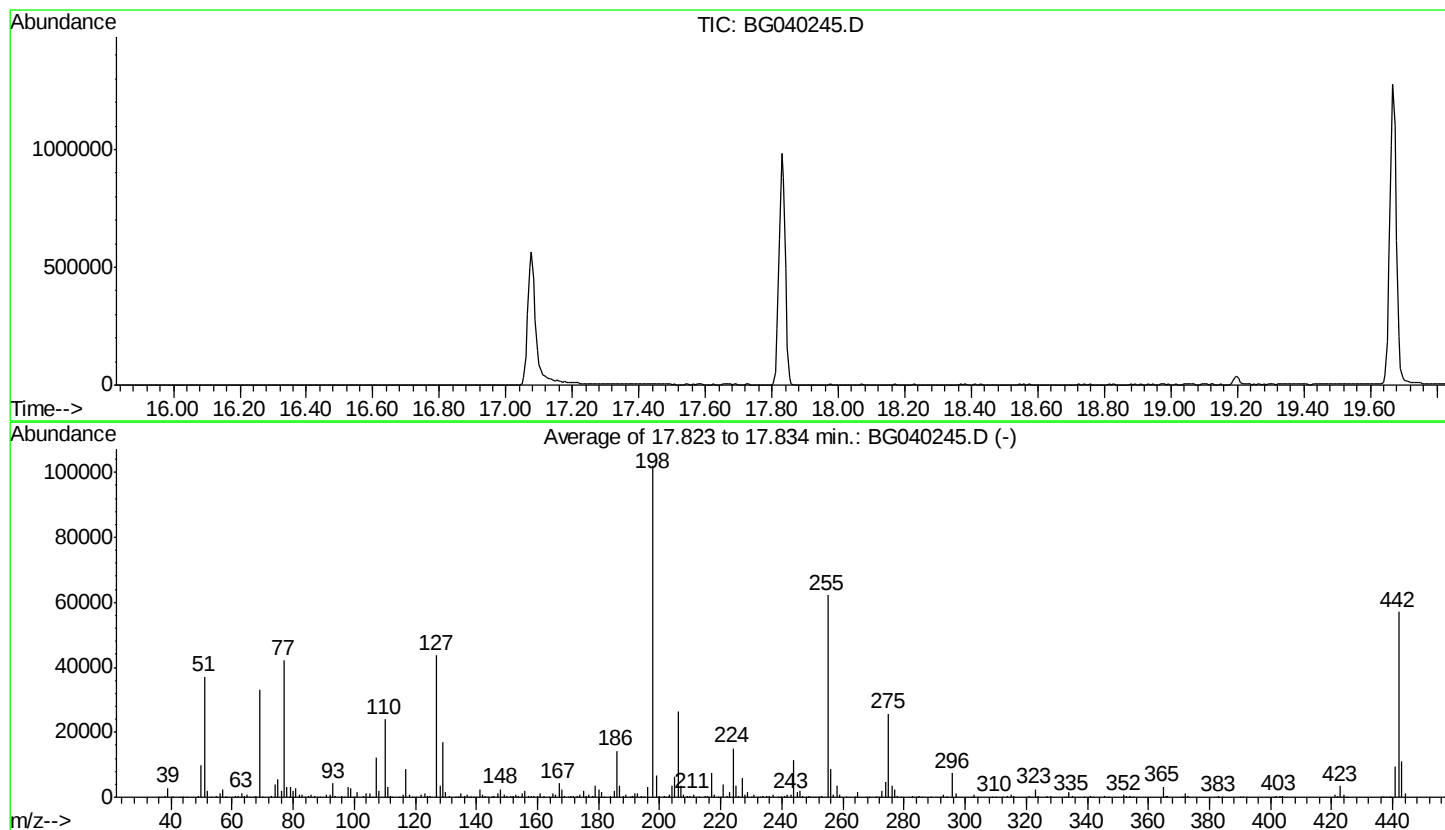

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	37194	PASS
68	69	0.00	2	1.1	365	PASS
69	198	0.00	100	32.5	33221	PASS
70	69	0.00	2	0.6	190	PASS
127	198	10	80	42.8	43682	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	102072	PASS
199	198	5	9	6.7	6838	PASS
275	198	10	60	25.1	25648	PASS
365	198	1	100	3.3	3351	PASS
441	198	0.01	100	9.1	9308	PASS
442	198	50	100	55.8	56994	PASS
443	442	15	24	19.6	11166	PASS