
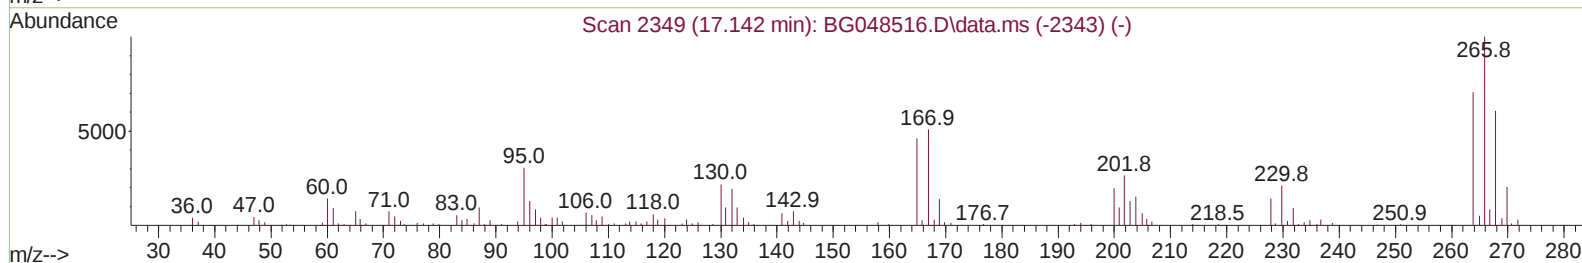
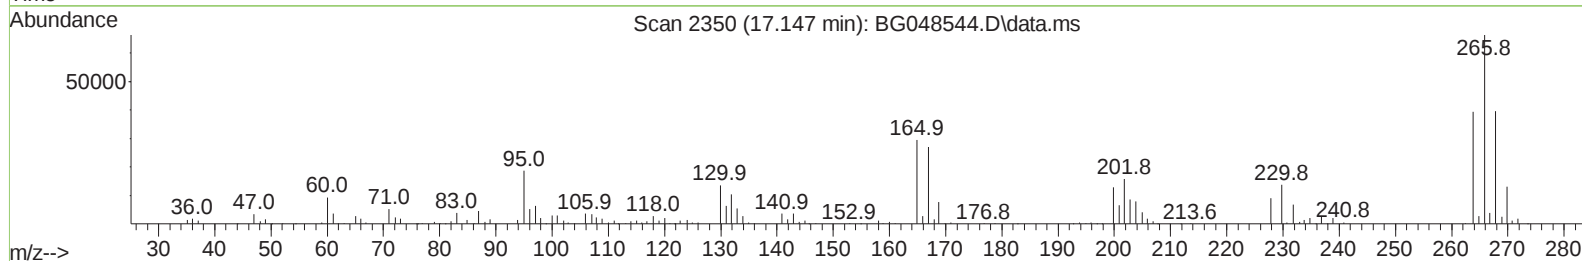


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040121\
Data File : BG048544.D
Acq On : 1 Apr 2021 14:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 15:52:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 11:19:59 2021
Response via : Initial Calibration

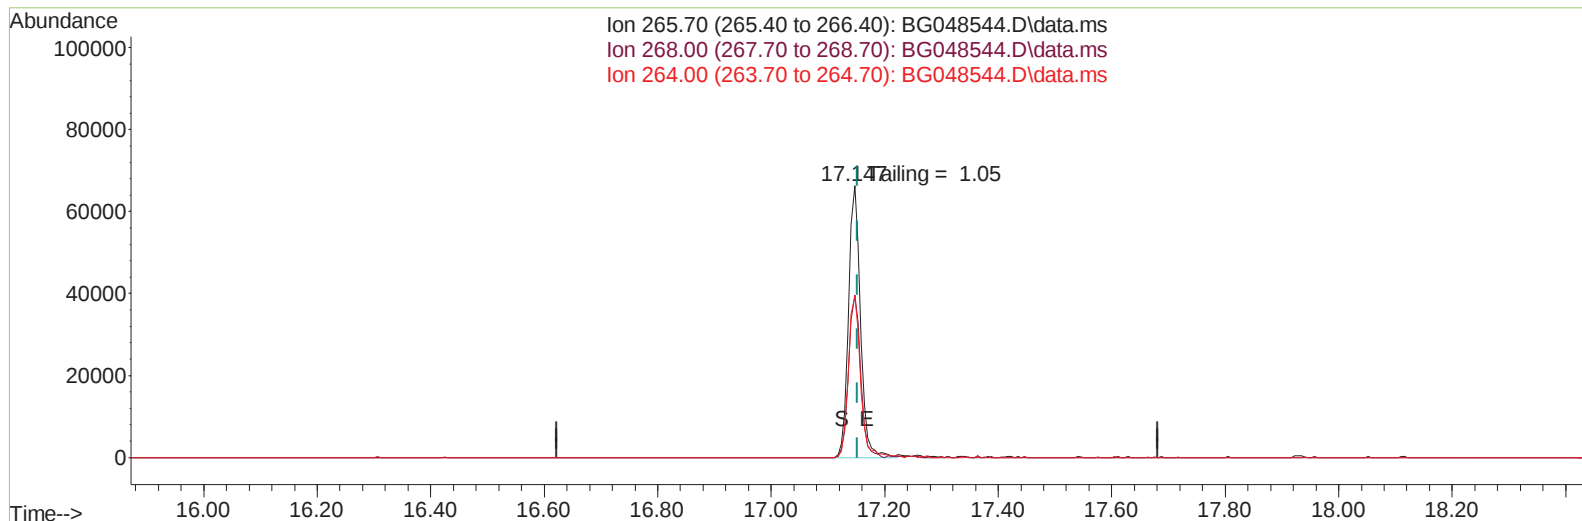

TIC: BG048544.D\data.ms

(70) Pentachlorophenol (C)




17.147min (-0.005) 227704.88 ng

response 96652

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	59.68
264.00	70.50	59.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040121\
 Data File : BG048544.D
 Acq On : 1 Apr 2021 14:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 15:52:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 11:19:59 2021
 Response via : Initial Calibration

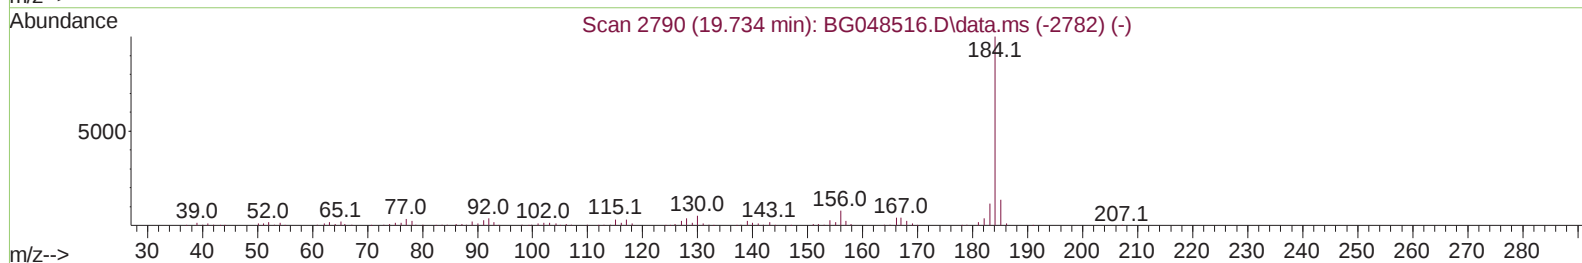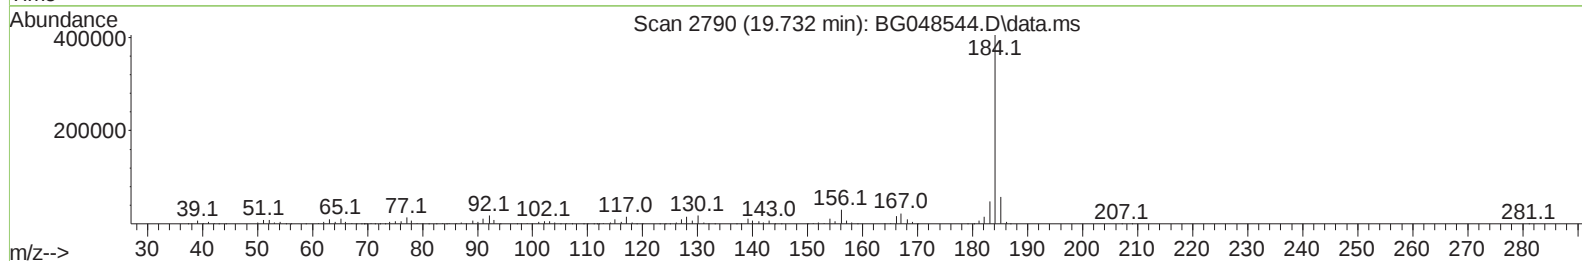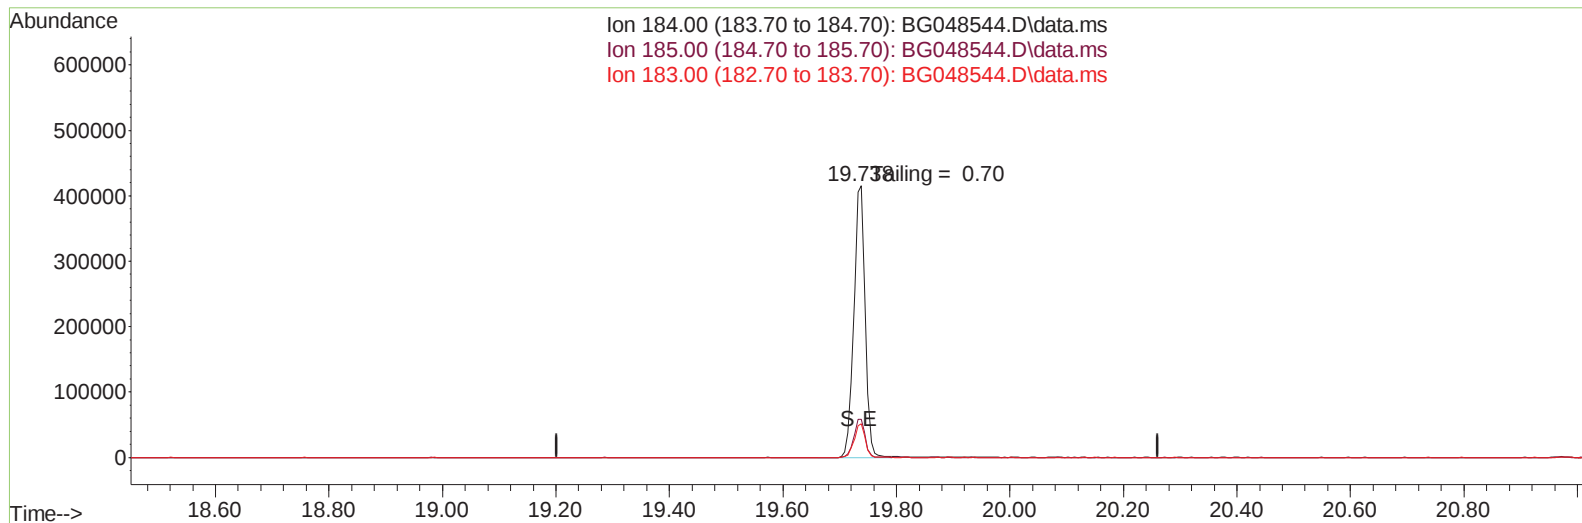

TIC: BG048544.D\data.ms

(77) Benzidine**19.731min (-19.731) 0.00 ng****response 0**

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	13.70	0.00#
183.00	11.50	0.00#
0.00	0.00	0.00