
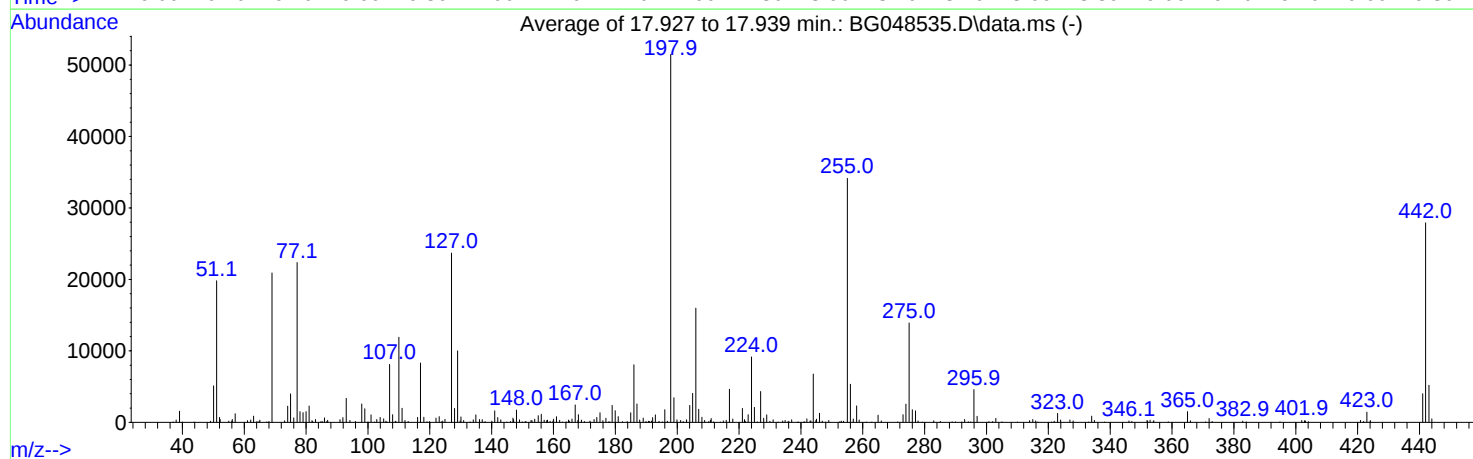


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040121\
 Data File : BG048535.D
 Acq On : 1 Apr 2021 8:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 02 10:20:56 2021

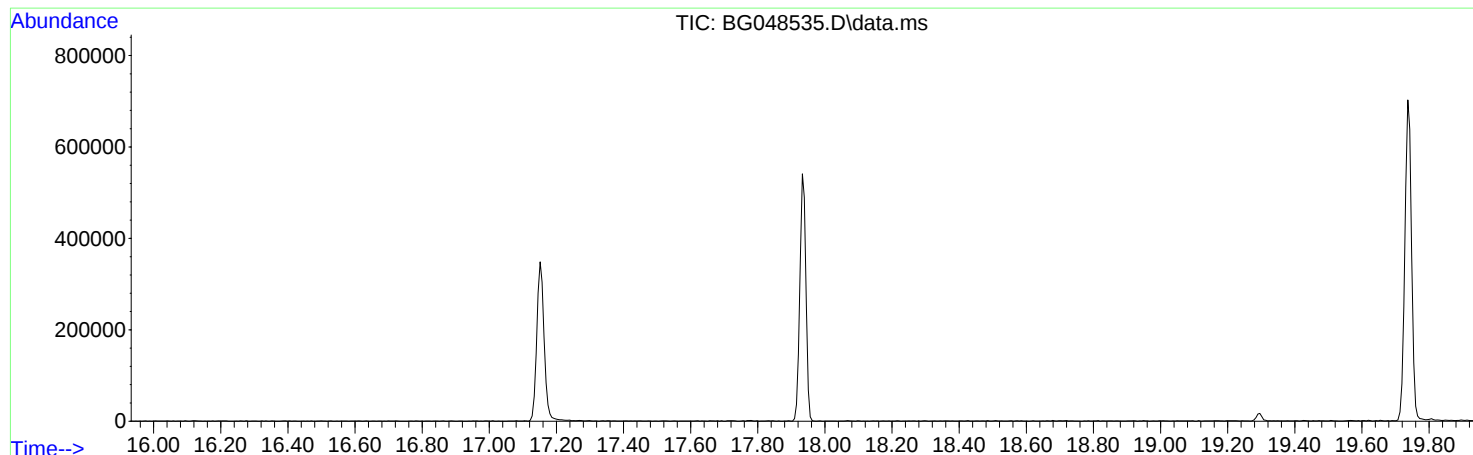




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	19803	PASS
68	69	0.00	2	0.6	122	PASS
69	198	0.00	100	40.6	20904	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.0	23685	PASS
197	198	0.00	2	0.3	154	PASS
198	198	100	100	100.0	51467	PASS
199	198	5	9	6.7	3449	PASS
275	198	10	60	27.0	13902	PASS
365	198	1	100	2.9	1492	PASS
441	198	0.01	100	7.8	3999	PASS
442	198	50	100	54.2	27917	PASS
443	442	15	24	18.6	5199	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040121\
 Data File : BG048535.D
 Acq On : 1 Apr 2021 8:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 01 11:13:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 31 11:41:32 2021
 Response via : Initial Calibration

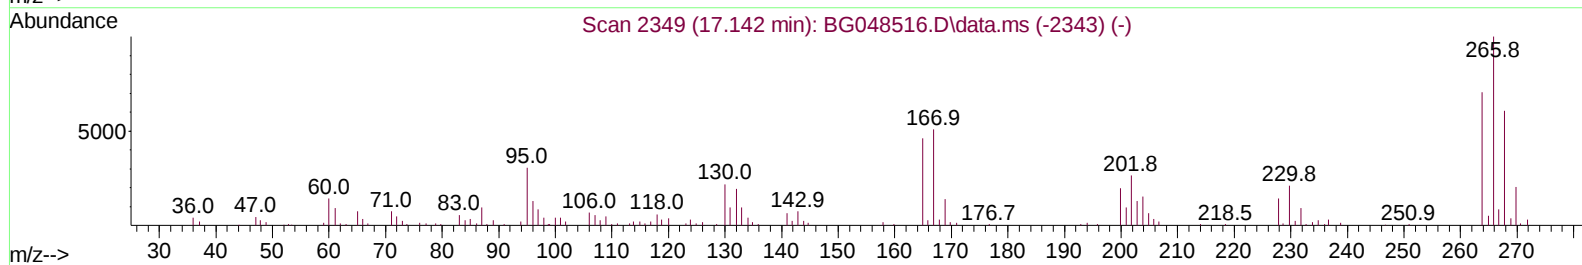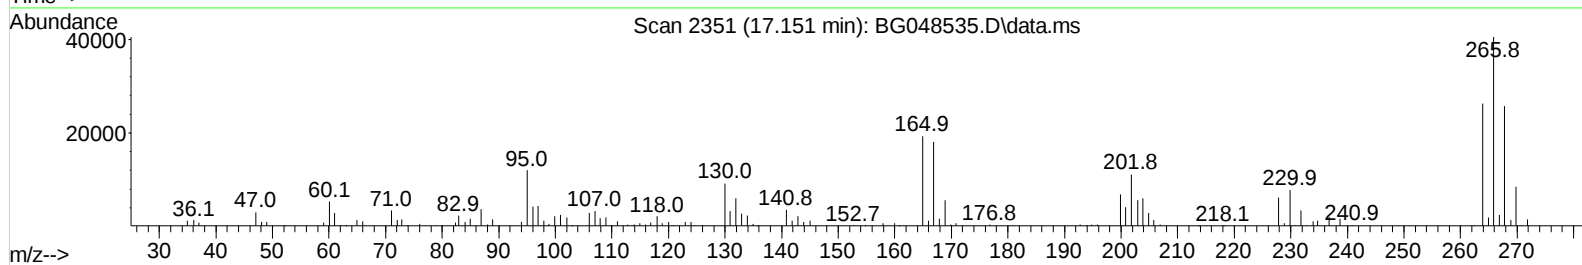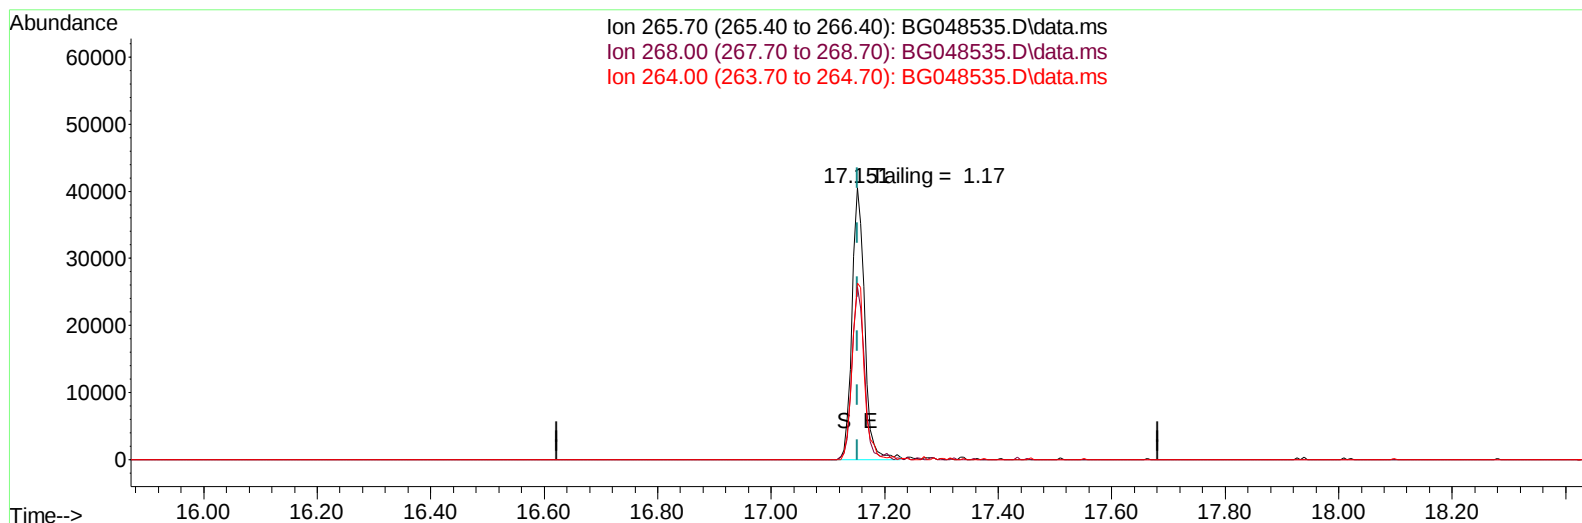

TIC: BG048535.D\data.ms

(70) Pentachlorophenol (C)

17.151min (-0.000) 23892.19 ng m




response 62223

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	63.47
264.00	70.50	65.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040121\
Data File : BG048535.D
Acq On : 1 Apr 2021 8:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 01 11:13:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 11:41:32 2021
Response via : Initial Calibration

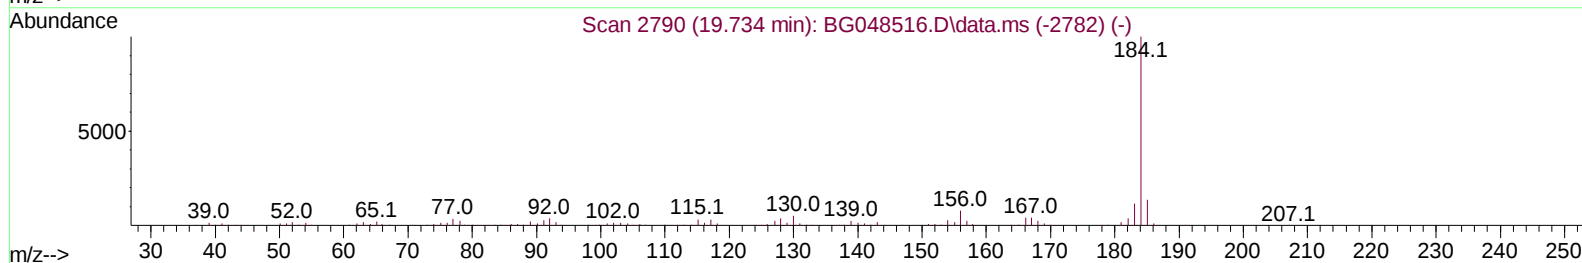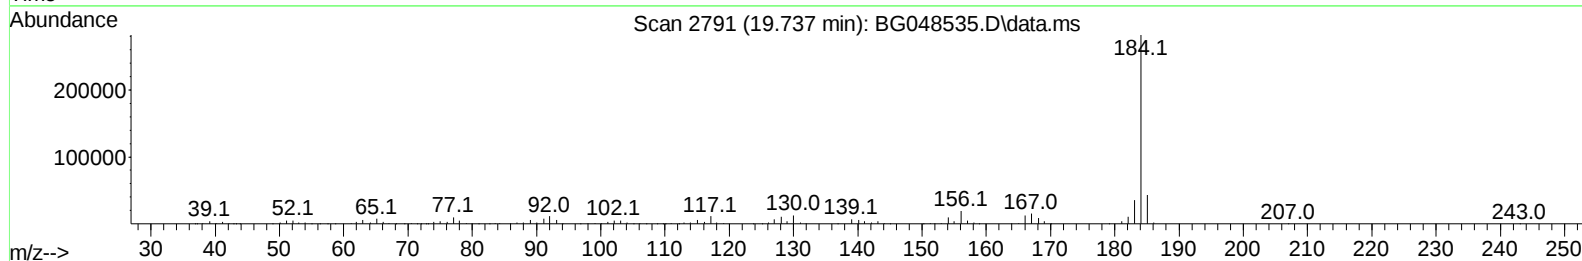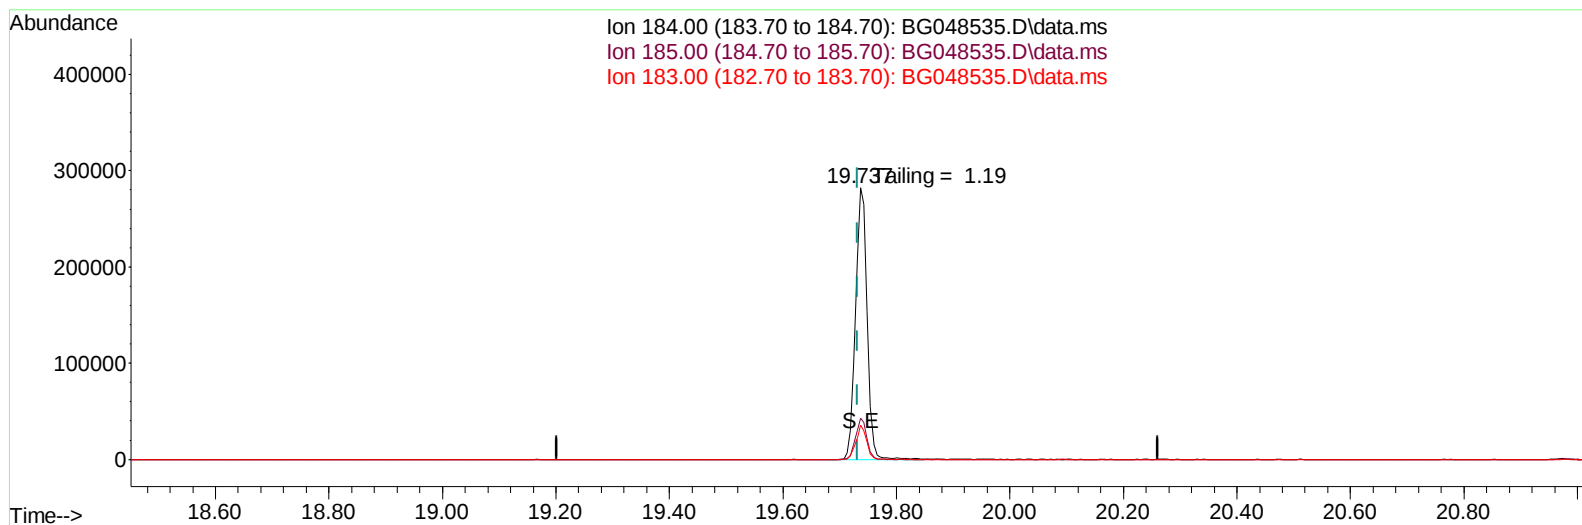

TIC: BG048535.D\data.ms

(77) Benzidine

19.737min (+ 0.005) 0.00 ng

response 397479

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	15.17
183.00	11.50	12.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/1/2021	BNA_G	BG048535.D
Compound Name	Response	Retention Time
DDT	196172	20.976
DDD	3189	20.53
DDE	94	20.019
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3283	199455	1.65

Instrument :
BNA_G
ClientSampleId :
DFTPP