
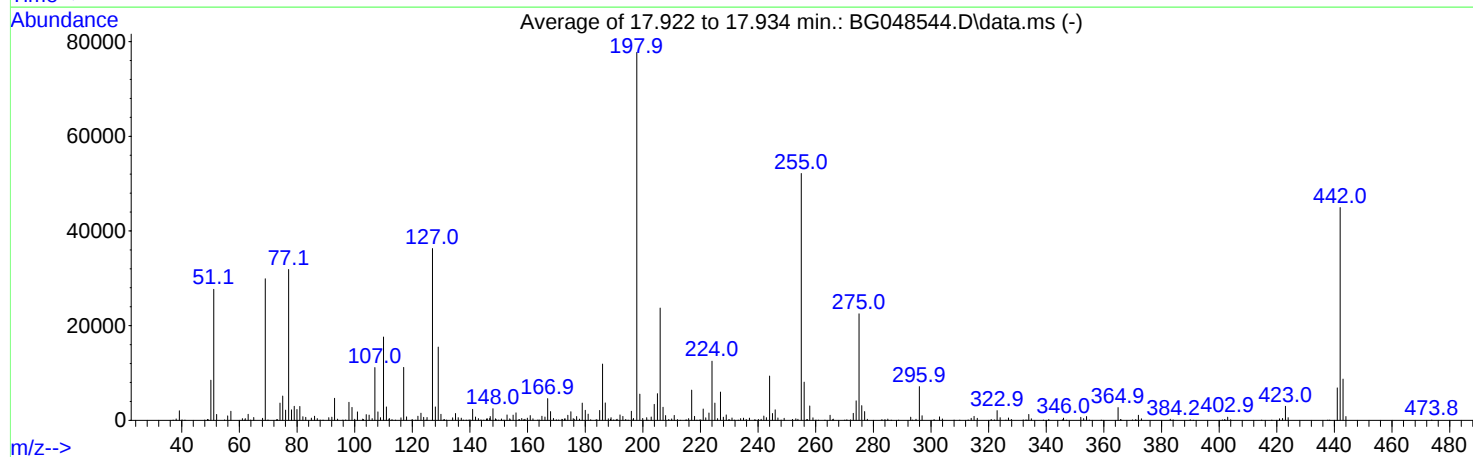


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040121\
 Data File : BG048544.D
 Acq On : 1 Apr 2021 14:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 02 10:20:56 2021

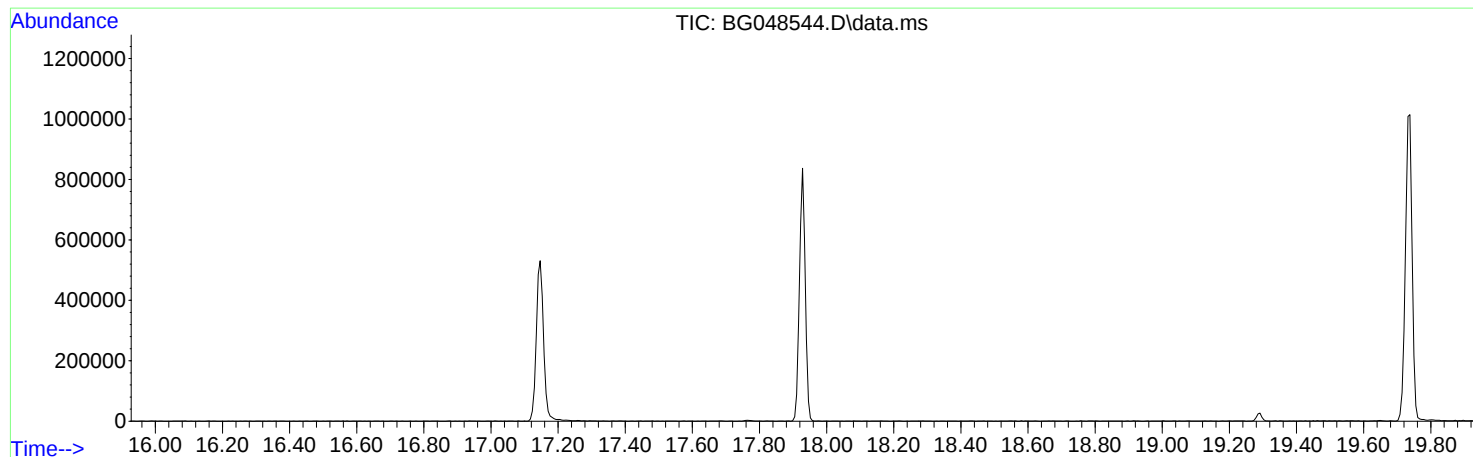




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	27680	PASS
68	69	0.00	2	1.5	455	PASS
69	198	0.00	100	38.5	29912	PASS
70	69	0.00	2	0.3	97	PASS
127	198	10	80	46.7	36307	PASS
197	198	0.00	2	0.5	422	PASS
198	198	100	100	100.0	77691	PASS
199	198	5	9	7.2	5555	PASS
275	198	10	60	29.0	22501	PASS
365	198	1	100	3.5	2702	PASS
441	198	0.01	100	8.9	6878	PASS
442	198	50	100	57.8	44944	PASS
443	442	15	24	19.4	8726	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040121\
 Data File : BG048544.D
 Acq On : 1 Apr 2021 14:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 01 15:52:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 11:19:59 2021
 Response via : Initial Calibration

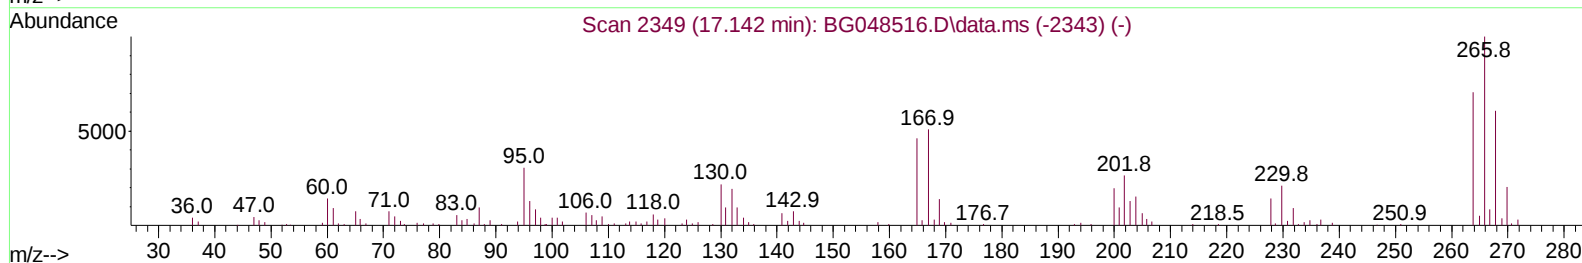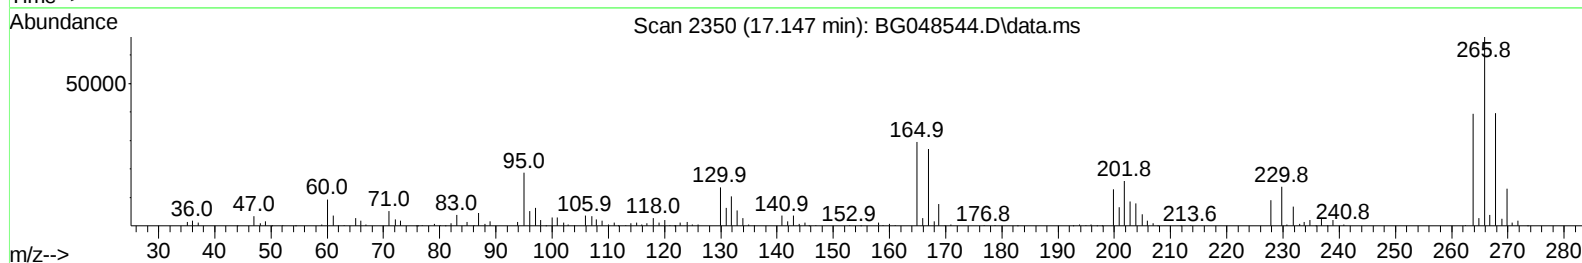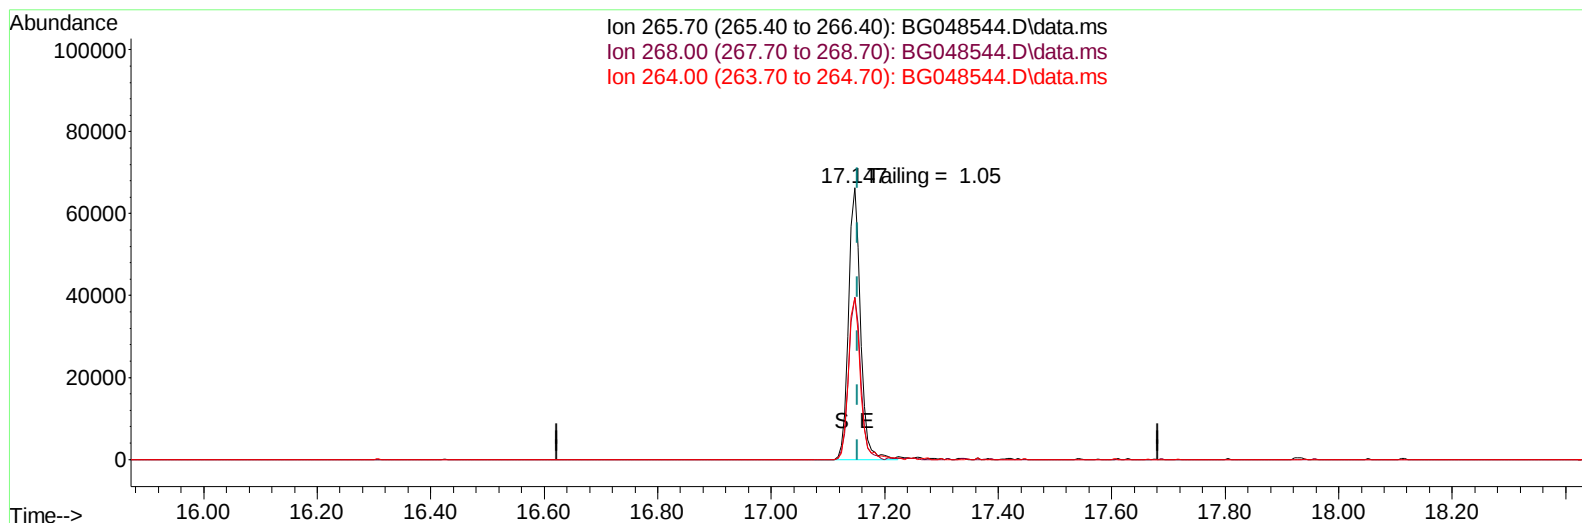

TIC: BG048544.D\data.ms

(70) Pentachlorophenol (C)

17.147min (-0.005) 227704.88 ng




response 96652

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	59.68
264.00	70.50	59.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040121\
 Data File : BG048544.D
 Acq On : 1 Apr 2021 14:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 01 15:52:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 11:19:59 2021
 Response via : Initial Calibration

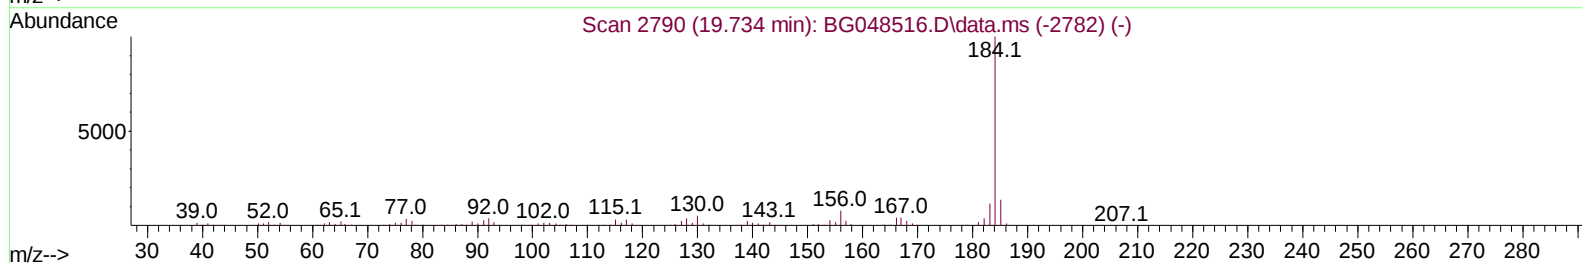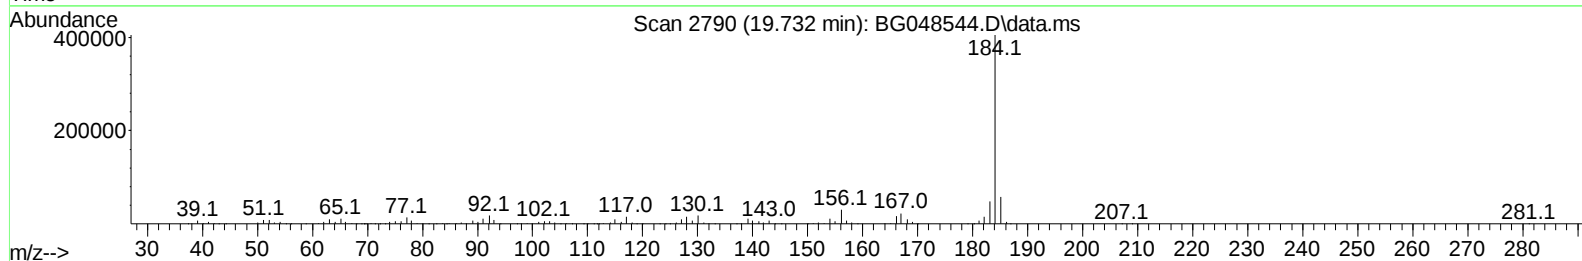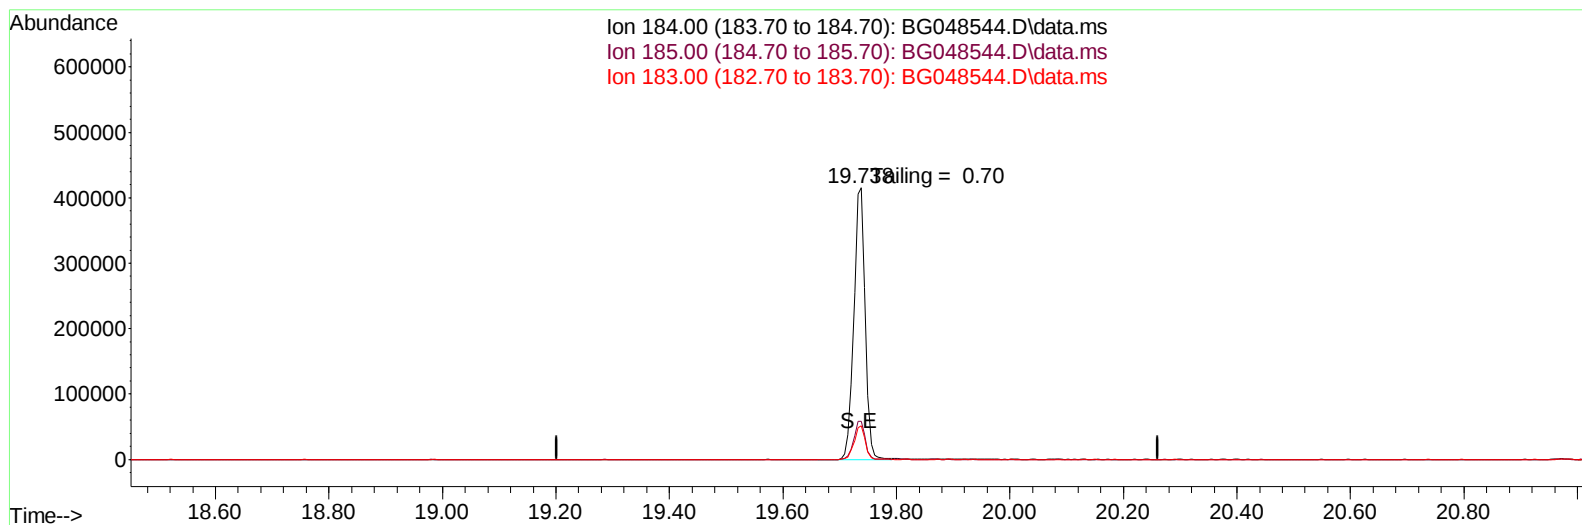

TIC: BG048544.D\data.ms

(77) Benzidine

19.731min (-19.731) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	13.70	0.00#
183.00	11.50	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/1/2021	BNA_G	BG048544.D
Compound Name	Response	Retention Time
DDT	306298	20.972
DDD	5529	20.519
DDE	377	20.02
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5906	312204	1.89