

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040219\
 Data File : BG040314.D
 Acq On : 3 Apr 2019 2:43
 Operator : JU/SJ
 Sample : K2182-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 S8A-S8B(12-16)COMP

Quant Time: Apr 03 03:53:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 28 05:47:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	58116	20.00	ng	-0.02
21) Naphthalene-d8	10.87	136	249002	20.00	ng	-0.02
39) Acenaphthene-d10	14.68	164	172362	20.00	ng	-0.02
64) Phenanthrene-d10	17.43	188	429343	20.00	ng	-0.02
76) Chrysene-d12	21.71	240	430169	20.00	ng	-0.02
87) Perylene-d12	25.01	264	429891	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	432031	123.58	ng	0.00
7) Phenol-d6	7.21	99	558707	115.64	ng	-0.02
23) Nitrobenzene-d5	9.23	82	414008	88.38	ng	-0.02
42) 2,4,6-Tribromophenol	16.17	330	193385	103.82	ng	-0.02
45) 2-Fluorobiphenyl	13.31	172	961638	82.67	ng	-0.02
79) Terphenyl-d14	20.03	244	1596235	83.48	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040219\
Data File : BG040314.D
Acq On : 3 Apr 2019 2:43
Operator : JU/SJ
Sample : K2182-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
S8A-S8B(12-16)COMP

Quant Time: Apr 03 03:53:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 28 05:47:00 2019
Response via : Initial Calibration

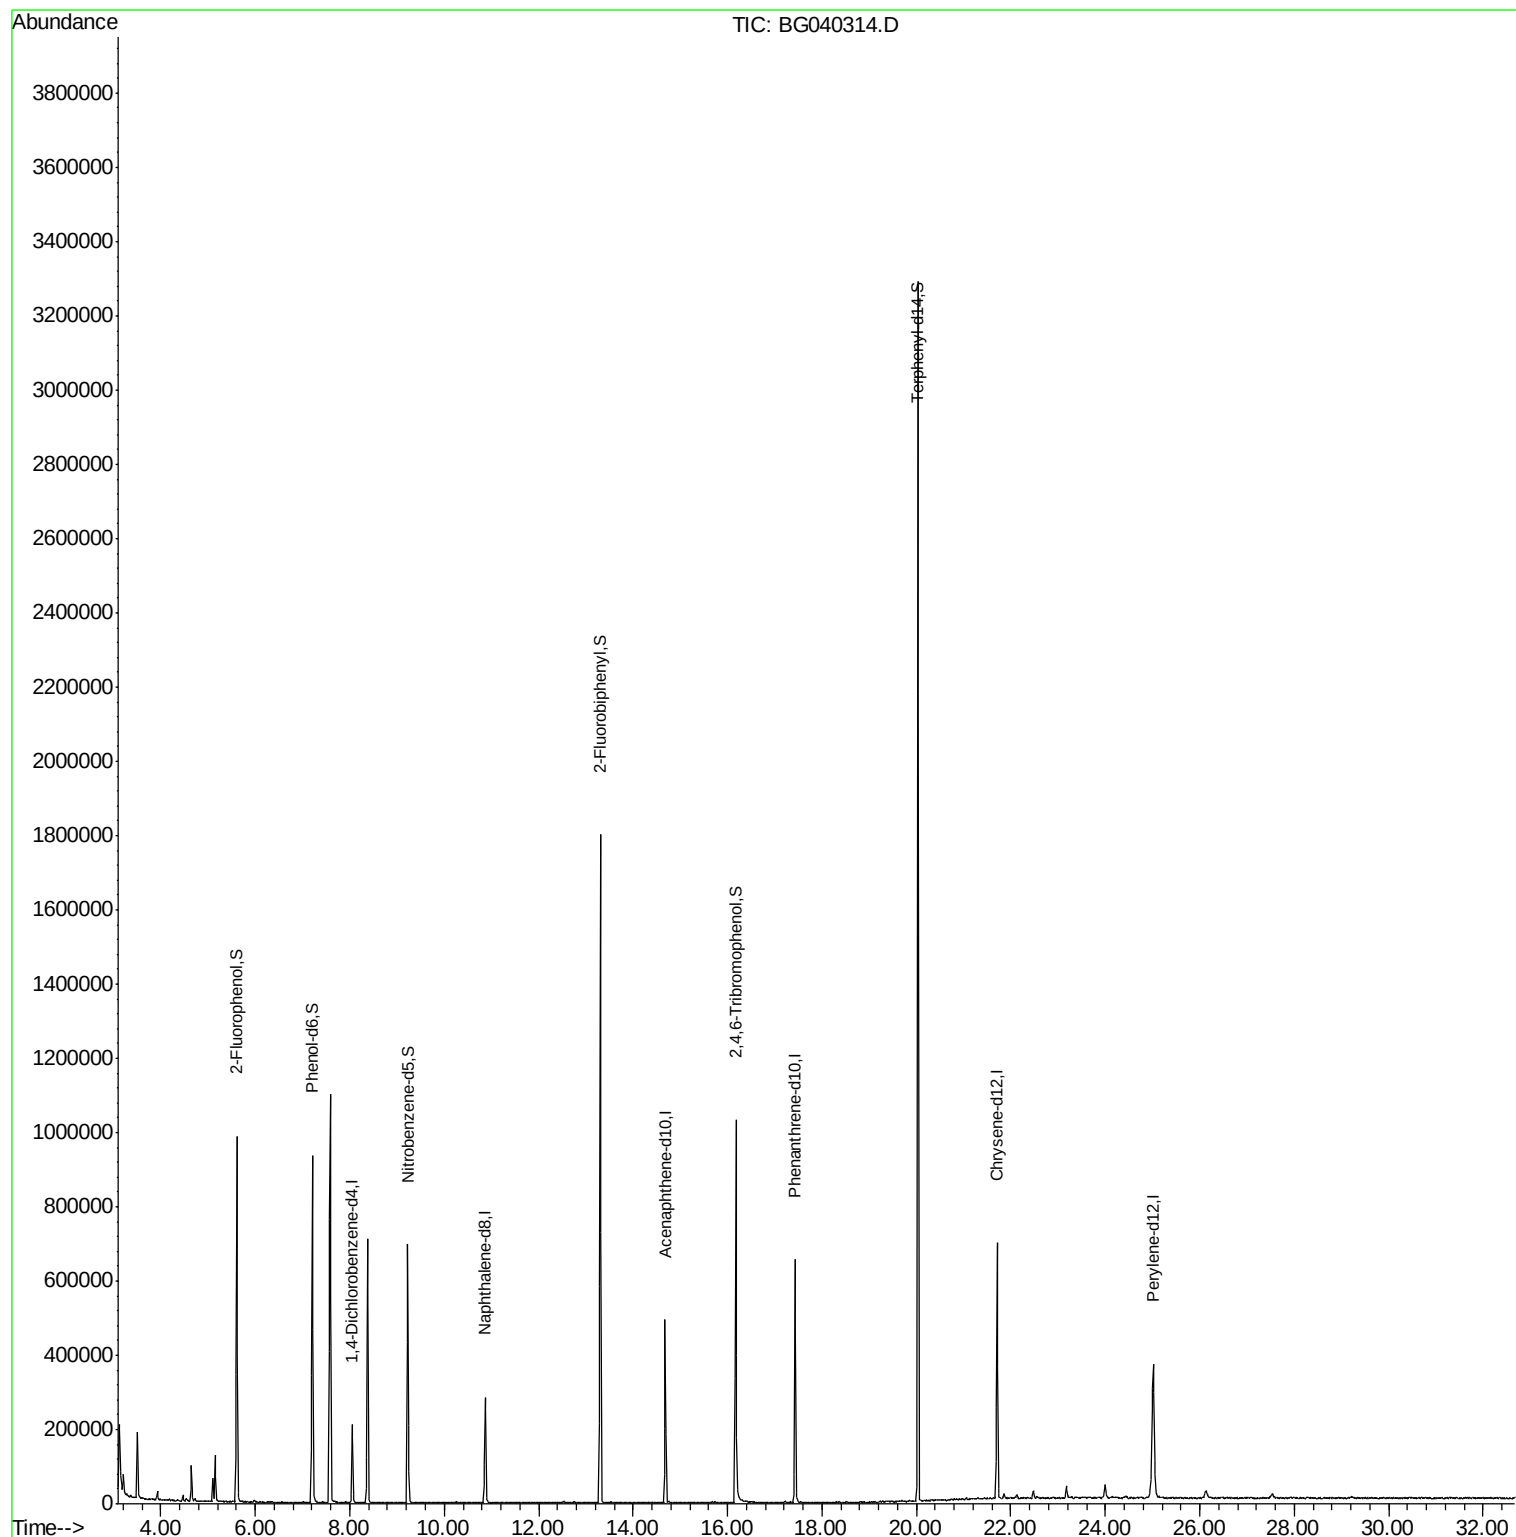


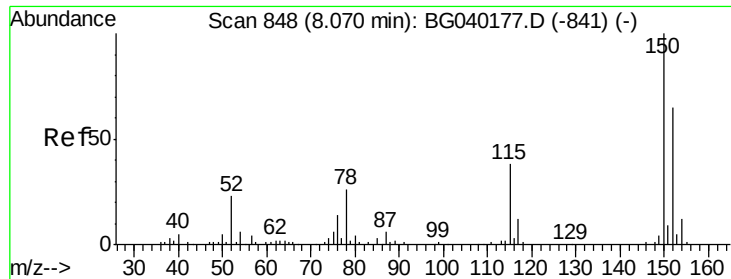




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.05 min Scan# 845
 Delta R.T. -0.02 min
 Lab File: BG040314.D
 Acq: 3 Apr 2019 2:43

Instrument :
 BNA_G
 ClientSampleId :
 S8A-S8B(12-16)COMP

Tgt Ion:152 Resp: 58116
 Ion Ratio Lower Upper
 152 100
 150 157.0 123.7 185.5
 115 56.3 46.9 70.3

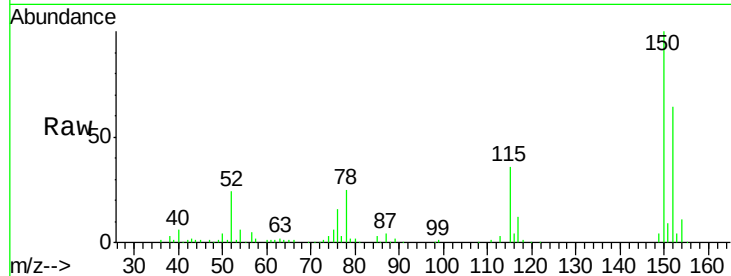


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

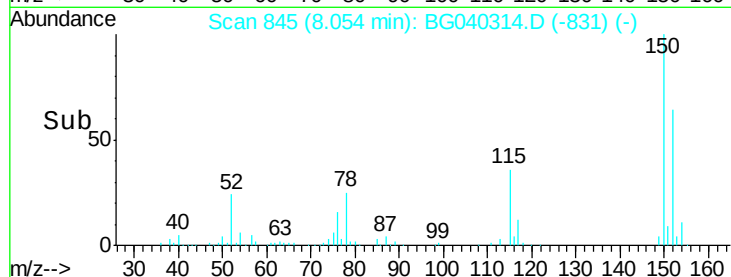
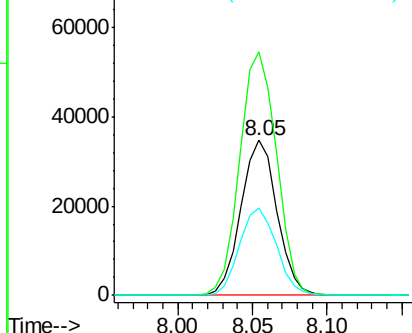



#5
 2-Fluorophenol
 Concen: 123.583 ng
 RT: 5.61 min Scan# 429
 Delta R.T. -0.01 min
 Lab File: BG040314.D
 Acq: 3 Apr 2019 2:43

Tgt Ion:112 Resp: 432031
 Ion Ratio Lower Upper
 112 100
 64 69.3 54.2 81.2
 63 32.5 26.4 39.6



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC

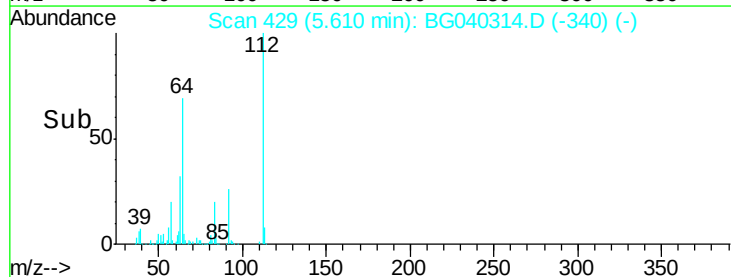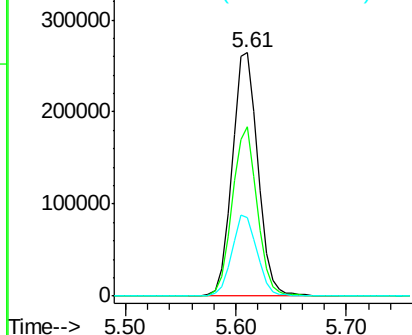

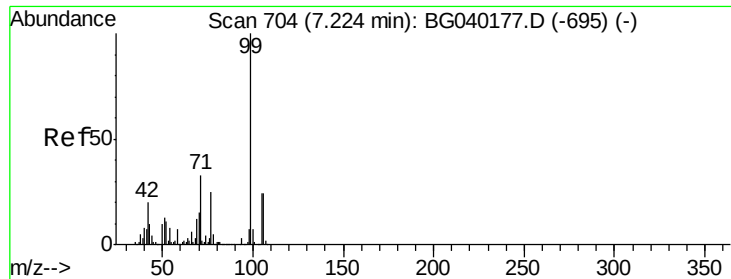

#7

Phenol-d6

Concen: 115.642 ng

RT: 7.21 min Scan# 701

Delta R.T. -0.02 min

Lab File: BG040314.D

Acq: 3 Apr 2019 2:43

Instrument :

BNA_G

ClientSampleId :

S8A-S8B(12-16)COMP


Tgt Ion: 99 Resp: 558707

Ion Ratio Lower Upper




99 100

42 18.3 16.2 24.2

71 32.2 26.8 40.2



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

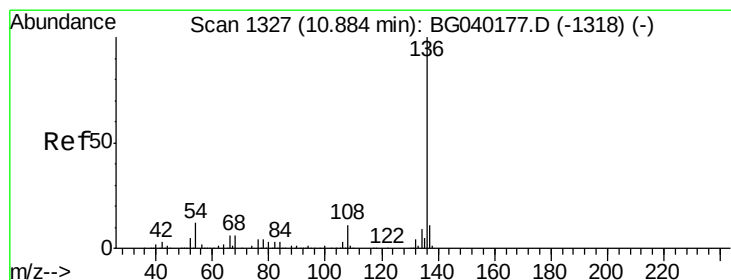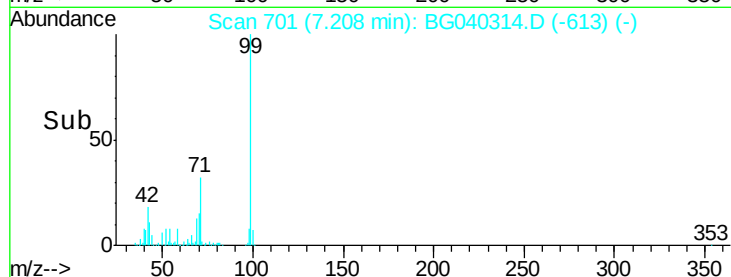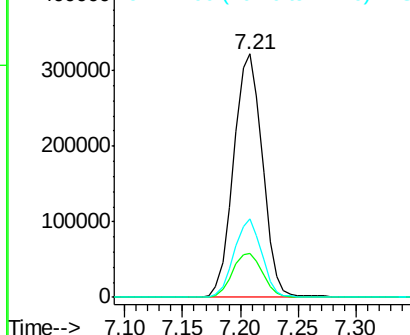

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.87 min Scan# 1324

Delta R.T. -0.02 min

Lab File: BG040314.D

Acq: 3 Apr 2019 2:43

Tgt Ion: 136 Resp: 249002


Ion Ratio Lower Upper

136 100



137 11.5 8.9 13.3


54 10.2 9.6 14.4

68 6.4 5.1 7.7

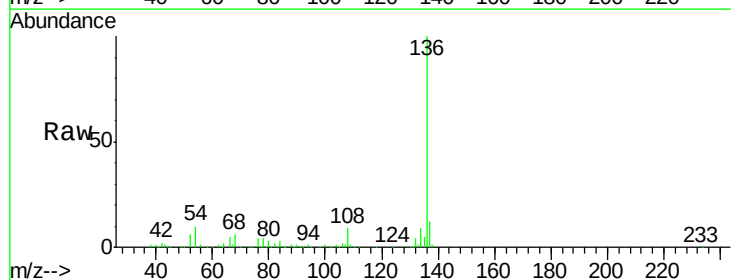

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



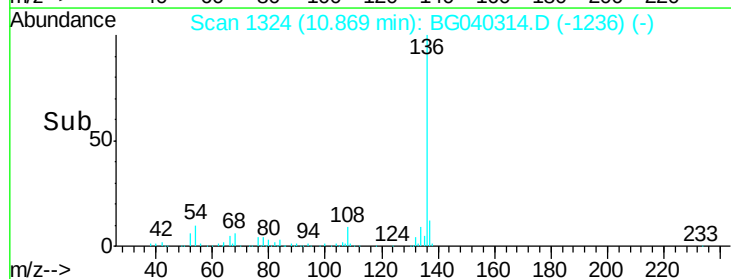
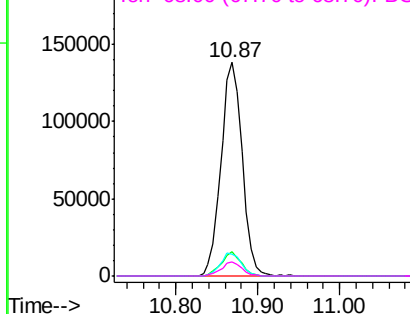


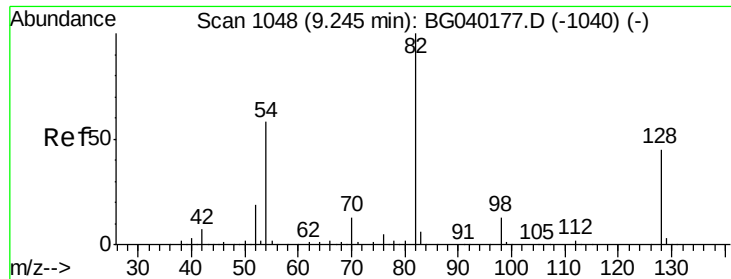

#23
Nitrobenzene-d5
Concen: 88.377 ng
RT: 9.23 min Scan# 1045
Delta R.T. -0.02 min
Lab File: BG040314.D
Acq: 3 Apr 2019 2:43




Instrument :
BNA_G
ClientSampleId :
S8A-S8B(12-16)COMP


Tgt Ion: 82 Resp: 414008
Ion Ratio Lower Upper
82 100
128 43.6 35.8 53.8
54 56.9 46.2 69.2

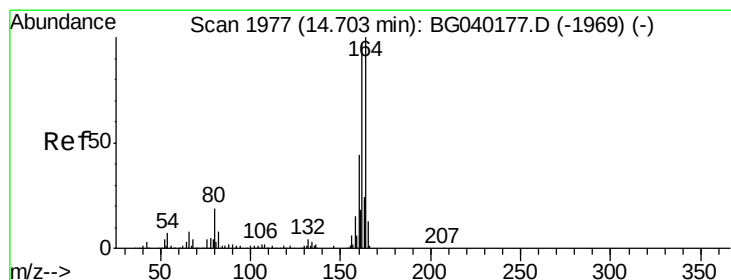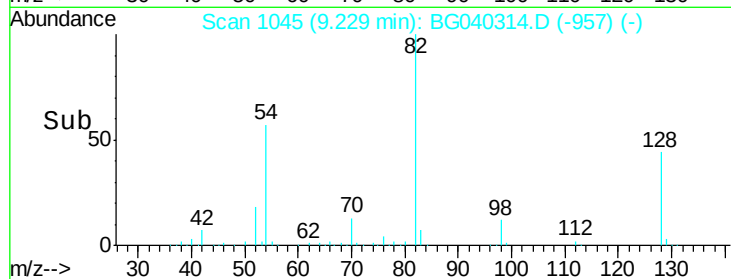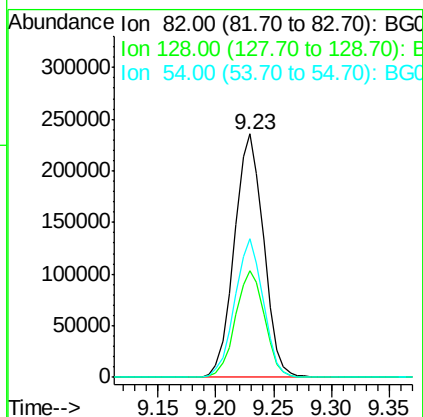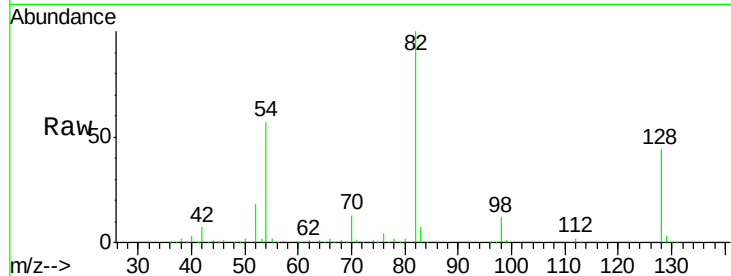

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.68 min Scan# 1973
Delta R.T. -0.02 min
Lab File: BG040314.D
Acq: 3 Apr 2019 2:43

Tgt Ion: 164 Resp: 172362
Ion Ratio Lower Upper
164 100
162 99.8 77.4 116.2
160 43.7 35.3 52.9

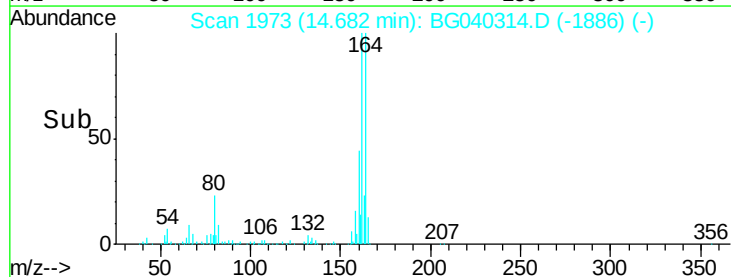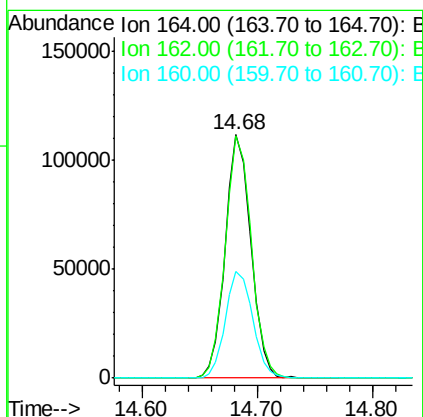


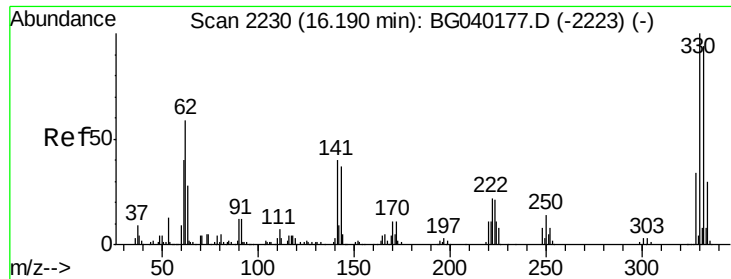




#42
 2,4,6-Tribromophenol
 Concen: 103.815 ng
 RT: 16.17 min Scan# 2227
 Delta R.T. -0.02 min
 Lab File: BG040314.D
 Acq: 3 Apr 2019 2:43

Instrument :
 BNA_G
 ClientSampleId :
 S8A-S8B(12-16)COMP

Tgt Ion	Ratio	Lower	Upper
330	100		
332	100.2	76.6	115.0
141	40.2	32.6	48.8




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

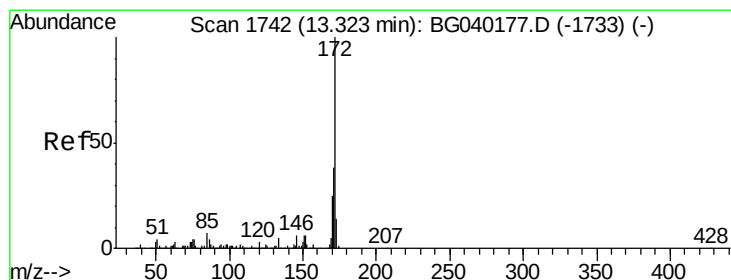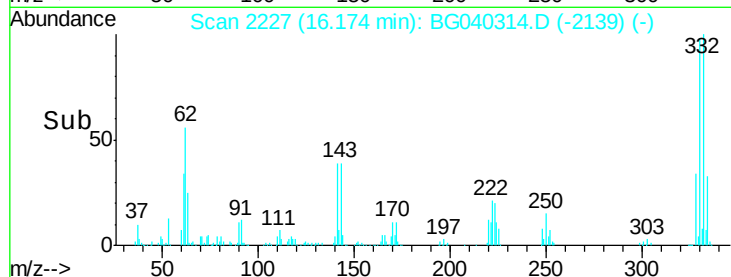
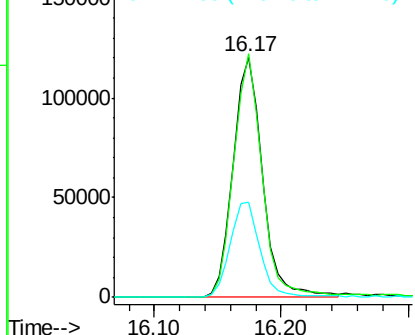



#45
 2-Fluorobiphenyl
 Concen: 82.670 ng
 RT: 13.31 min Scan# 1739
 Delta R.T. -0.02 min
 Lab File: BG040314.D
 Acq: 3 Apr 2019 2:43

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.7	30.5	45.7
170	24.3	20.1	30.1



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

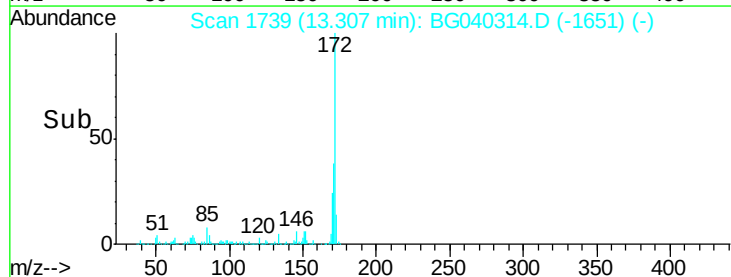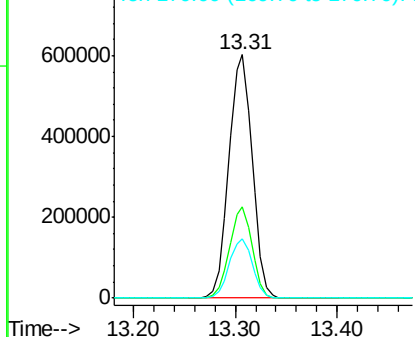

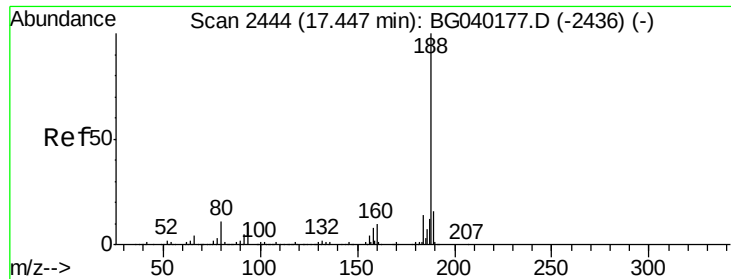

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.43 min Scan# 2440

Delta R.T. -0.02 min

Lab File: BG040314.D

Acq: 3 Apr 2019 2:43

Instrument :

BNA_G

ClientSampleId :

S8A-S8B(12-16)COMP


Tgt Ion:188 Resp: 429343

Ion Ratio Lower Upper

188 100

94 8.8 7.0 10.4




80 10.7 8.6 13.0

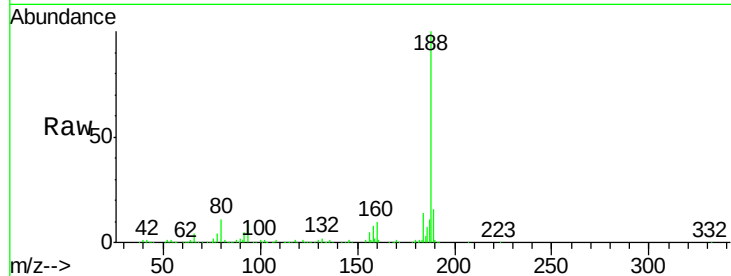

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

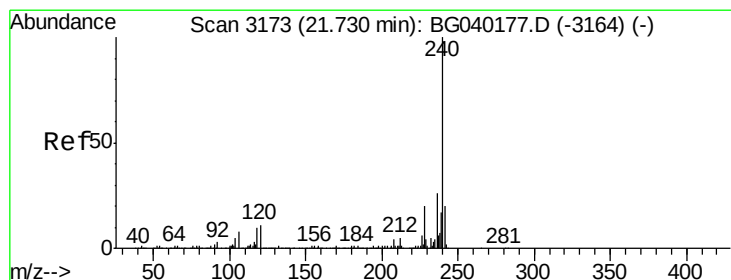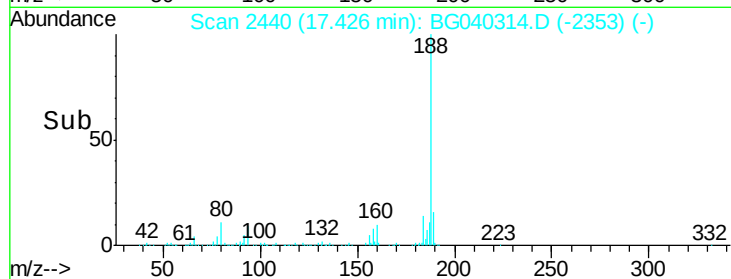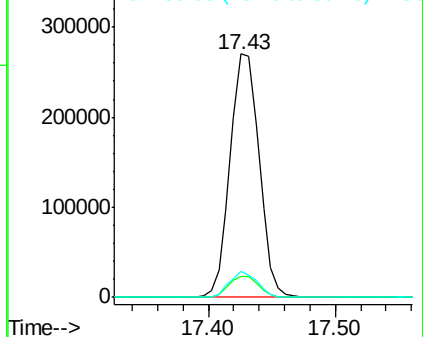

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.71 min Scan# 3169

Delta R.T. -0.02 min

Lab File: BG040314.D

Acq: 3 Apr 2019 2:43


Tgt Ion:240 Resp: 430169

Ion Ratio Lower Upper

240 100

120 10.6 8.4 12.6



236 25.1 20.8 31.2




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

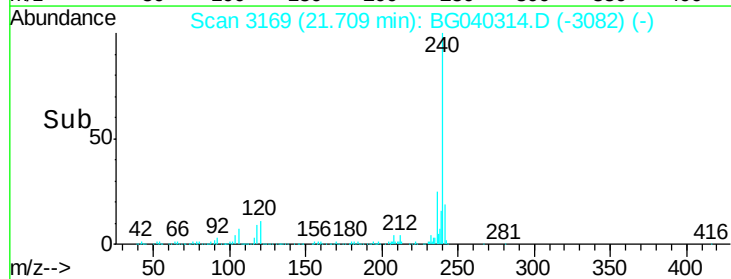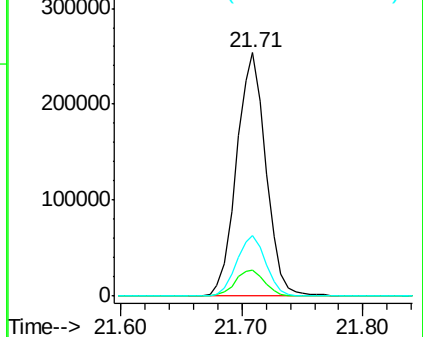

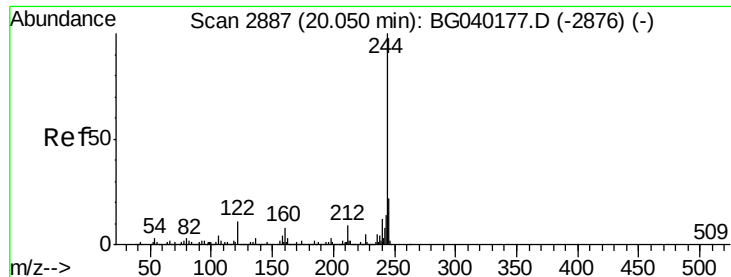

#79

Terphenyl-d14

Concen: 83.478 ng

RT: 20.03 min Scan# 2884

Delta R.T. -0.02 min

Lab File: BG040314.D

Acq: 3 Apr 2019 2:43

Instrument :

BNA_G

ClientSampleId :

S8A-S8B(12-16)COMP


Tgt Ion:244 Resp: 1596235

Ion Ratio Lower Upper

244 100

212 8.6 7.0 10.6




122 11.0 8.5 12.7



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

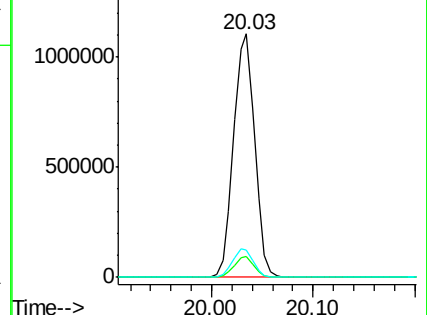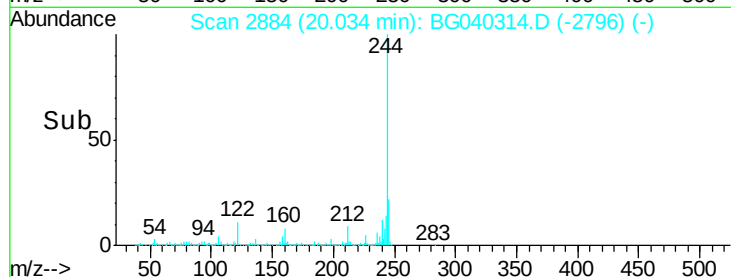

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.01 min Scan# 3731

Delta R.T. -0.02 min

Lab File: BG040314.D

Acq: 3 Apr 2019 2:43


Tgt Ion:264 Resp: 429891

Ion Ratio Lower Upper

264 100

260 23.1 17.9 26.9

265 20.8 16.8 25.2



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

