


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040219\
 Data File : BG040317.D
 Acq On : 3 Apr 2019 5:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 28 05:47:00 2019

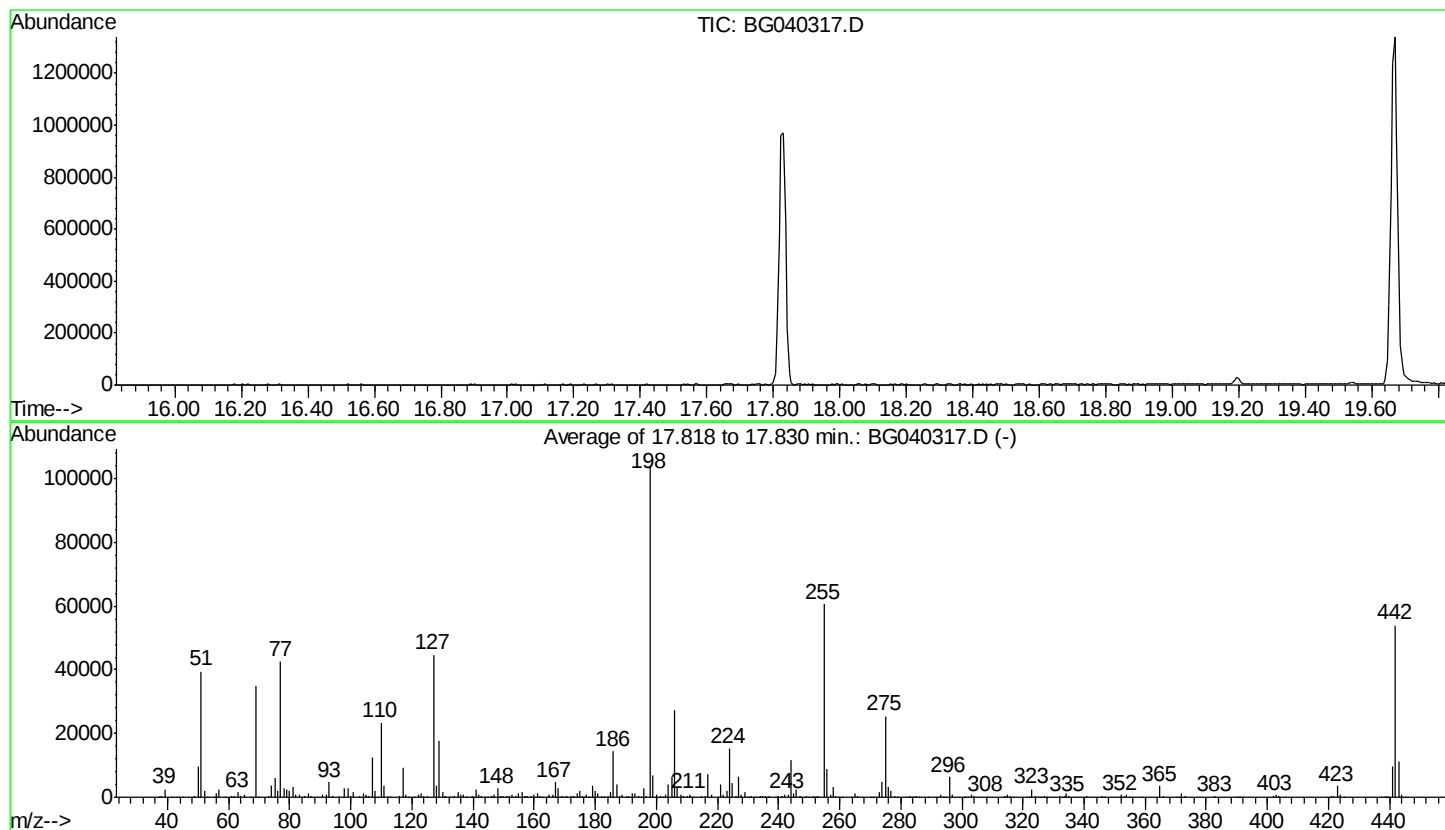

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	39549	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.8	35146	PASS
70	69	0.00	2	0.4	148	PASS
127	198	10	80	42.9	44666	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	104069	PASS
199	198	5	9	6.5	6799	PASS
275	198	10	60	24.5	25480	PASS
365	198	1	100	3.4	3498	PASS
441	198	0.01	100	9.2	9551	PASS
442	198	50	100	51.9	53976	PASS
443	442	15	24	20.9	11263	PASS