


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040224\
Data File : BG060733.D
Acq On : 2 Apr 2024 9:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 30 03:12:26 2024

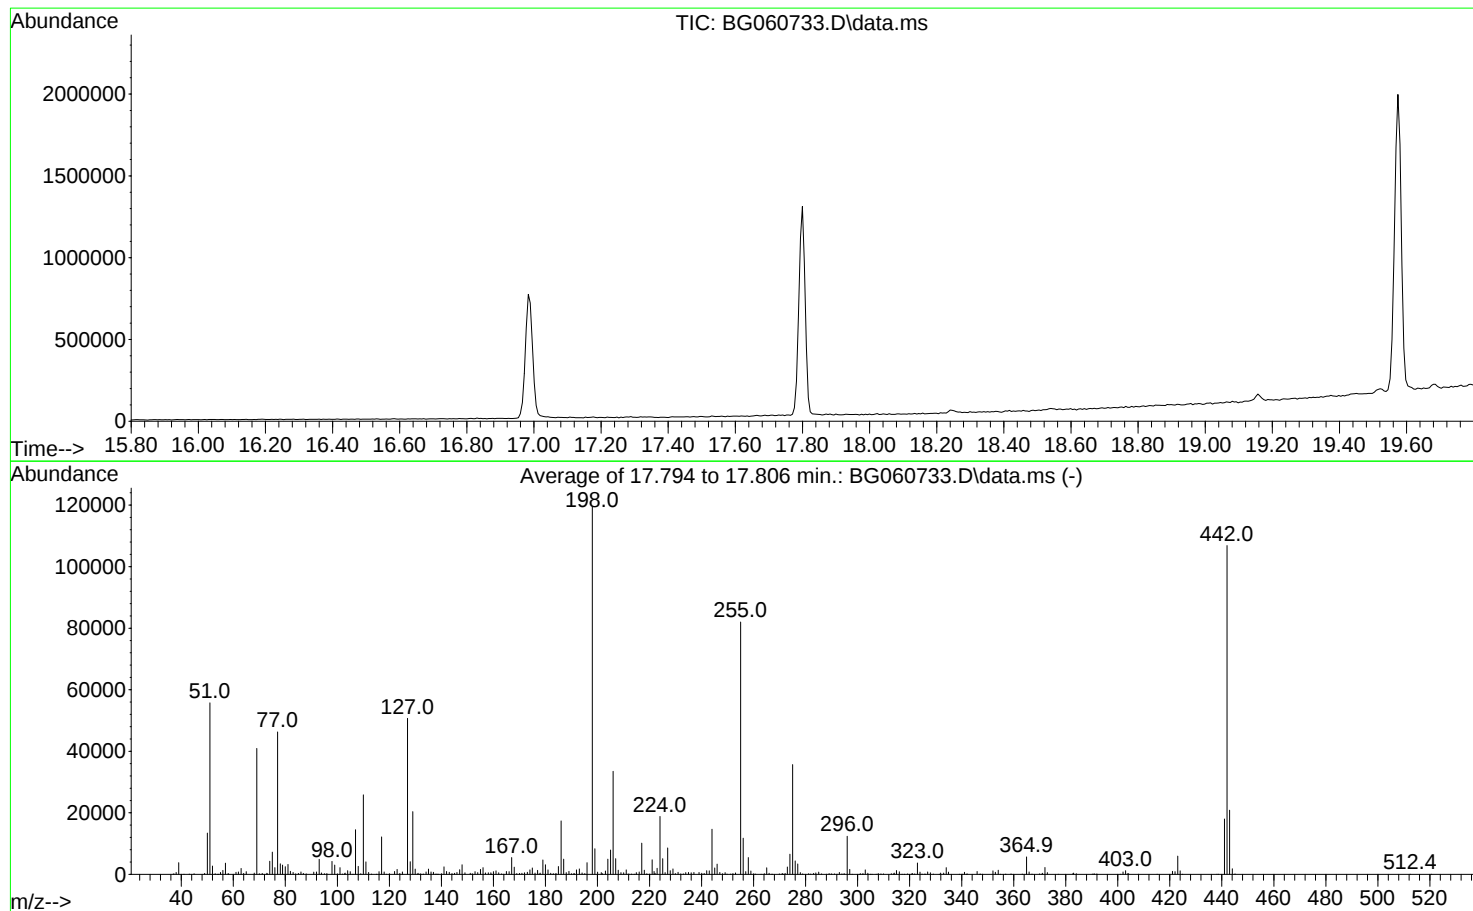




AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.6	55747	PASS
68	69	0.00	2	1.0	398	PASS
69	198	0.00	100	34.2	40936	PASS
70	69	0.00	2	0.5	210	PASS
127	198	10	80	42.4	50690	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	119555	PASS
199	198	5	9	7.0	8315	PASS
275	198	10	60	29.9	35701	PASS
365	198	1	100	4.8	5695	PASS
441	198	0.01	100	15.0	17974	PASS
442	442	50	100	100.0	106888	PASS
443	442	15	24	19.5	20856	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040224\
Data File : BG060733.D
Acq On : 2 Apr 2024 9:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 02 12:36:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

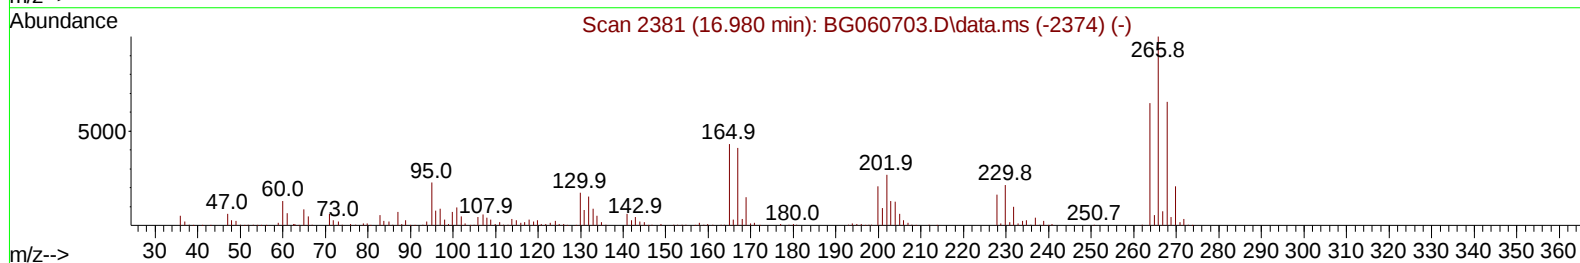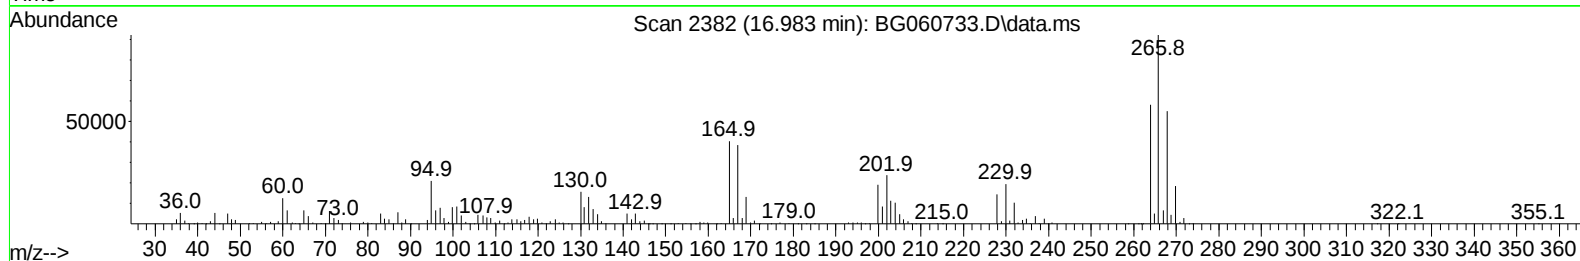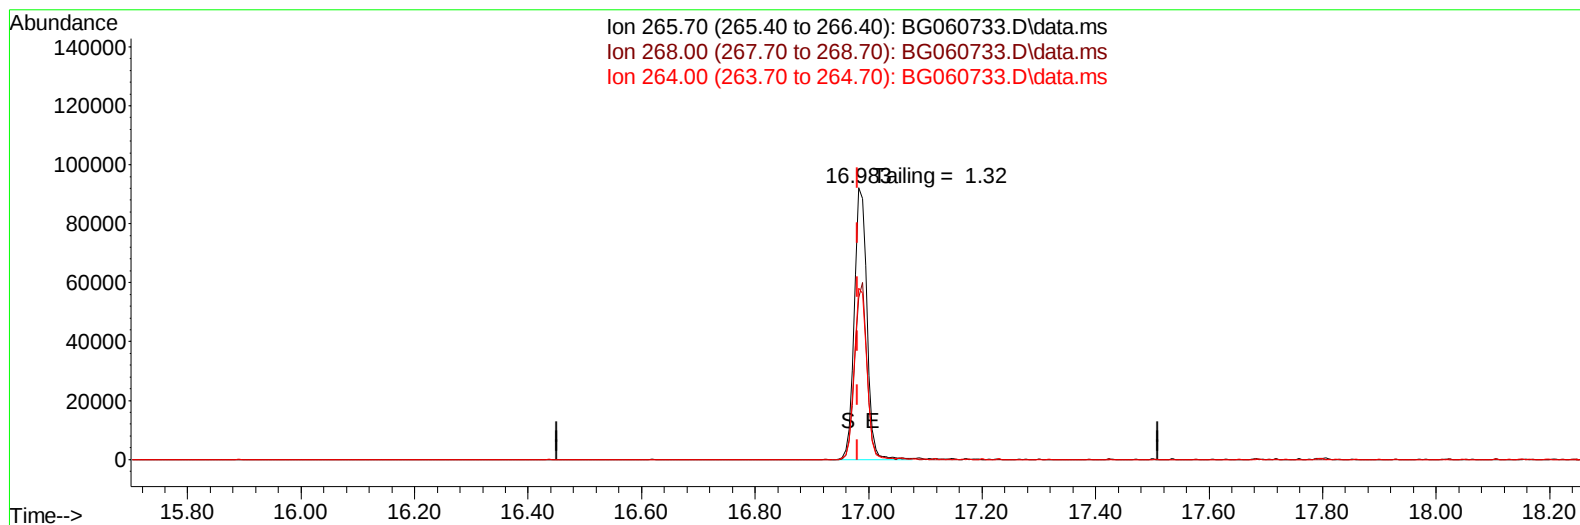

TIC: BG060733.D\data.ms

(70) Pentachlorophenol (C)

16.983min (+ 0.003) 311409.69 ng




response 142003

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	59.60
264.00	64.70	63.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040224\
Data File : BG060733.D
Acq On : 2 Apr 2024 9:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 02 12:36:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

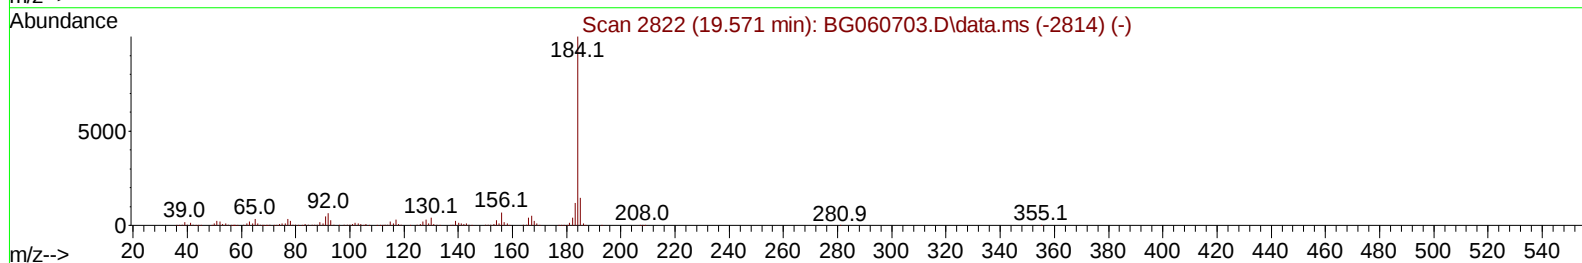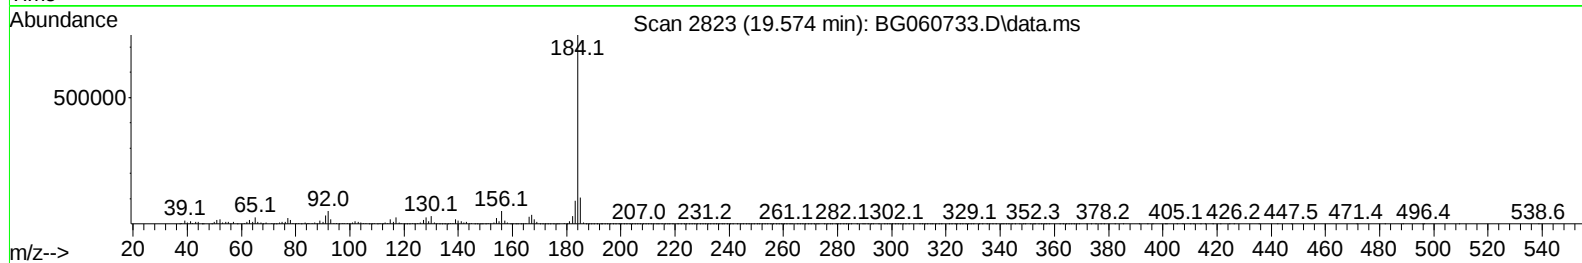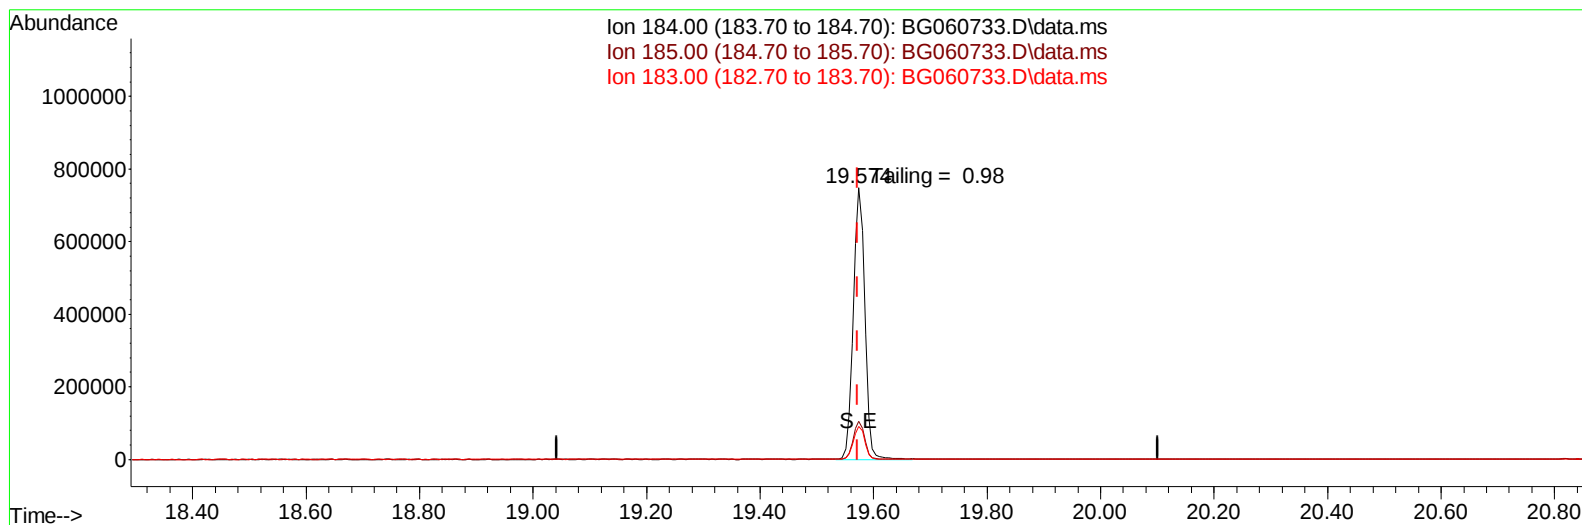

TIC: BG060733.D\data.ms

(77) Benzidine**19.574min (+ 0.003) 139592.51 ng****response 1051271**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.98
183.00	11.90	12.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/2/2024	BNA_G	<u>BG060733.D</u>
Compound Name	Response	Retention Time
DDT	466000	20.82
DDD	10738	20.432
DDE	0	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10738	476738	2.25

Instrument :
BNA_G
ClientSampleId :
DFTPP