


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040224\
Data File : BG060739.D
Acq On : 2 Apr 2024 15:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 30 03:12:26 2024

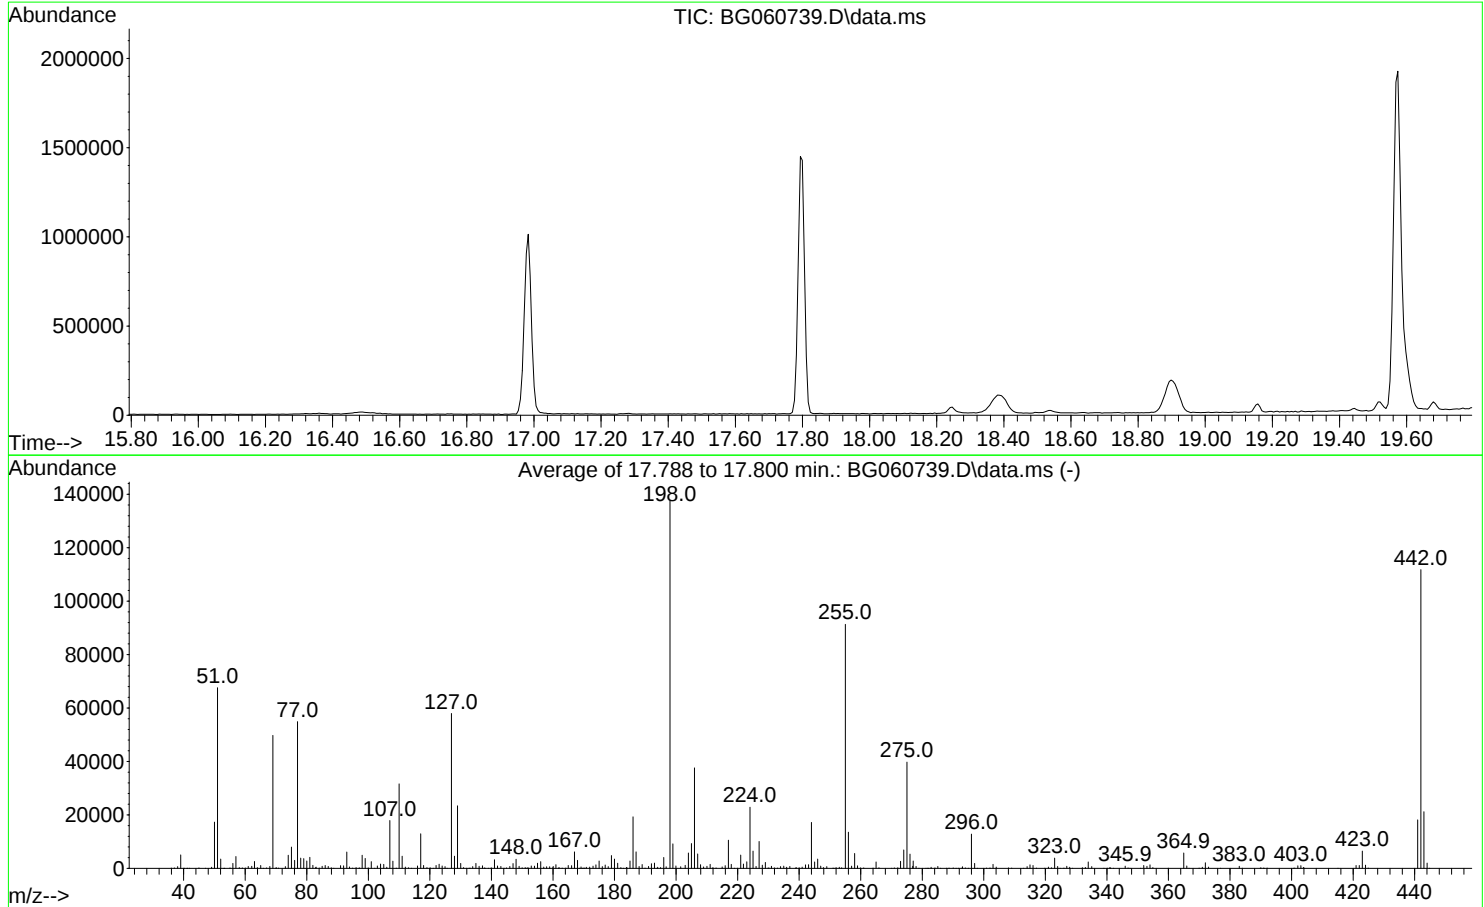




AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.1	67589	PASS
68	69	0.00	2	1.4	719	PASS
69	198	0.00	100	36.1	49751	PASS
70	69	0.00	2	0.5	239	PASS
127	198	10	80	42.1	57965	PASS
197	198	0.00	2	0.4	595	PASS
198	198	100	100	100.0	137664	PASS
199	198	5	9	6.7	9171	PASS
275	198	10	60	28.9	39739	PASS
365	198	1	100	4.2	5752	PASS
441	198	0.01	100	13.2	18169	PASS
442	442	50	100	100.0	111781	PASS
443	442	15	24	19.0	21225	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040224\
Data File : BG060739.D
Acq On : 2 Apr 2024 15:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 03 04:12:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

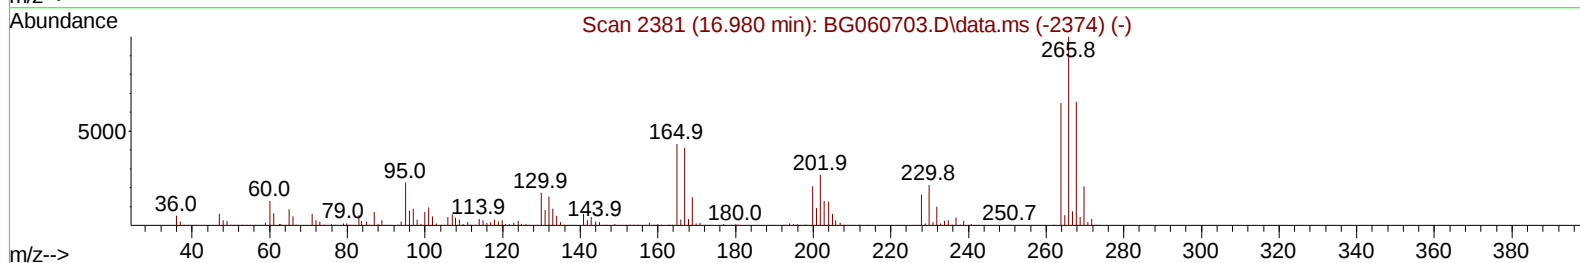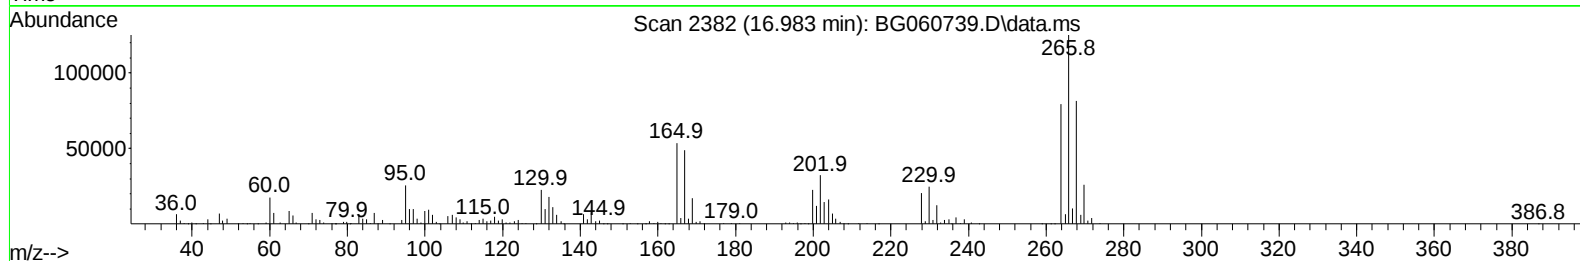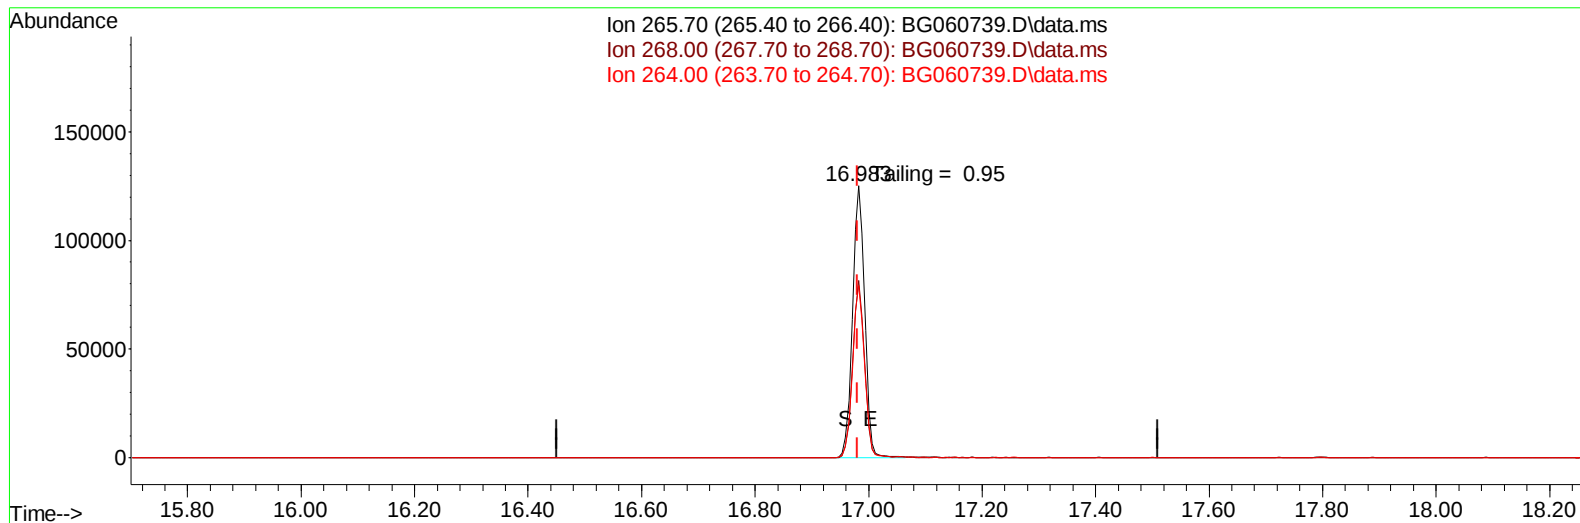

TIC: BG060739.D\data.ms

(70) Pentachlorophenol (C)

16.983min (+ 0.003) 22476.19 ng




response 186165

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.24
264.00	64.70	63.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040224\
Data File : BG060739.D
Acq On : 2 Apr 2024 15:56
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 03 04:12:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

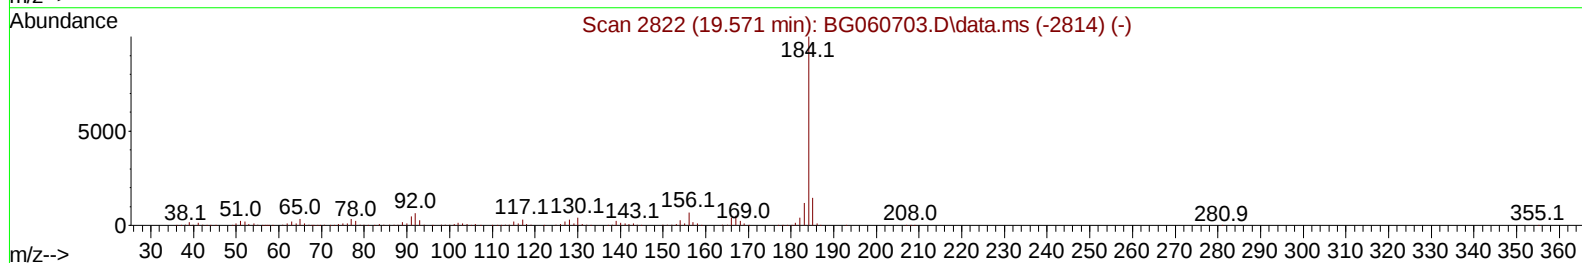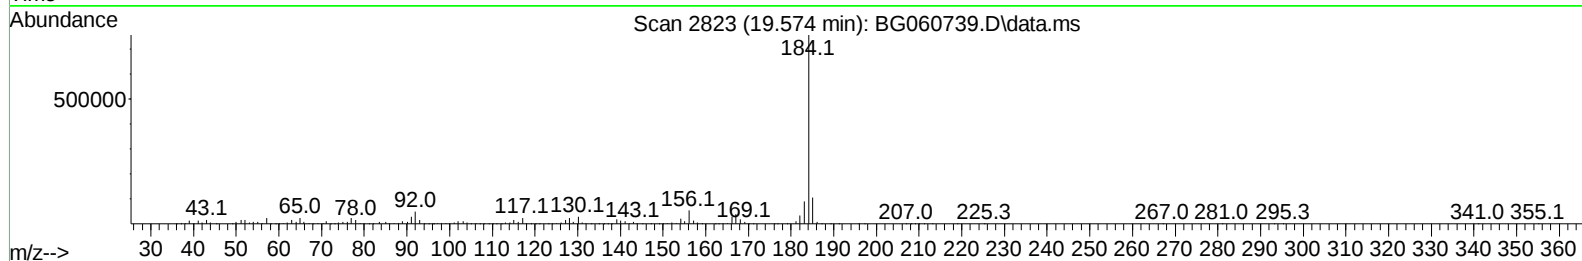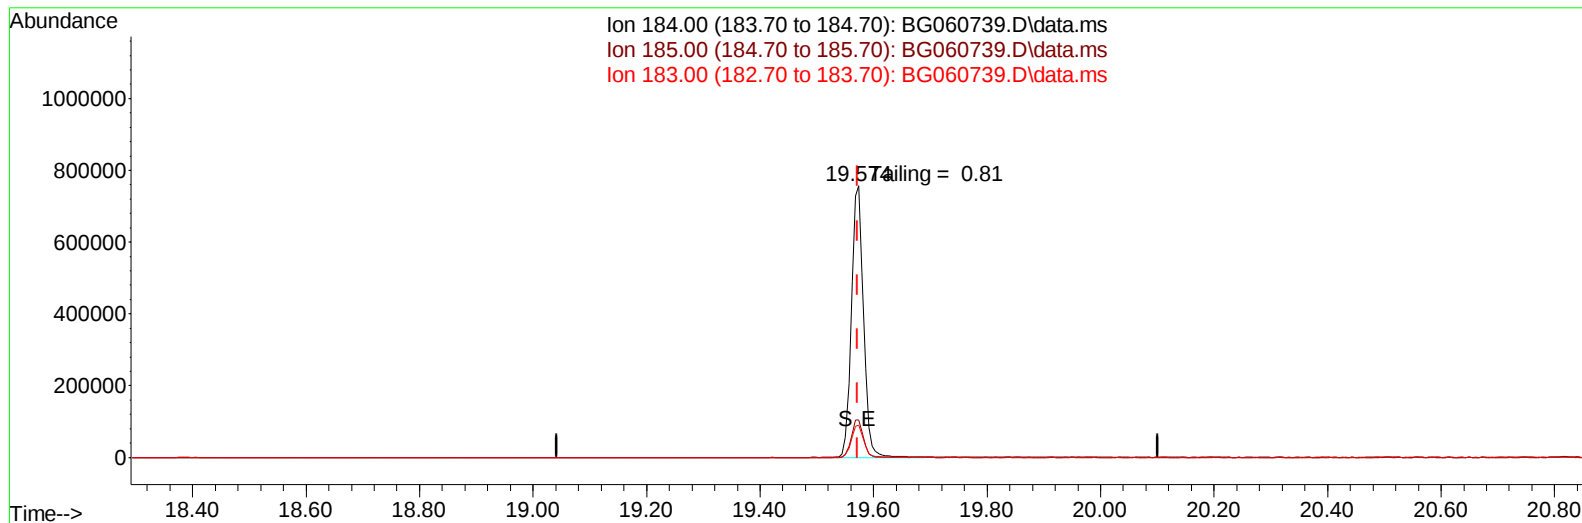

TIC: BG060739.D\data.ms

(77) Benzidine

19.574min (+ 0.003) 567594.34 ng

response 1091057

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.89
183.00	11.90	11.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/2/2024	BNA_G	<u>BG060739.D</u>
Compound Name	Response	Retention Time
DDT	534741	20.82
DDD	10838	20.432
DDE	102	19.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10940	545681	2.00

Instrument :
BNA_G
ClientSampleId :
DFTPP