

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG040319\
 Data File : BG040334.D
 Acq On : 3 Apr 2019 20:26
 Operator : JU/SJ
 Sample : K2182-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Apr 04 01:24:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 28 05:47:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	60678	20.00	ng	-0.02
21) Naphthalene-d8	10.86	136	240352	20.00	ng	-0.02
39) Acenaphthene-d10	14.68	164	150996	20.00	ng	-0.02
64) Phenanthrene-d10	17.42	188	368233	20.00	ng	-0.02
76) Chrysene-d12	21.70	240	408128	20.00	ng	-0.04
87) Perylene-d12	24.98	264	418534	20.00	ng	-0.05

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.60	112	372817	102.14	ng	-0.02
7) Phenol-d6	7.20	99	528895	104.85	ng	-0.02
23) Nitrobenzene-d5	9.22	82	309074	68.35	ng	-0.02
42) 2,4,6-Tribromophenol	16.17	330	189480	116.11	ng	-0.02
45) 2-Fluorobiphenyl	13.30	172	727347	71.38	ng	-0.02
79) Terphenyl-d14	20.03	244	1182257	65.17	ng	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
10) Phenol	7.23	94	14997	2.739	ng	96
19) n-Nitroso-di-n-propylamine	9.22	70	38344	10.602	ng	# 74
50) Dimethylphthalate	14.13	163	53799	4.552	ng	97
51) 2,6-Dinitrotoluene	14.68	165	18781	7.078	ng	# 25
57) 2,4-Dinitrotoluene	14.68	165	18781	5.094	ng	# 25
67) 4-Bromophenyl-phenylether	16.17	248	14204	3.428	ng	# 1
75) Fluoranthene	19.47	202	152426	6.651	ng	95
78) Pyrene	19.83	202	169042	6.298	ng	97
81) Benzo(a)anthracene	21.68	228	71041	2.826	ng	97
83) Chrysene	21.74	228	96569	3.997	ng	98
88) Benzo(b)fluoranthene	23.92	252	140598	5.487	ng	100
89) Benzo(k)fluoranthene	23.92	252	140598	5.967	ng	98
90) Benzo(a)pyrene	24.66	252	59591	2.479	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG040319\
Data File : BG040334.D
Acq On : 3 Apr 2019 20:26
Operator : JU/SJ
Sample : K2182-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Apr 04 01:24:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 28 05:47:00 2019
Response via : Initial Calibration

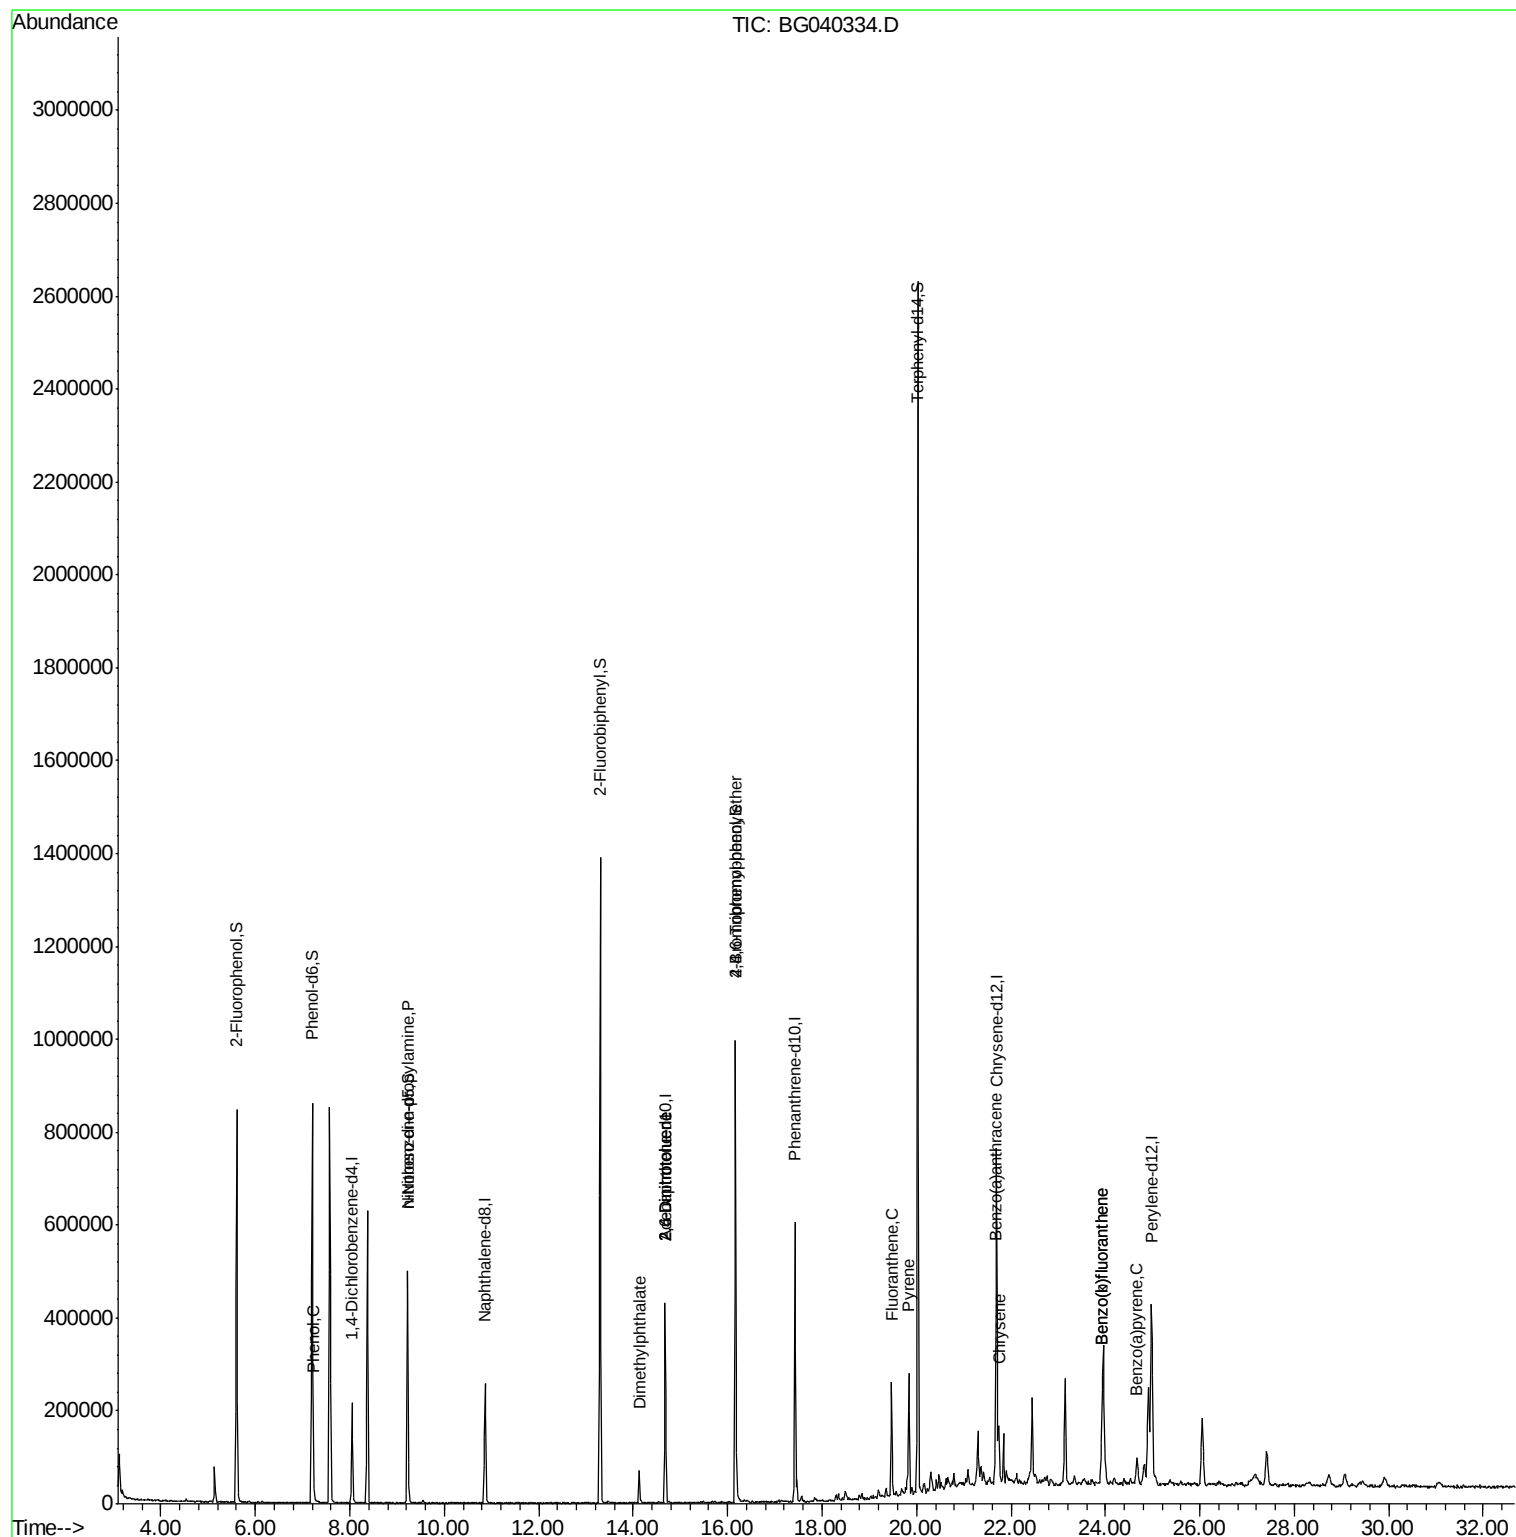




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 844
Delta R.T. -0.02 min
Lab File: BG040334.D
Acq: 3 Apr 2019 20:26

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 60678
Ion Ratio Lower Upper
152 100
150 149.6 123.7 185.5
115 54.0 46.9 70.3

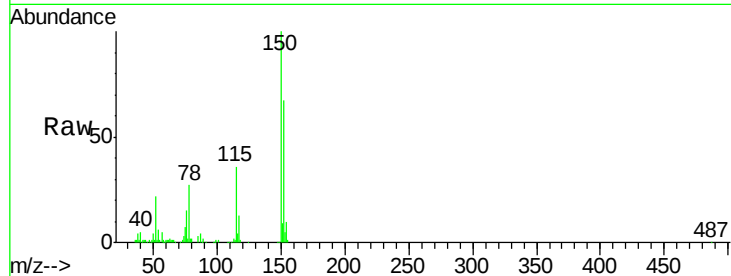


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

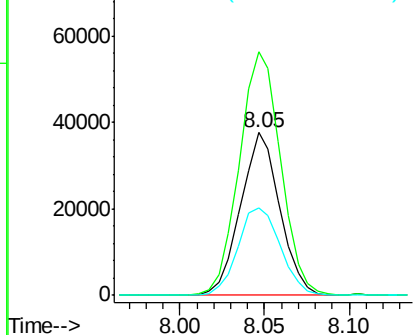



#5


2-Fluorophenol
Concen: 102.142 ng
RT: 5.60 min Scan# 428
Delta R.T. -0.02 min
Lab File: BG040334.D
Acq: 3 Apr 2019 20:26

Tgt Ion:112 Resp: 372817
Ion Ratio Lower Upper
112 100
64 67.8 54.2 81.2
63 33.8 26.4 39.6

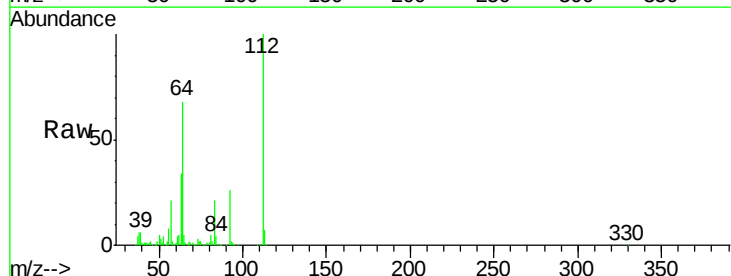

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

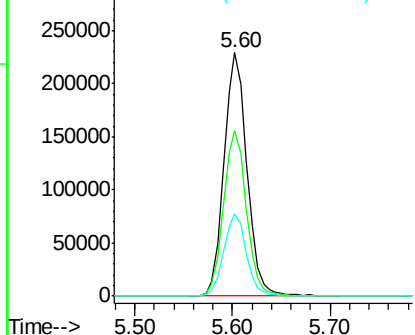



#7

Phenol-d6

Concen: 104.849 ng

RT: 7.20 min Scan# 700

Delta R.T. -0.02 min

Lab File: BG040334.D

Acq: 3 Apr 2019 20:26

Instrument :

BNA_G

ClientSampled :


Tot Ion: 99 Resp: 528895

Ion Ratio Lower Upper




99 100

42 18.4 16.2 24.2

71 31.4 26.8 40.2

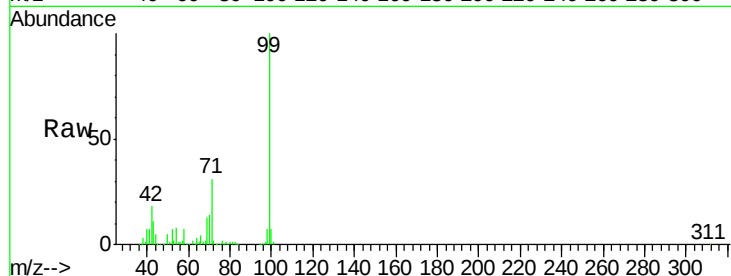

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

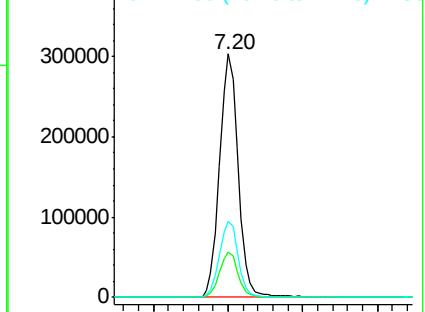

#10

Phenol

Concen: 2.739 ng

RT: 7.23 min Scan# 705

Delta R.T. -0.02 min

Lab File: BG040334.D

Acq: 3 Apr 2019 20:26


Tgt Ion: 94 Resp: 14997

Ion Ratio Lower Upper



94 100




65 29.0 10.5 50.5

66 39.5 16.9 56.9



Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

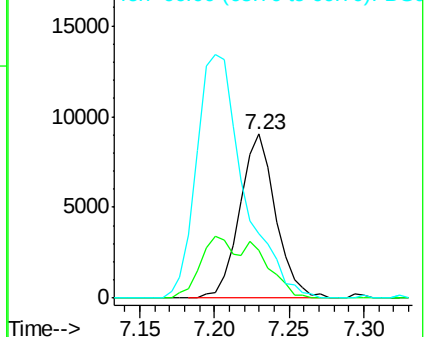

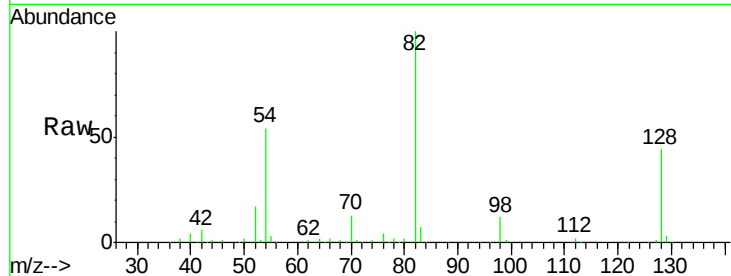

#19

n-Nitroso-di-n-propylamine

Concen: 10.602 ng

RT: 9.22 min Scan# 1044

Delta R.T. 0.35 min

Lab File: BG040334.D

Acq: 3 Apr 2019 20:26

Instrument :

BNA_G

ClientSampleId :

Tot Ion: 70 Resp: 38344





Ion Ratio Lower Upper

70 100

42 51.1 54.0 81.0#

101 0.0 8.6 13.0#

130 1.9 18.2 27.2#

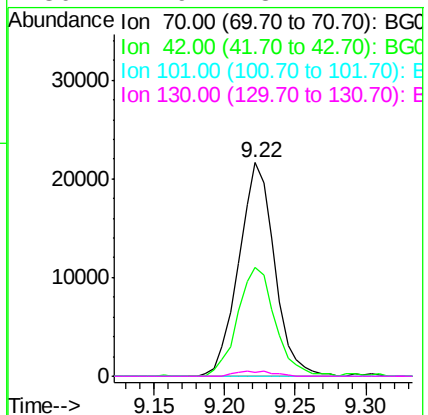

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1323

Delta R.T. -0.02 min

Lab File: BG040334.D

Acq: 3 Apr 2019 20:26

Tgt Ion: 136 Resp: 240352


Ion Ratio Lower Upper


136 100

137 10.7 8.9 13.3

54 10.0 9.6 14.4

68 5.4 5.1 7.7




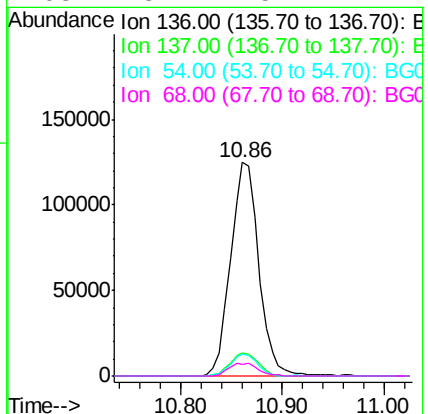




#23
Nitrobenzene-d5
Concen: 68.351 ng
RT: 9.22 min Scan# 1044
Delta R.T. -0.02 min
Lab File: BG040334.D
Acq: 3 Apr 2019 20:26




Instrument :
BNA_G
ClientSampleId :


Tot Ion: 82 Resp: 309074
Ion Ratio Lower Upper
82 100
128 43.9 35.8 53.8
54 53.8 46.2 69.2

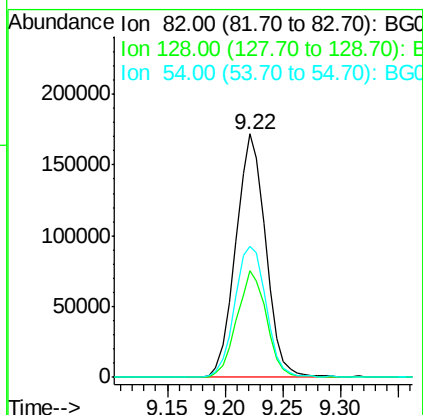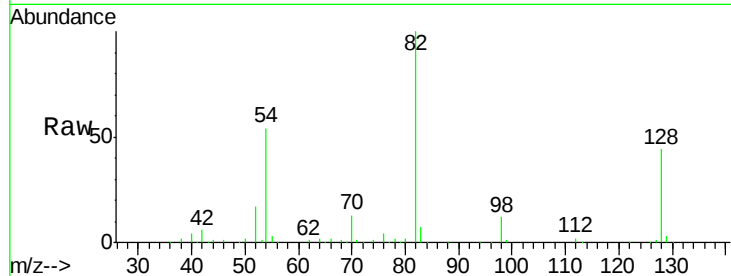

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.68 min Scan# 1973
Delta R.T. -0.02 min
Lab File: BG040334.D
Acq: 3 Apr 2019 20:26

Tgt Ion:164 Resp: 150996
Ion Ratio Lower Upper
164 100
162 96.3 77.4 116.2
160 42.3 35.3 52.9

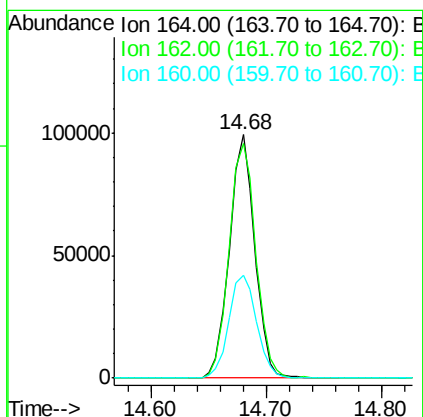

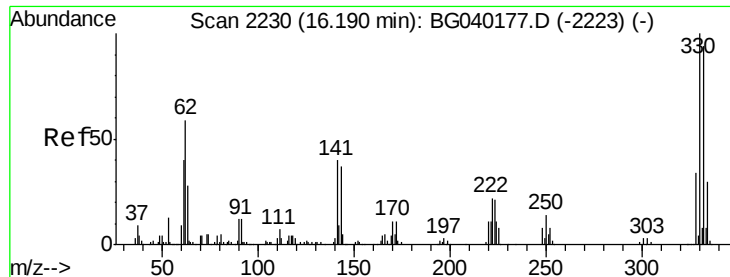

#42

2,4,6-Tribromophenol

Concen: 116.112 ng

RT: 16.17 min Scan# 2227

Delta R.T. -0.02 min

Lab File: BG040334.D

Acq: 3 Apr 2019 20:26

Instrument :

BNA_G

ClientSampleId :


Tot Ion:330 Resp: 189480

Ion Ratio Lower Upper




330 100

332 97.3 76.6 115.0

141 38.8 32.6 48.8

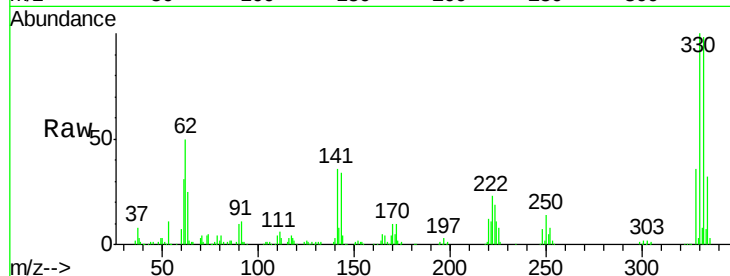

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

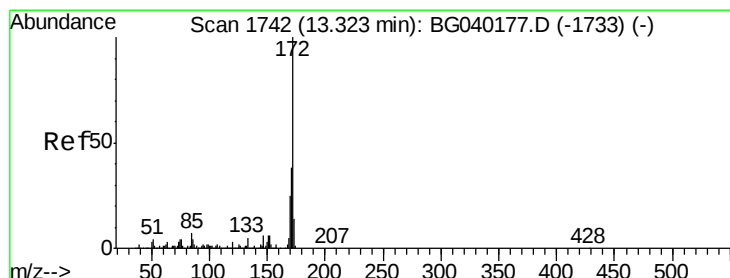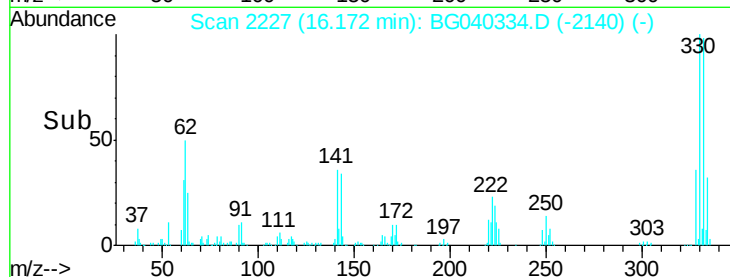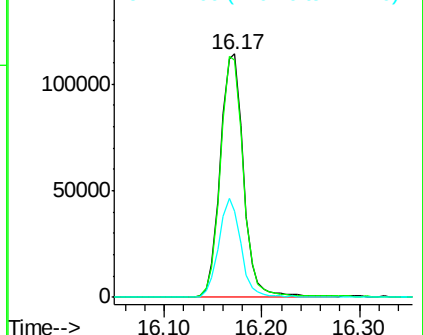

#45

2-Fluorobiphenyl

Concen: 71.376 ng

RT: 13.30 min Scan# 1738

Delta R.T. -0.02 min

Lab File: BG040334.D

Acq: 3 Apr 2019 20:26


Tgt Ion:172 Resp: 727347

Ion Ratio Lower Upper



172 100


171 37.4 30.5 45.7

170 24.6 20.1 30.1

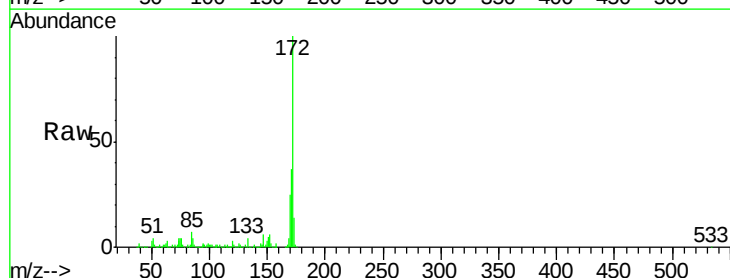

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E



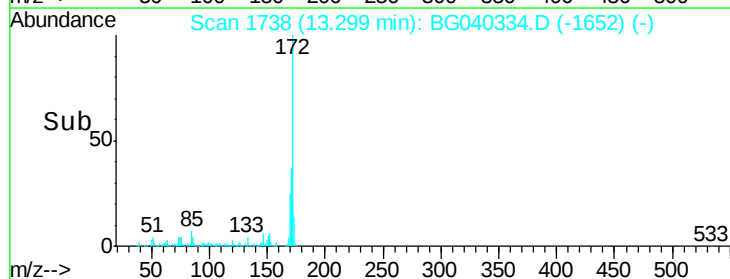
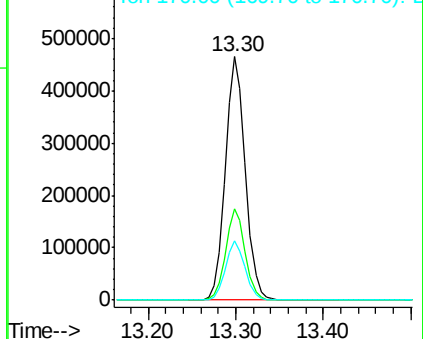




#50
Dimethylphthalate
Concen: 4.552 ng
RT: 14.13 min Scan# 1879
Delta R.T. -0.02 min
Lab File: BG040334.D
Acq: 3 Apr 2019 20:26




Instrument :
BNA_G
ClientSampleId :


Tot Ion:163 Resp: 53799
Ion Ratio Lower Upper
163 100
194 5.4 4.1 6.1
164 9.1 8.6 13.0

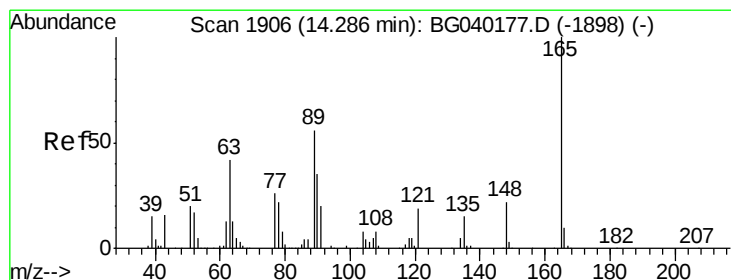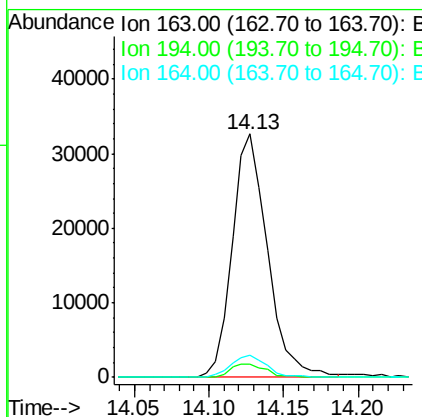

#51
2,6-Dinitrotoluene
Concen: 7.078 ng
RT: 14.68 min Scan# 1973
Delta R.T. 0.39 min
Lab File: BG040334.D
Acq: 3 Apr 2019 20:26

Tgt Ion:165 Resp: 18781
Ion Ratio Lower Upper
165 100
63 0.0 44.1 66.1#
89 1.6 44.9 67.3#

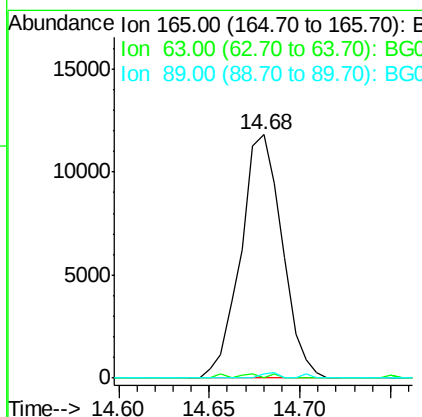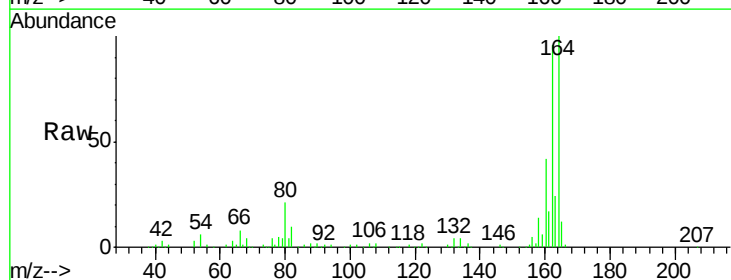




#57
 2,4-Dinitrotoluene
 Concen: 5.094 ng
 RT: 14.68 min Scan# 1973
 Delta R.T. -0.39 min
 Lab File: BG040334.D
 Acq: 3 Apr 2019 20:26

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	0.0	33.8	50.6#
89	1.6	55.4	83.2#
182	0.0	2.2	3.4#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC


Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

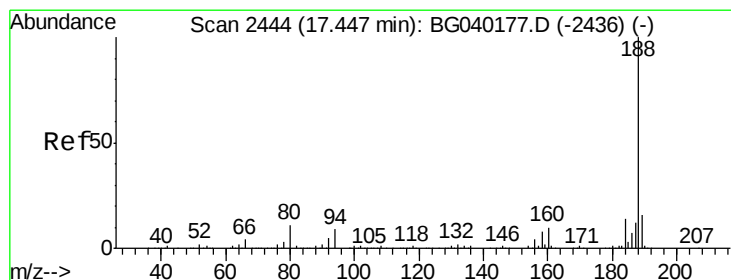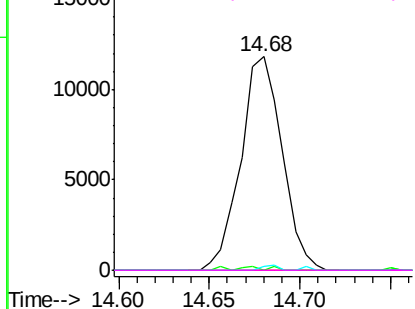

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.42 min Scan# 2440
 Delta R.T. -0.02 min
 Lab File: BG040334.D
 Acq: 3 Apr 2019 20:26



Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.7	7.0	10.4
80	10.1	8.6	13.0

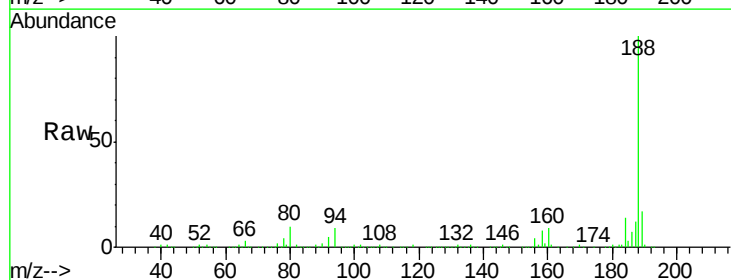


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

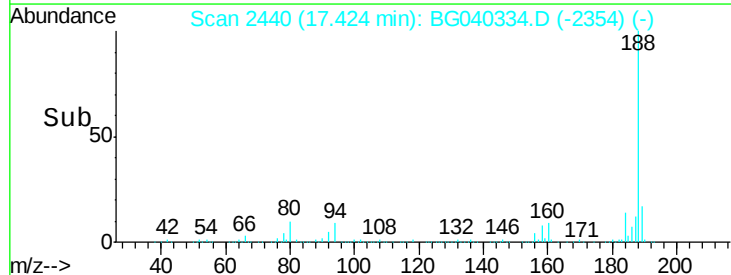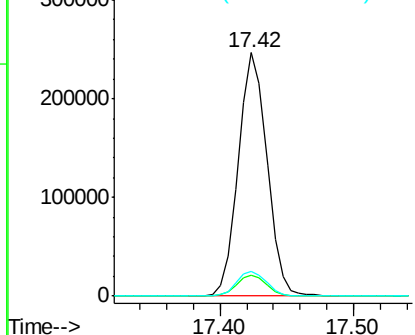







#67
4-Bromophenyl-phenylether
Concen: 3.428 ng
RT: 16.17 min Scan# 2226
Delta R.T. -0.46 min
Lab File: BG040334.D
Acq: 3 Apr 2019 20:26

Instrument :
BNA_G
ClientSampleId :

Tot Ion:248 Resp: 14204
Ion Ratio Lower Upper
248 100
250 201.3 76.4 114.6#
141 500.7 53.8 80.8#




Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

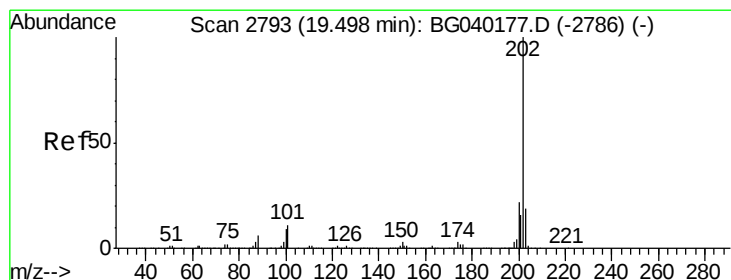
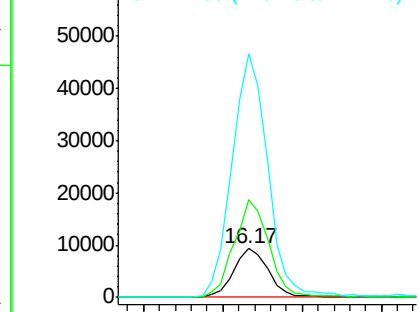



#75
Fluoranthene
Concen: 6.651 ng
RT: 19.47 min Scan# 2789
Delta R.T. -0.02 min
Lab File: BG040334.D
Acq: 3 Apr 2019 20:26

Tgt Ion:202 Resp: 152426
Ion Ratio Lower Upper
202 100
101 10.0 0.0 30.8
203 15.9 0.0 38.9

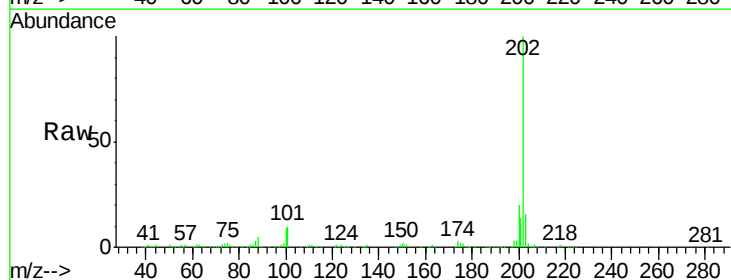

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E




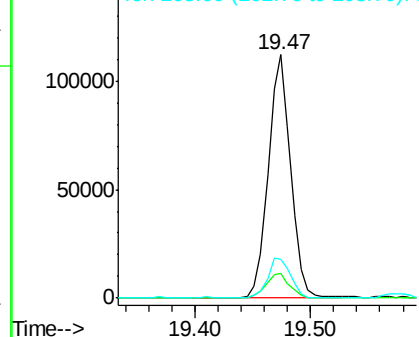




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.70 min Scan# 3167
Delta R.T. -0.04 min
Lab File: BG040334.D
Acq: 3 Apr 2019 20:26




Instrument :
BNA_G
ClientSampleId :


Tot Ion:240 Resp: 408128
Ion Ratio Lower Upper
240 100
120 10.4 8.4 12.6
236 26.5 20.8 31.2

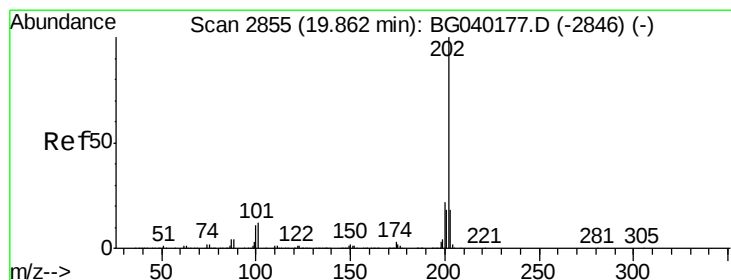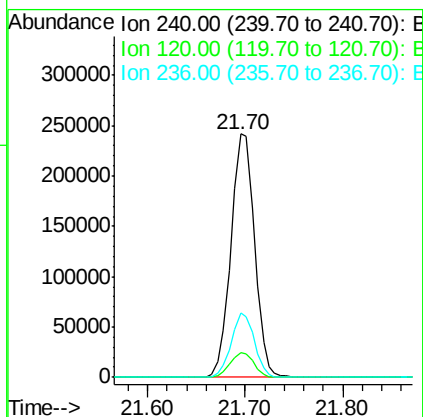

#78
Pyrene
Concen: 6.298 ng
RT: 19.83 min Scan# 2850
Delta R.T. -0.03 min
Lab File: BG040334.D
Acq: 3 Apr 2019 20:26

Tgt Ion:202 Resp: 169042
Ion Ratio Lower Upper
202 100
200 19.5 17.3 25.9
203 18.0 14.6 22.0

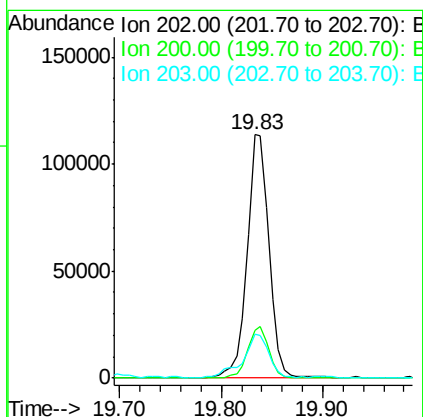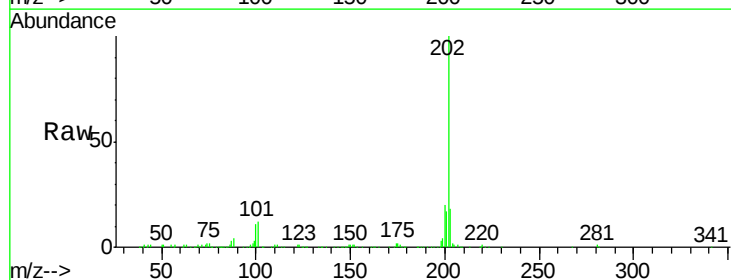



#79

Terphenyl-d14

Concen: 65.167 ng

RT: 20.03 min Scan# 2883

Delta R.T. -0.02 min

Lab File: BG040334.D

Acq: 3 Apr 2019 20:26





Instrument :

BNA_G

ClientSampled :

Tot Ion:244 Resp: 1182257

Ion	Ratio	Lower	Upper
244	100		
212	8.6	7.0	10.6
122	11.0	8.5	12.7

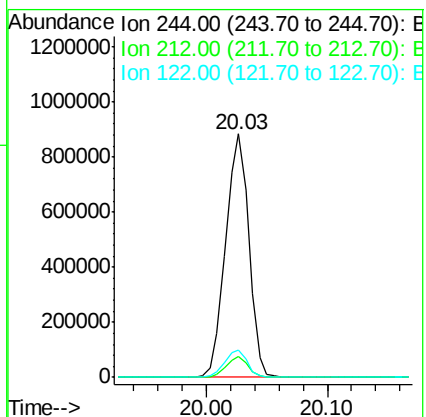

#81

Benzo(a)anthracene

Concen: 2.826 ng

RT: 21.68 min Scan# 3164




Delta R.T. -0.03 min


Lab File: BG040334.D

Acq: 3 Apr 2019 20:26

Tgt Ion:228 Resp: 71041

Ion	Ratio	Lower	Upper
228	100		
226	27.2	22.6	34.0
229	18.4	16.1	24.1




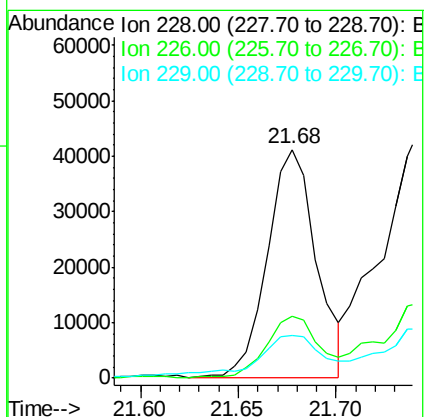




#83
Chrysene
Concen: 3.997 ng
RT: 21.74 min Scan# 3175
Delta R.T. -0.04 min
Lab File: BG040334.D
Acq: 3 Apr 2019 20:26




Instrument :
BNA_G
ClientSampled :


Tot Ion:228 Resp: 96569
Ion Ratio Lower Upper
228 100
226 30.8 25.4 38.0
229 20.3 17.0 25.4

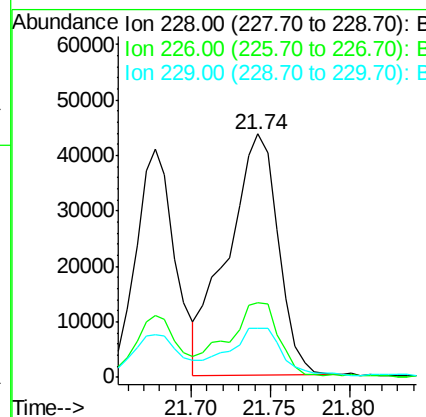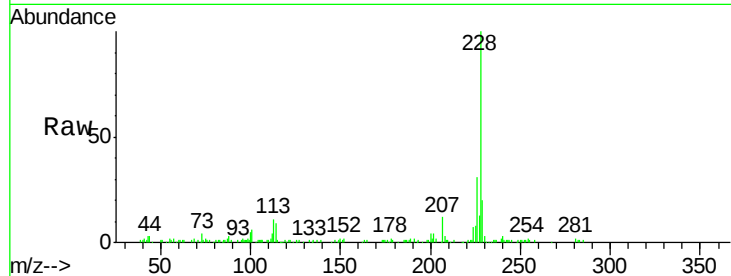

#87
Perylene-d12
Concen: 20.000 ng
RT: 24.98 min Scan# 3726
Delta R.T. -0.05 min
Lab File: BG040334.D
Acq: 3 Apr 2019 20:26

Tgt Ion:264 Resp: 418534
Ion Ratio Lower Upper
264 100
260 23.5 17.9 26.9
265 22.1 16.8 25.2



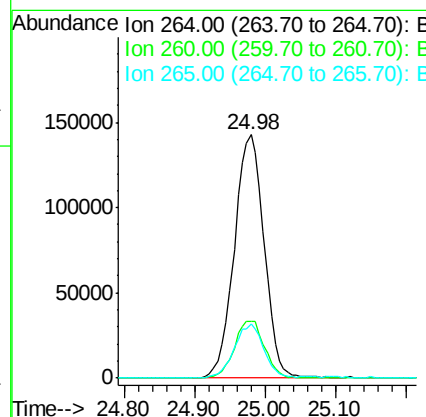
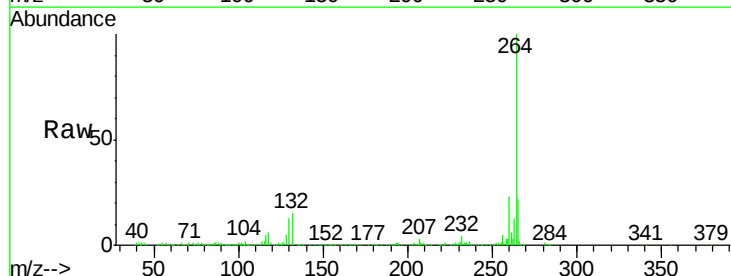


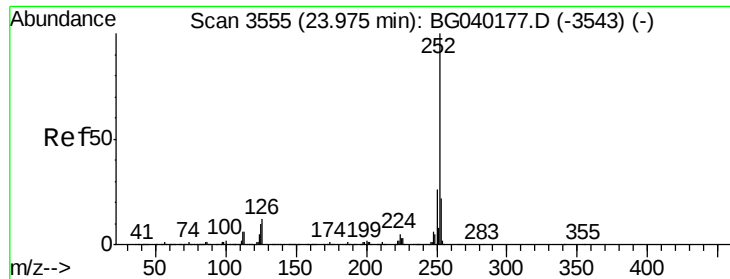

#88
Benzo(b)fluoranthene
Concen: 5.487 ng
RT: 23.92 min Scan# 3546
Delta R.T. -0.05 min
Lab File: BG040334.D
Acq: 3 Apr 2019 20:26




Instrument :
BNA_G
ClientSampleId :




Tot Ion	Ratio	Lower	Upper
252	100		
253	22.1	17.6	26.4
125	10.1	8.2	12.4

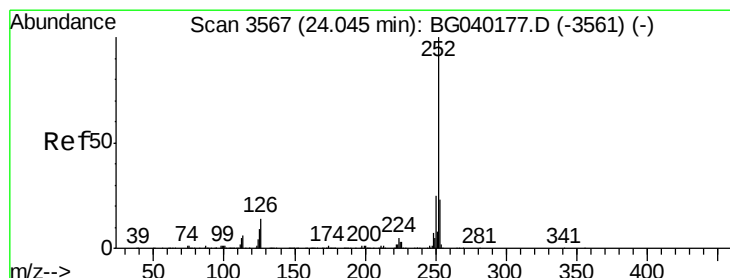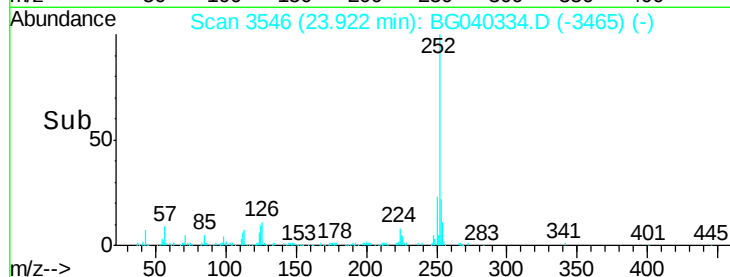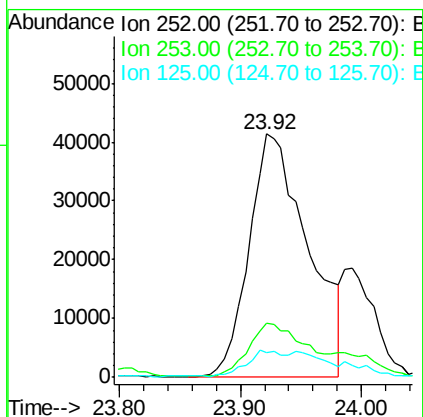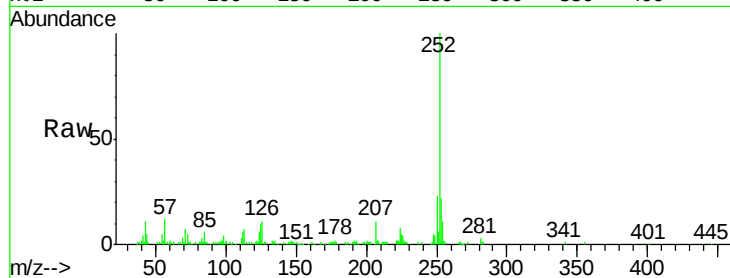

#89
Benzo(k)fluoranthene
Concen: 5.967 ng
RT: 23.92 min Scan# 3546
Delta R.T. -0.12 min
Lab File: BG040334.D
Acq: 3 Apr 2019 20:26

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.1	18.6	28.0
125	10.1	7.3	10.9

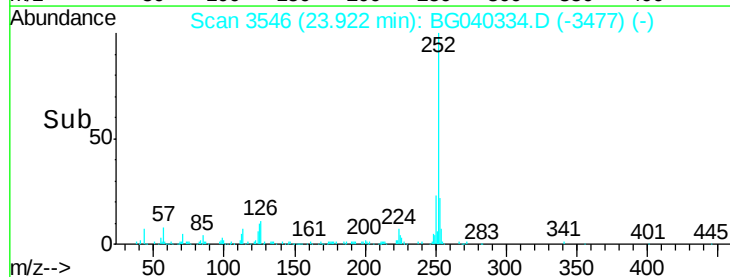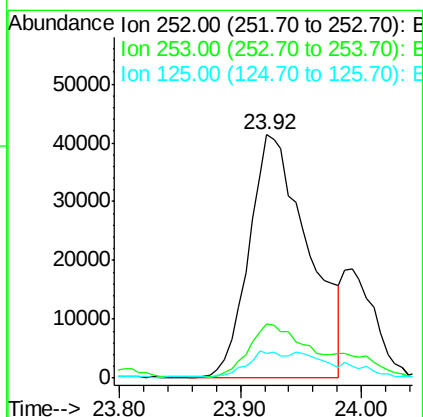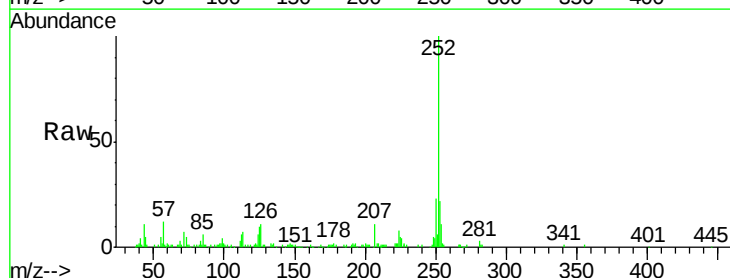



#90

Benzo(a)pyrene

Concen: 2.479 ng

RT: 24.66 min Scan# 3672

Delta R.T. -0.21 min

Lab File: BG040334.D

Acq: 3 Apr 2019 20:26

Instrument :

BNA_G

ClientSampleId :

Tot Ion: 252 Resp: 59591

Ion Ratio Lower Upper

252 100

253 21.9 17.8 26.8

125 11.5 8.3 12.5

