

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040319\
 Data File : BG040348.D
 Acq On : 4 Apr 2019 6:35
 Operator : JU/SJ
 Sample : PB118527BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB118527BL

Quant Time: Apr 04 08:30:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 28 05:47:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	57730	20.00	ng	-0.03
21) Naphthalene-d8	10.86	136	225445	20.00	ng	-0.02
39) Acenaphthene-d10	14.68	164	137761	20.00	ng	-0.03
64) Phenanthrene-d10	17.42	188	342617	20.00	ng	-0.03
76) Chrysene-d12	21.69	240	385537	20.00	ng	-0.04
87) Perylene-d12	24.98	264	394442	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	257512	74.15	ng	-0.01
7) Phenol-d6	7.20	99	341021	71.06	ng	-0.02
23) Nitrobenzene-d5	9.22	82	304621	71.82	ng	-0.02
42) 2,4,6-Tribromophenol	16.17	330	118325	79.47	ng	-0.02
45) 2-Fluorobiphenyl	13.30	172	706293	75.97	ng	-0.03
79) Terphenyl-d14	20.02	244	1066272	62.22	ng	-0.03


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040319\
Data File : BG040348.D
Acq On : 4 Apr 2019 6:35
Operator : JU/SJ
Sample : PB118527BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB118527BL

Quant Time: Apr 04 08:30:25 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 28 05:47:00 2019
Response via : Initial Calibration

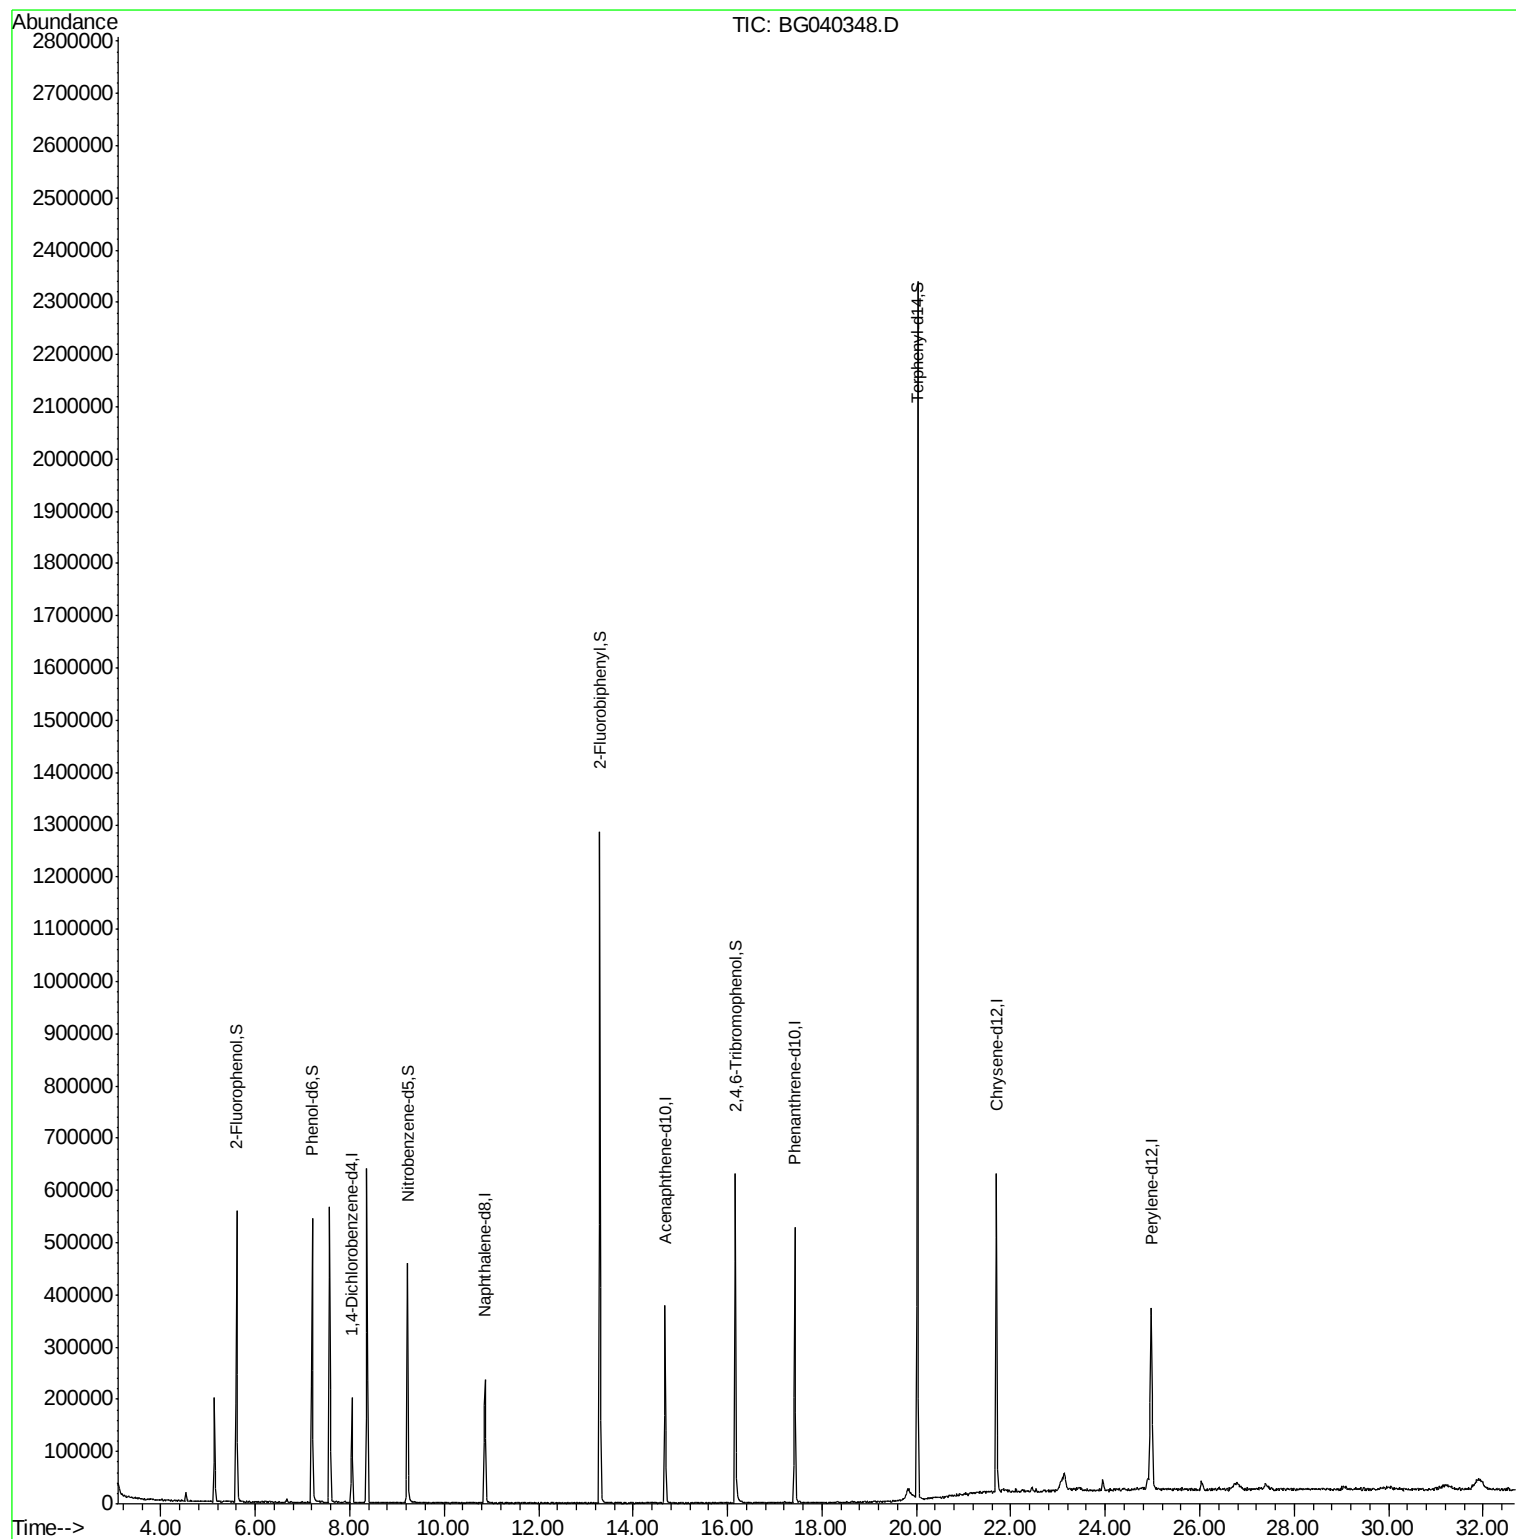




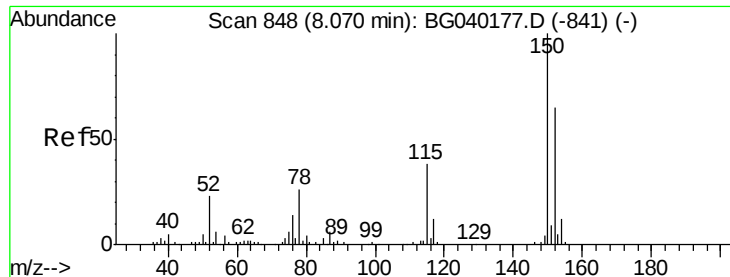


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.04 min Scan# 843
Delta R.T. -0.03 min
Lab File: BG040348.D
Acq: 4 Apr 2019 6:35

Instrument :
BNA_G
ClientSampleId :
PB118527BL




Tgt Ion:152 Resp: 57730
Ion Ratio Lower Upper
152 100
150 159.0 123.7 185.5
115 62.4 46.9 70.3

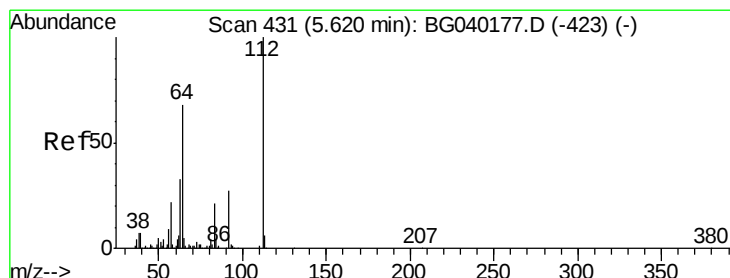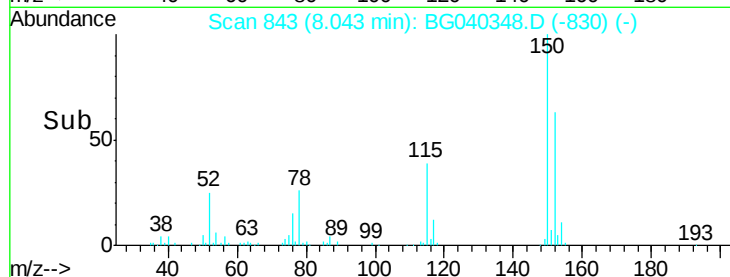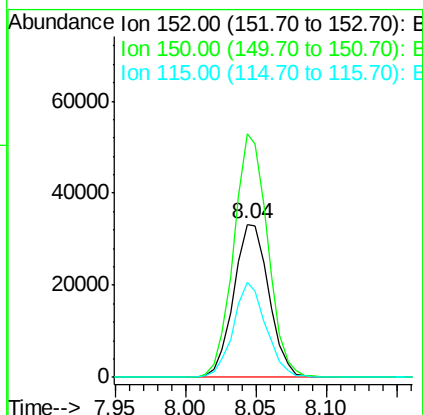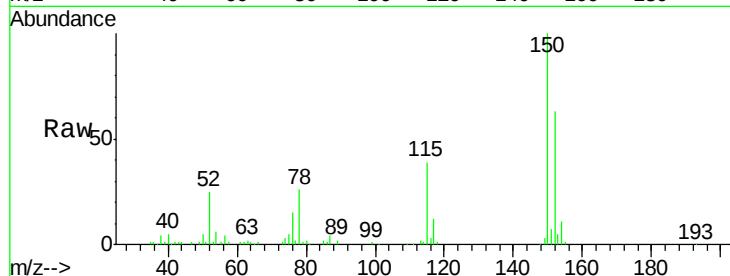


#5

2-Fluorophenol
Concen: 74.154 ng
RT: 5.61 min Scan# 428
Delta R.T. -0.01 min
Lab File: BG040348.D
Acq: 4 Apr 2019 6:35

Tgt Ion:112 Resp: 257512
Ion Ratio Lower Upper
112 100
64 65.1 54.2 81.2
63 32.7 26.4 39.6

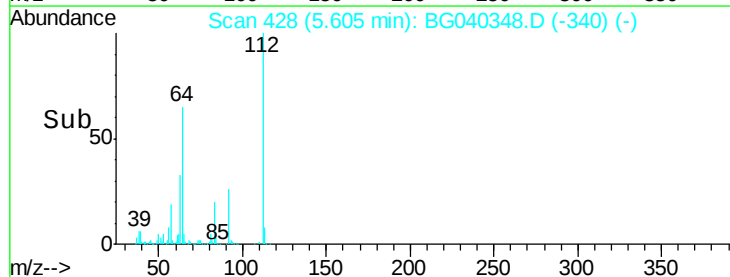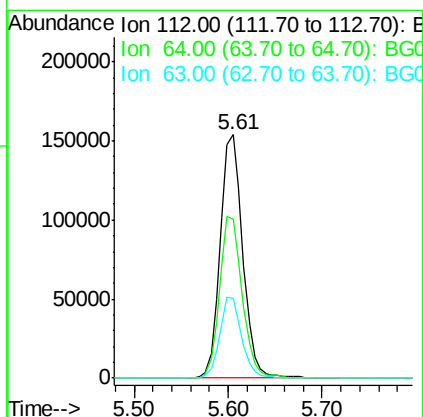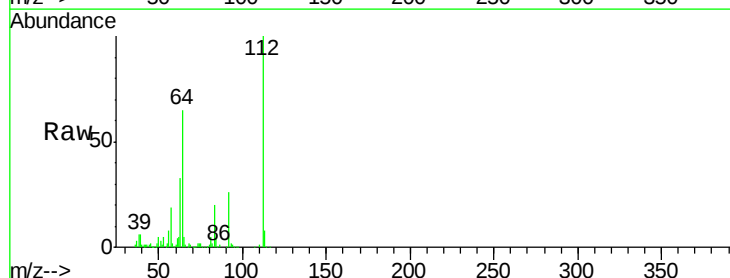

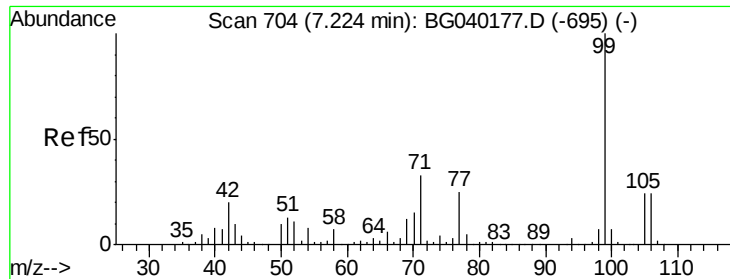

#7

Phenol-d6

Concen: 71.057 ng

RT: 7.20 min Scan# 700

Delta R.T. -0.02 min

Lab File: BG040348.D

Acq: 4 Apr 2019 6:35

Instrument :

BNA_G

ClientSampleId :

PB118527BL


Tgt Ion: 99 Resp: 341021

Ion Ratio Lower Upper




99 100

42 20.2 16.2 24.2

71 32.0 26.8 40.2

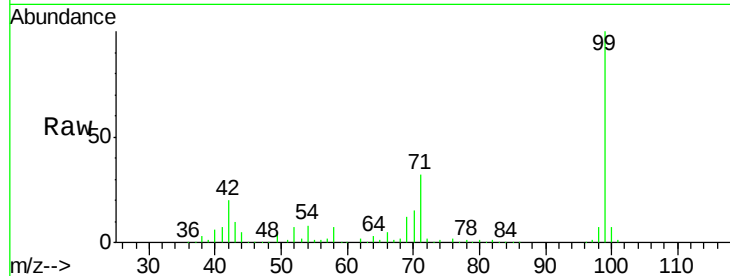

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

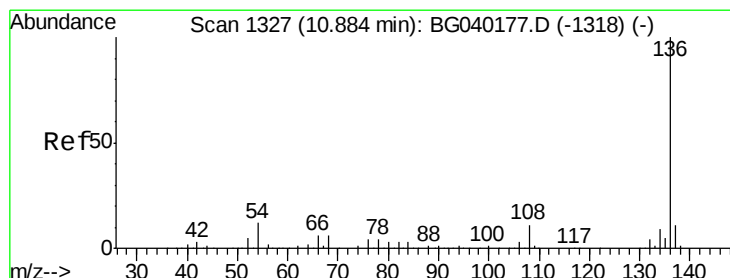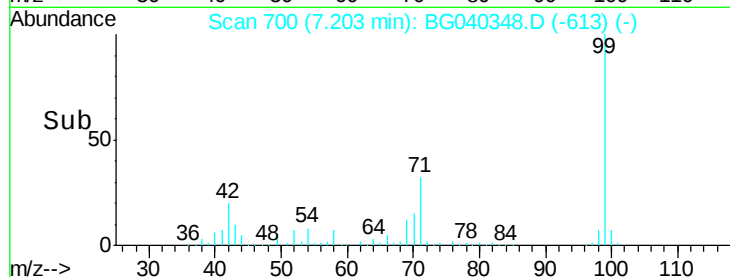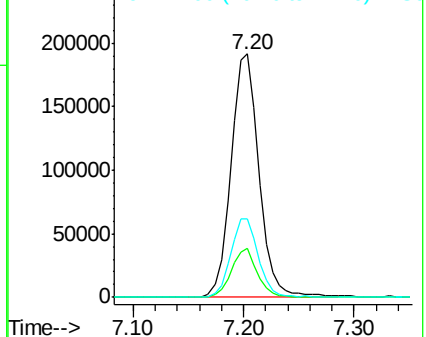

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1323

Delta R.T. -0.02 min

Lab File: BG040348.D

Acq: 4 Apr 2019 6:35

Tgt Ion: 136 Resp: 225445


Ion Ratio Lower Upper

136 100



137 11.0 8.9 13.3


54 10.2 9.6 14.4

68 6.3 5.1 7.7

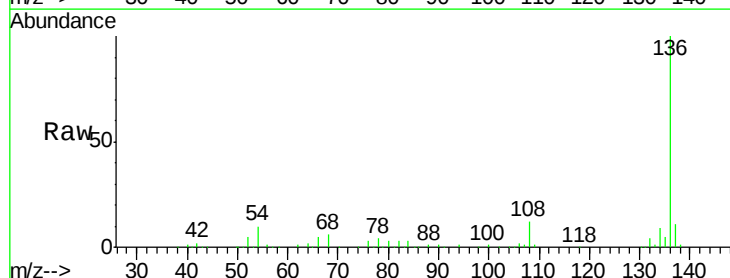

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



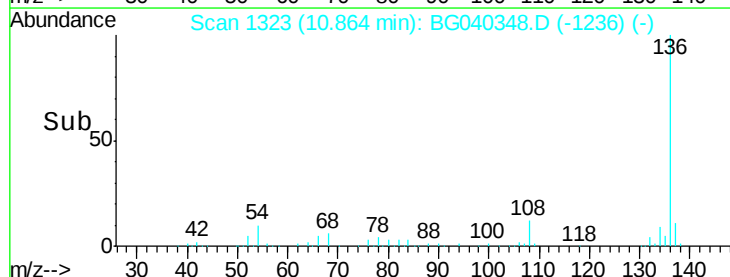
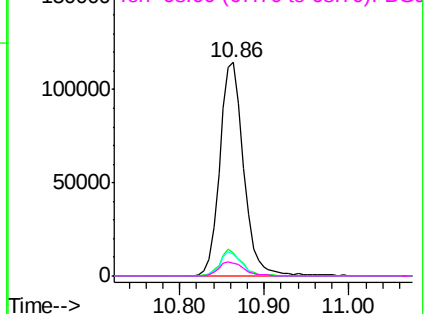


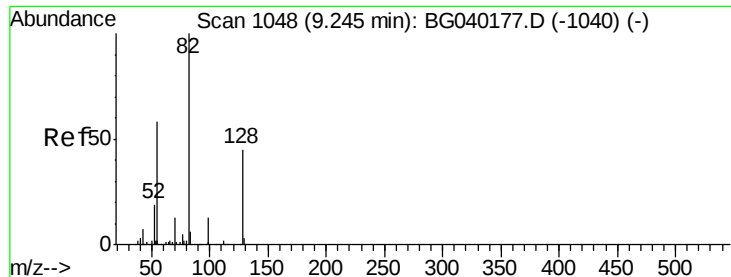

#23
 Nitrobenzene-d5
 Concen: 71.821 ng
 RT: 9.22 min Scan# 1044
 Delta R.T. -0.02 min
 Lab File: BG040348.D
 Acq: 4 Apr 2019 6:35




Instrument :
 BNA_G
 ClientSampleID :
 PB118527BL


Tgt Ion: 82 Resp: 304621
 Ion Ratio Lower Upper
 82 100
 128 44.4 35.8 53.8
 54 52.6 46.2 69.2

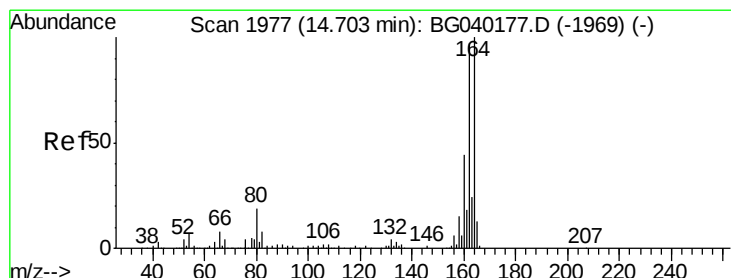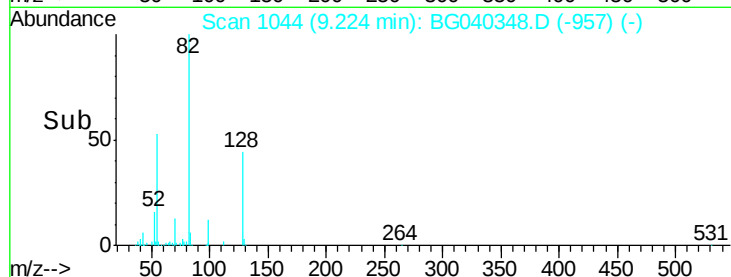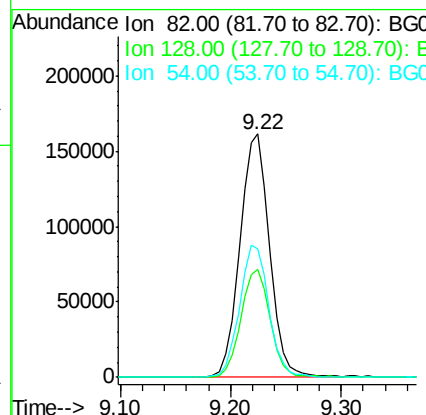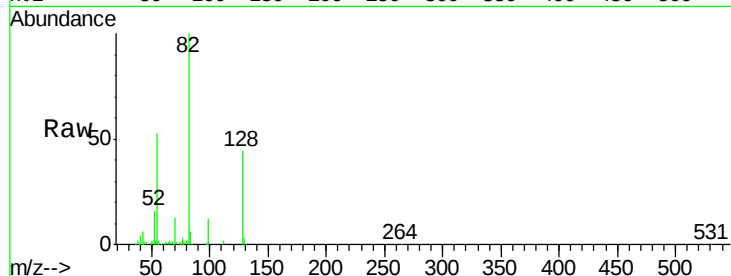

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.68 min Scan# 1972
 Delta R.T. -0.03 min
 Lab File: BG040348.D
 Acq: 4 Apr 2019 6:35

Tgt Ion: 164 Resp: 137761
 Ion Ratio Lower Upper
 164 100
 162 107.4 77.4 116.2
 160 45.3 35.3 52.9

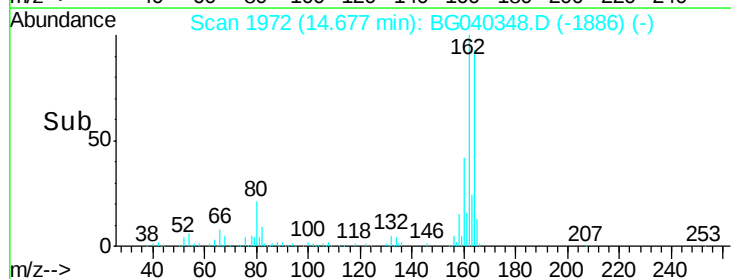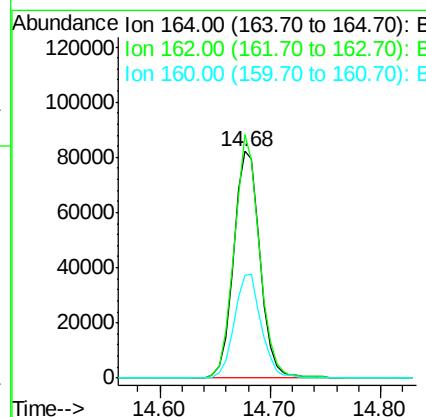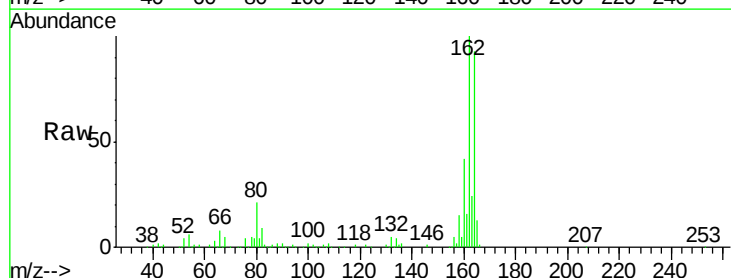


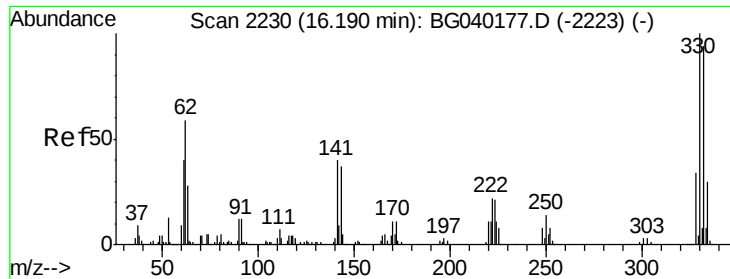

#42
 2,4,6-Tribromophenol
 Concen: 79.475 ng
 RT: 16.17 min Scan# 2226
 Delta R.T. -0.02 min
 Lab File: BG040348.D
 Acq: 4 Apr 2019 6:35

Instrument :
 BNA_G
 ClientSampleId :
 PB118527BL

Tgt Ion	Ratio	Resp	Lower	Upper
330	100	118325		
332	98.6	76.6	115.0	
141	39.1	32.6	48.8	



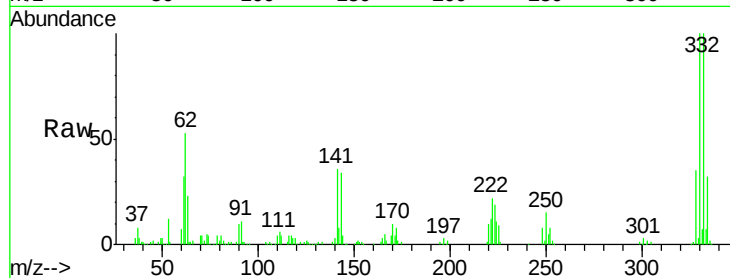


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

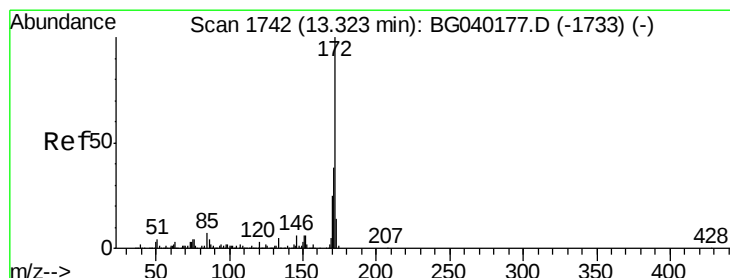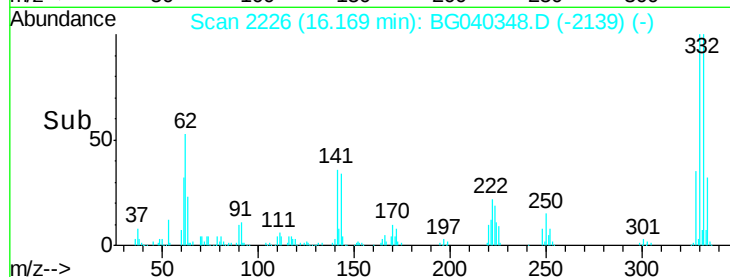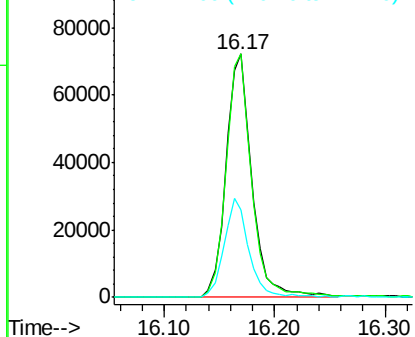

#45
 2-Fluorobiphenyl
 Concen: 75.969 ng
 RT: 13.30 min Scan# 1737
 Delta R.T. -0.03 min
 Lab File: BG040348.D
 Acq: 4 Apr 2019 6:35

Tgt Ion	Ratio	Resp	Lower	Upper
172	100	706293		
171	36.1	30.5	45.7	
170	23.7	20.1	30.1	


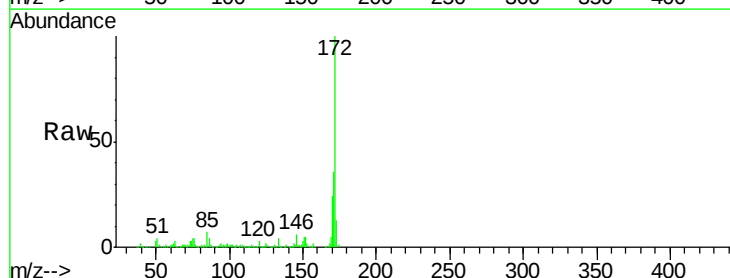



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

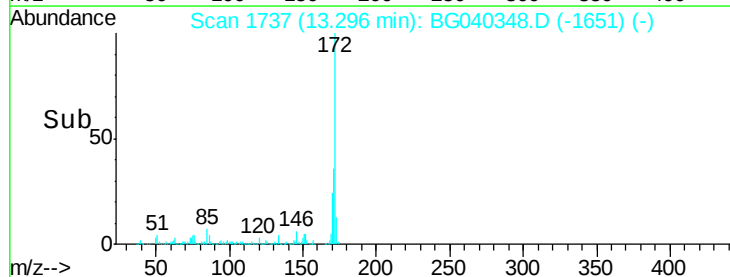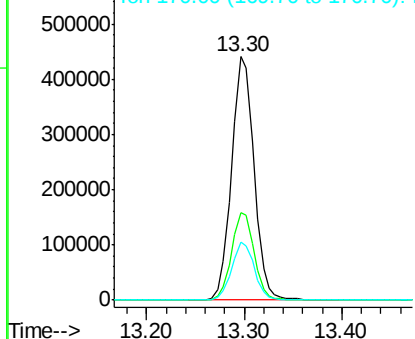

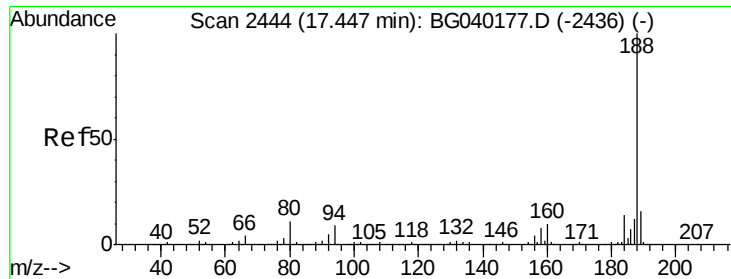

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2439

Delta R.T. -0.03 min

Lab File: BG040348.D

Acq: 4 Apr 2019 6:35

Instrument :

BNA_G

ClientSampleId :

PB118527BL


Tgt Ion:188 Resp: 342617

Ion Ratio Lower Upper

188 100

94 8.2 7.0 10.4




80 11.0 8.6 13.0

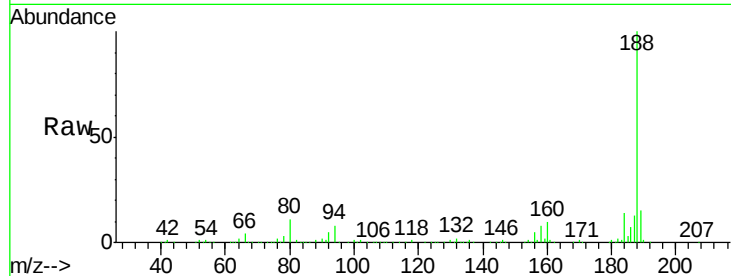

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): B

Ion 80.00 (79.70 to 80.70): B

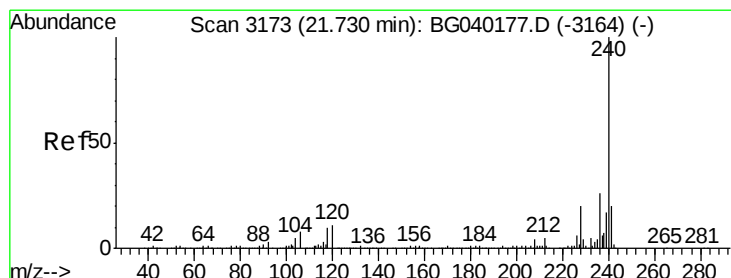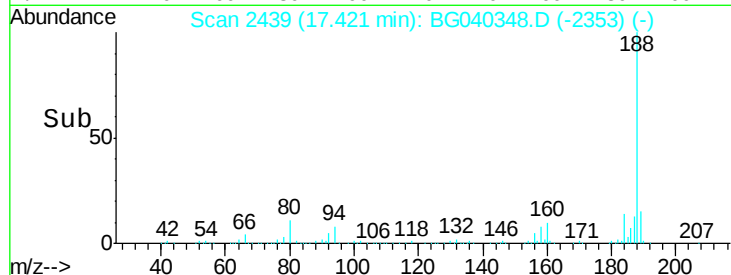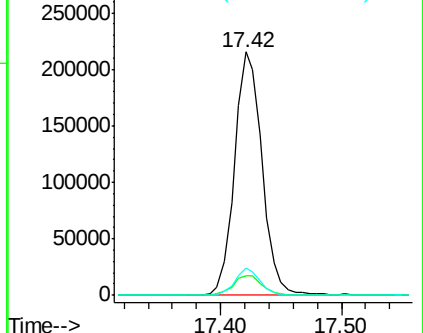

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3166

Delta R.T. -0.04 min

Lab File: BG040348.D

Acq: 4 Apr 2019 6:35


Tgt Ion:240 Resp: 385537

Ion Ratio Lower Upper

240 100

120 10.8 8.4 12.6



236 24.0 20.8 31.2

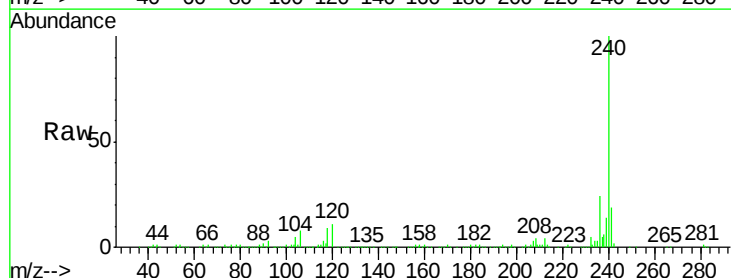


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

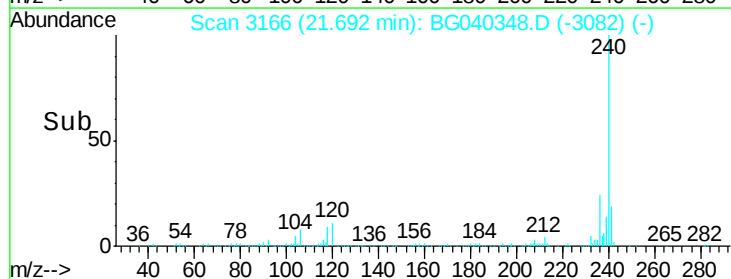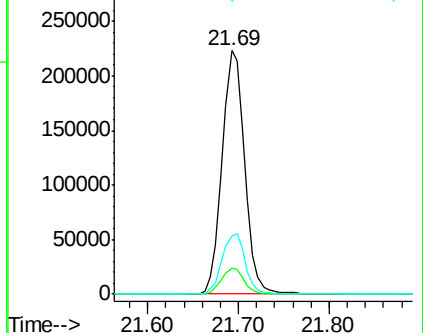

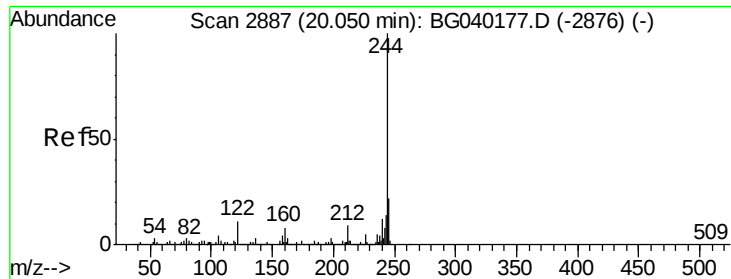

#79

Terphenyl-d14

Concen: 62.218 ng

RT: 20.02 min Scan# 2882

Delta R.T. -0.03 min

Lab File: BG040348.D

Acq: 4 Apr 2019 6:35

Instrument :

BNA_G

ClientSampleId :

PB118527BL


Tgt Ion:244 Resp: 1066272

Ion Ratio Lower Upper

244 100

212 8.3 7.0 10.6




122 11.1 8.5 12.7

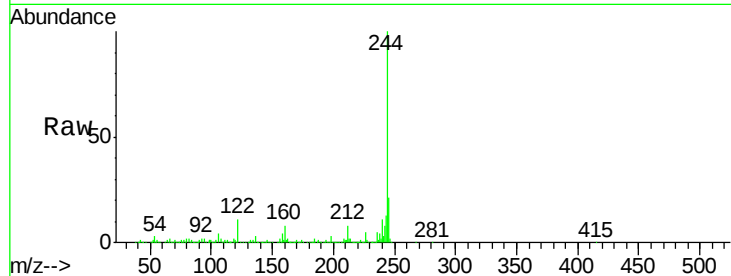

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

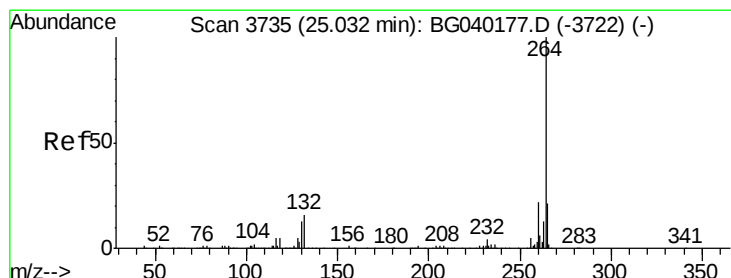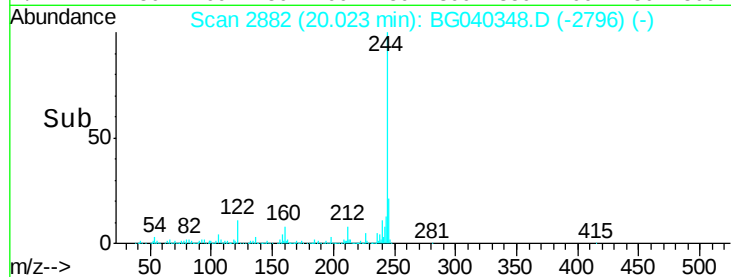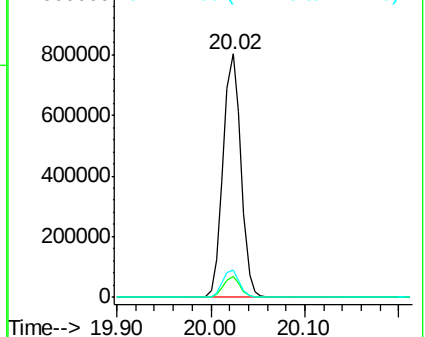

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.98 min Scan# 3725

Delta R.T. -0.06 min

Lab File: BG040348.D

Acq: 4 Apr 2019 6:35


Tgt Ion:264 Resp: 394442

Ion Ratio Lower Upper

264 100

260 22.6 17.9 26.9

265 20.1 16.8 25.2

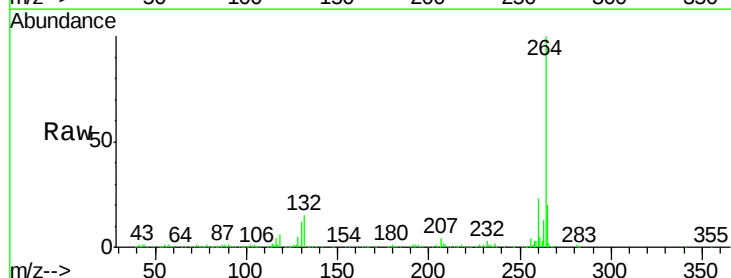

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

