

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040319\
 Data File : BG040343.D
 Acq On : 4 Apr 2019 2:33
 Operator : JU/SJ
 Sample : K2219-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CON-COMP-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.925	136	142	152	rVB	342241	513091	3.22%	1.421%
2	4.548	239	248	268	rVB	8011099	15940980	100.00%	44.144%
3	5.147	341	350	370	rVB	2252728	3645658	22.87%	10.096%
4	7.204	693	700	710	rBV	119703	214351	1.34%	0.594%
5	8.050	837	844	856	rBV	206616	374873	2.35%	1.038%
6	8.367	890	898	909	rBV	624977	1118971	7.02%	3.099%
7	8.702	947	955	964	rBV	430882	749686	4.70%	2.076%
8	9.219	1035	1043	1051	rBV	479363	893627	5.61%	2.475%
9	9.466	1077	1085	1094	rBV	96021	159708	1.00%	0.442%
10	9.777	1131	1138	1148	rBV	148685	255137	1.60%	0.707%
11	10.864	1315	1323	1333	rVB	256006	475877	2.99%	1.318%
12	13.297	1729	1737	1744	rBV	1315831	2118897	13.29%	5.868%
13	14.677	1965	1972	1981	rBV2	418828	679129	4.26%	1.881%
14	17.421	2431	2439	2446	rBV2	552980	899243	5.64%	2.490%
15	20.024	2876	2882	2889	rBV	2603723	3498526	21.95%	9.688%
16	21.293	3093	3098	3115	rBV2	112764	190818	1.20%	0.528%
17	21.693	3160	3166	3176	rBV2	707716	1143247	7.17%	3.166%
18	22.445	3289	3294	3302	rVB	135928	221044	1.39%	0.612%
19	23.138	3405	3412	3423	rBV2	184240	358081	2.25%	0.992%
20	23.949	3543	3550	3560	rBV2	210628	456470	2.86%	1.264%
21	24.901	3703	3712	3717	rBV3	174282	445128	2.79%	1.233%
22	24.971	3717	3724	3739	rVB2	382464	1112006	6.98%	3.079%
23	26.035	3895	3905	3917	rBV3	131798	409941	2.57%	1.135%
24	27.409	4128	4139	4150	rBV3	64147	236646	1.48%	0.655%


Sum of corrected areas: 36111135

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040319\
Data File : BG040343.D
Acq On : 4 Apr 2019 2:33
Operator : JU/SJ
Sample : K2219-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CON-COMP-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

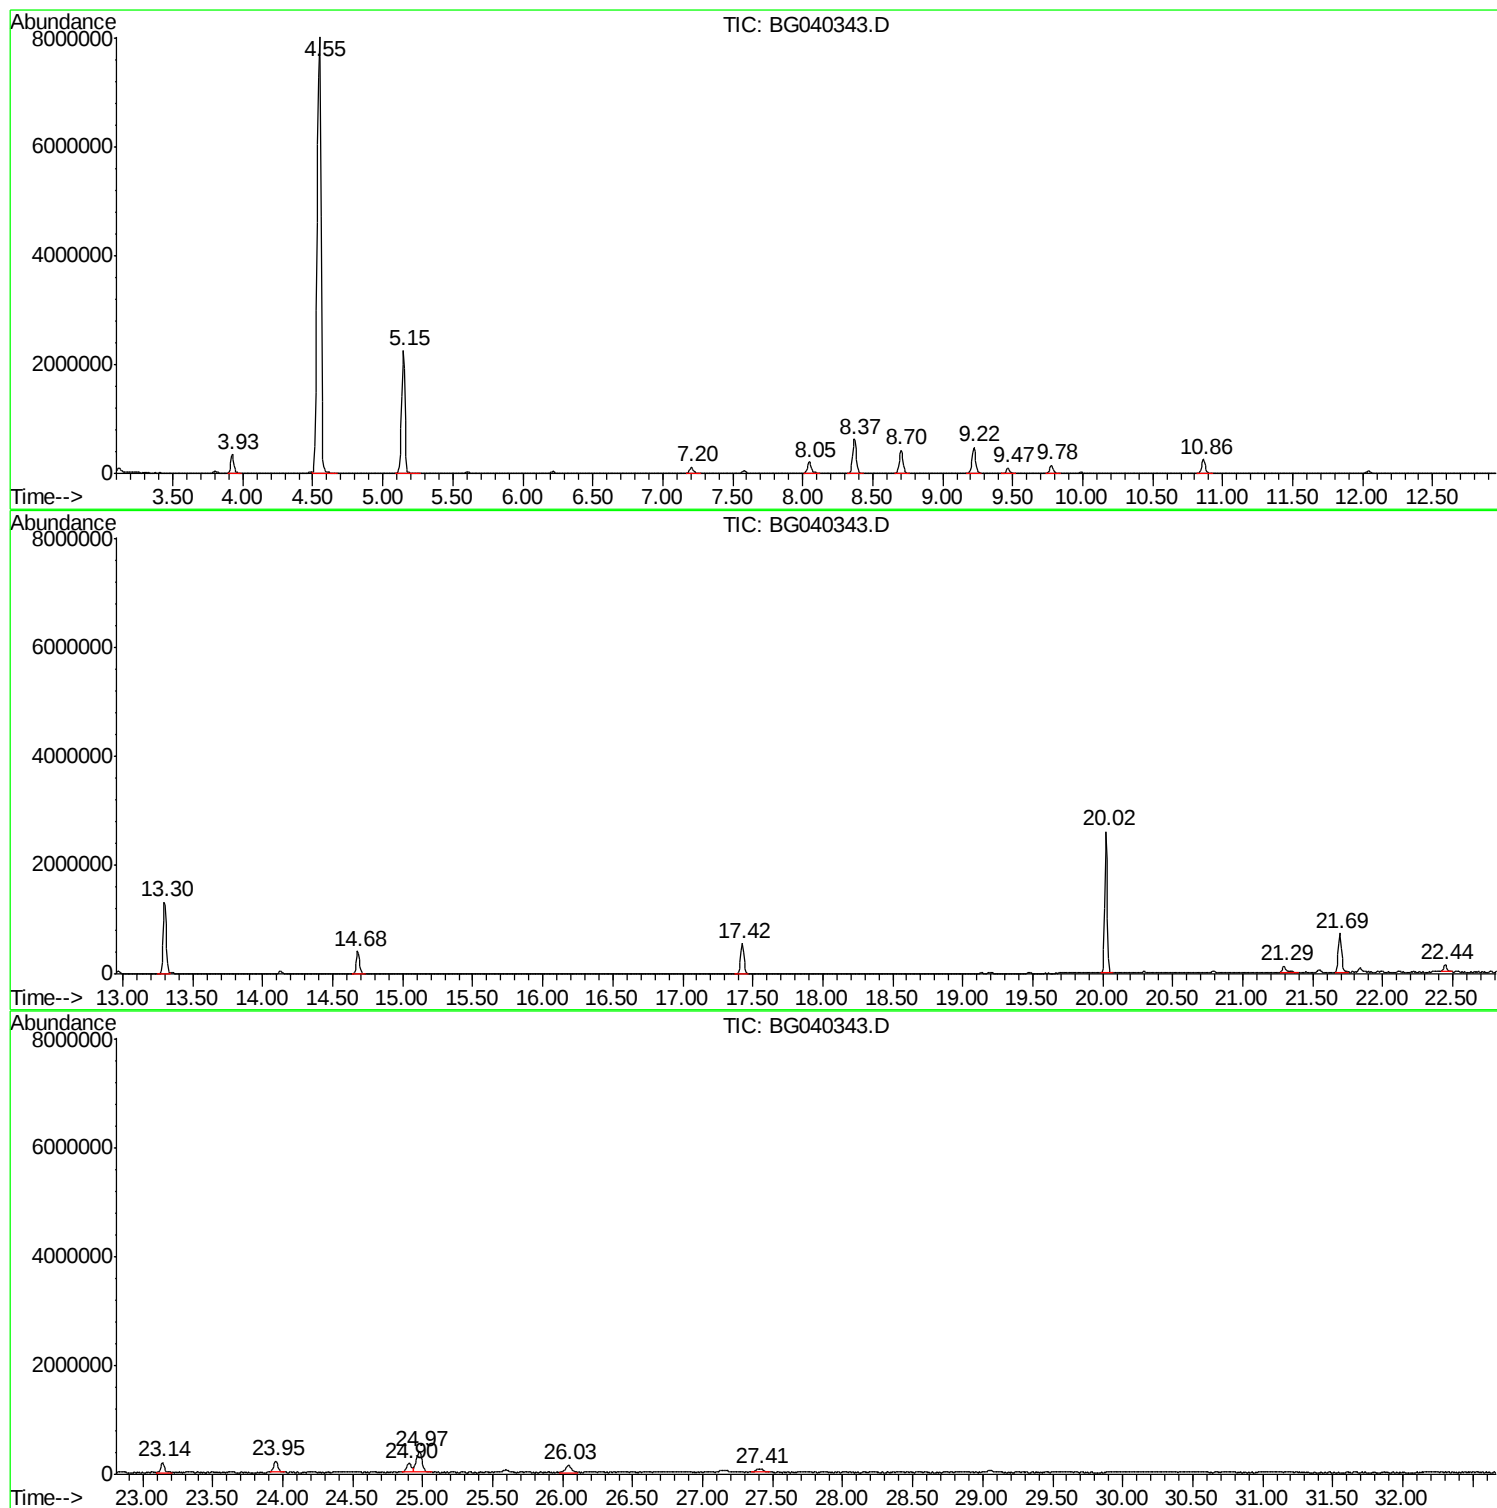

DbaaaPath::ZZ\SSV0ASRVNRPBEM1BBAAGGDATA\BB0000319\
 DbaaaFile::BB0000313DD
 AcqQ00n :: 44Apr2009 22333
 Operator::JUUSJ
 Sample::K0229008
 Misc::
 ASSVaal::199 SampleMultiplier:11

Instrument :
 BNA_G
 ClientSampleId :
 CON-COMP-2

QqaantMebbdd::ZZ\SSV0ASRVNRPBEM1BBAAGGMEH0DS82Z0BB002ZT9MM
 QqaantTitle::ASBPBNASSANDABBSF0QR55P000NTC6AIBRATION

TICLibrary::CC\DaababbaeN0\$T11LL
 TICIntegratíonParameters:LS6C0NTPP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
