


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040319\
 Data File : BG040325.D
 Acq On : 3 Apr 2019 14:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 28 05:47:00 2019

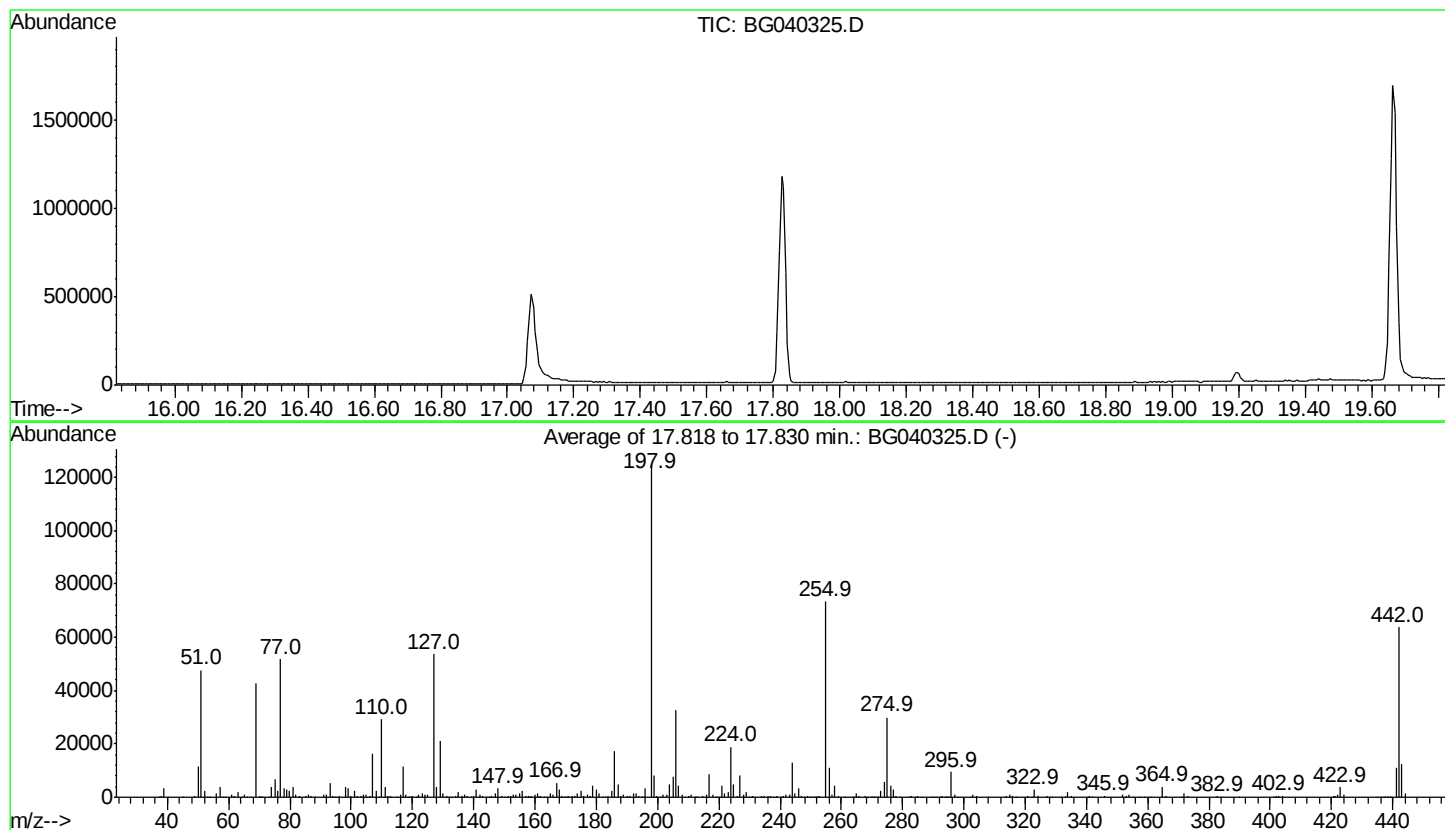

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	47570	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.3	42714	PASS
70	69	0.00	2	0.6	258	PASS
127	198	10	80	43.2	53776	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	124429	PASS
199	198	5	9	6.7	8296	PASS
275	198	10	60	24.0	29818	PASS
365	198	1	100	3.2	4034	PASS
441	198	0.01	100	8.9	11033	PASS
442	198	50	100	51.3	63786	PASS
443	442	15	24	19.5	12468	PASS