


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040319\
 Data File : BG040344.D
 Acq On : 4 Apr 2019 3:54
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 28 05:47:00 2019

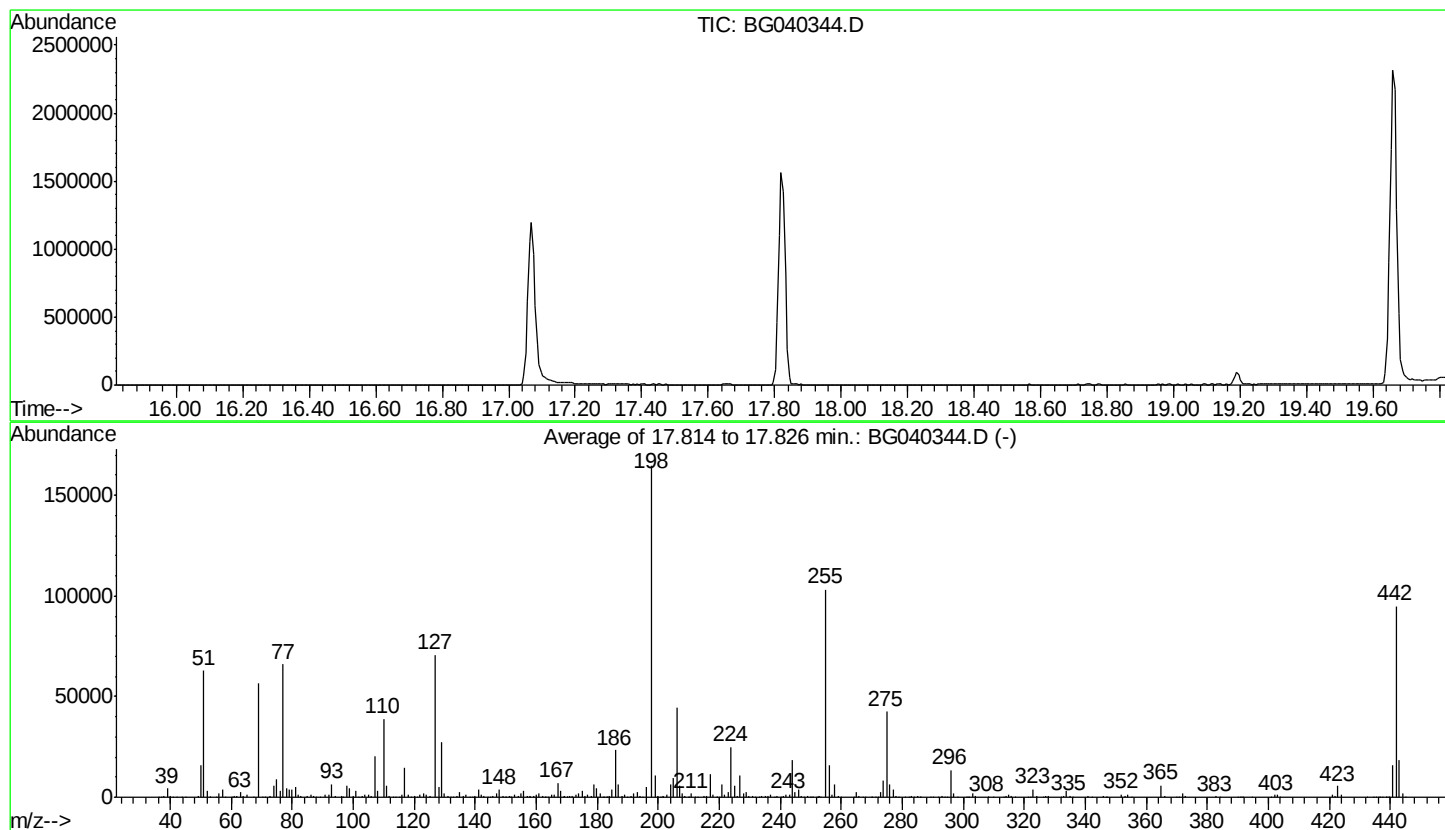

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	62914	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.3	56469	PASS
70	69	0.00	2	0.5	298	PASS
127	198	10	80	43.0	70773	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	164736	PASS
199	198	5	9	6.6	10891	PASS
275	198	10	60	25.8	42426	PASS
365	198	1	100	3.5	5732	PASS
441	198	0.01	100	9.6	15873	PASS
442	198	50	100	57.7	95064	PASS
443	442	15	24	19.5	18581	PASS