


Abundance

Ion 265.70 (265.40 to 266.40): BG060755.D\data.ms
 Ion 268.00 (267.70 to 268.70): BG060755.D\data.ms
 Ion 264.00 (263.70 to 264.70): BG060755.D\data.ms

16.985 Tailing = 1.02

S E




Time--> 15.80 16.00 16.20 16.40 16.60 16.80 17.00 17.20 17.40 17.60 17.80 18.00 18.20



Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.70
264.00	64.70	61.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040324\
Data File : BG060755.D
Acq On : 3 Apr 2024 9:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 00:47:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

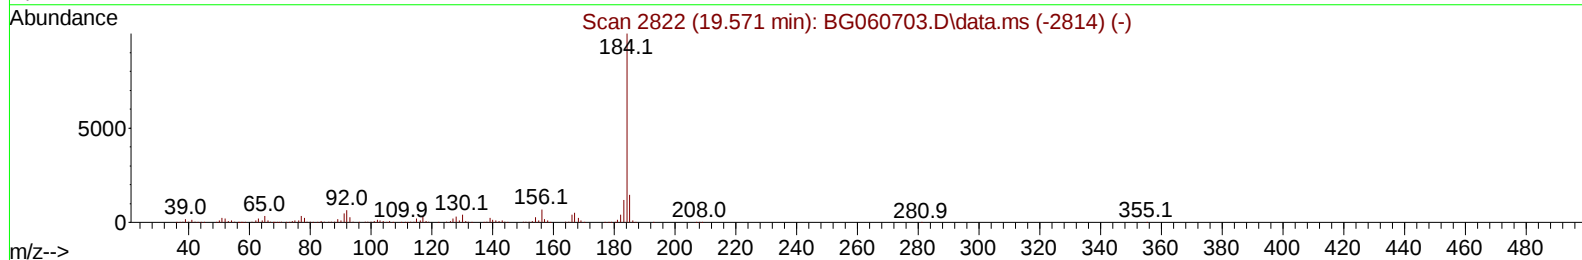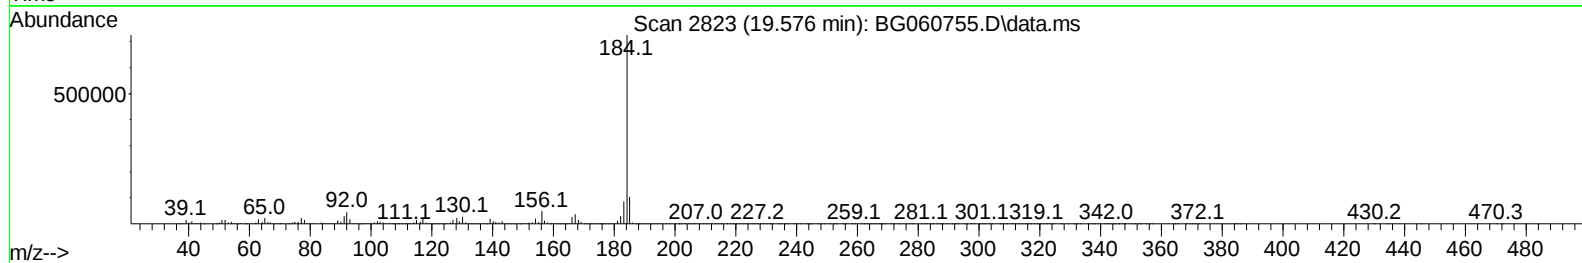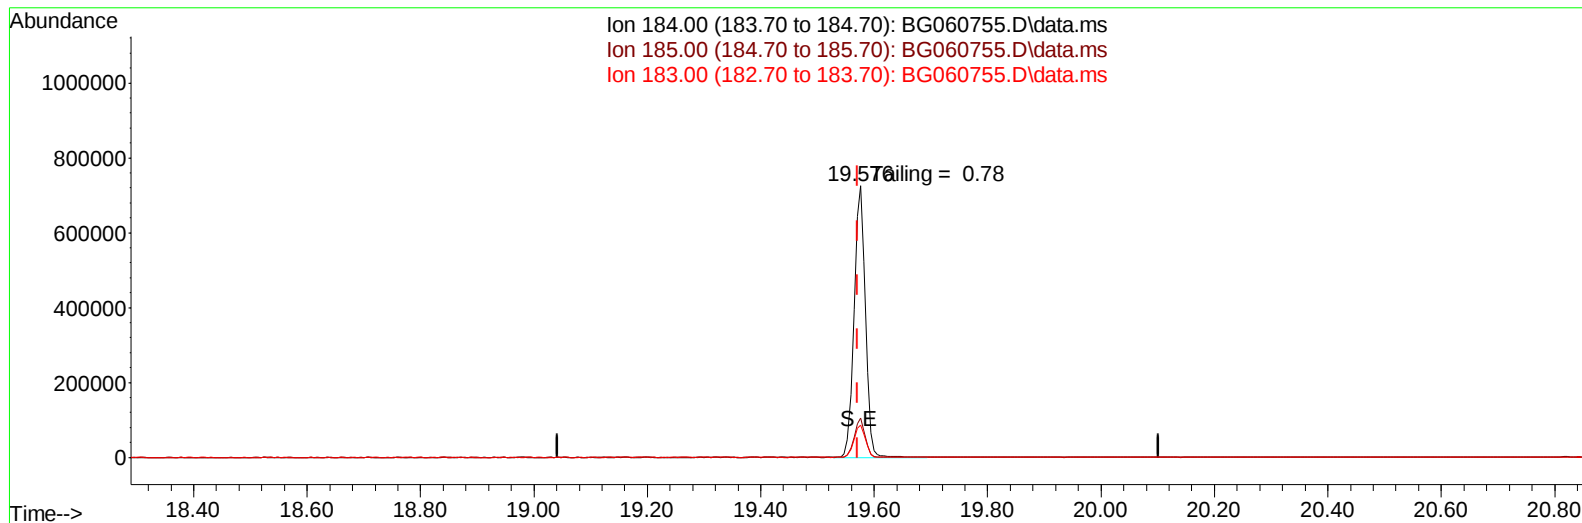

TIC: BG060755.D\data.ms

(77) Benzidine**19.576min (+ 0.005) 85429.04 ng****response 1007790**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.43
183.00	11.90	12.04
0.00	0.00	0.00