
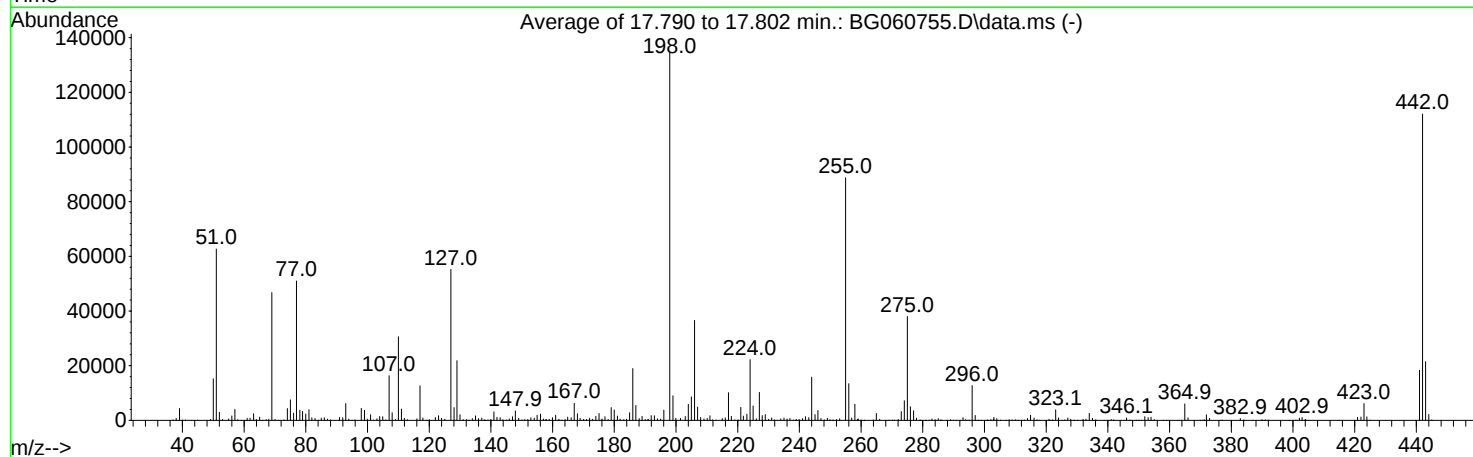


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040324\
Data File : BG060755.D
Acq On : 3 Apr 2024 9:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 30 03:12:26 2024

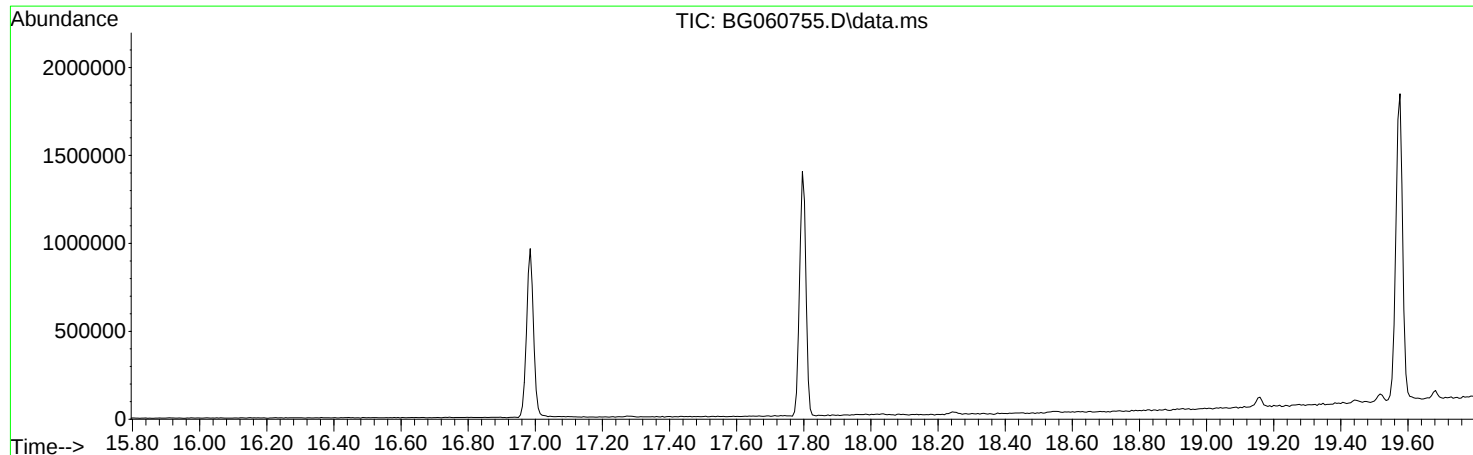




AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.6	62672	PASS
68	69	0.00	2	0.8	388	PASS
69	198	0.00	100	34.8	46789	PASS
70	69	0.00	2	0.8	370	PASS
127	198	10	80	41.0	55189	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	134579	PASS
199	198	5	9	6.7	9027	PASS
275	198	10	60	28.2	37981	PASS
365	198	1	100	4.5	6033	PASS
441	198	0.01	100	13.6	18309	PASS
442	442	50	100	100.0	112016	PASS
443	442	15	24	19.2	21519	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040324\
Data File : BG060755.D
Acq On : 3 Apr 2024 9:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 04 00:47:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

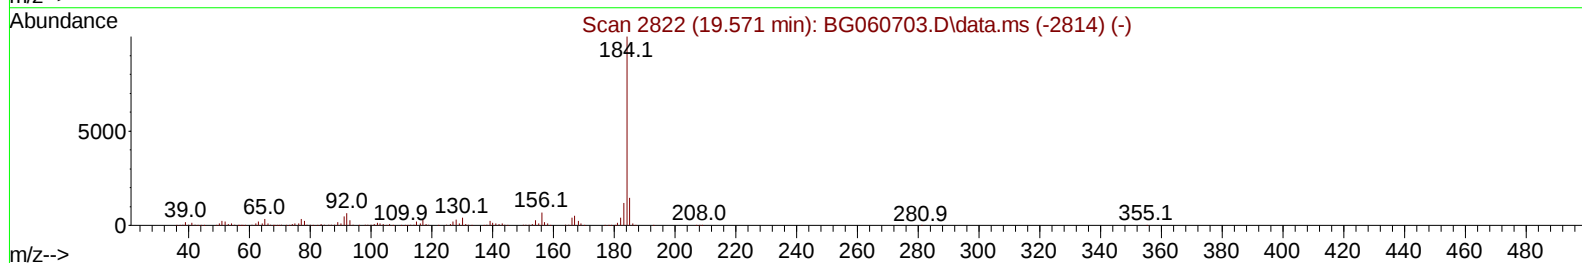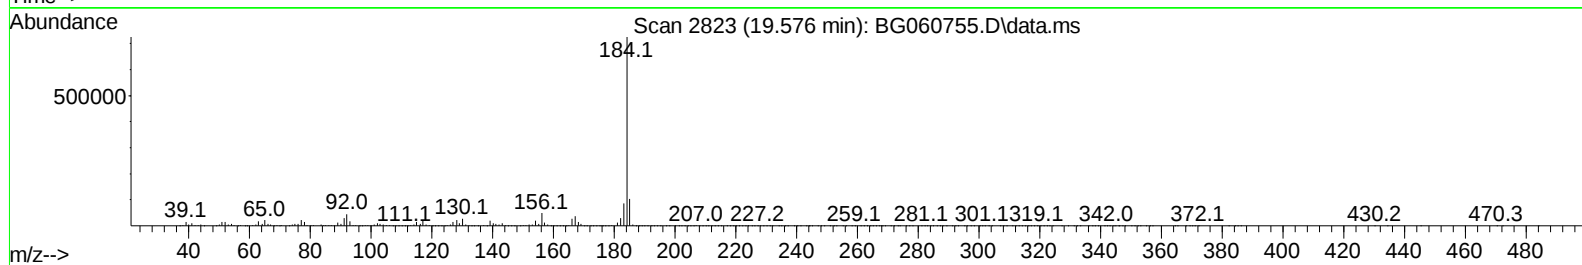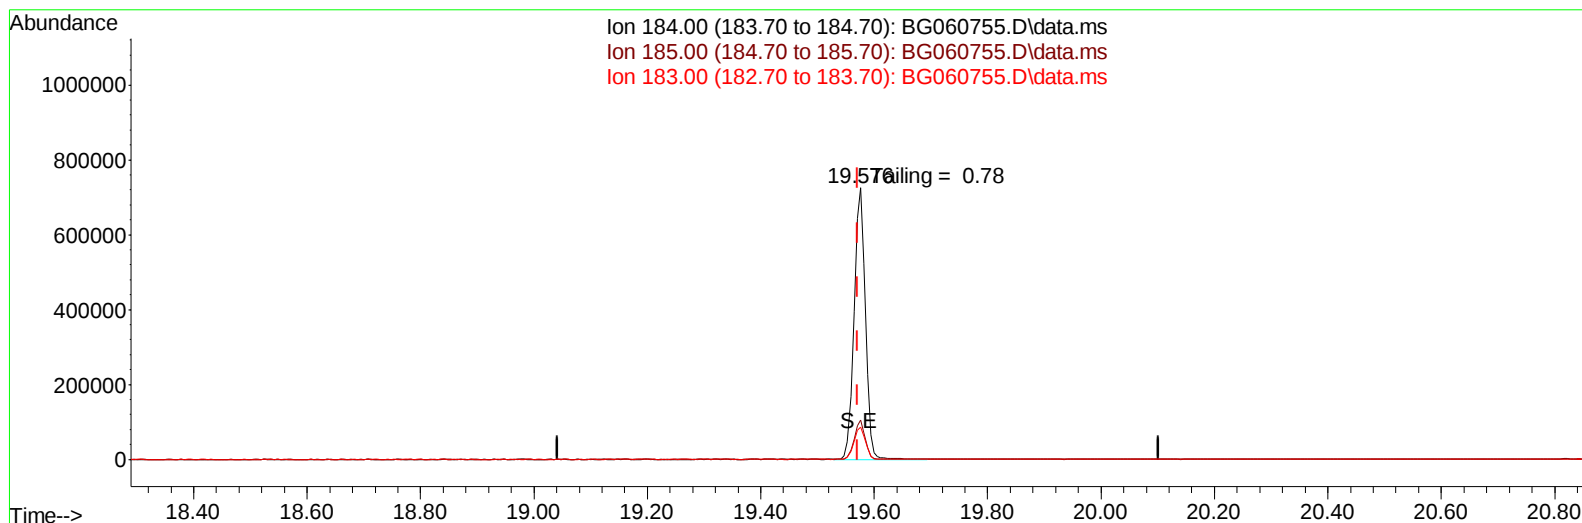

TIC: BG060755.D\data.ms

(77) Benzidine

19.576min (+ 0.005) 85429.04 ng

response 1007790

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.43
183.00	11.90	12.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/3/2024	BNA_G	<u>BG060755.D</u>
Compound Name	Response	Retention Time
DDT	507928	20.816
DDD	19111	20.375
DDE	0	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19111	527039	3.63

Instrument :
BNA_G
ClientSampleId :
DFTPP