

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG040419\
 Data File : BG040367.D
 Acq On : 4 Apr 2019 19:58
 Operator : JU/SJ
 Sample : PB118524BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Apr 05 01:21:13 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 28 05:47:00 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	59382	20.00	ng	-0.02
21) Naphthalene-d8	10.86	136	237254	20.00	ng	-0.02
39) Acenaphthene-d10	14.68	164	145868	20.00	ng	-0.02
64) Phenanthrene-d10	17.42	188	362370	20.00	ng	-0.02
76) Chrysene-d12	21.69	240	413925	20.00	ng	-0.04
87) Perylene-d12	24.97	264	418786	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	449235	125.76	ng	-0.02
7) Phenol-d6	7.21	99	615775	124.74	ng	-0.02
23) Nitrobenzene-d5	9.22	82	360637	80.80	ng	-0.02
42) 2,4,6-Tribromophenol	16.17	330	212107	134.55	ng	-0.02
45) 2-Fluorobiphenyl	13.30	172	843691	85.70	ng	-0.02
79) Terphenyl-d14	20.02	244	1386506	75.36	ng	-0.03
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.22	70	45618	12.888	ng	# 72
51) 2,6-Dinitrotoluene	14.67	165	19074	7.441	ng	# 25
57) 2,4-Dinitrotoluene	14.67	165	19074	5.355	ng	# 25
67) 4-Bromophenyl-phenylether	16.17	248	16515	4.050	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG040419\
Data File : BG040367.D
Acq On : 4 Apr 2019 19:58
Operator : JU/SJ
Sample : PB118524BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Apr 05 01:21:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 28 05:47:00 2019
Response via : Initial Calibration

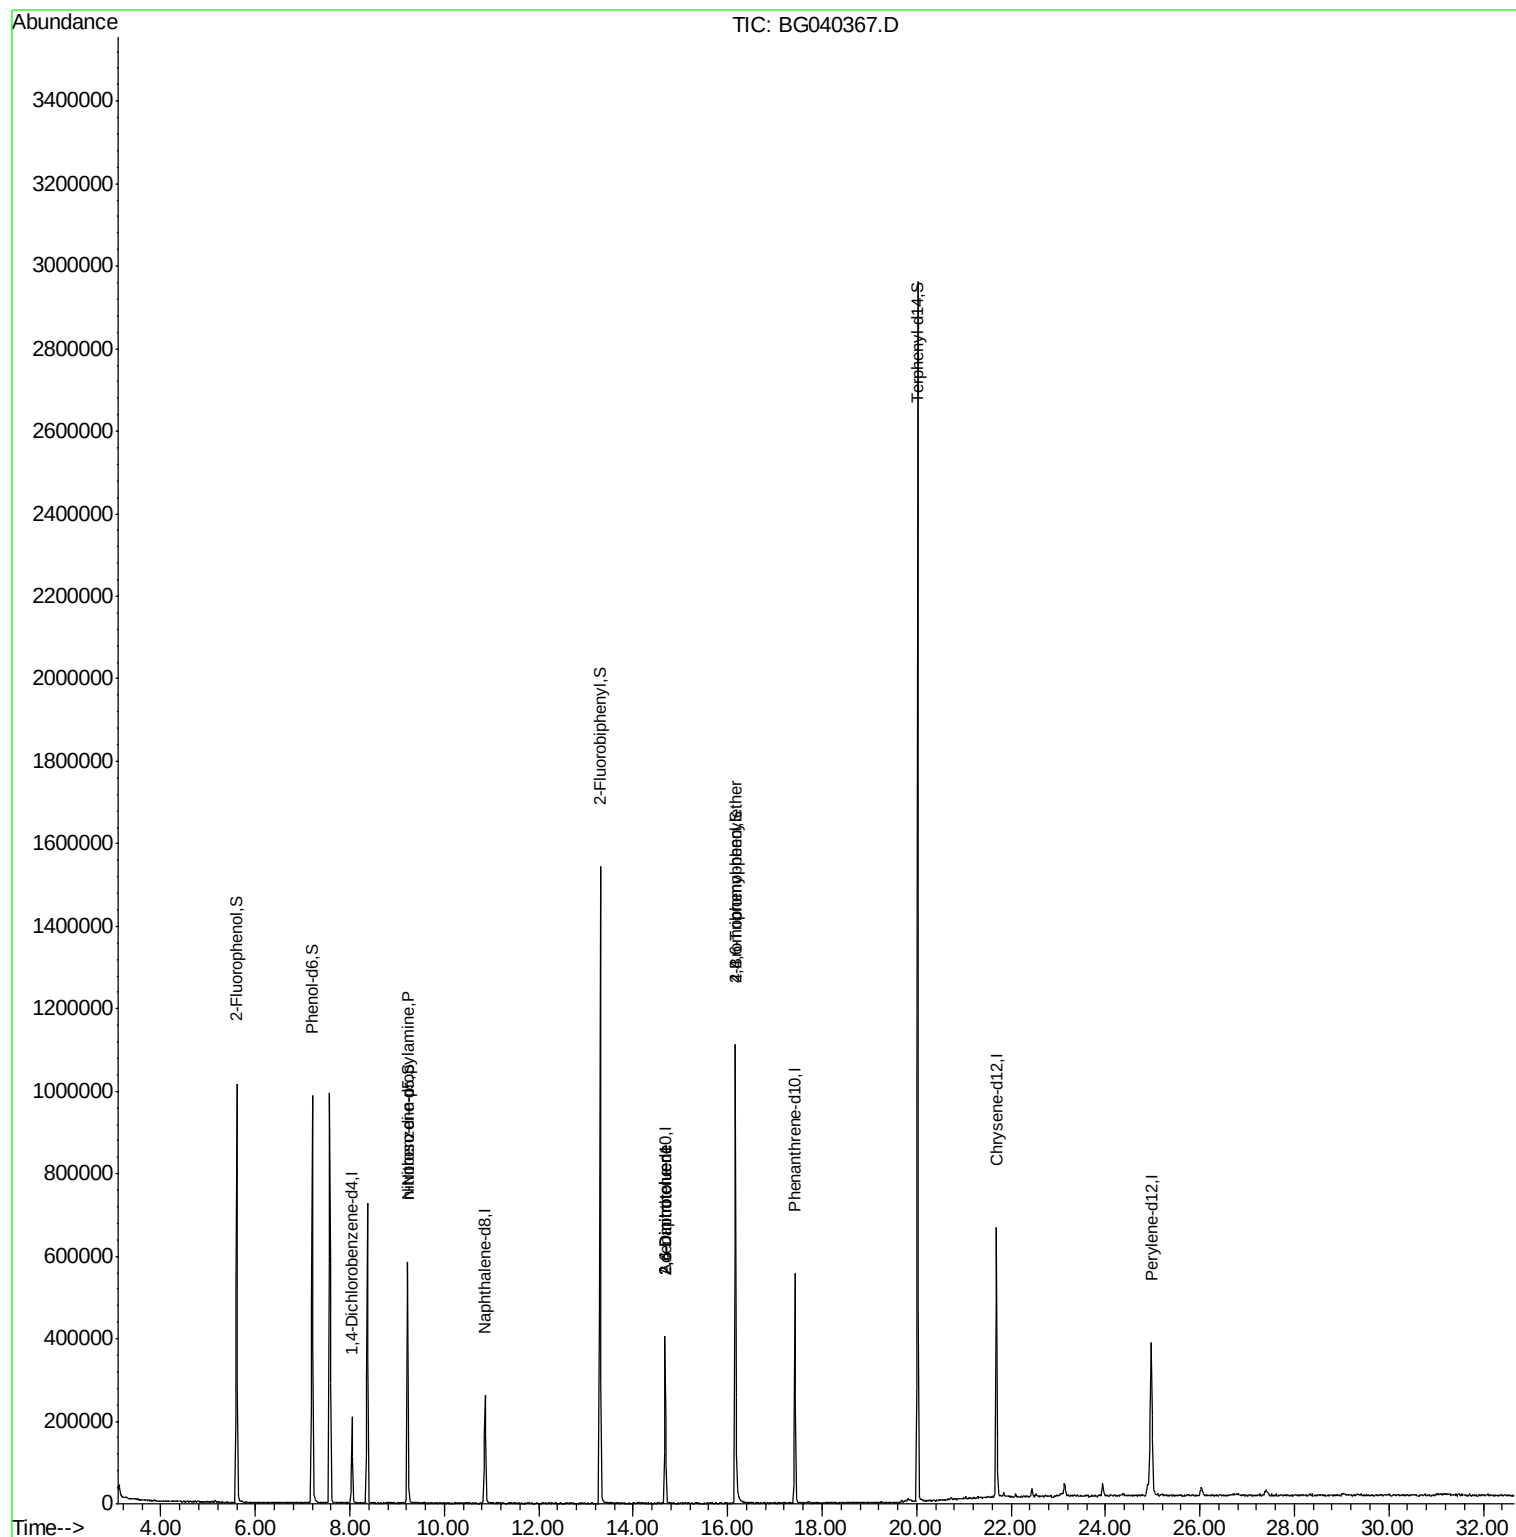

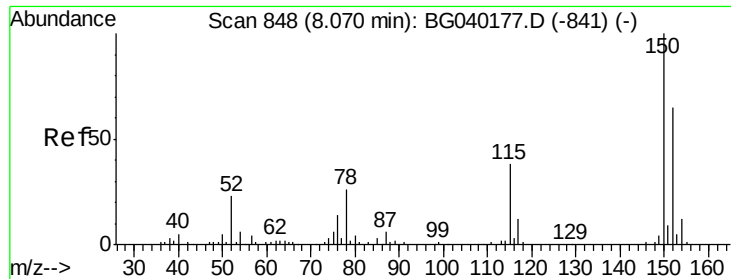


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 844
Delta R.T. -0.02 min
Lab File: BG040367.D
Acq: 4 Apr 2019 19:58

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 59382
Ion Ratio Lower Upper
152 100
150 157.5 123.7 185.5
115 57.2 46.9 70.3

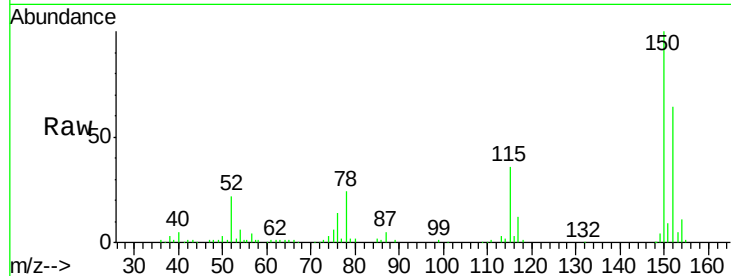


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

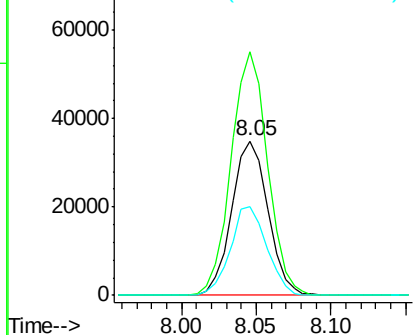



#5


2-Fluorophenol
Concen: 125.764 ng
RT: 5.60 min Scan# 428
Delta R.T. -0.02 min
Lab File: BG040367.D
Acq: 4 Apr 2019 19:58

Tgt Ion:112 Resp: 449235
Ion Ratio Lower Upper
112 100
64 66.1 54.2 81.2
63 33.8 26.4 39.6

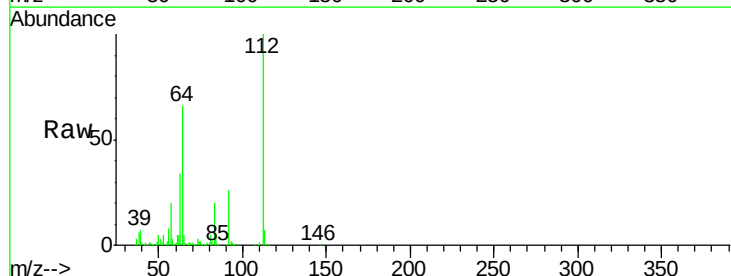

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

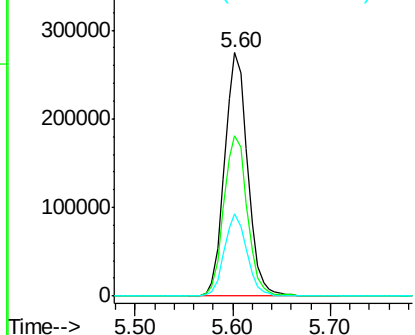

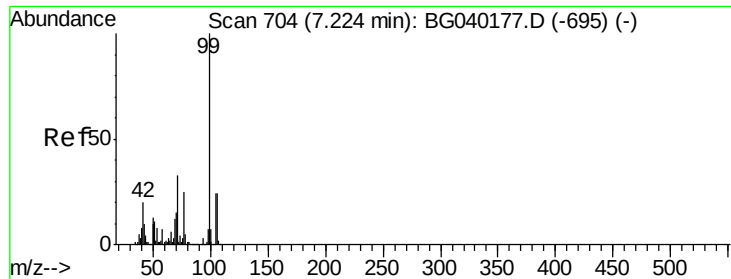

#7

Phenol-d6

Concen: 124.736 ng

RT: 7.21 min Scan# 701

Delta R.T. -0.02 min

Lab File: BG040367.D

Acq: 4 Apr 2019 19:58

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 615775

Ion Ratio Lower Upper




99 100

42 18.4 16.2 24.2

71 32.6 26.8 40.2



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

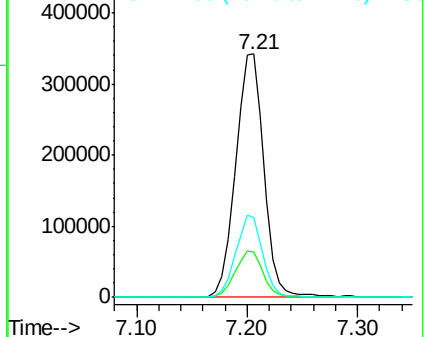

#19

n-Nitroso-di-n-propylamine

Concen: 12.888 ng

RT: 9.22 min Scan# 1044

Delta R.T. 0.35 min

Lab File: BG040367.D

Acq: 4 Apr 2019 19:58

Tgt Ion: 70 Resp: 45618


Ion Ratio Lower Upper

70 100



42 49.4 54.0 81.0#


101 0.0 8.6 13.0#

130 2.1 18.2 27.2#



Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

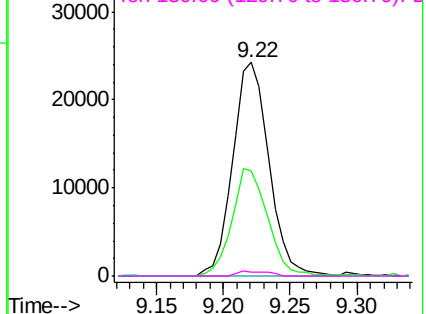


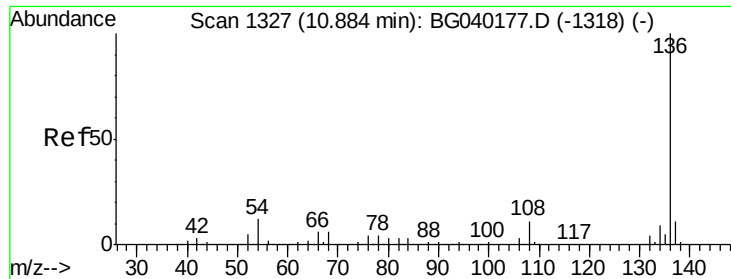




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.86 min Scan# 1323
Delta R.T. -0.02 min
Lab File: BG040367.D
Acq: 4 Apr 2019 19:58

Instrument :
BNA_G
ClientSampleId :

Tot Ion:136	Resp:	237254
Ion Ratio	Lower	Upper
136	100	
137	11.3	8.9 13.3
54	10.3	9.6 14.4
68	7.1	5.1 7.7




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


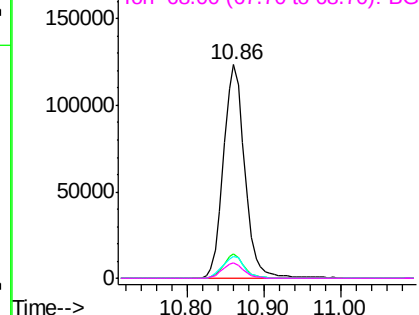



#23
Nitrobenzene-d5
Concen: 80.796 ng
RT: 9.22 min Scan# 1044
Delta R.T. -0.02 min
Lab File: BG040367.D
Acq: 4 Apr 2019 19:58

Tgt Ion: 82	Resp:	360637
Ion Ratio	Lower	Upper
82	100	
128	45.3	35.8 53.8
54	55.6	46.2 69.2



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

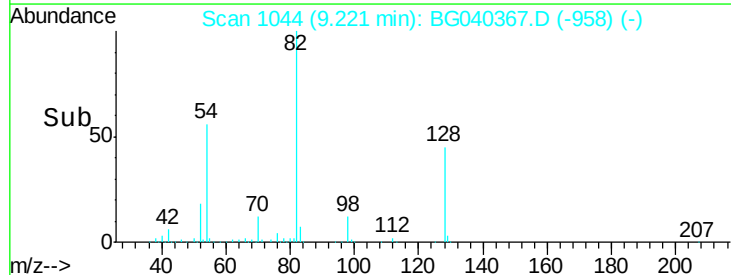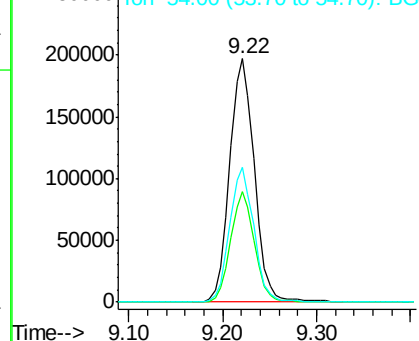


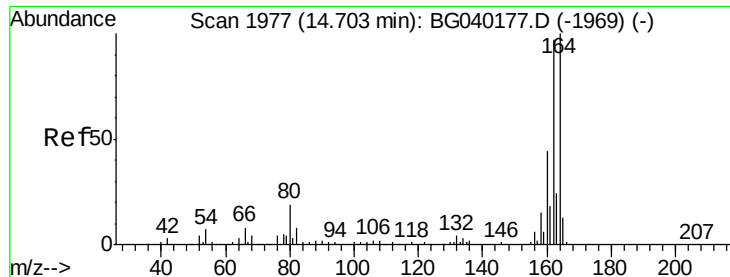




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.68 min Scan# 1973
Delta R.T. -0.02 min
Lab File: BG040367.D
Acq: 4 Apr 2019 19:58

Instrument :
BNA_G
ClientSampleId :

Tot Ion:164 Resp: 145868
Ion Ratio Lower Upper
164 100
162 100.4 77.4 116.2
160 44.7 35.3 52.9

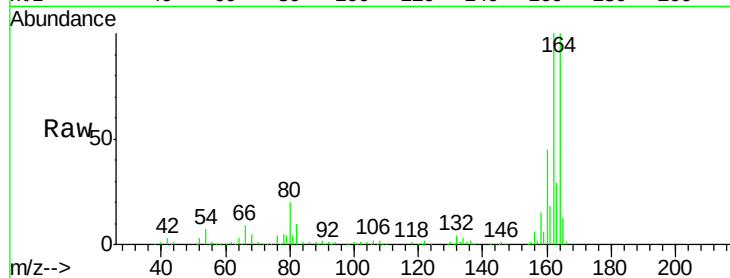


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

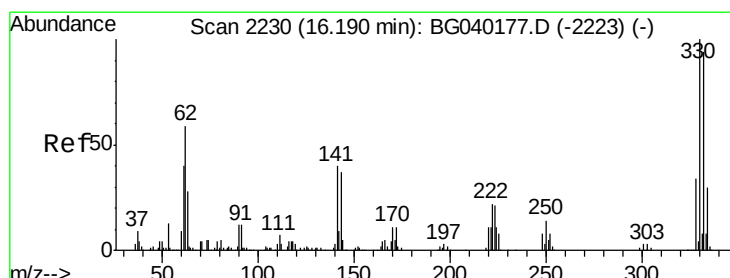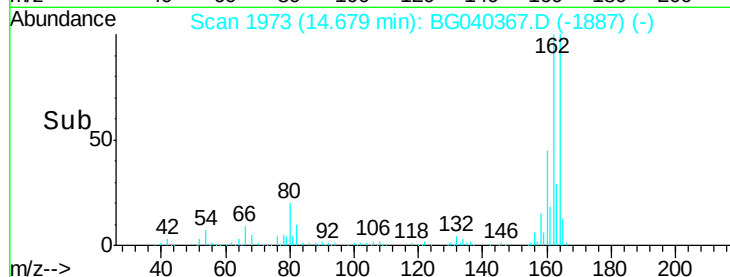
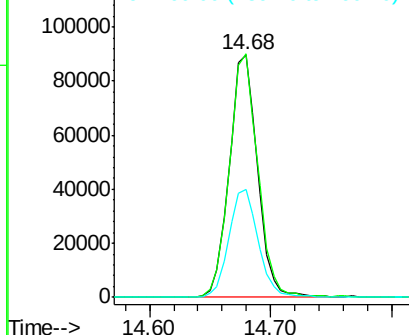



#42
2,4,6-Tribromophenol
Concen: 134.547 ng
RT: 16.17 min Scan# 2226
Delta R.T. -0.02 min
Lab File: BG040367.D
Acq: 4 Apr 2019 19:58

Tgt Ion:330 Resp: 212107
Ion Ratio Lower Upper
330 100
332 98.8 76.6 115.0
141 38.8 32.6 48.8

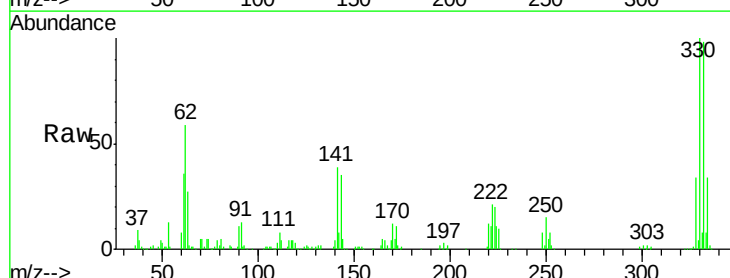

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E



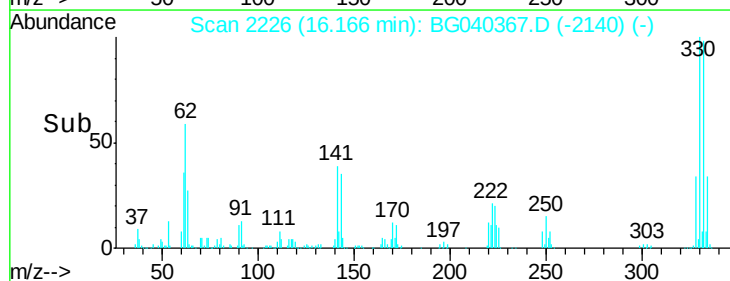
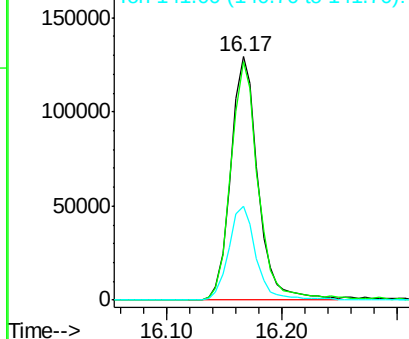




#45
2-Fluorobiphenyl
Concen: 85.704 ng
RT: 13.30 min Scan# 1738
Delta R.T. -0.02 min
Lab File: BG040367.D
Acq: 4 Apr 2019 19:58




Instrument :
BNA_G
ClientSampleId :


Tot Ion:172 Resp: 843691
Ion Ratio Lower Upper
172 100
171 37.8 30.5 45.7
170 23.8 20.1 30.1

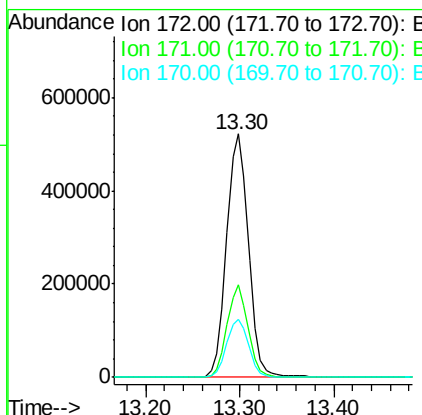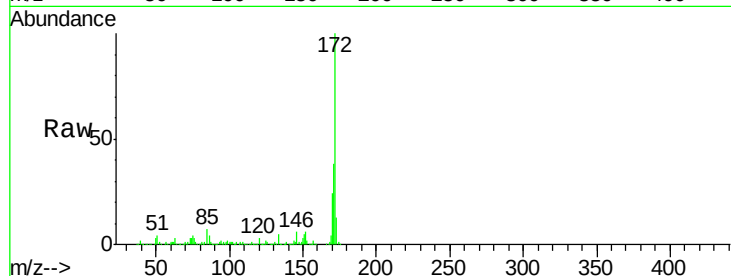

#51
2,6-Dinitrotoluene
Concen: 7.441 ng
RT: 14.67 min Scan# 1972
Delta R.T. 0.39 min
Lab File: BG040367.D
Acq: 4 Apr 2019 19:58

Tgt Ion:165 Resp: 19074
Ion Ratio Lower Upper
165 100
63 2.1 44.1 66.1#
89 0.0 44.9 67.3#

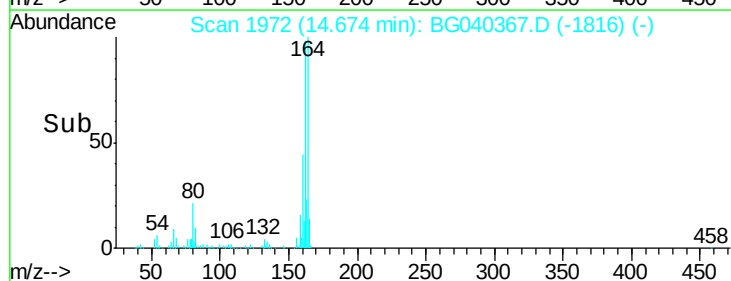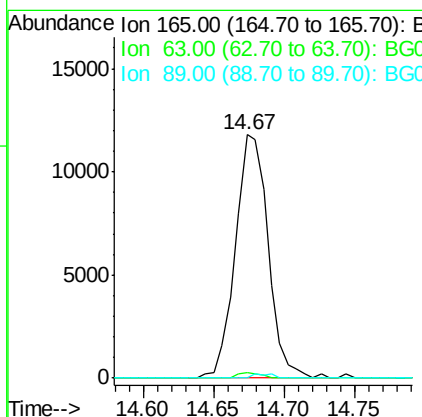

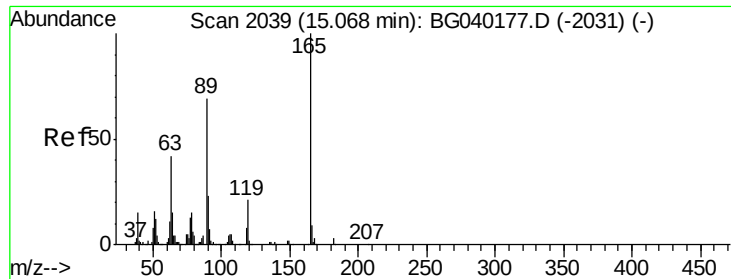

#57

2,4-Dinitrotoluene

Concen: 5.355 ng

RT: 14.67 min Scan# 1972

Delta R.T. -0.39 min


Lab File: BG040367.D

Acq: 4 Apr 2019 19:58

Instrument :

BNA_G

ClientSampleId :






Tot Ion:	165	Resp:	19074
Ion	Ratio	Lower	Upper
165	100		
63	2.1	33.8	50.6#
89	0.0	55.4	83.2#
182	0.0	2.2	3.4#

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC

Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

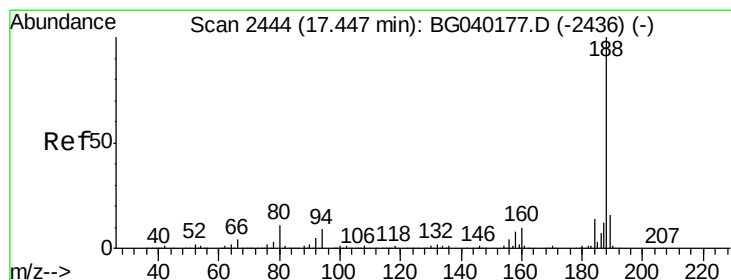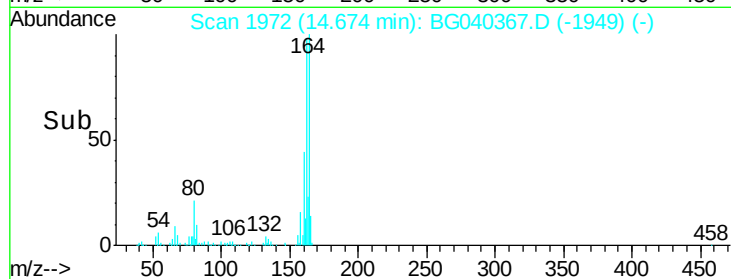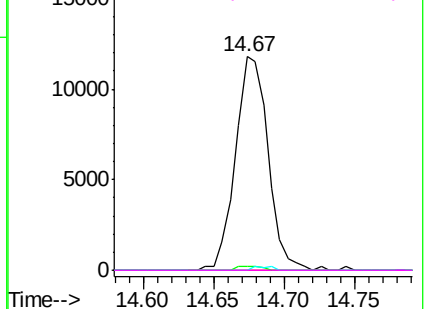

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2440

Delta R.T. -0.02 min

Lab File: BG040367.D




Acq: 4 Apr 2019 19:58


Tgt Ion:	188	Resp:	362370
Ion	Ratio	Lower	Upper
188	100		
94	9.4	7.0	10.4
80	10.3	8.6	13.0

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

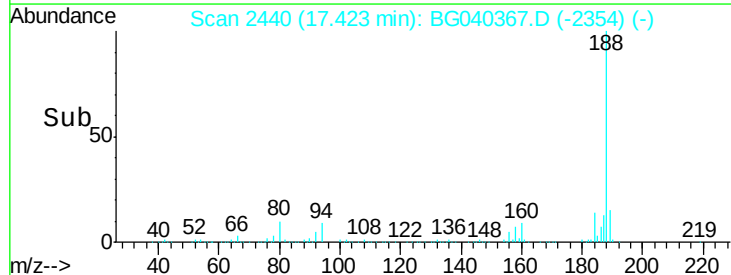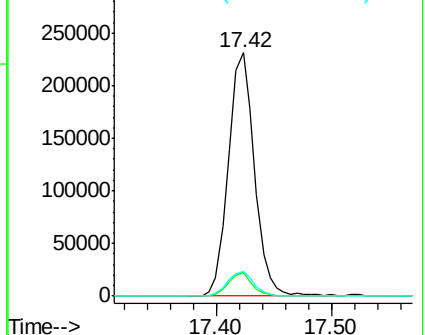

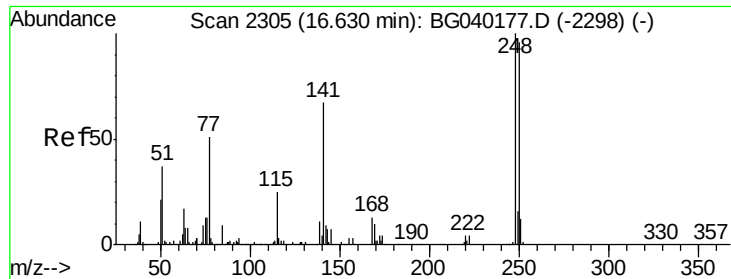

#67

4-Bromophenyl-phenylether

Concen: 4.050 ng

RT: 16.17 min Scan# 2226

Delta R.T. -0.46 min

Lab File: BG040367.D

Acq: 4 Apr 2019 19:58


Instrument :

BNA_G

ClientSampleId :

Tot Ion:248 Resp: 16515

Ion	Ratio	Lower	Upper
248	100		
250	194.2	76.4	114.6#
141	485.9	53.8	80.8#



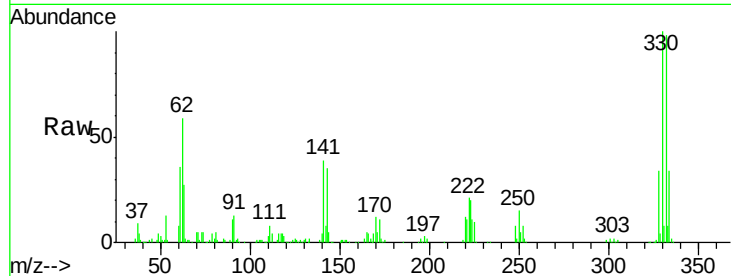


Abundance

Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

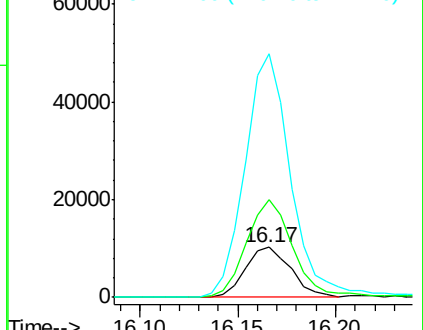

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3167


Delta R.T. -0.04 min

Lab File: BG040367.D

Acq: 4 Apr 2019 19:58

Tgt Ion:240 Resp: 413925

Ion	Ratio	Lower	Upper
240	100		
120	10.0	8.4	12.6
236	25.3	20.8	31.2






Abundance

Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

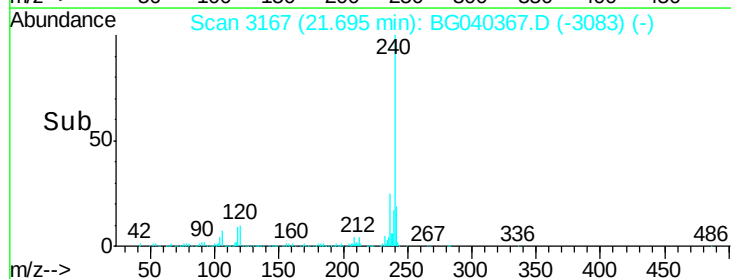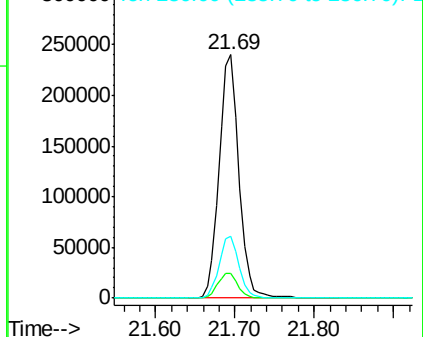



#79

Terphenyl-d14

Concen: 75.356 ng

RT: 20.02 min Scan# 2882

Delta R.T. -0.03 min

Lab File: BG040367.D

Acq: 4 Apr 2019 19:58

Instrument :

BNA_G

ClientSampled :


Tot Ion:244 Resp: 1386506

Ion Ratio Lower Upper

244 100

212 8.6 7.0 10.6




122 11.6 8.5 12.7



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

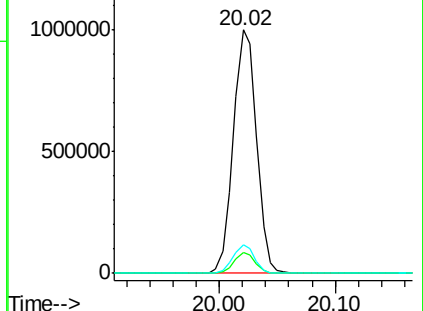

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.97 min Scan# 3724

Delta R.T. -0.06 min

Lab File: BG040367.D

Acq: 4 Apr 2019 19:58


Tgt Ion:264 Resp: 418786

Ion Ratio Lower Upper

264 100

260 23.5 17.9 26.9

265 21.6 16.8 25.2



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

