

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040419\
 Data File : BG040367.D
 Acq On : 4 Apr 2019 19:58
 Operator : JU/SJ
 Sample : PB118524BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB118524BL

Quant Time: Apr 05 02:28:09 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 28 05:47:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	59382	20.00	ng	-0.02
21) Naphthalene-d8	10.86	136	237254	20.00	ng	-0.02
39) Acenaphthene-d10	14.68	164	145868	20.00	ng	-0.02
64) Phenanthrene-d10	17.42	188	362370	20.00	ng	-0.02
76) Chrysene-d12	21.69	240	413925	20.00	ng	-0.04
87) Perylene-d12	24.97	264	418786	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	449235	125.76	ng	-0.02
7) Phenol-d6	7.21	99	615775	124.74	ng	-0.02
23) Nitrobenzene-d5	9.22	82	360637	80.80	ng	-0.02
42) 2,4,6-Tribromophenol	16.17	330	212107	134.55	ng	-0.02
45) 2-Fluorobiphenyl	13.30	172	843691	85.70	ng	-0.02
79) Terphenyl-d14	20.02	244	1386506	75.36	ng	-0.03


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040419\
Data File : BG040367.D
Acq On : 4 Apr 2019 19:58
Operator : JU/SJ
Sample : PB118524BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB118524BL

Quant Time: Apr 05 02:28:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 28 05:47:00 2019
Response via : Initial Calibration

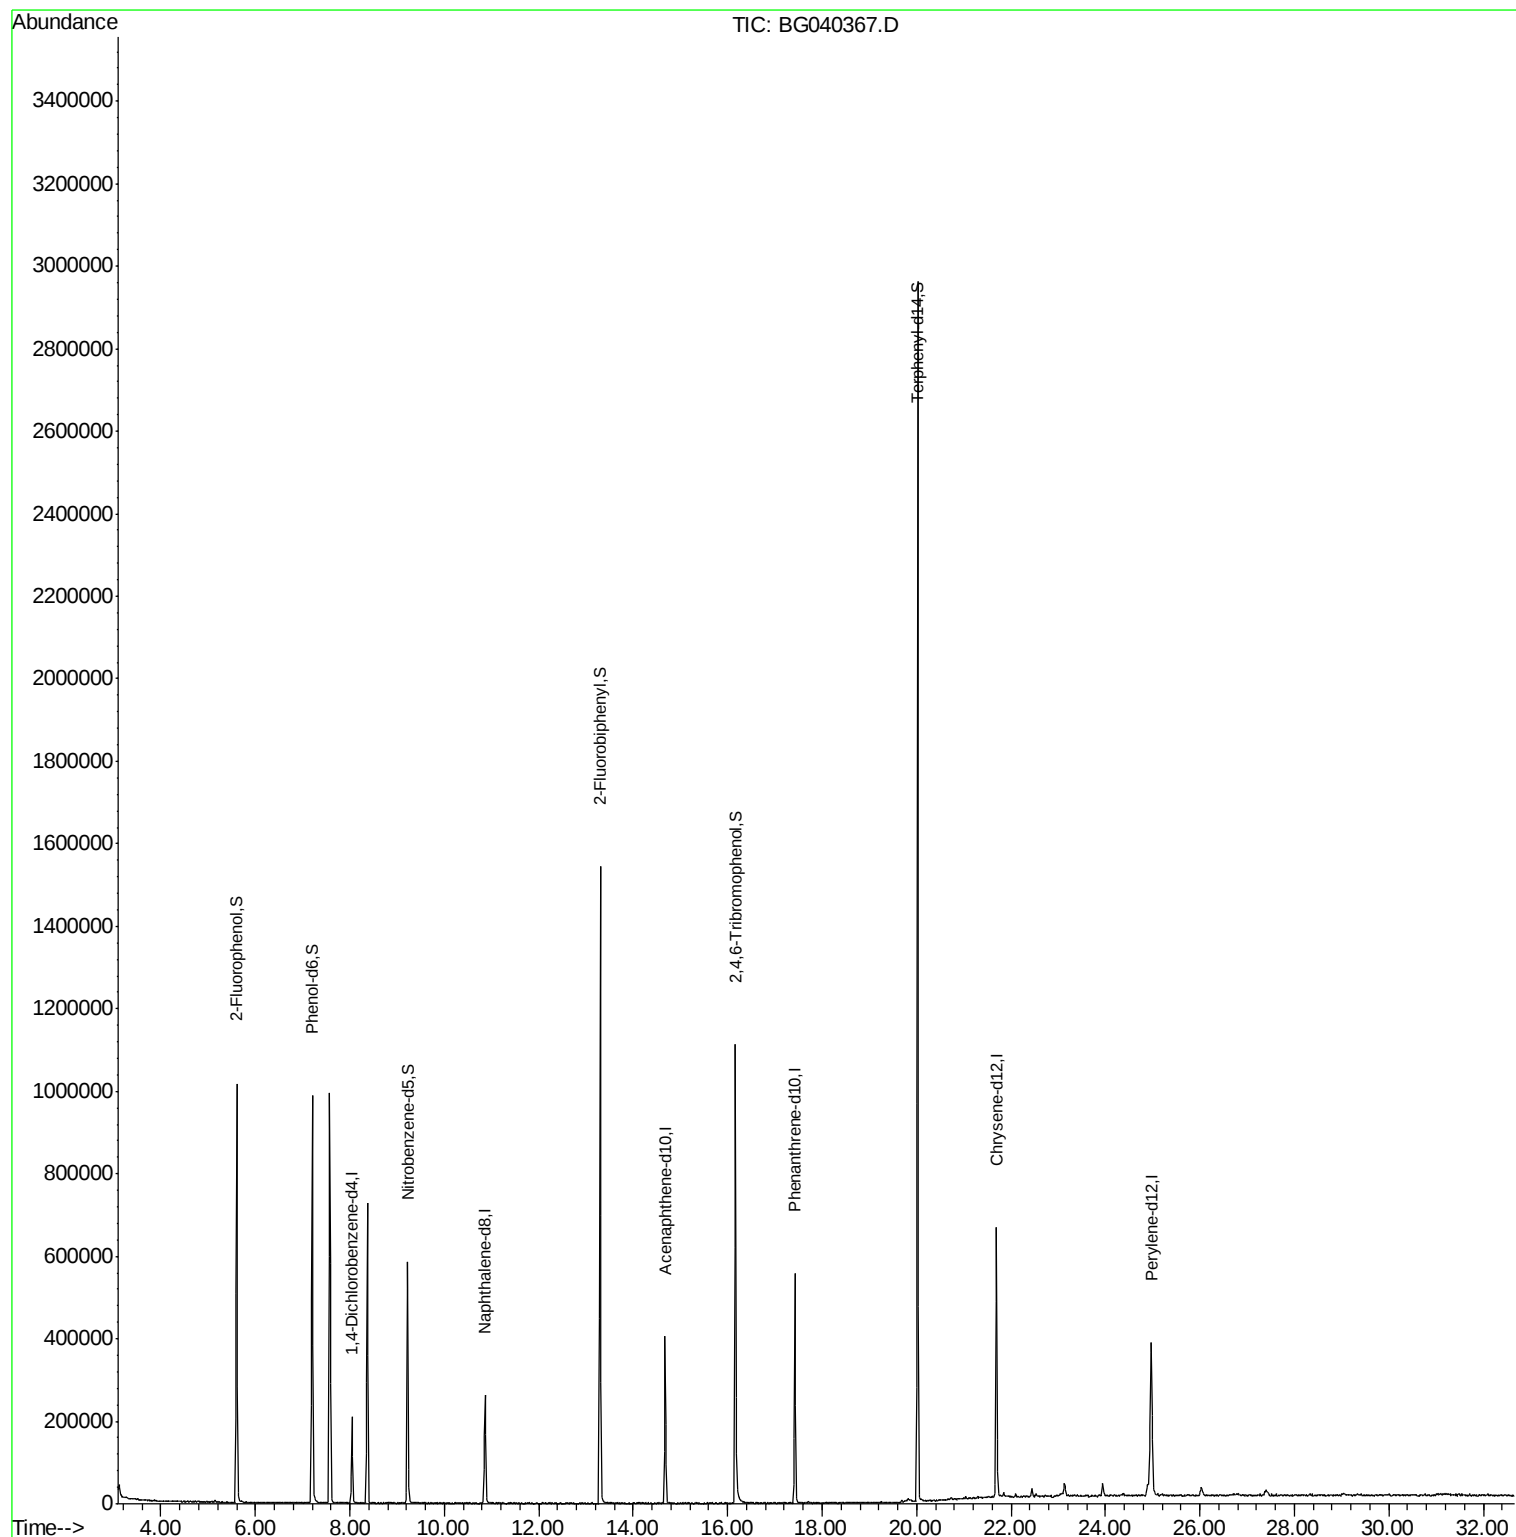




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 844
Delta R.T. -0.02 min
Lab File: BG040367.D
Acq: 4 Apr 2019 19:58

Instrument :
BNA_G
ClientSampleId :
PB118524BL

Tgt Ion:152 Resp: 59382
Ion Ratio Lower Upper
152 100
150 157.5 123.7 185.5
115 57.2 46.9 70.3

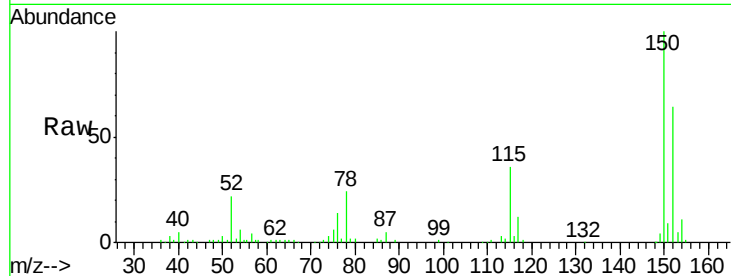


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

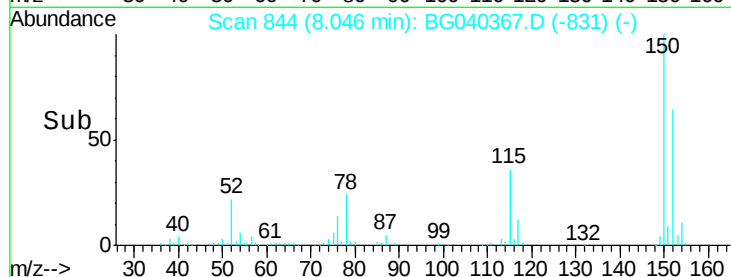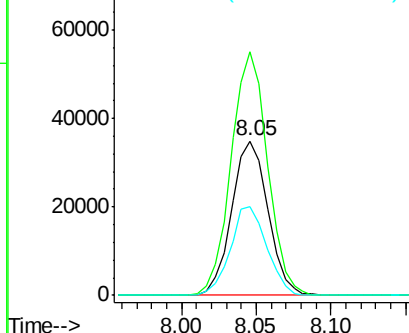



#5


2-Fluorophenol
Concen: 125.764 ng
RT: 5.60 min Scan# 428
Delta R.T. -0.02 min
Lab File: BG040367.D
Acq: 4 Apr 2019 19:58

Tgt Ion:112 Resp: 449235
Ion Ratio Lower Upper
112 100
64 66.1 54.2 81.2
63 33.8 26.4 39.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

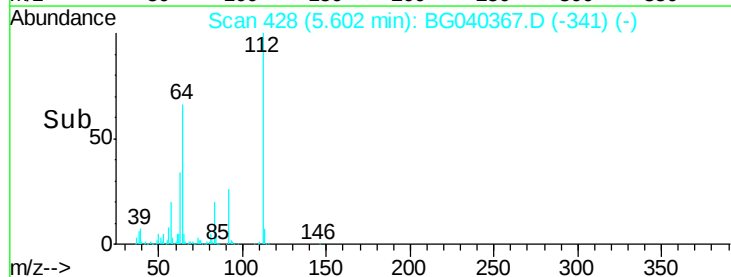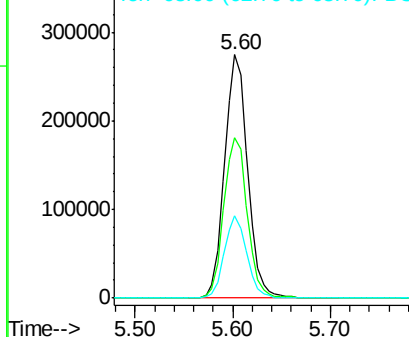

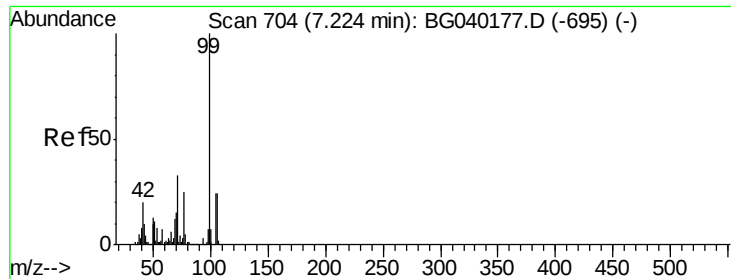

#7

Phenol-d6

Concen: 124.736 ng

RT: 7.21 min Scan# 701

Delta R.T. -0.02 min

Lab File: BG040367.D

Acq: 4 Apr 2019 19:58

Instrument :

BNA_G

ClientSampleId :

PB118524BL


Tgt Ion: 99 Resp: 615775

Ion Ratio Lower Upper




99 100

42 18.4 16.2 24.2

71 32.6 26.8 40.2



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

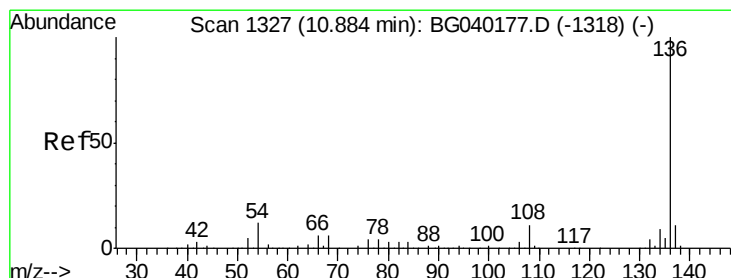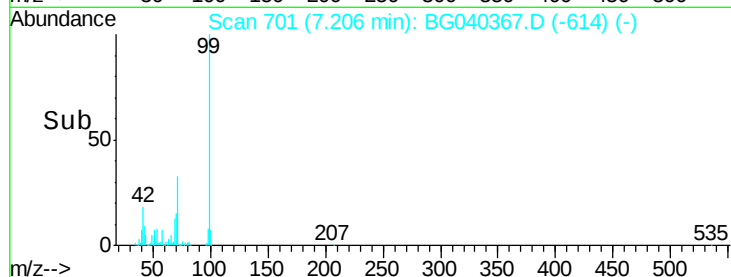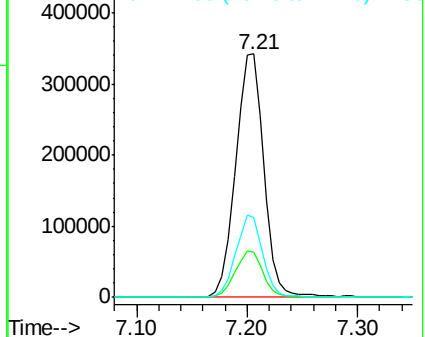

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1323

Delta R.T. -0.02 min

Lab File: BG040367.D

Acq: 4 Apr 2019 19:58

Tgt Ion: 136 Resp: 237254


Ion Ratio Lower Upper

136 100



137 11.3 8.9 13.3


54 10.3 9.6 14.4

68 7.1 5.1 7.7



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


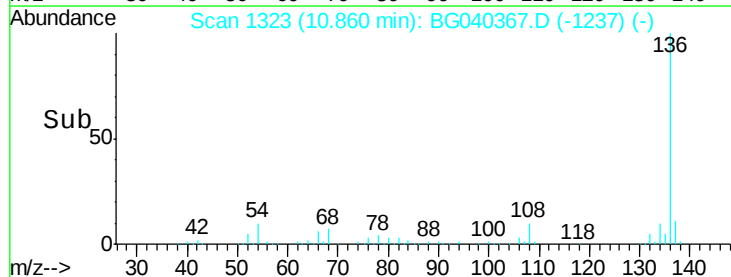
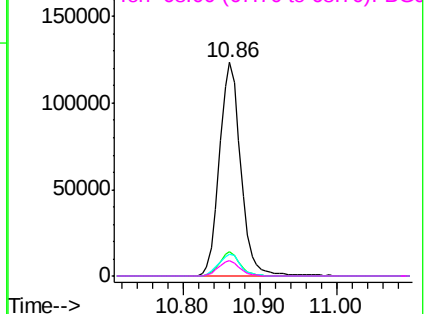


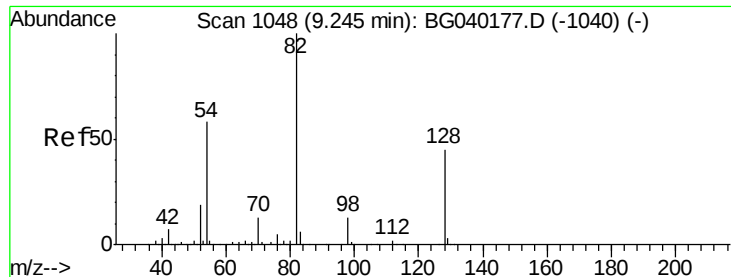

#23
 Nitrobenzene-d5
 Concen: 80.796 ng
 RT: 9.22 min Scan# 1044
 Delta R.T. -0.02 min
 Lab File: BG040367.D
 Acq: 4 Apr 2019 19:58




Instrument :
 BNA_G
 ClientSampleId :
 PB118524BL

Tgt Ion: 82 Resp: 360637
 Ion Ratio Lower Upper
 82 100
 128 45.3 35.8 53.8
 54 55.6 46.2 69.2

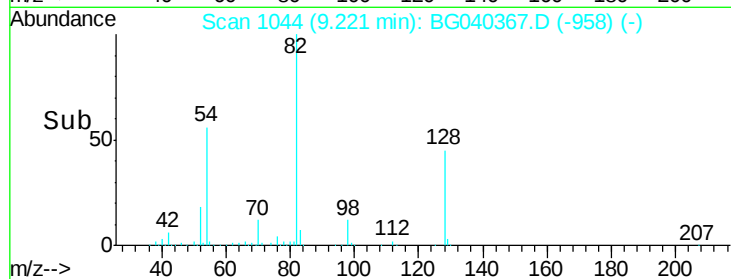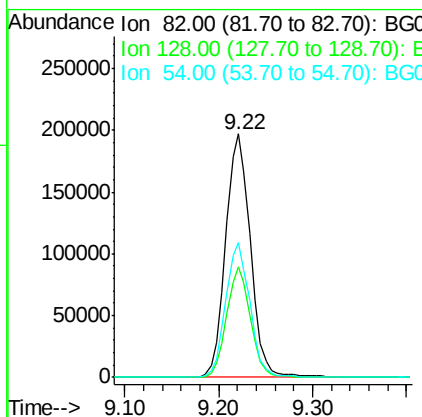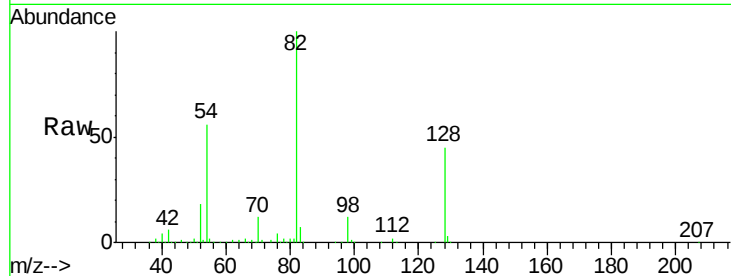

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.68 min Scan# 1973
 Delta R.T. -0.02 min
 Lab File: BG040367.D
 Acq: 4 Apr 2019 19:58

Tgt Ion: 164 Resp: 145868
 Ion Ratio Lower Upper
 164 100
 162 100.4 77.4 116.2
 160 44.7 35.3 52.9

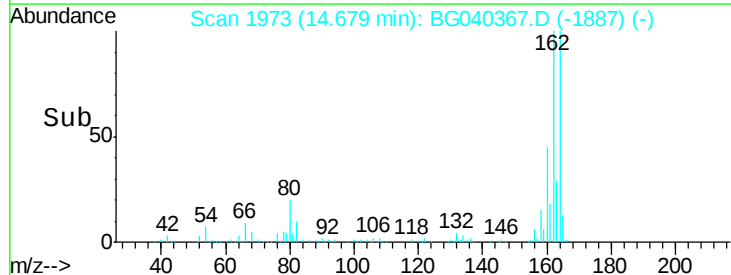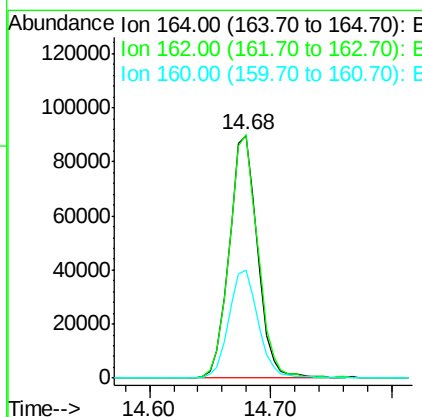






#42
 2,4,6-Tribromophenol
 Concen: 134.547 ng
 RT: 16.17 min Scan# 2226
 Delta R.T. -0.02 min
 Lab File: BG040367.D
 Acq: 4 Apr 2019 19:58

Instrument :
 BNA_G
 ClientSampleId :
 PB118524BL

Tgt Ion:330 Resp: 212107
 Ion Ratio Lower Upper
 330 100
 332 98.8 76.6 115.0
 141 38.8 32.6 48.8

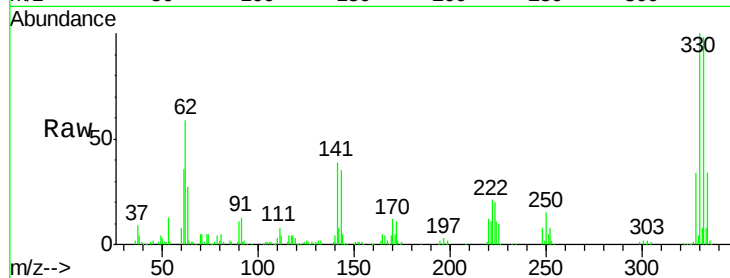


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

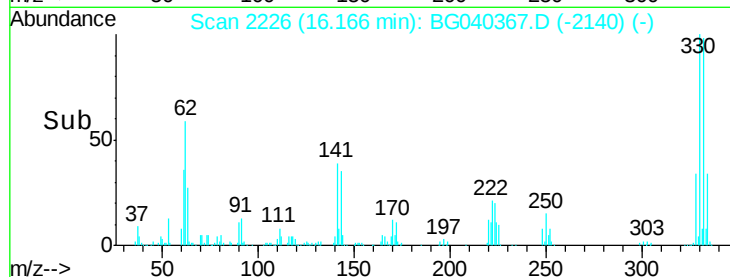
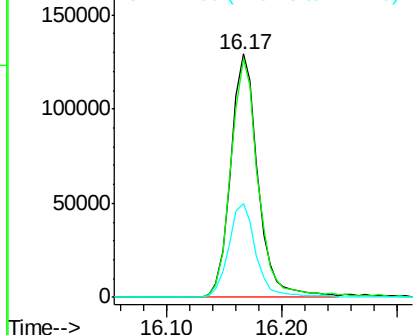



#45
 2-Fluorobiphenyl
 Concen: 85.704 ng
 RT: 13.30 min Scan# 1738
 Delta R.T. -0.02 min
 Lab File: BG040367.D
 Acq: 4 Apr 2019 19:58

Tgt Ion:172 Resp: 843691
 Ion Ratio Lower Upper
 172 100
 171 37.8 30.5 45.7
 170 23.8 20.1 30.1

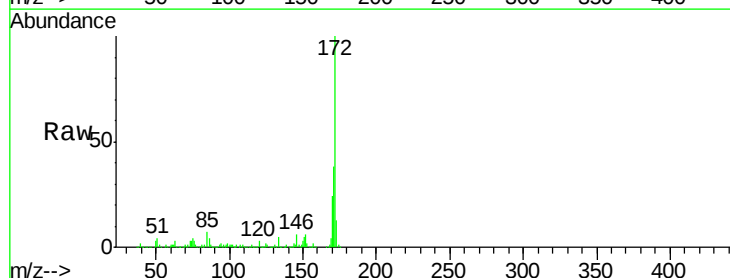

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

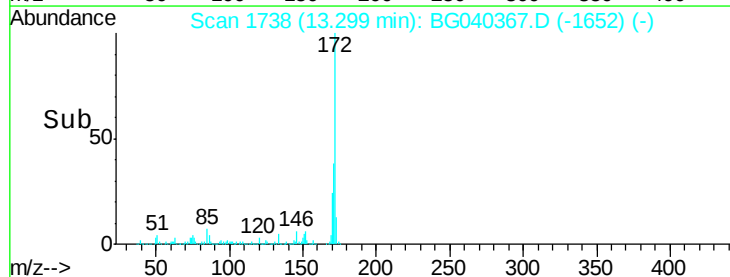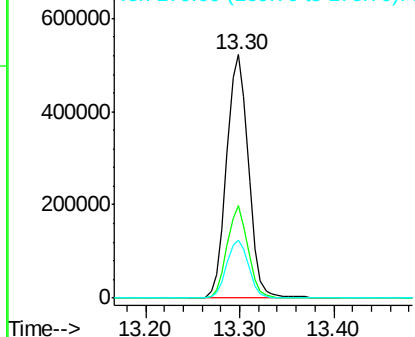

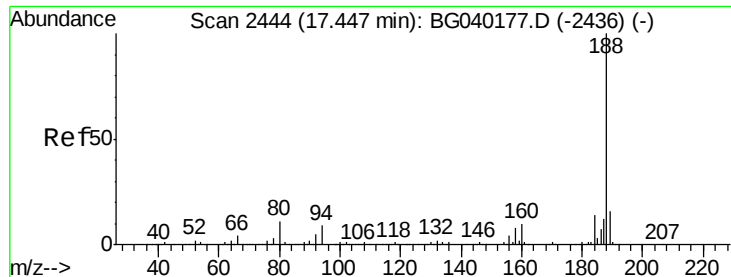

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2440

Delta R.T. -0.02 min

Lab File: BG040367.D

Acq: 4 Apr 2019 19:58

Instrument :

BNA_G

ClientSampleId :

PB118524BL


Tgt Ion:188 Resp: 362370

Ion Ratio Lower Upper

188 100

94 9.4 7.0 10.4




80 10.3 8.6 13.0



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

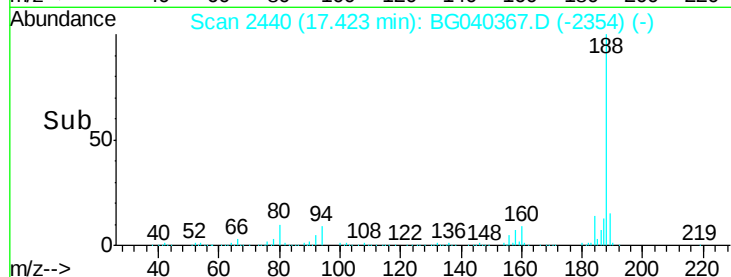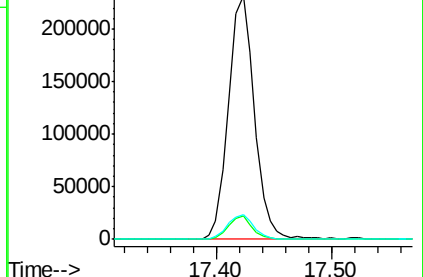

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.69 min Scan# 3167

Delta R.T. -0.04 min

Lab File: BG040367.D

Acq: 4 Apr 2019 19:58


Tgt Ion:240 Resp: 413925

Ion Ratio Lower Upper

240 100

120 10.0 8.4 12.6



236 25.3 20.8 31.2



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

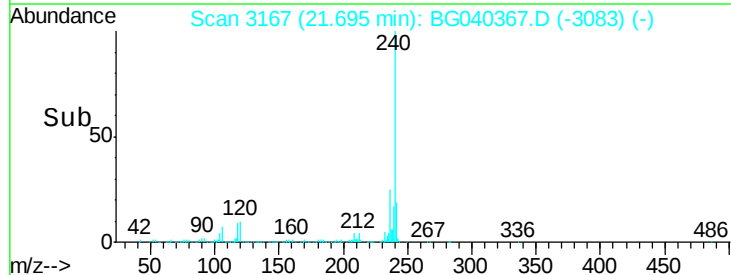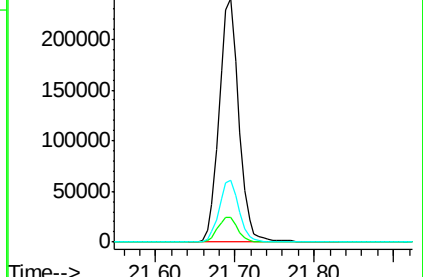



#79

Terphenyl-d14

Concen: 75.356 ng

RT: 20.02 min Scan# 2882

Delta R.T. -0.03 min

Lab File: BG040367.D

Acq: 4 Apr 2019 19:58

Instrument :

BNA_G

ClientSampleId :

PB118524BL


Tgt Ion:244 Resp: 1386506

Ion Ratio Lower Upper

244 100

212 8.6 7.0 10.6




122 11.6 8.5 12.7



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

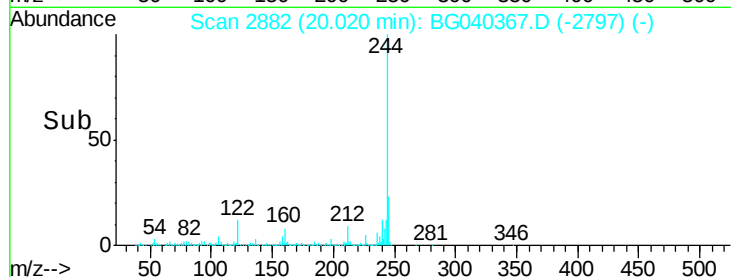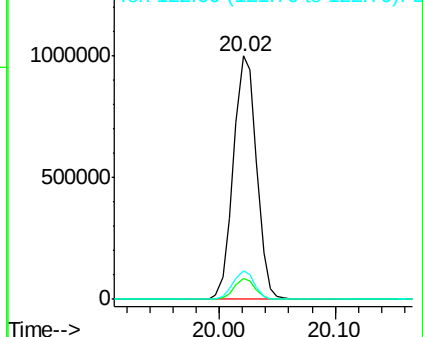

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.97 min Scan# 3724

Delta R.T. -0.06 min

Lab File: BG040367.D

Acq: 4 Apr 2019 19:58


Tgt Ion:264 Resp: 418786

Ion Ratio Lower Upper

264 100

260 23.5 17.9 26.9

265 21.6 16.8 25.2



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

