

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040419\
 Data File : BG040372.D
 Acq On : 4 Apr 2019 23:19
 Operator : JU/SJ
 Sample : K2240-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-01-(13.5-14)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.602	420	428	444	rBV	980286	1596222	51.31%	7.936%
2	7.200	692	700	716	rBV	1003699	1768782	56.85%	8.794%
3	7.576	756	764	779	rBV	987345	1699517	54.63%	8.449%
4	8.046	836	844	855	rBV	213738	376963	12.12%	1.874%
5	8.369	890	899	910	rBV	672492	1205549	38.75%	5.993%
6	9.221	1036	1044	1052	rBV	580315	1049761	33.74%	5.219%
7	10.860	1314	1323	1332	rBV	258623	498068	16.01%	2.476%
8	13.299	1731	1738	1750	rBV	1306519	2059532	66.20%	10.239%
9	14.121	1871	1878	1888	rBV	136686	221928	7.13%	1.103%
10	14.679	1966	1973	1982	rBV2	406598	699949	22.50%	3.480%
11	16.166	2219	2226	2243	rBV	1130296	1810057	58.18%	8.999%
12	17.423	2431	2440	2449	rBV2	560612	884750	28.44%	4.399%
13	18.275	2581	2585	2591	rBV6	20239	38451	1.24%	0.191%
14	20.020	2876	2882	2892	rBV	2363092	3111160	100.00%	15.467%
15	20.925	3033	3036	3043	rVB2	27341	39043	1.25%	0.194%
16	21.289	3094	3098	3114	rBV	175720	333979	10.73%	1.660%
17	21.689	3159	3166	3179	rBV2	652606	1129510	36.31%	5.615%
18	21.836	3184	3191	3196	rBV4	23114	40388	1.30%	0.201%
19	22.441	3290	3294	3300	rBV2	25804	36545	1.17%	0.182%
20	23.064	3389	3400	3401	rBV6	22894	60543	1.95%	0.301%
21	23.134	3408	3412	3419	rVB3	50345	98435	3.16%	0.489%
22	23.945	3543	3550	3558	rBV4	39630	91581	2.94%	0.455%
23	24.903	3706	3713	3715	rBV3	33342	75446	2.43%	0.375%
24	24.967	3715	3724	3737	rVB3	370228	1096151	35.23%	5.450%
25	26.037	3896	3906	3918	rVB5	30794	92303	2.97%	0.459%


Sum of corrected areas: 20114613

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040419\
Data File : BG040372.D
Acq On : 4 Apr 2019 23:19
Operator : JU/SJ
Sample : K2240-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-01-(13.5-14)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

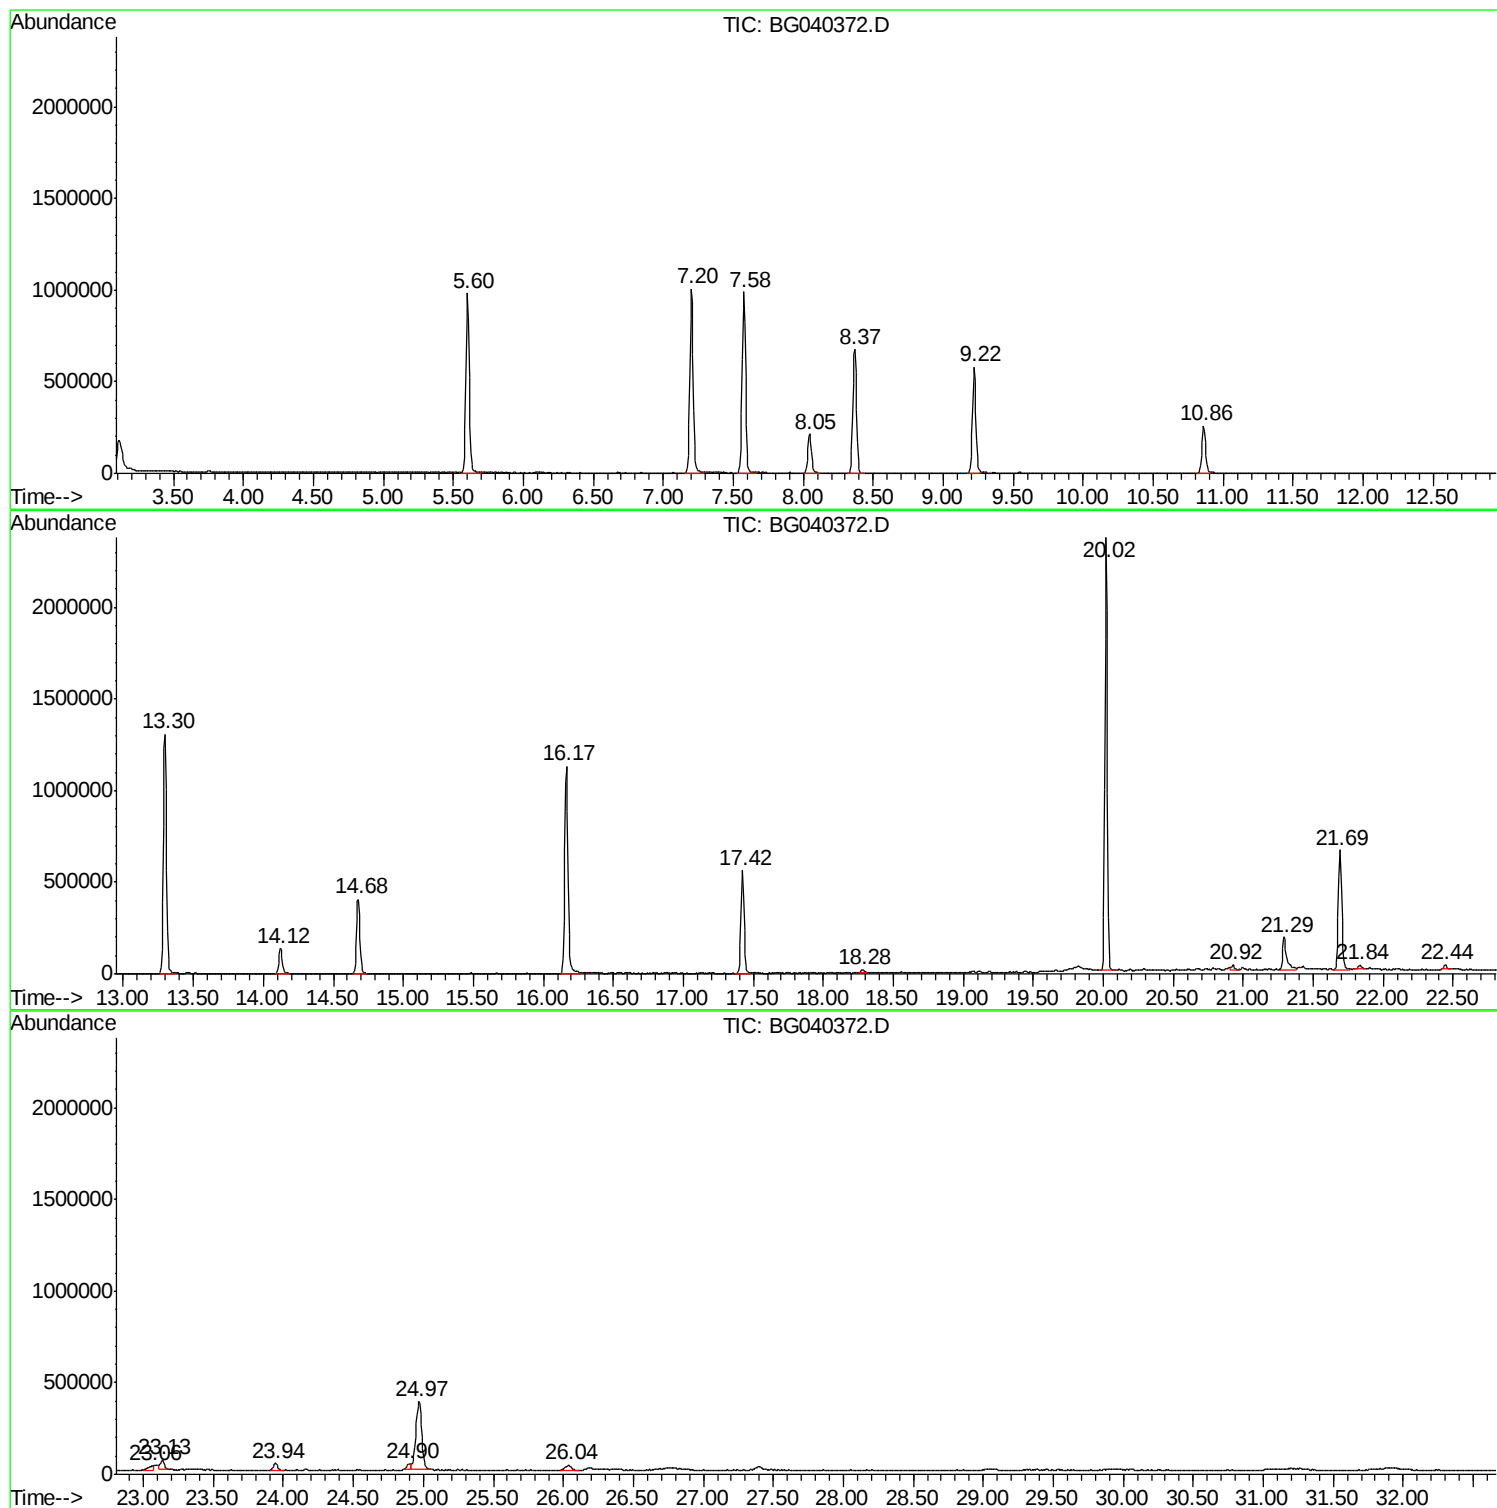

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040419\
Data File : BG040372.D
Acq On : 4 Apr 2019 23:19
Operator : JU/SJ
Sample : K2240-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-01-(13.5-14)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.58 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.58	90.17 ng	1699520	1,4-Dichlorobenzene-d4	8.05

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			1H-Tetrazaborole, 5-chloro-4,5-d...	132	C2H6BClN4	021960-49-6	16
3			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
4			Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
5			5-Aminoindole	132	C8H8N2	005192-03-0	12

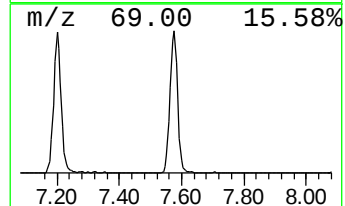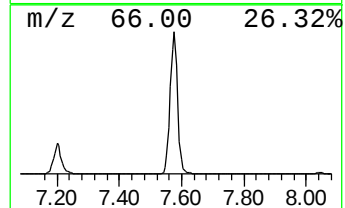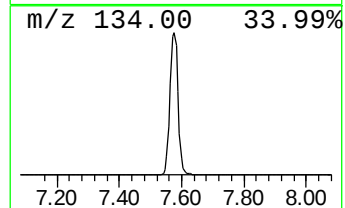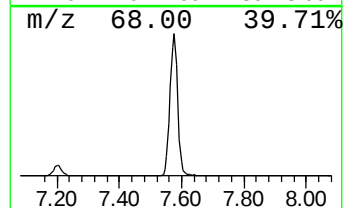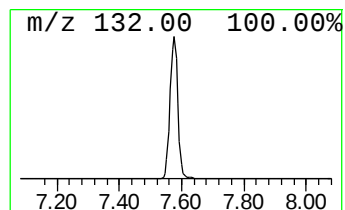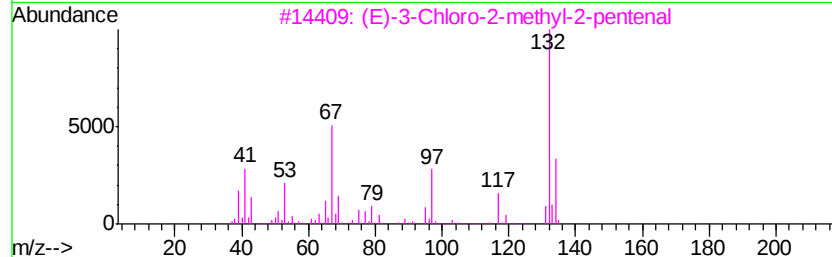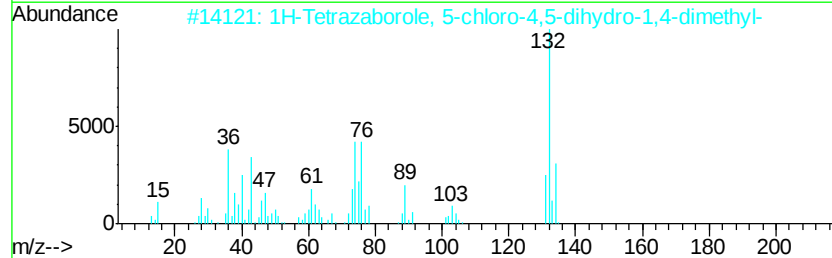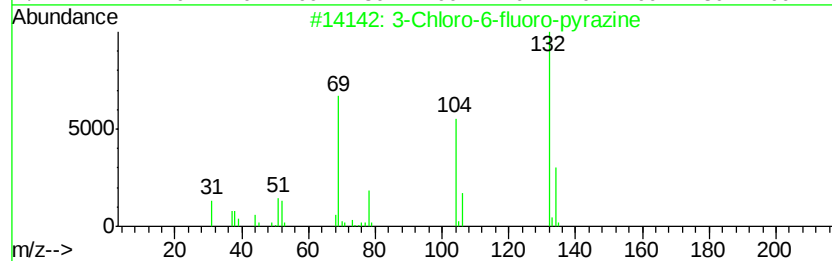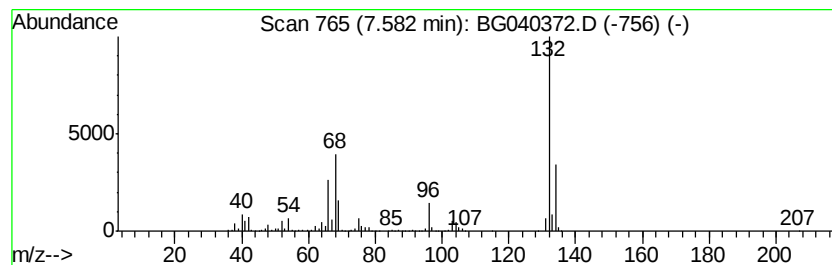

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040419\
 Data File : BG040372.D
 Acq On : 4 Apr 2019 23:19
 Operator : JU/SJ
 Sample : K2240-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-01-(13.5-14)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
 TIC Integration Parameters: LSCINT.P

 Peak Number 3 Trichloroacetic acid, hexad... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.29	5.91 ng	333979	Chrysene-d12	21.69

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	95
2			1-Docosene	308	C22H44	001599-67-3	95
3			1-Tricosene	322	C23H46	018835-32-0	94
4			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	94
5			Octacosanol	410	C28H58O	000557-61-9	94

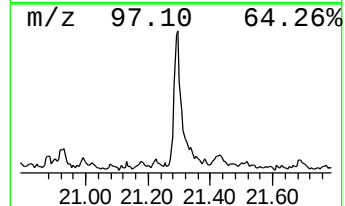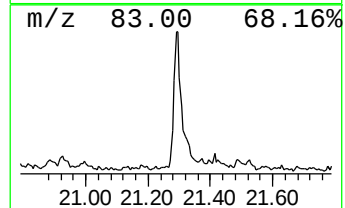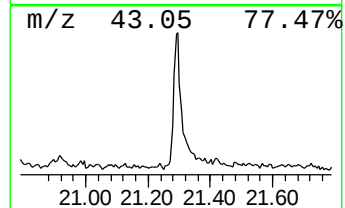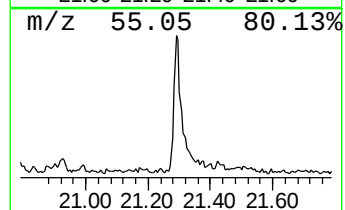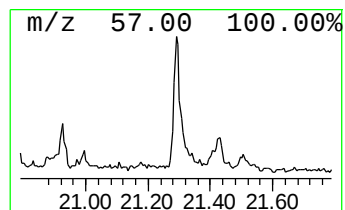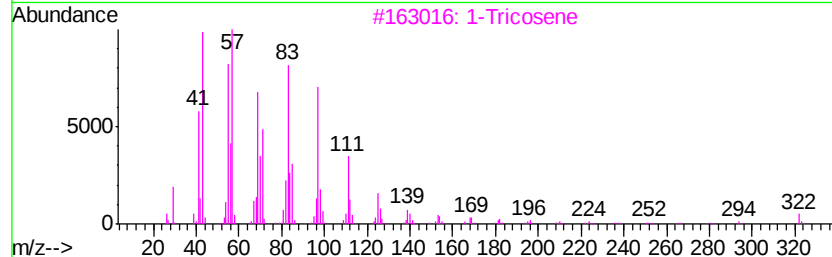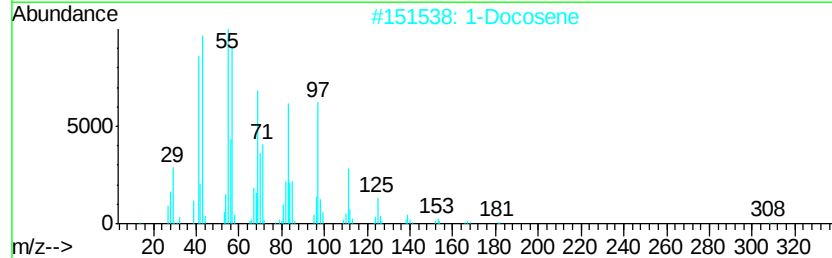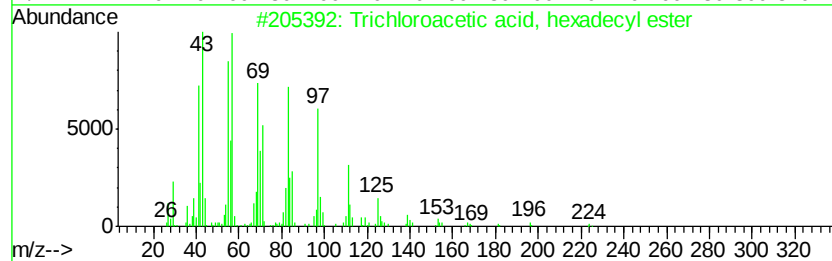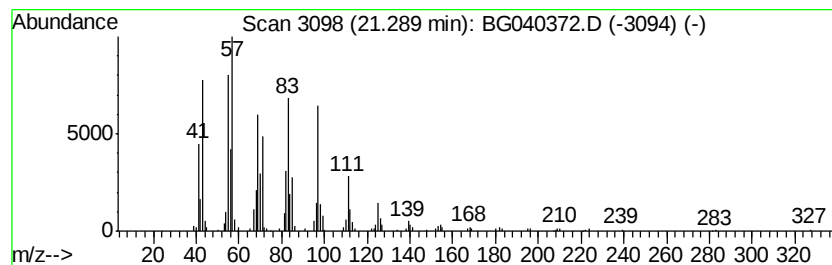

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040419\
Data File : BG040372.D
Acq On : 4 Apr 2019 23:19
Operator : JU/SJ
Sample : K2240-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-01-(13.5-14)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.58	7.58	90.2	ng	1699520	1	8.05	376963	20.0
Trichloroacetic a...	21.29	5.9	ng	333979	5	21.69	1129510	20.0