
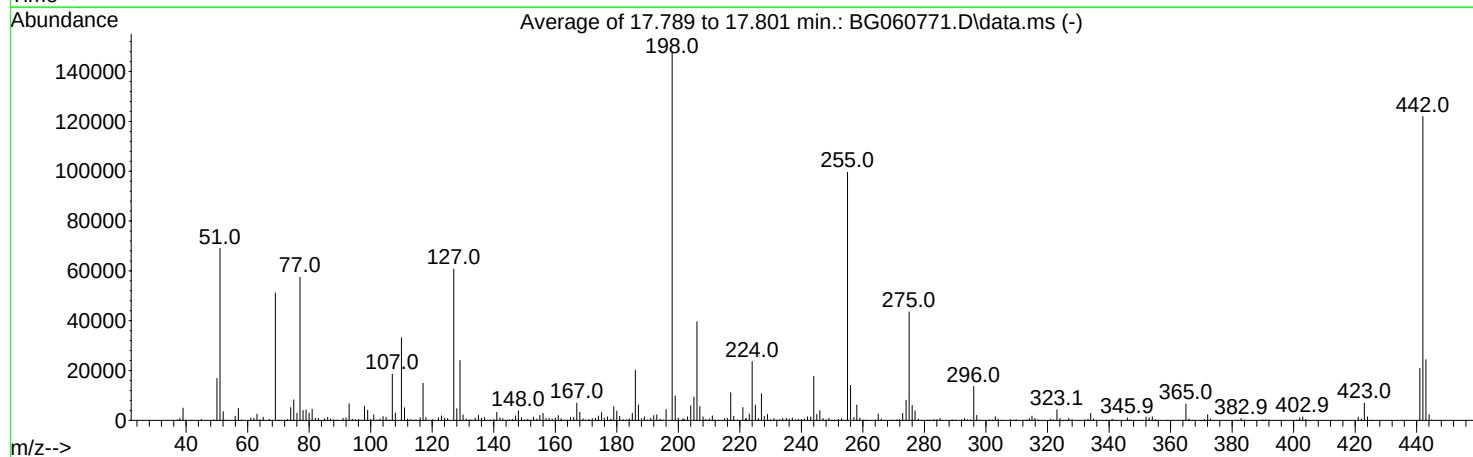


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040424\
Data File : BG060771.D
Acq On : 4 Apr 2024 9:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 30 03:12:26 2024

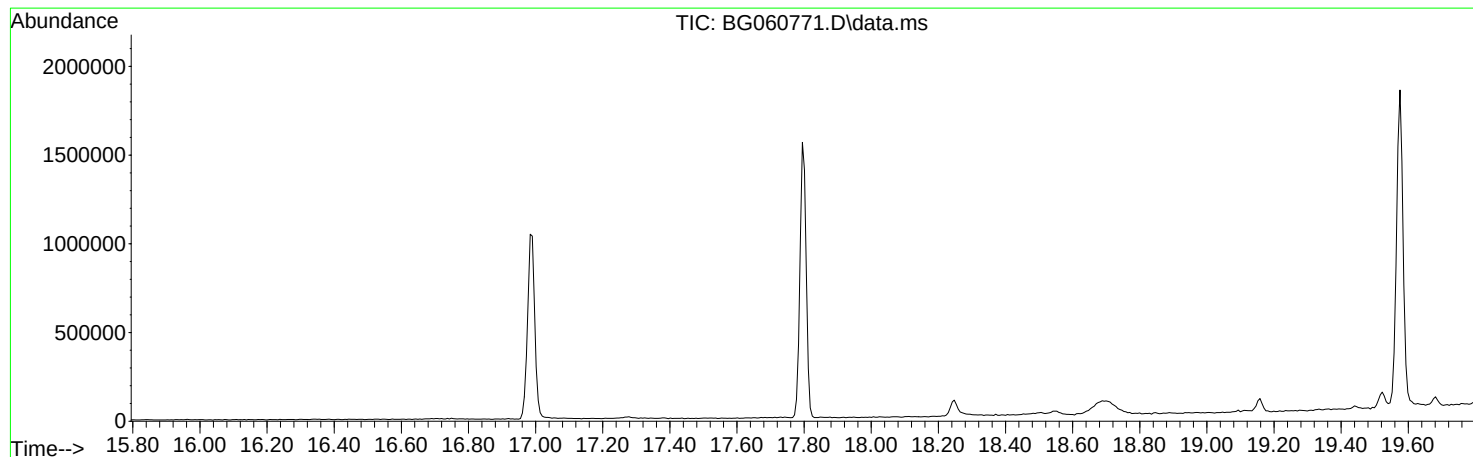




AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2512

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	46.8	69035	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.6	51129	PASS
70	69	0.00	2	0.0	18	PASS
127	198	10	80	41.1	60699	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	147667	PASS
199	198	5	9	6.7	9843	PASS
275	198	10	60	29.5	43557	PASS
365	198	1	100	4.5	6611	PASS
441	198	0.01	100	14.1	20888	PASS
442	442	50	100	100.0	121984	PASS
443	442	15	24	20.0	24349	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040424\
Data File : BG060771.D
Acq On : 4 Apr 2024 9:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 04 10:55:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

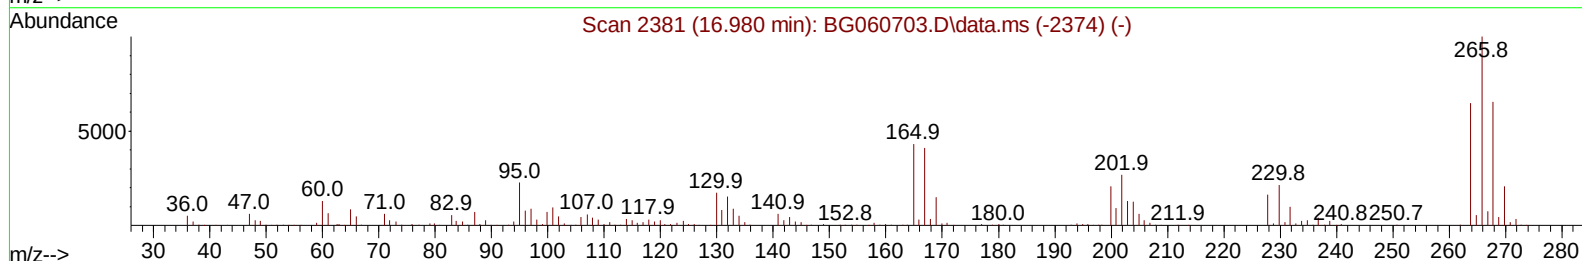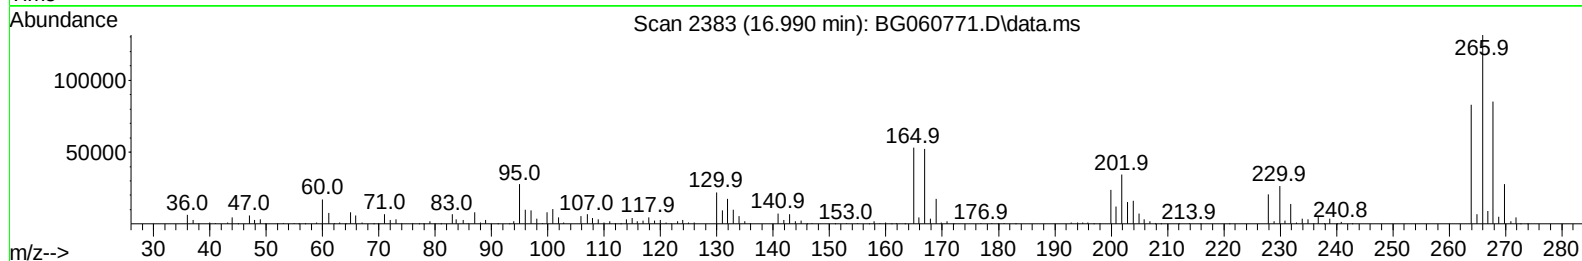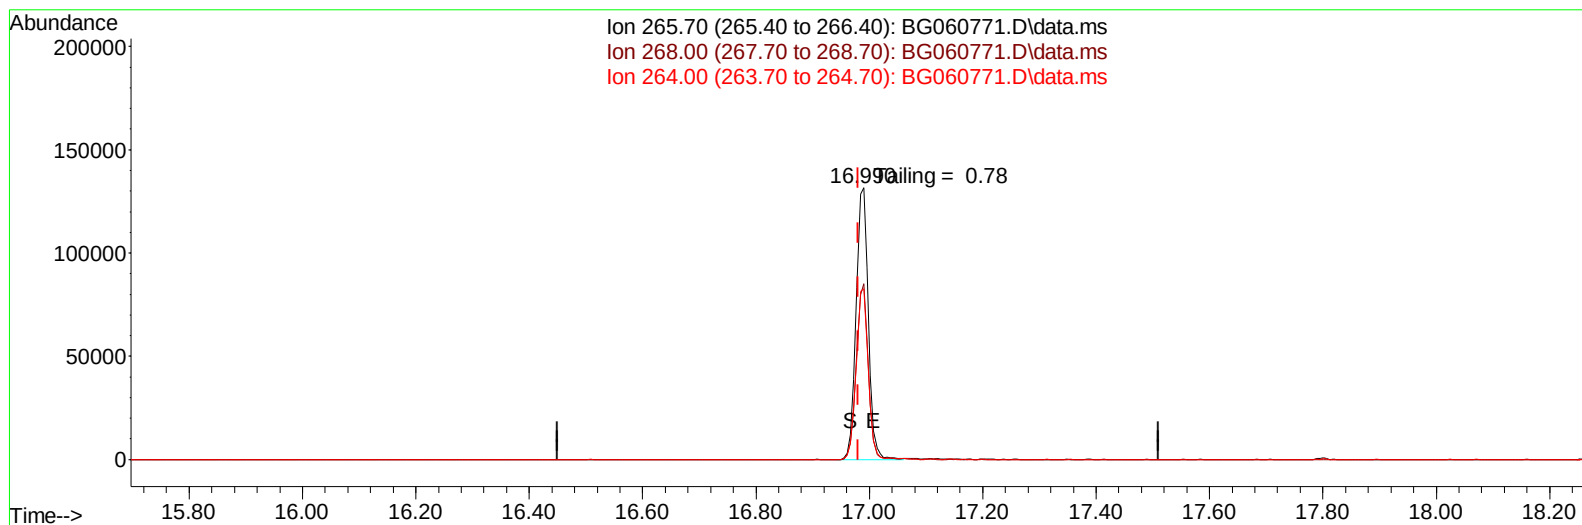

TIC: BG060771.D\data.ms

(70) Pentachlorophenol (C)

16.990min (+ 0.010) 404126.54 ng




response 196366

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	64.83
264.00	64.70	62.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040424\
Data File : BG060771.D
Acq On : 4 Apr 2024 9:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 04 10:55:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

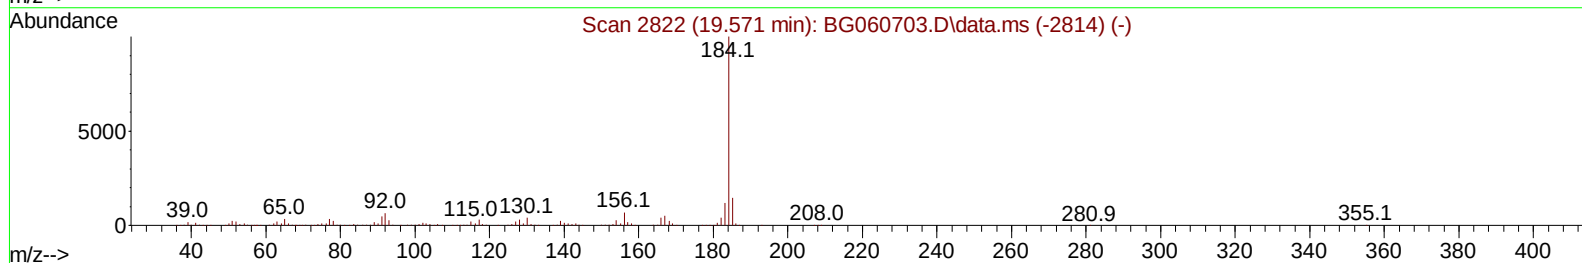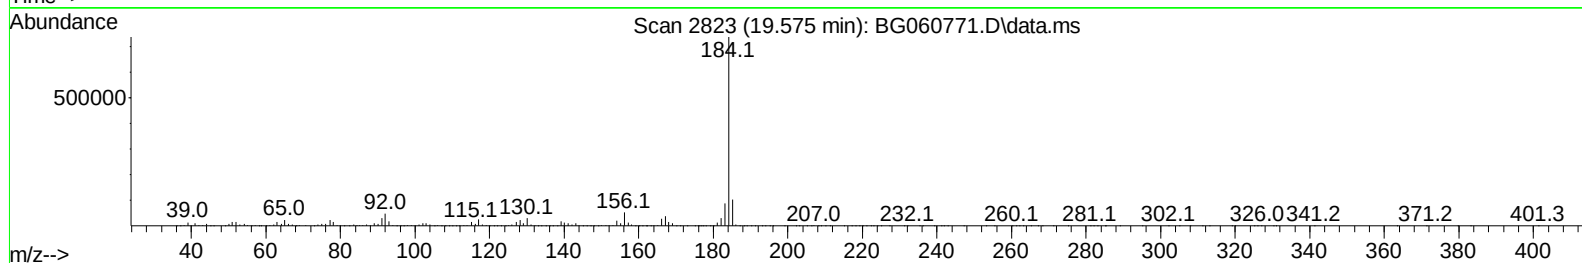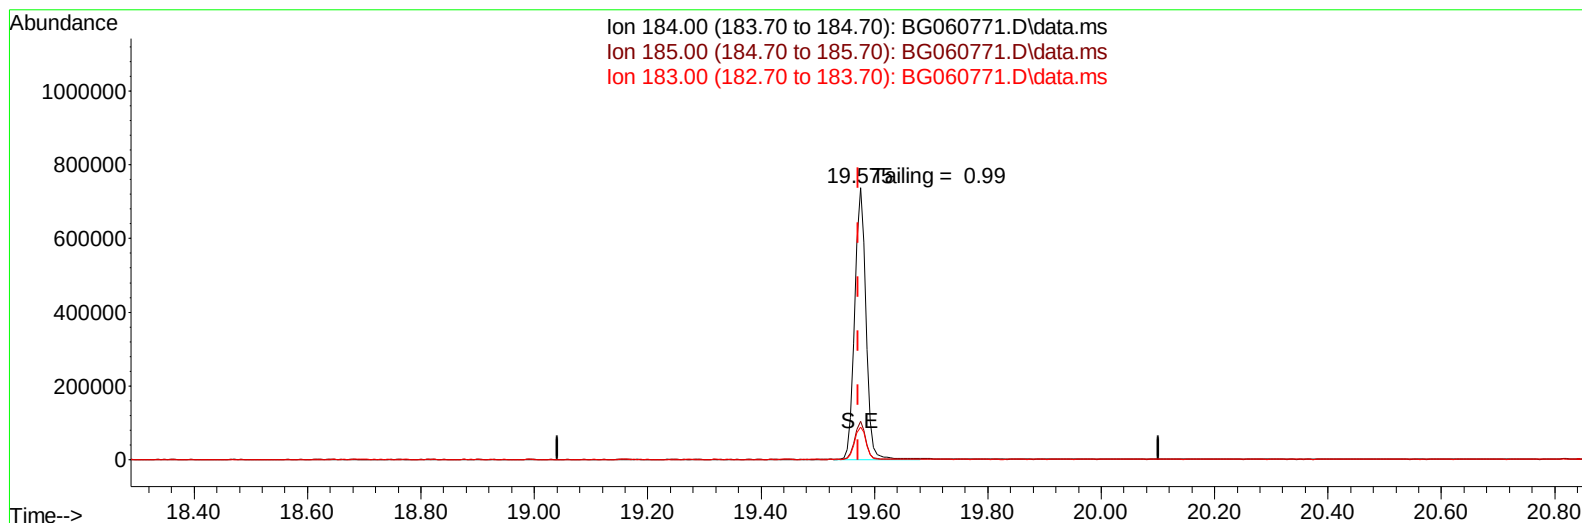

TIC: BG060771.D\data.ms

(77) Benzidine

19.575min (+ 0.004) 185798.76 ng

response 1012744

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.02
183.00	11.90	12.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/4/2024	BNA_G	<u>BG060771.D</u>
Compound Name	Response	Retention Time
DDT	535411	20.821
DDD	14959	20.374
DDE	0	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14959	550370	2.72

Instrument :
BNA_G
ClientSampleId :
DFTPP