
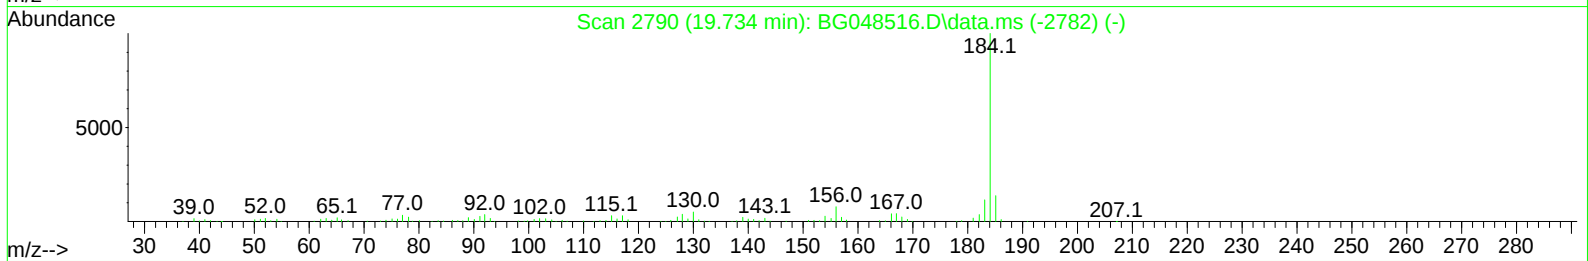
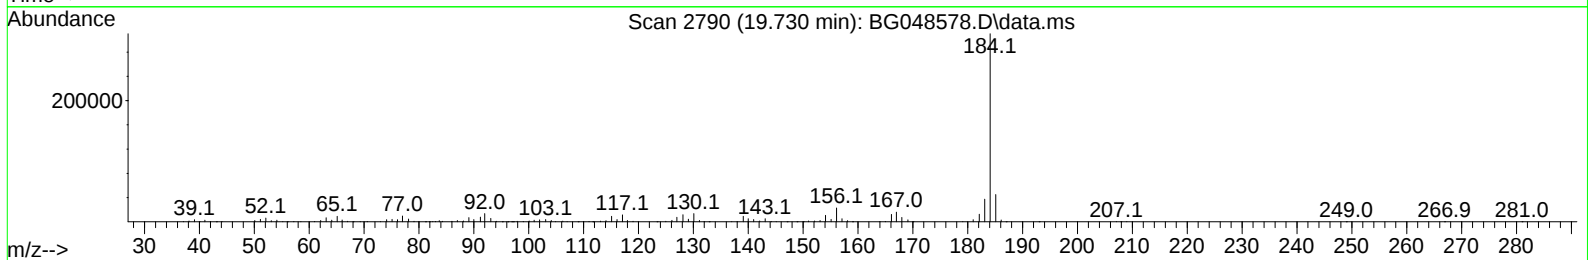


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040521\
Data File : BG048578.D
Acq On : 5 Apr 2021 10:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 11:49:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 02 10:20:56 2021
Response via : Initial Calibration

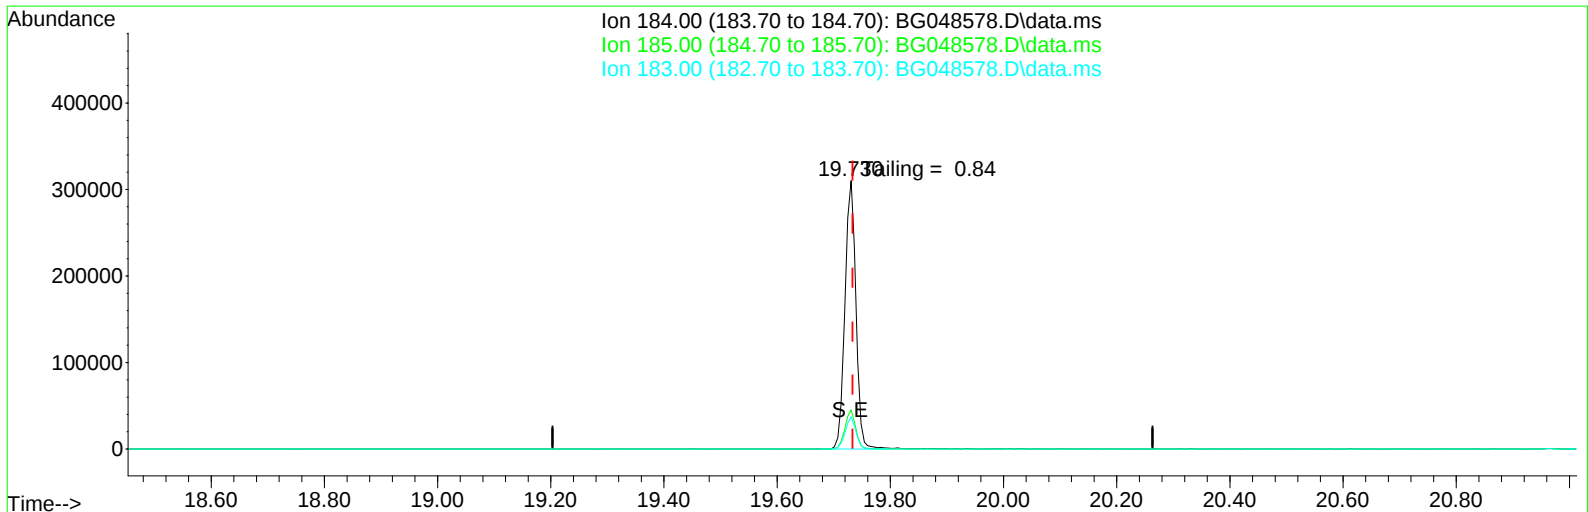




TIC: BG048578.D\data.ms

(77) Benzidine**19.730min (-0.003) 90654.82 ng****response 417499**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.54
183.00	11.50	12.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040521\
 Data File : BG048578.D
 Acq On : 5 Apr 2021 10:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 11:49:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 02 10:20:56 2021
 Response via : Initial Calibration

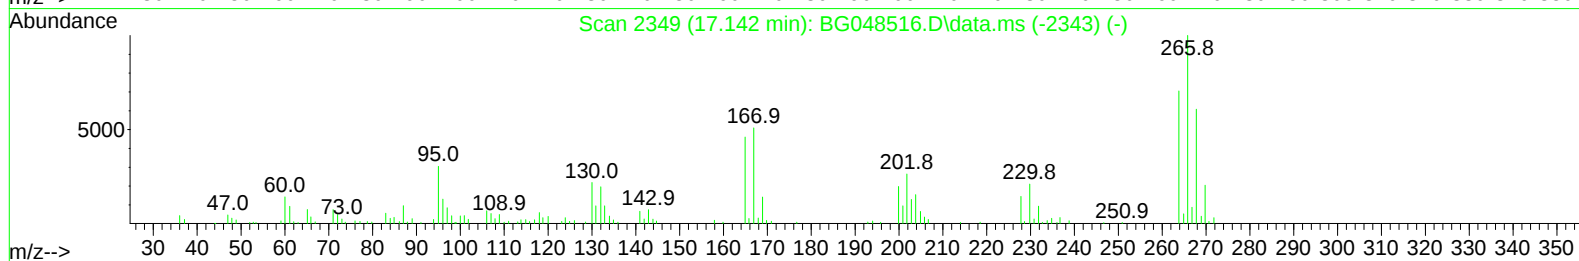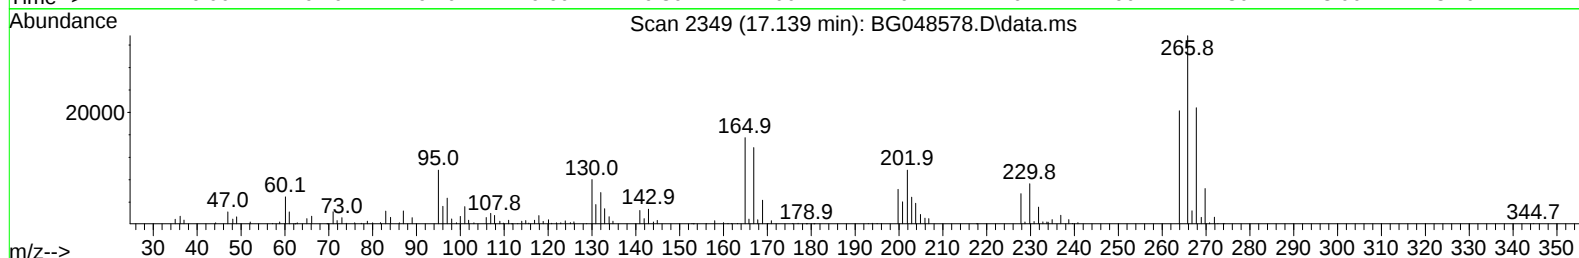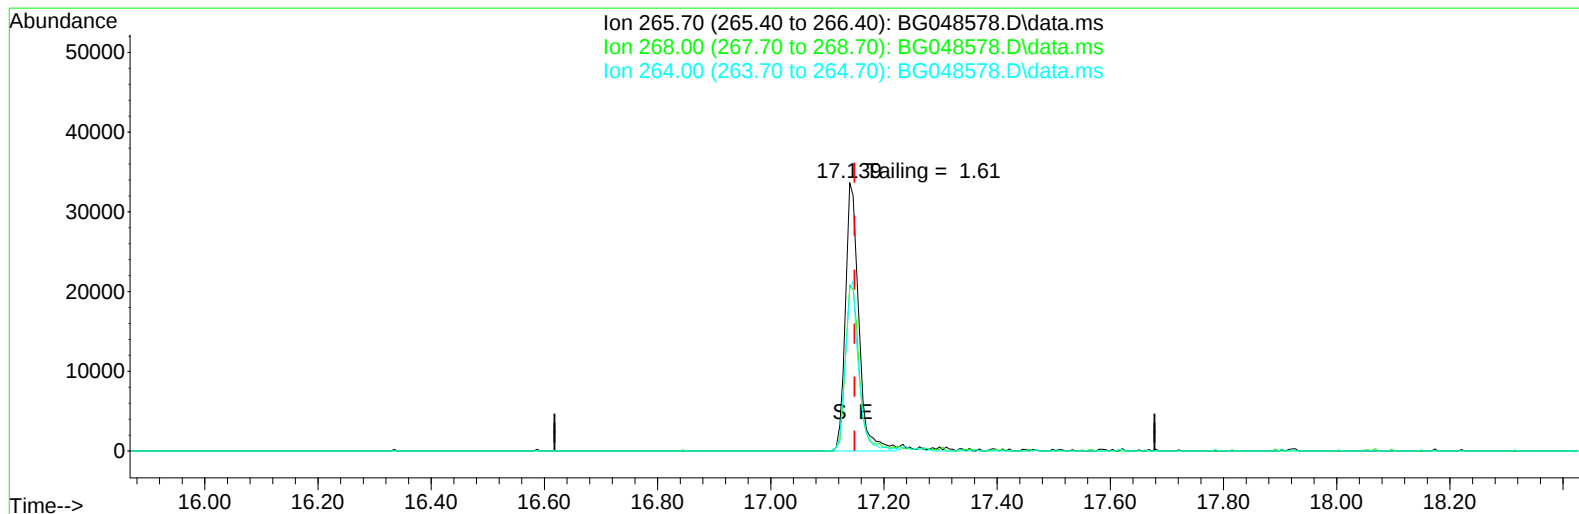

TIC: BG048578.D\data.ms

(70) Pentachlorophenol (C)

17.139min (-0.008) 18992.83 ng

response 55339

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	61.88
264.00	70.50	60.27
0.00	0.00	0.00