

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040521\
 Data File : BG048594.D
 Acq On : 5 Apr 2021 22:01
 Operator : CG/JU
 Sample : M1836-12DL 2X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B5-19-21DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.738	65	68	76	rVB5	24322	45616	1.46%	0.107%
2	3.984	101	110	121	rBV	80535	196151	6.28%	0.462%
3	4.078	121	126	132	rVV	116172	238391	7.63%	0.562%
4	4.125	132	134	144	rVB3	38556	79636	2.55%	0.188%
5	4.231	144	152	164	rBV2	74432	158815	5.09%	0.374%
6	4.337	165	170	179	rBV	72598	131168	4.20%	0.309%
7	4.578	207	211	223	rVB3	47797	99629	3.19%	0.235%
8	5.095	294	299	302	rBV2	28312	49779	1.59%	0.117%
9	5.512	364	370	371	rBV3	52693	81621	2.61%	0.192%
10	5.577	376	381	388	rVV	553921	1035915	33.17%	2.440%
11	5.641	388	392	398	rVV2	284094	503553	16.12%	1.186%
12	5.712	398	404	421	rVB	1055633	2794566	89.49%	6.584%
13	5.847	421	427	437	rBV3	43412	102896	3.29%	0.242%
14	6.082	453	467	479	rVB	680582	1336709	42.80%	3.149%
15	6.346	506	512	522	rBV3	54530	129816	4.16%	0.306%
16	6.464	525	532	541	rVB4	35026	80311	2.57%	0.189%
17	6.564	541	549	556	rBV2	156798	333589	10.68%	0.786%
18	6.628	556	560	566	rVV2	39194	67505	2.16%	0.159%
19	6.716	570	575	583	rVV6	44716	94290	3.02%	0.222%
20	6.957	610	616	618	rBV2	30466	52889	1.69%	0.125%
21	7.069	625	635	641	rBV2	703917	1392668	44.60%	3.281%
22	7.128	641	645	647	rVV	81525	113616	3.64%	0.268%
23	7.175	647	653	658	rVV	809423	1398087	44.77%	3.294%
24	7.239	658	664	670	rVV2	685790	1381047	44.22%	3.254%
25	7.310	670	676	686	rVB	621531	1066669	34.16%	2.513%
26	7.421	688	695	699	rBV	50242	102464	3.28%	0.241%
27	7.480	699	705	712	rVB	430329	727895	23.31%	1.715%
28	7.615	724	728	730	rBV3	43844	63786	2.04%	0.150%
29	7.739	739	749	758	rBV	1759748	3122849	100.00%	7.357%
30	7.968	783	788	789	rBV	31139	46908	1.50%	0.111%
31	7.991	790	792	799	rVB2	66406	96225	3.08%	0.227%
32	8.074	799	806	814	rBV2	246382	593634	19.01%	1.399%
33	8.132	814	816	820	rVB	46312	49121	1.57%	0.116%
34	8.209	824	829	837	rVB2	620801	1106245	35.42%	2.606%
35	8.326	843	849	856	rBV	284192	494592	15.84%	1.165%
36	8.473	867	874	886	rVB	430523	786755	25.19%	1.853%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040521\
 Data File : BG048594.D
 Acq On : 5 Apr 2021 22:01
 Operator : CG/JU
 Sample : M1836-12DL 2X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B5-19-21DL

Integration Parameters: rteint.p

Integrator: RTE

Smoother: ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	8.585	886	893	897	rBV2	314739	551112	17.65%	1.298%
38	8.644	897	903	913	rVB3	498728	1036860	33.20%	2.443%
39	8.738	913	919	932	rVB3	709976	1605574	51.41%	3.783%
40	8.849	932	938	942	rBV4	49801	93506	2.99%	0.220%
41	8.902	942	947	953	rVB	169998	261770	8.38%	0.617%
42	8.978	954	960	963	rBV	104155	166608	5.34%	0.393%
43	9.055	968	973	977	rVV	247057	413670	13.25%	0.975%
44	9.108	977	982	989	rVV2	214898	411708	13.18%	0.970%
45	9.208	993	999	1005	rVV	890630	1551789	49.69%	3.656%
46	9.290	1005	1013	1030	rVB4	274488	947064	30.33%	2.231%
47	9.454	1030	1041	1050	rBV5	88987	222907	7.14%	0.525%
48	9.543	1050	1056	1074	rVV3	124231	358122	11.47%	0.844%
49	9.678	1074	1079	1083	rVV2	56098	109883	3.52%	0.259%
50	9.736	1083	1089	1094	rVV	490027	838417	26.85%	1.975%
51	9.795	1094	1099	1105	rVV	372462	637449	20.41%	1.502%
52	9.995	1124	1133	1137	rVV	121182	214754	6.88%	0.506%
53	10.036	1137	1140	1145	rVV2	67427	104267	3.34%	0.246%
54	10.107	1145	1152	1156	rVV3	117280	238760	7.65%	0.562%
55	10.159	1156	1161	1172	rVV	325830	713579	22.85%	1.681%
56	10.259	1172	1178	1181	rVV3	83299	170579	5.46%	0.402%
57	10.312	1181	1187	1193	rVV2	638639	1234433	39.53%	2.908%
58	10.377	1194	1198	1203	rVV4	156010	297186	9.52%	0.700%
59	10.430	1203	1207	1210	rVV4	39848	80966	2.59%	0.191%
60	10.494	1210	1218	1223	rVV4	120672	267315	8.56%	0.630%
61	10.547	1223	1227	1230	rVV3	41318	69009	2.21%	0.163%
62	10.612	1233	1238	1246	rVB	139433	246675	7.90%	0.581%
63	10.900	1278	1287	1289	rBV4	169367	419260	13.43%	0.988%
64	10.970	1294	1299	1305	rVV2	490584	1026053	32.86%	2.417%
65	11.029	1305	1309	1313	rVB	73120	106411	3.41%	0.251%
66	11.129	1321	1326	1334	rVB2	99891	165535	5.30%	0.390%
67	11.323	1356	1359	1366	rVV5	27215	53805	1.72%	0.127%
68	11.387	1366	1370	1378	rVB10	19303	49500	1.59%	0.117%
69	11.528	1389	1394	1398	rBV8	23719	49350	1.58%	0.116%
70	11.581	1398	1403	1407	rVV2	79969	137663	4.41%	0.324%
71	11.628	1407	1411	1417	rVB6	33617	61389	1.97%	0.145%
72	11.752	1426	1432	1439	rVB7	33440	76895	2.46%	0.181%
73	11.834	1439	1446	1452	rBV2	136863	249748	8.00%	0.588%
74	12.022	1473	1478	1484	rVB2	73394	120760	3.87%	0.284%
75	12.110	1488	1493	1501	rBV7	41949	110847	3.55%	0.261%
76	12.239	1507	1515	1521	rVB2	45716	88236	2.83%	0.208%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040521\
 Data File : BG048594.D
 Acq On : 5 Apr 2021 22:01
 Operator : CG/JU
 Sample : M1836-12DL 2X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B5-19-21DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	12.304	1521	1526	1528	rBV2	55805	100259	3.21%	0.236%
78	12.574	1561	1572	1581	rVB	559165	975006	31.22%	2.297%
79	12.798	1599	1610	1619	rBV	273996	531560	17.02%	1.252%
80	13.367	1697	1707	1713	rBV	446404	679585	21.76%	1.601%
81	13.555	1735	1739	1747	rVB5	25925	49152	1.57%	0.116%
82	13.773	1770	1776	1785	rVB2	39796	87738	2.81%	0.207%
83	13.908	1793	1799	1800	rBV	63256	94388	3.02%	0.222%
84	14.067	1818	1826	1831	rBV	92629	182586	5.85%	0.430%
85	14.120	1831	1835	1841	rVB2	56200	84582	2.71%	0.199%
86	14.302	1861	1866	1870	rBV3	34664	63518	2.03%	0.150%
87	14.748	1929	1942	1949	rBV	337842	573038	18.35%	1.350%
88	14.825	1949	1955	1959	rVB5	26314	52694	1.69%	0.124%
89	14.954	1971	1977	1985	rBV3	23404	52027	1.67%	0.123%
90	15.142	2005	2009	2014	rVB3	32731	50962	1.63%	0.120%
91	16.235	2187	2195	2203	rBV	339917	539836	17.29%	1.272%
92	17.498	2403	2410	2415	rBV	399013	623118	19.95%	1.468%
93	17.539	2415	2417	2424	rVB2	72635	102194	3.27%	0.241%
94	18.379	2556	2560	2564	rBV6	49269	72010	2.31%	0.170%
95	19.548	2756	2759	2764	rVB	52263	71943	2.30%	0.169%
96	19.601	2765	2768	2772	rVB3	50600	64692	2.07%	0.152%
97	19.913	2819	2821	2826	rVB2	43254	57232	1.83%	0.135%
98	20.107	2850	2854	2860	rVB	601231	767077	24.56%	1.807%
99	21.799	3136	3142	3148	rBV	271739	457301	14.64%	1.077%
100	25.142	3707	3711	3722	rVB3	153975	399958	12.81%	0.942%




Sum of corrected areas: 42447276

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040521\
Data File : BG048594.D
Acq On : 5 Apr 2021 22:01
Operator : CG/JU
Sample : M1836-12DL 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :
B5-19-21DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

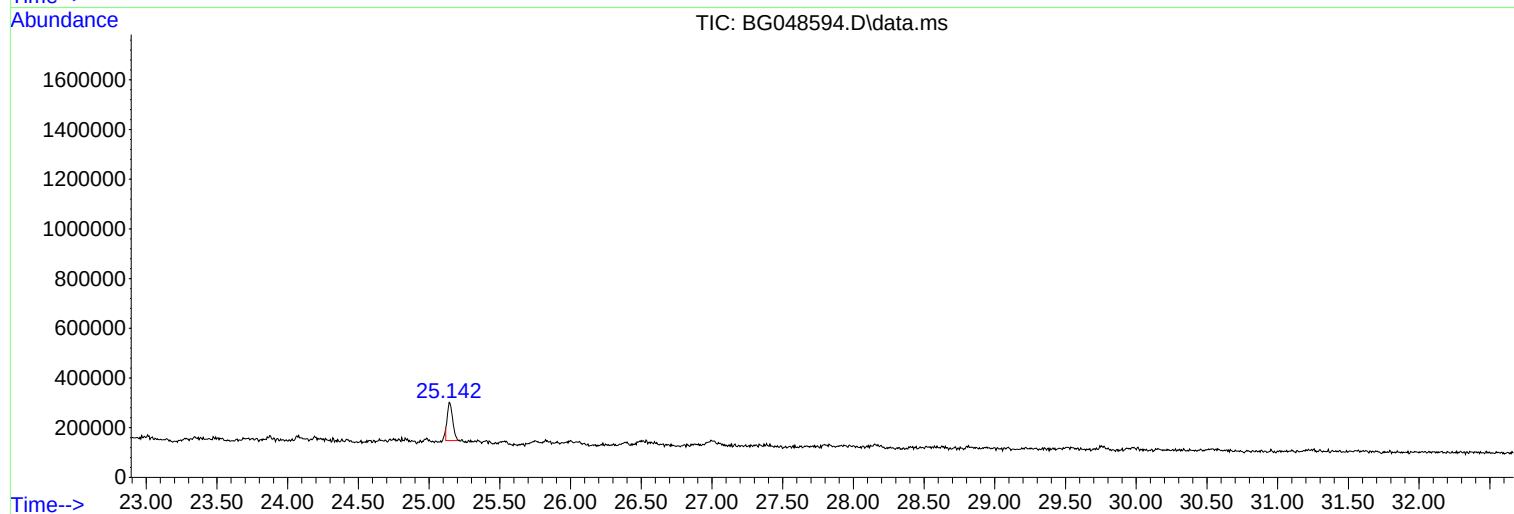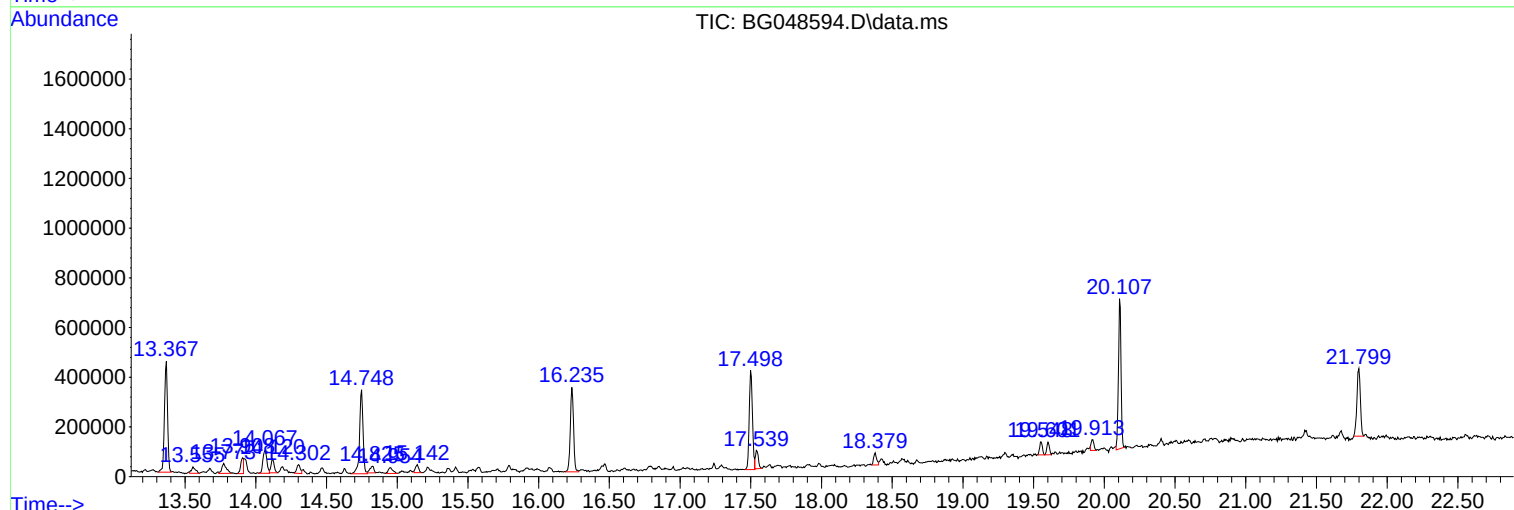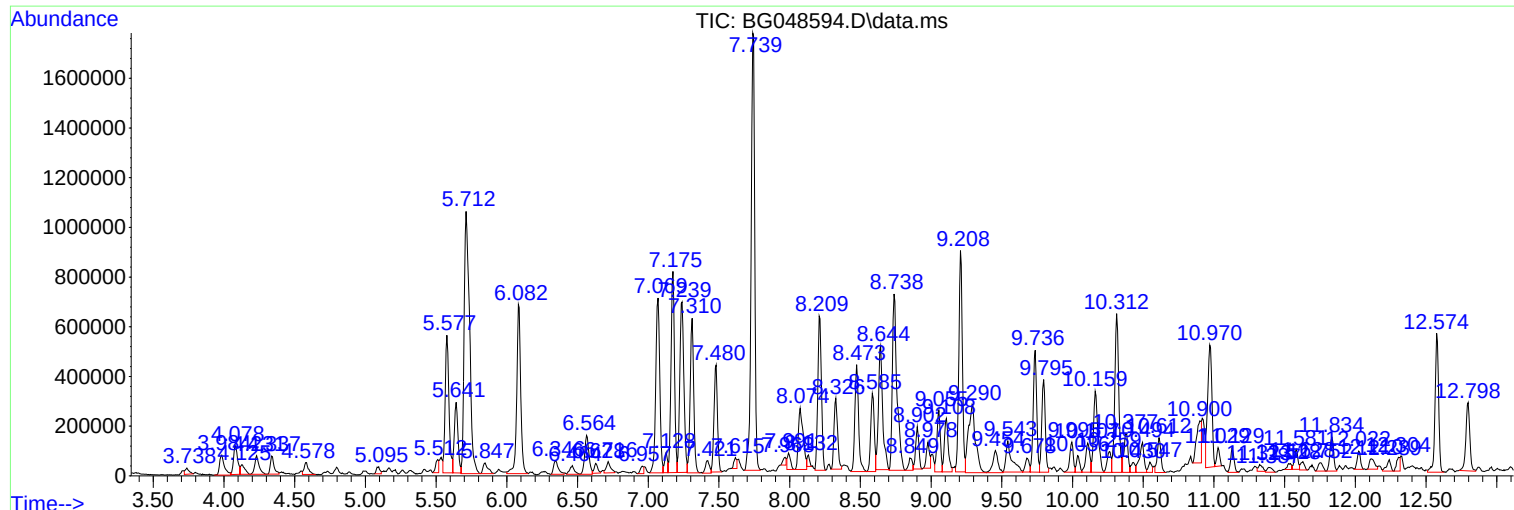

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040521\
Data File : BG048594.D
Acq On : 5 Apr 2021 22:01
Operator : CG/JU
Sample : M1836-12DL 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B5-19-21DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040521\
Data File : BG048594.D
Acq On : 5 Apr 2021 22:01
Operator : CG/JU
Sample : M1836-12DL 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B5-19-21DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------