
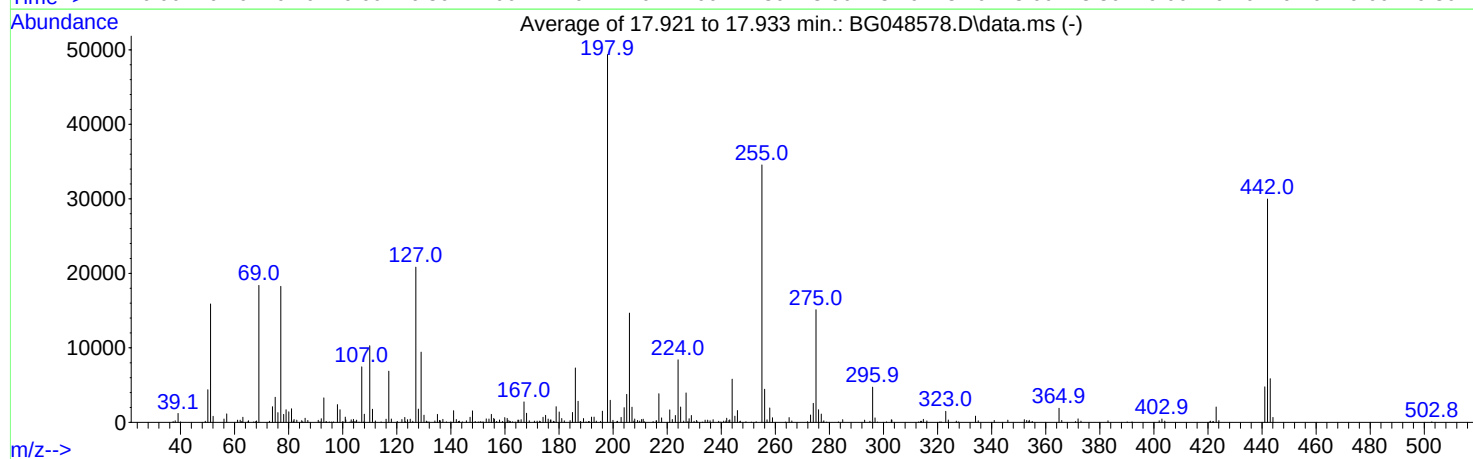


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040521\
 Data File : BG048578.D
 Acq On : 5 Apr 2021 10:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 02 10:20:56 2021

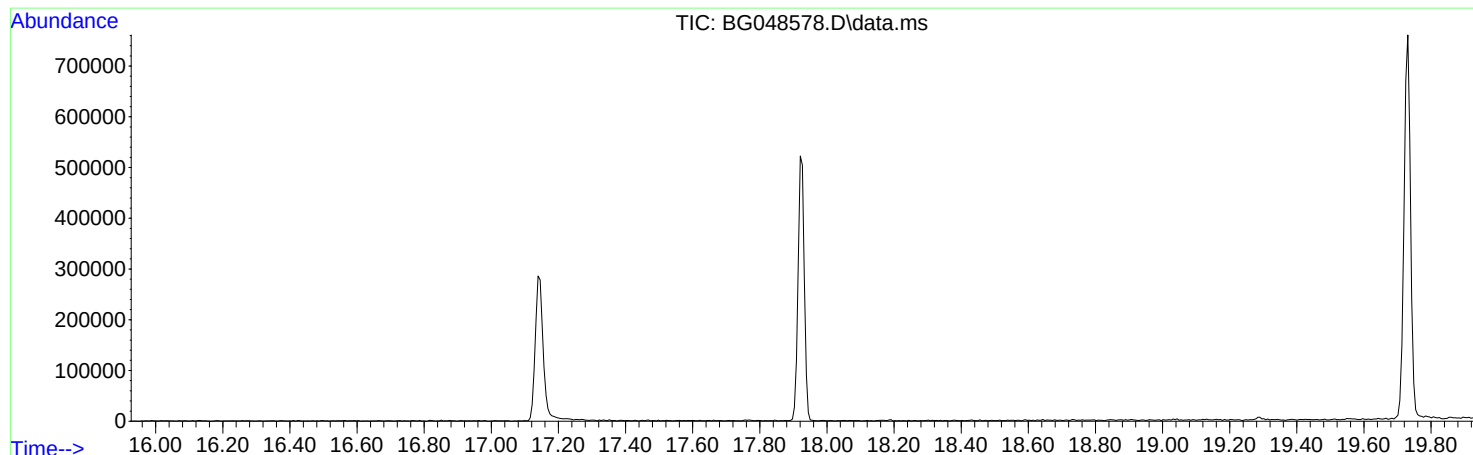




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	15901	PASS
68	69	0.00	2	1.0	190	PASS
69	198	0.00	100	37.2	18391	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.2	20834	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49373	PASS
199	198	5	9	6.0	2970	PASS
275	198	10	60	30.6	15129	PASS
365	198	1	100	3.8	1894	PASS
441	198	0.01	100	9.7	4774	PASS
442	198	50	100	60.7	29984	PASS
443	442	15	24	19.5	5855	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040521\
Data File : BG048578.D
Acq On : 5 Apr 2021 10:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 05 11:49:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 02 10:20:56 2021
Response via : Initial Calibration

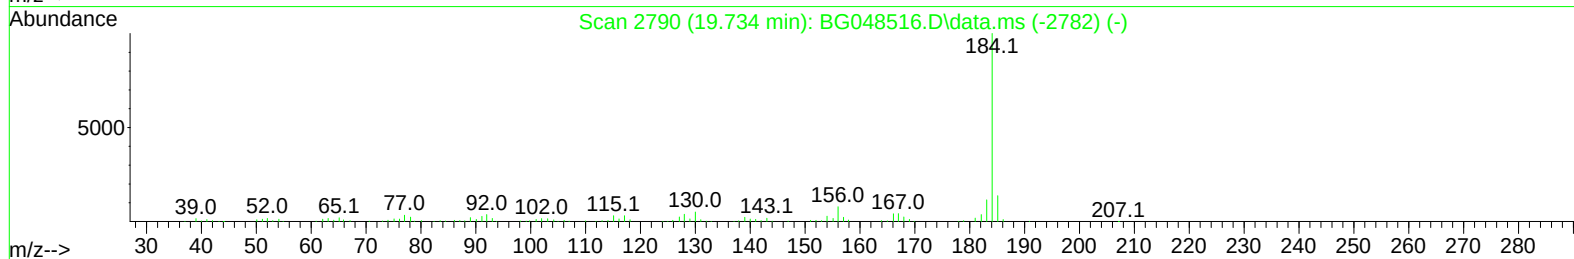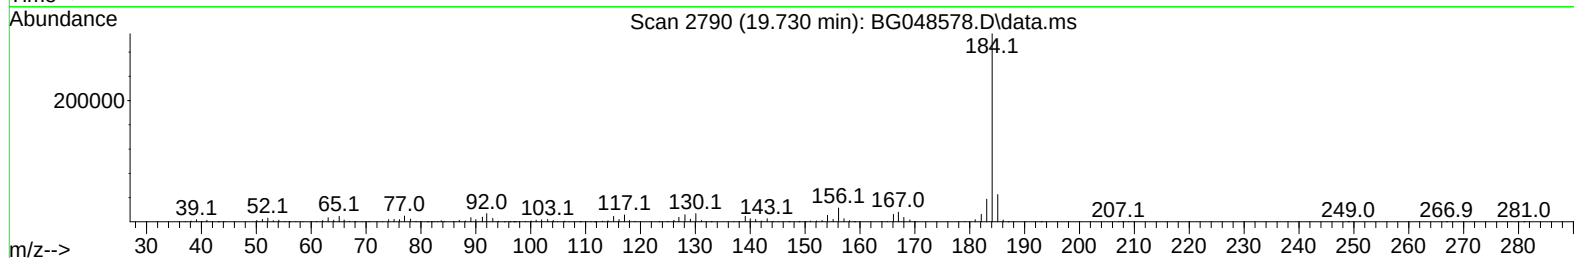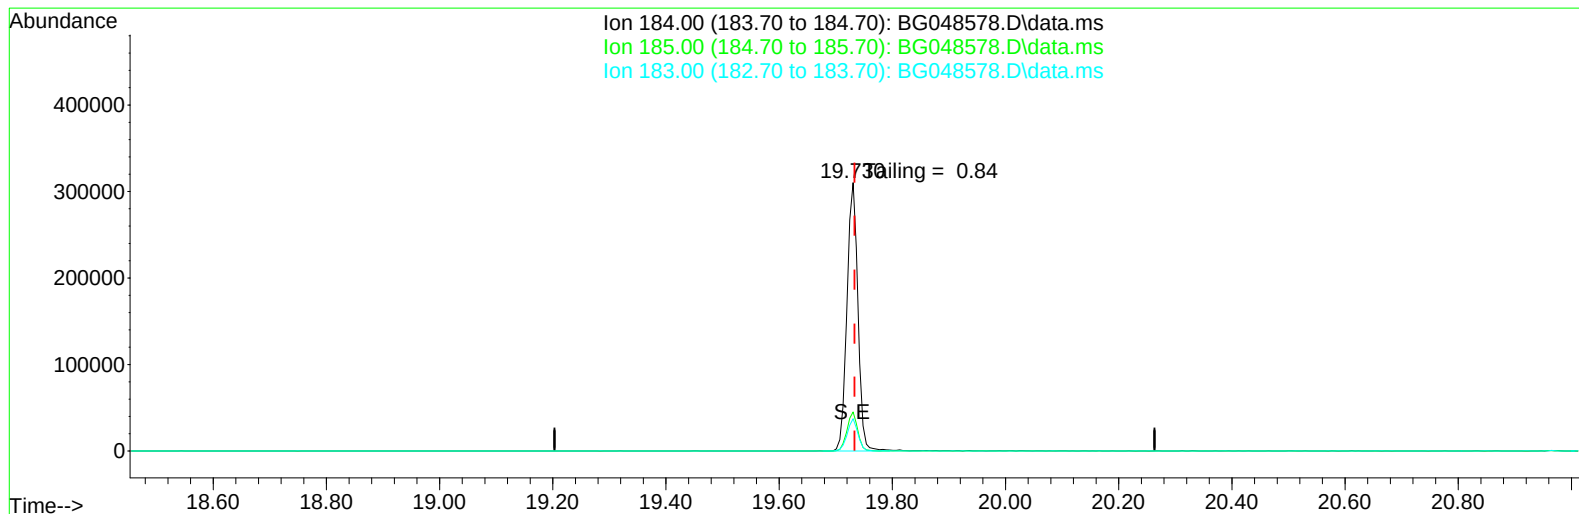

TIC: BG048578.D\data.ms

(77) Benzidine

19.730min (-0.003) 90654.82 ng




response 417499

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.54
183.00	11.50	12.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040521\
Data File : BG048578.D
Acq On : 5 Apr 2021 10:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 05 11:49:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 02 10:20:56 2021
Response via : Initial Calibration

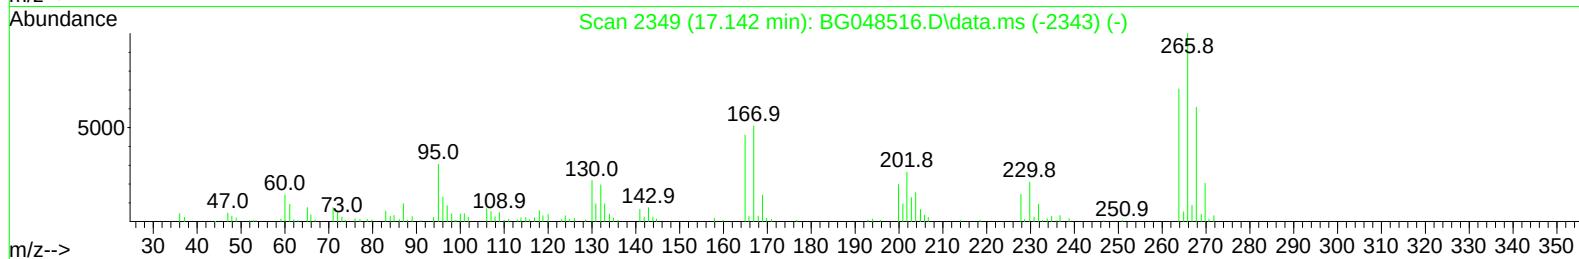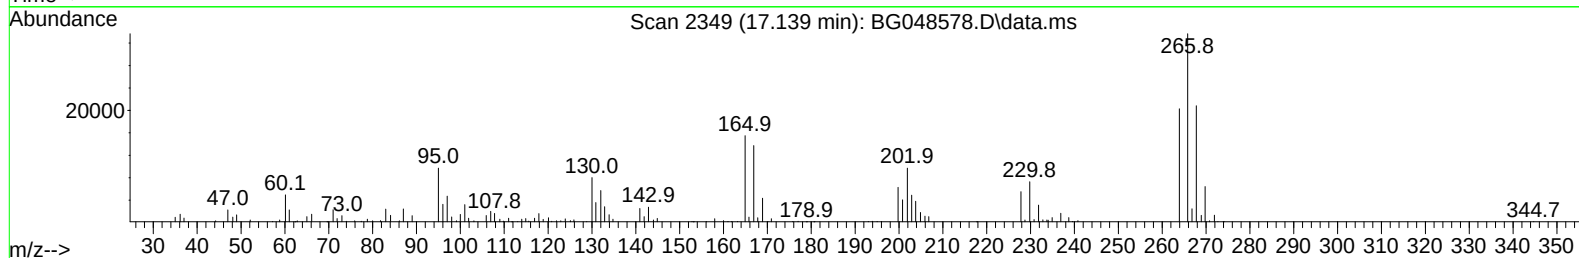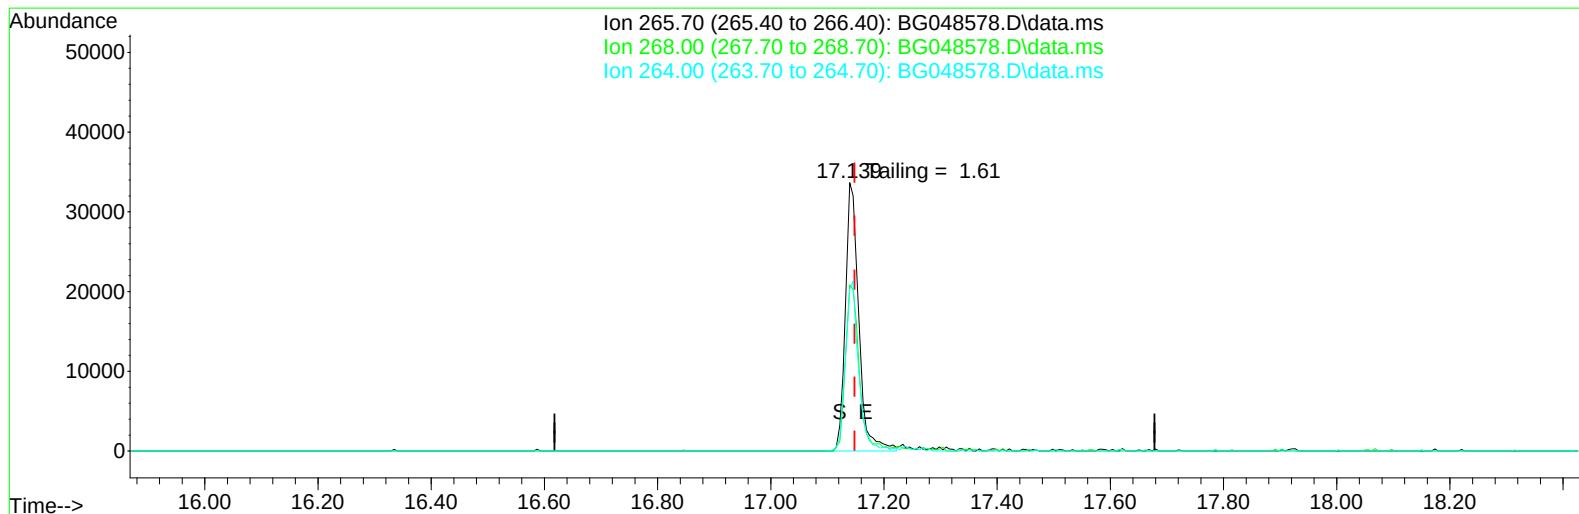

TIC: BG048578.D\data.ms

(70) Pentachlorophenol (C)

17.139min (-0.008) 18992.83 ng

response 55339

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	61.88
264.00	70.50	60.27
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/5/2021	BNA_G	BG048578.D
Compound Name	Response	Retention Time
DDT	158383	20.96
DDD	19682	20.51
DDE	545	20.02
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20227	178610	11.32