
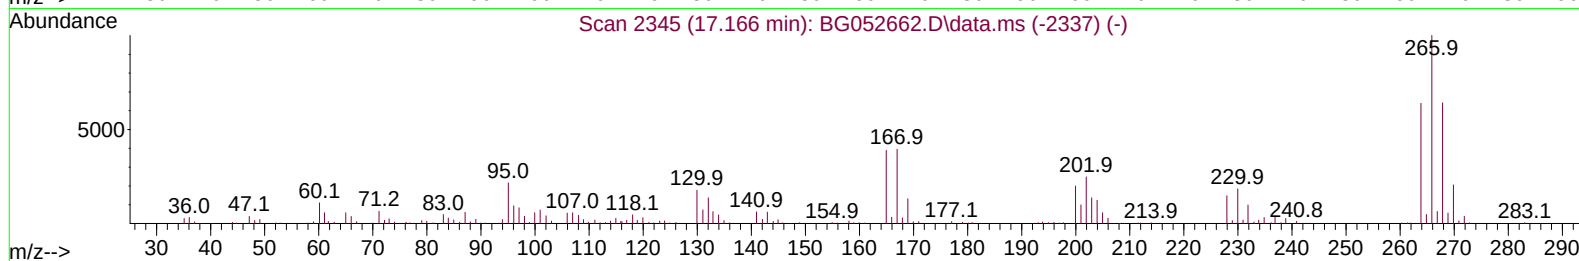
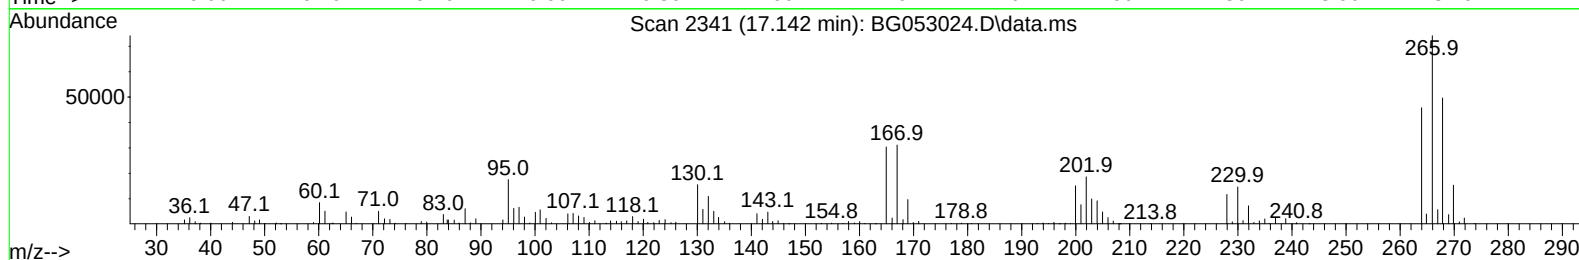


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
Data File : BG053024.D
Acq On : 5 Apr 2022 9:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 14:35:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 14:24:42 2022
Response via : Initial Calibration

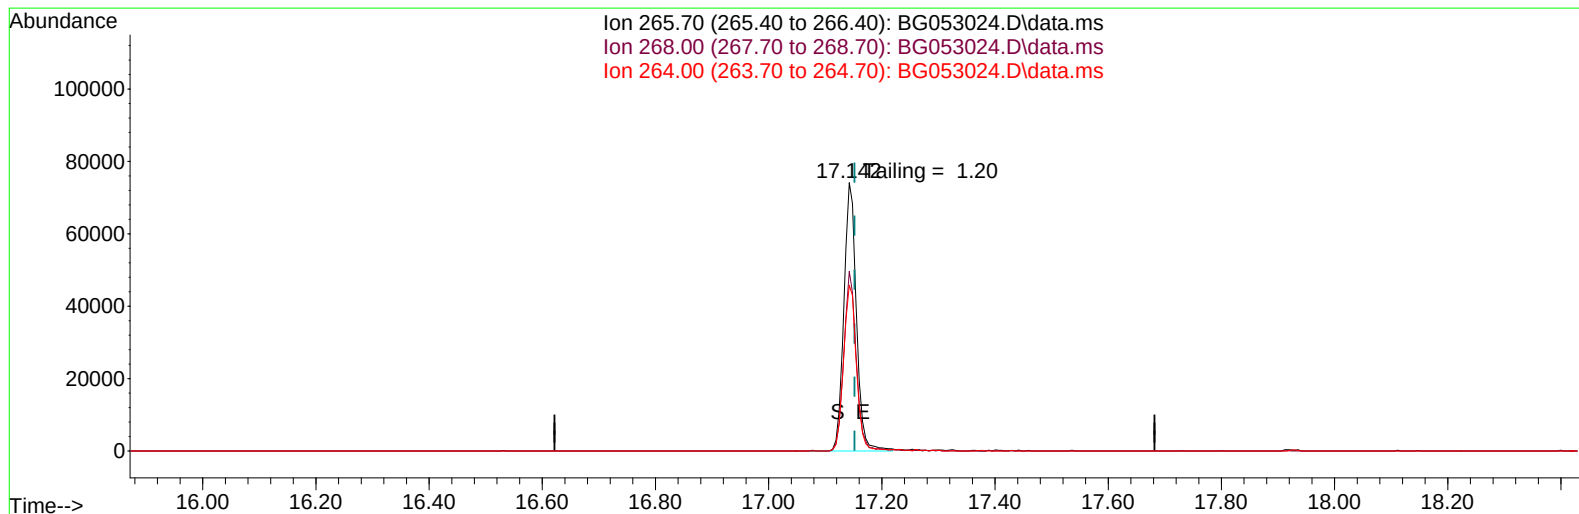

TIC: BG053024.D\data.ms

(70) Pentachlorophenol (C)




17.142min (-0.009) 18785.40 ng

response 114780

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	66.95
264.00	56.60	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
Data File : BG053024.D
Acq On : 5 Apr 2022 9:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 14:35:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 14:24:42 2022
Response via : Initial Calibration

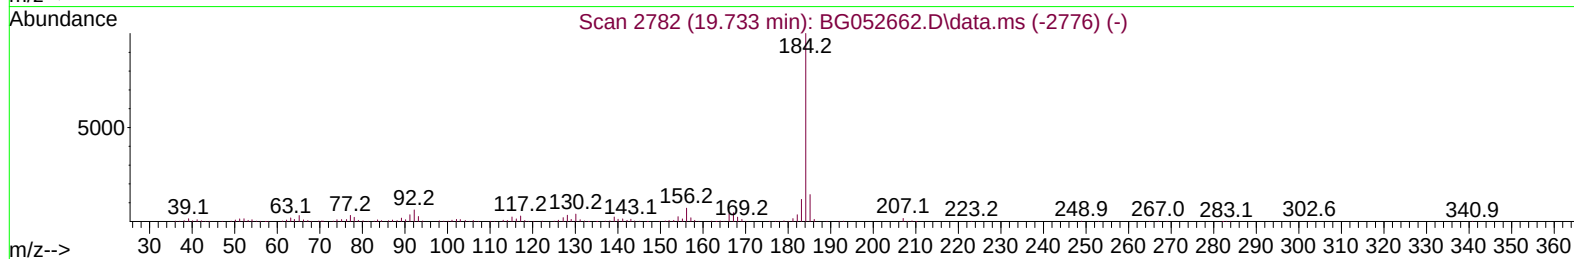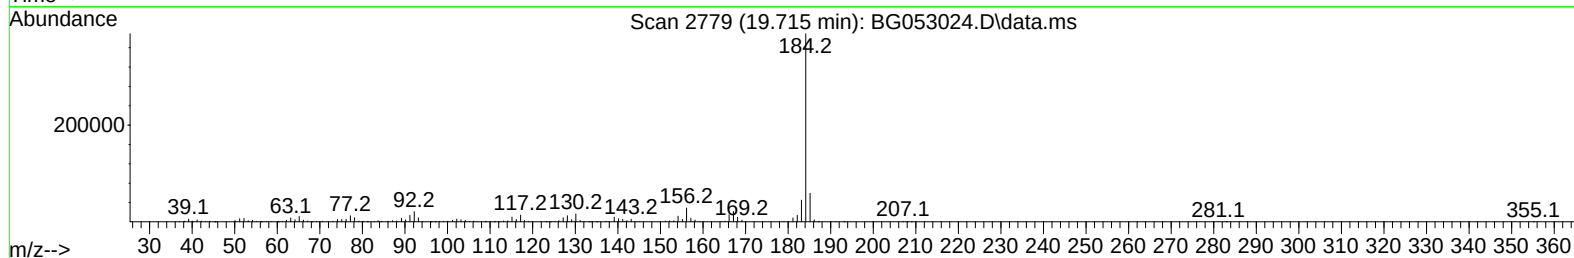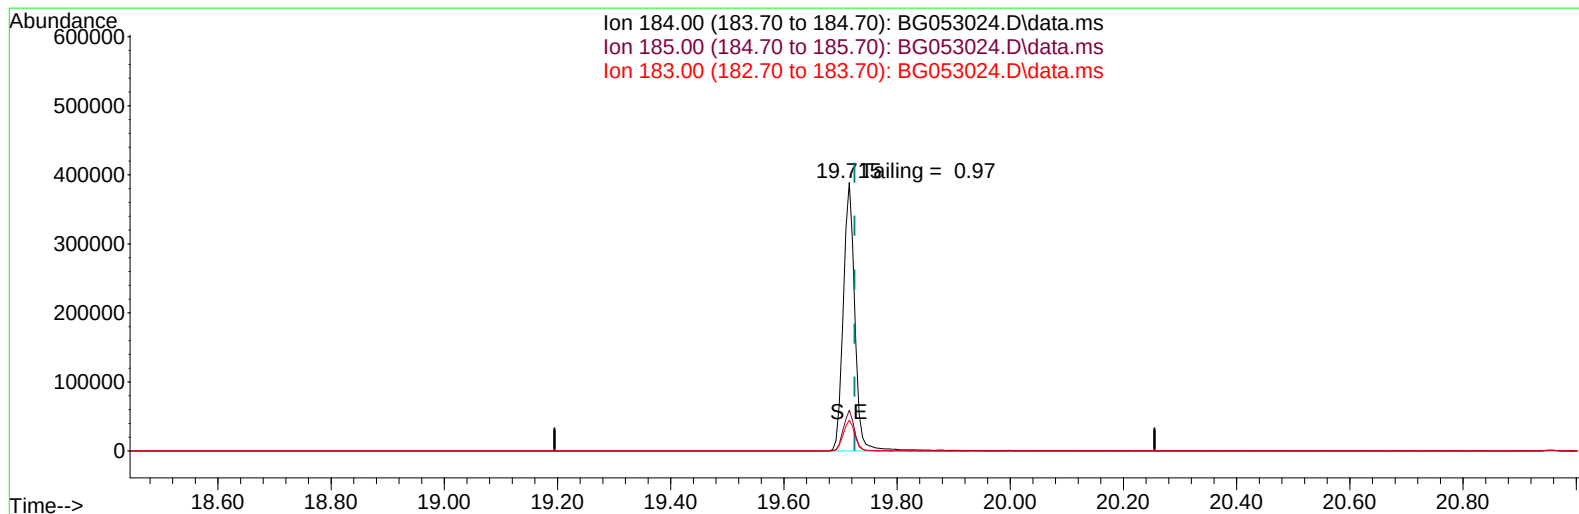

TIC: BG053024.D\data.ms

(77) Benzidine

19.715min (-0.009) 0.00 ng

response 549814

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.22
183.00	11.80	11.54
0.00	0.00	0.00