
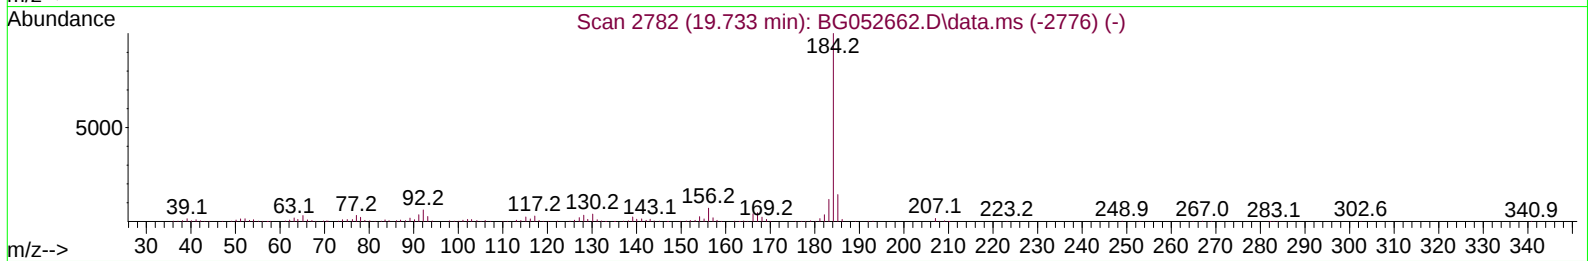
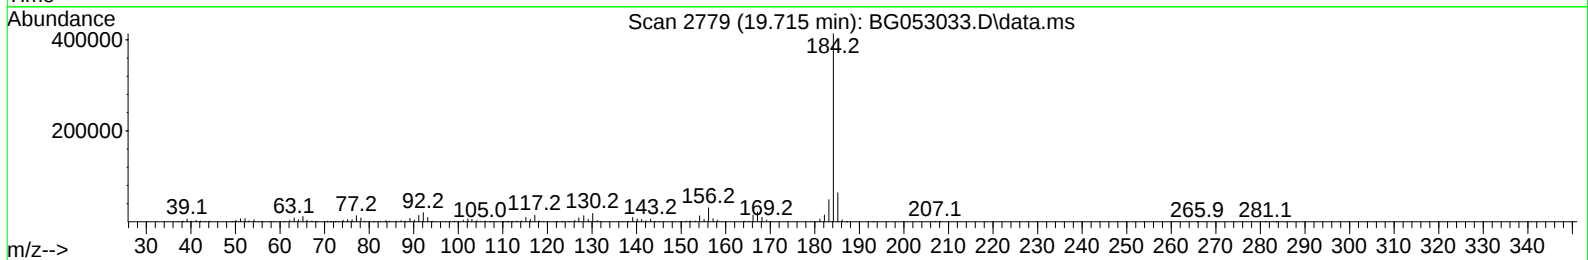


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
 Data File : BG053033.D
 Acq On : 5 Apr 2022 15:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 16:39:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 14:24:42 2022
 Response via : Initial Calibration

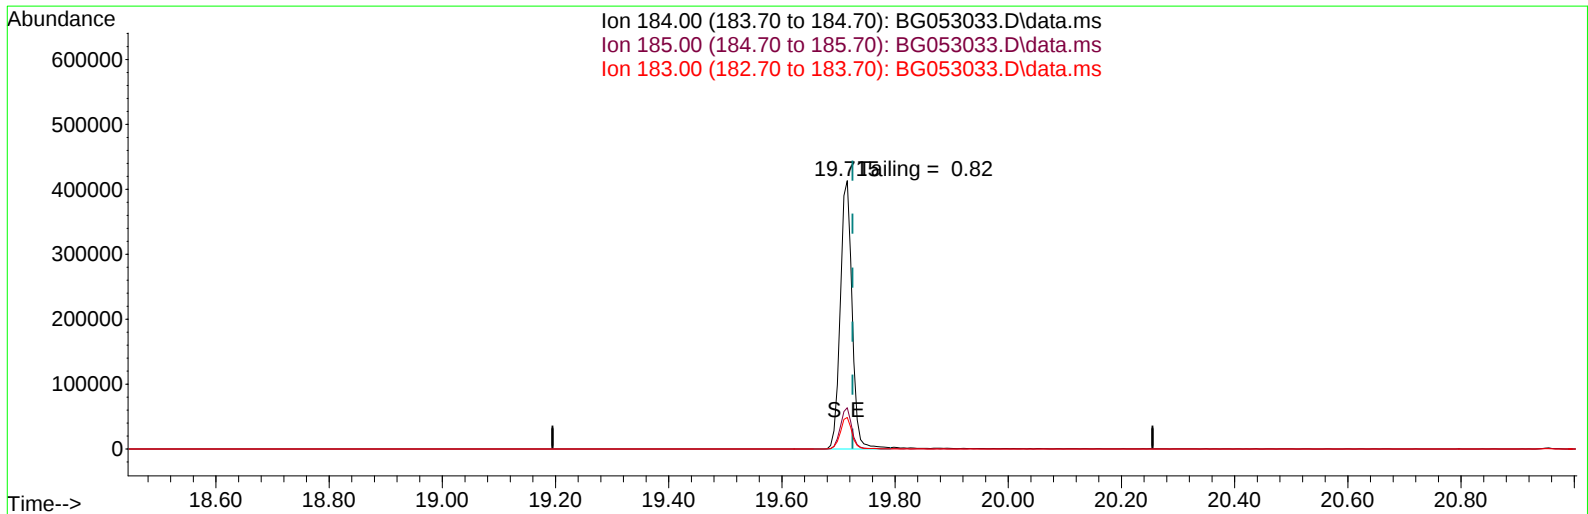




TIC: BG053033.D\data.ms

(77) Benzidine**19.715min (-0.009) 368428.44 ng****response 598658**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.42
183.00	11.80	11.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
Data File : BG053033.D
Acq On : 5 Apr 2022 15:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 16:39:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 14:24:42 2022
Response via : Initial Calibration

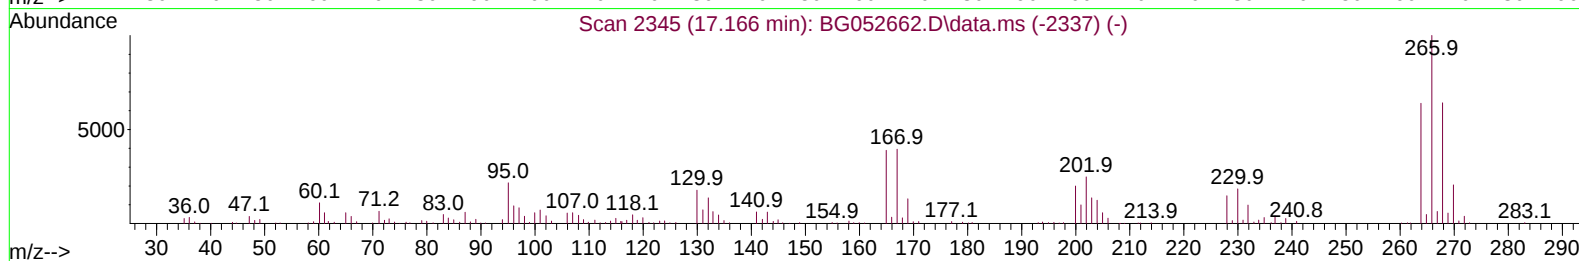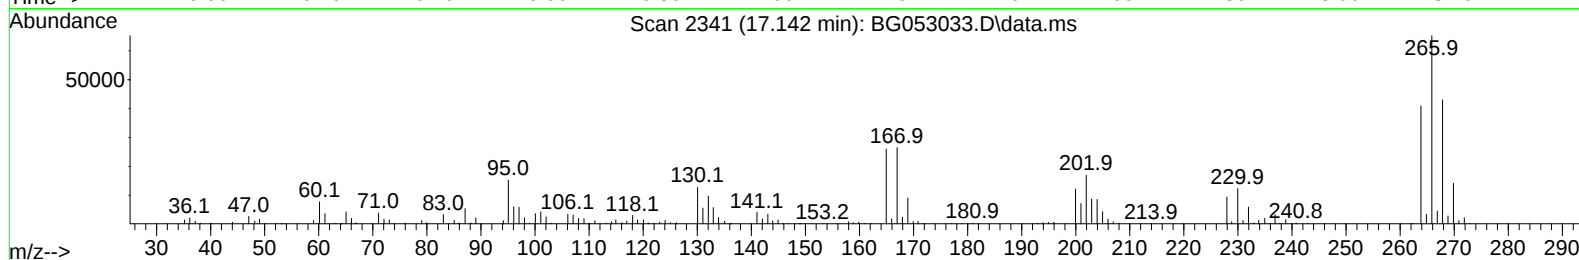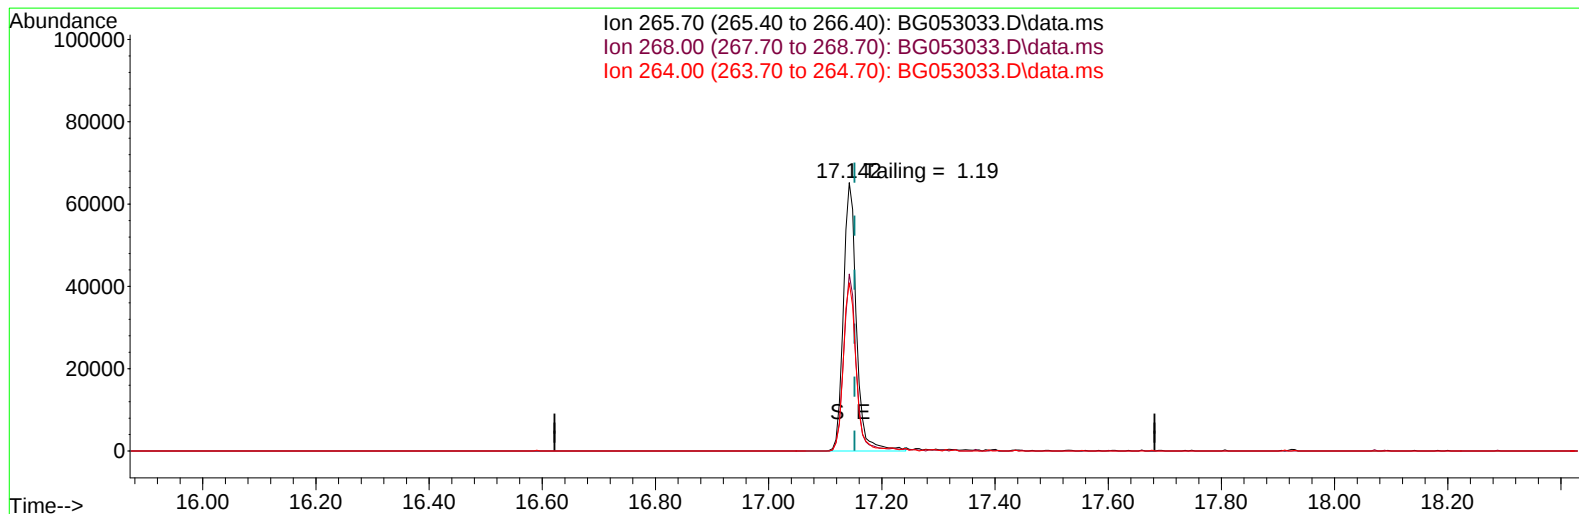

TIC: BG053033.D\data.ms

(70) Pentachlorophenol (C)

17.142min (-0.009) 25512.06 ng

response 104809

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	65.92
264.00	56.60	62.70
0.00	0.00	0.00