

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
 Data File : BG053026.D
 Acq On : 5 Apr 2022 11:13
 Operator : CG/JU
 Sample : PB143839BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB143839BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.696	386	393	406	rBV	703907	1129444	31.15%	8.635%
2	7.287	655	664	674	rBV	689512	1230636	33.94%	9.408%
3	8.133	802	808	816	rVB	119137	200644	5.53%	1.534%
4	9.291	997	1005	1013	rBV	433896	783749	21.62%	5.992%
5	10.941	1277	1286	1295	rVB	153817	279234	7.70%	2.135%
6	13.379	1693	1701	1708	rBV	1168734	1837261	50.68%	14.046%
7	14.754	1927	1935	1947	rVB	261642	416124	11.48%	3.181%
8	16.234	2180	2187	2200	rBV	1066382	1608565	44.37%	12.298%
9	17.497	2394	2402	2409	rBV	372583	574607	15.85%	4.393%
10	20.100	2838	2845	2850	rBV	2718079	3625520	100.00%	27.718%
11	21.774	3123	3130	3139	rBV	412125	698964	19.28%	5.344%
12	25.081	3682	3693	3707	rVB2	234823	695329	19.18%	5.316%




Sum of corrected areas: 13080077

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
Data File : BG053026.D
Acq On : 5 Apr 2022 11:13
Operator : CG/JU
Sample : PB143839BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143839BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

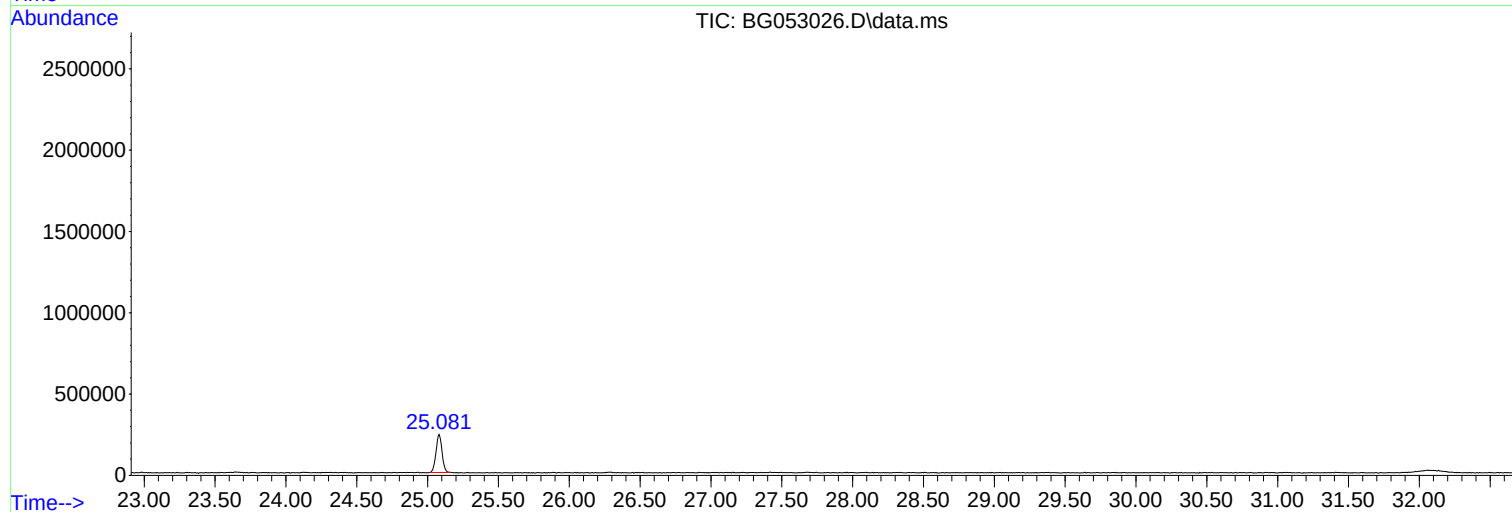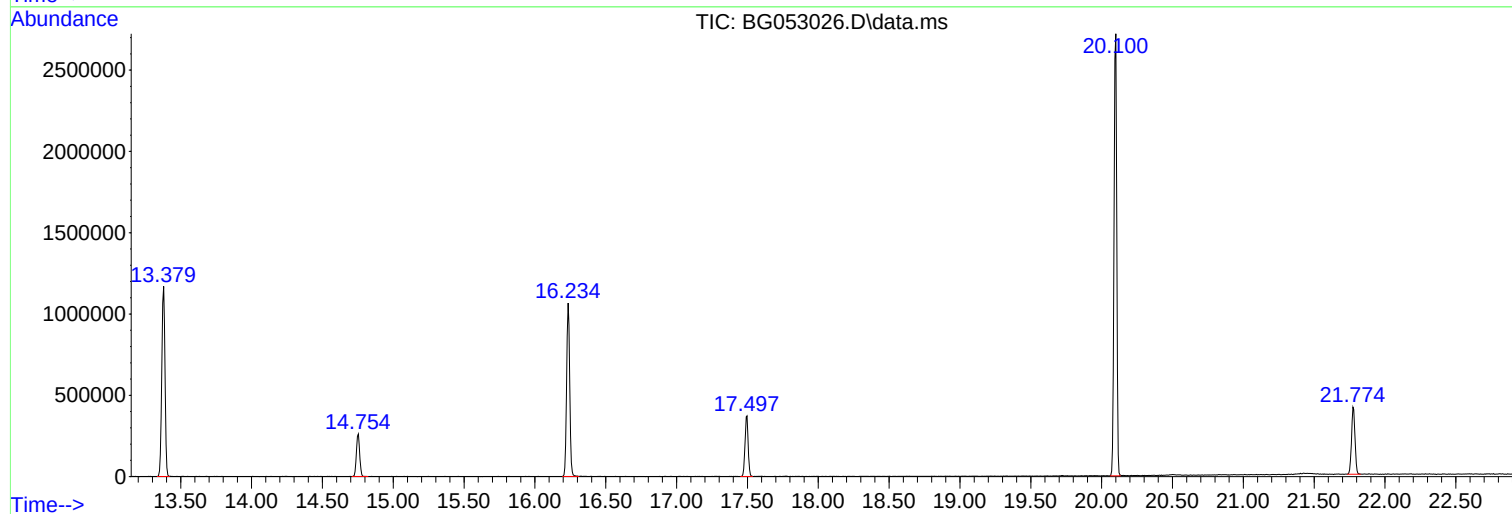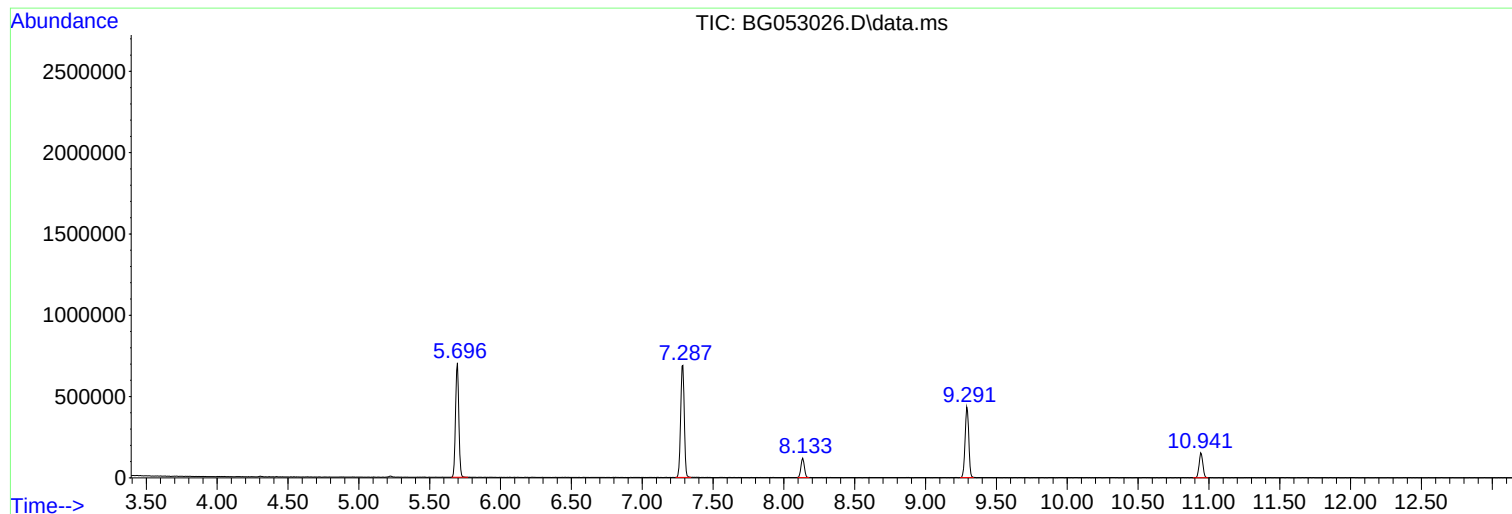

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
Data File : BG053026.D
Acq On : 5 Apr 2022 11:13
Operator : CG/JU
Sample : PB143839BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143839BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
Data File : BG053026.D
Acq On : 5 Apr 2022 11:13
Operator : CG/JU
Sample : PB143839BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB143839BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------