

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
 Data File : BG053036.D
 Acq On : 5 Apr 2022 17:54
 Operator : CG/JU
 Sample : N2239-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.588	30	34	42	rVB	105169	147044	4.18%	1.010%
2	4.739	224	230	236	rBV	120764	177384	5.04%	1.218%
3	5.191	302	307	310	rBV	67437	103470	2.94%	0.710%
4	5.221	310	312	319	rVB	48921	68576	1.95%	0.471%
5	5.691	385	392	402	rVB	715564	1158822	32.93%	7.956%
6	7.277	655	662	671	rBV	647659	1148757	32.65%	7.887%
7	8.129	799	807	814	rVB	138467	239762	6.81%	1.646%
8	9.286	996	1004	1014	rBV	511668	927037	26.35%	6.365%
9	10.937	1277	1285	1292	rBV	173337	312297	8.88%	2.144%
10	13.374	1693	1700	1708	rVB	1187103	1925049	54.71%	13.216%
11	14.185	1833	1838	1847	rBV	24822	35906	1.02%	0.247%
12	14.743	1927	1933	1939	rVB2	271489	420484	11.95%	2.887%
13	16.229	2177	2186	2195	rBV	1112209	1711857	48.65%	11.753%
14	17.486	2393	2400	2405	rBV	387480	574942	16.34%	3.947%
15	17.528	2405	2407	2413	rVB	28577	37096	1.05%	0.255%
16	17.880	2461	2467	2473	rBV	26772	44995	1.28%	0.309%
17	19.707	2772	2778	2785	rBV	256244	353506	10.05%	2.427%
18	20.095	2837	2844	2850	rBV	2701709	3518643	100.00%	24.157%
19	20.330	2879	2884	2890	rBV2	63603	94005	2.67%	0.645%
20	20.829	2964	2969	2976	rVB	154959	205266	5.83%	1.409%
21	21.769	3122	3129	3137	rBV	393767	677108	19.24%	4.649%
22	25.064	3680	3690	3703	rVB2	227696	683583	19.43%	4.693%




Sum of corrected areas: 14565589

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
Data File : BG053036.D
Acq On : 5 Apr 2022 17:54
Operator : CG/JU
Sample : N2239-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

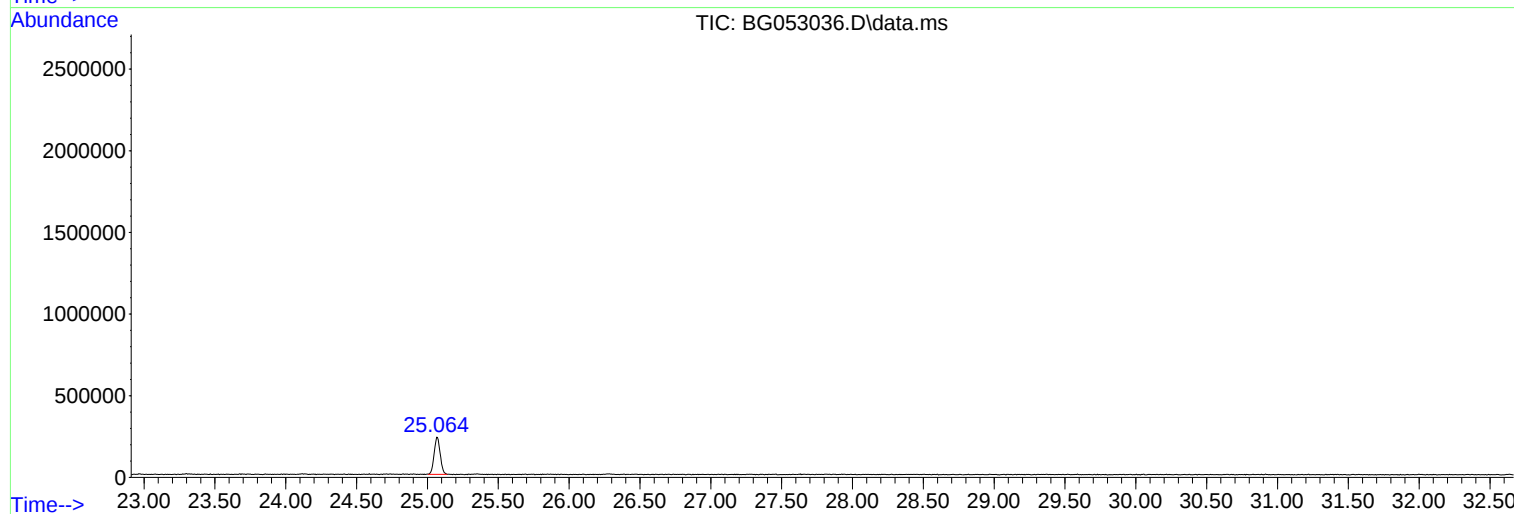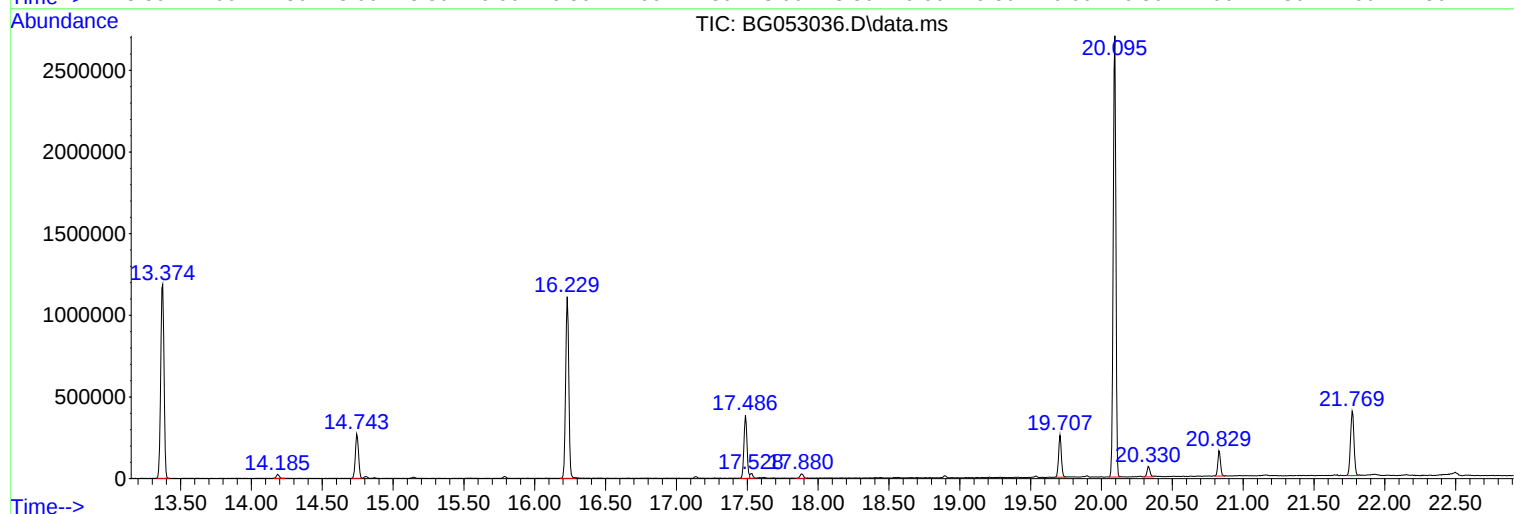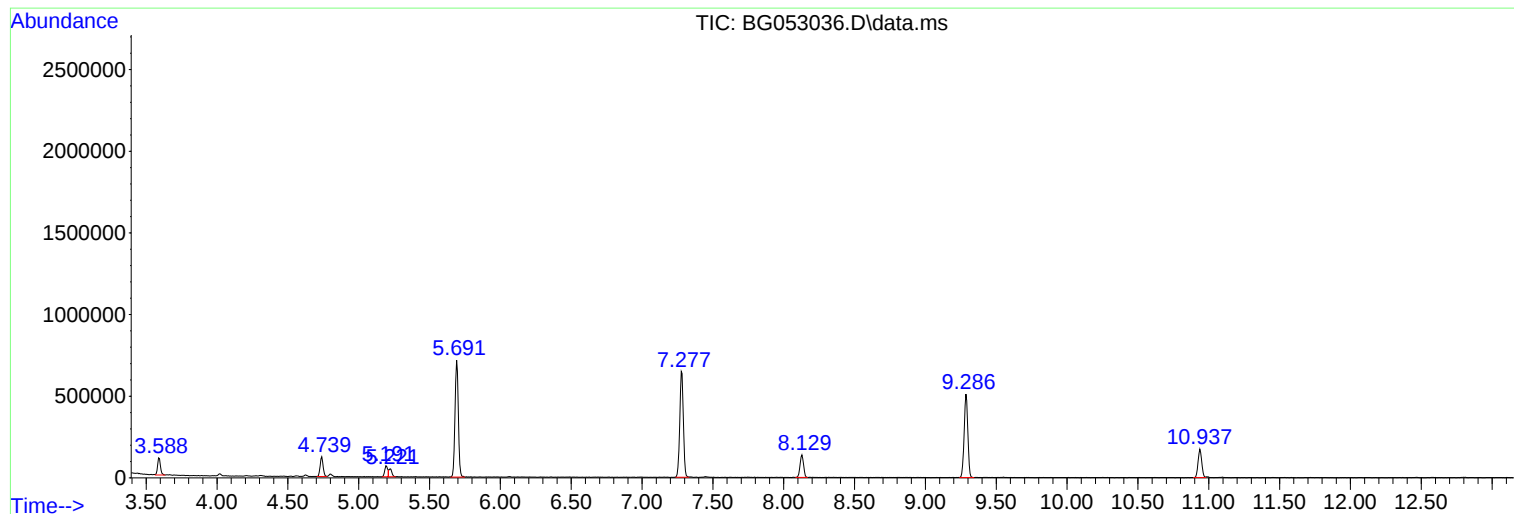

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
Data File : BG053036.D
Acq On : 5 Apr 2022 17:54
Operator : CG/JU
Sample : N2239-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
Data File : BG053036.D
Acq On : 5 Apr 2022 17:54
Operator : CG/JU
Sample : N2239-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------