
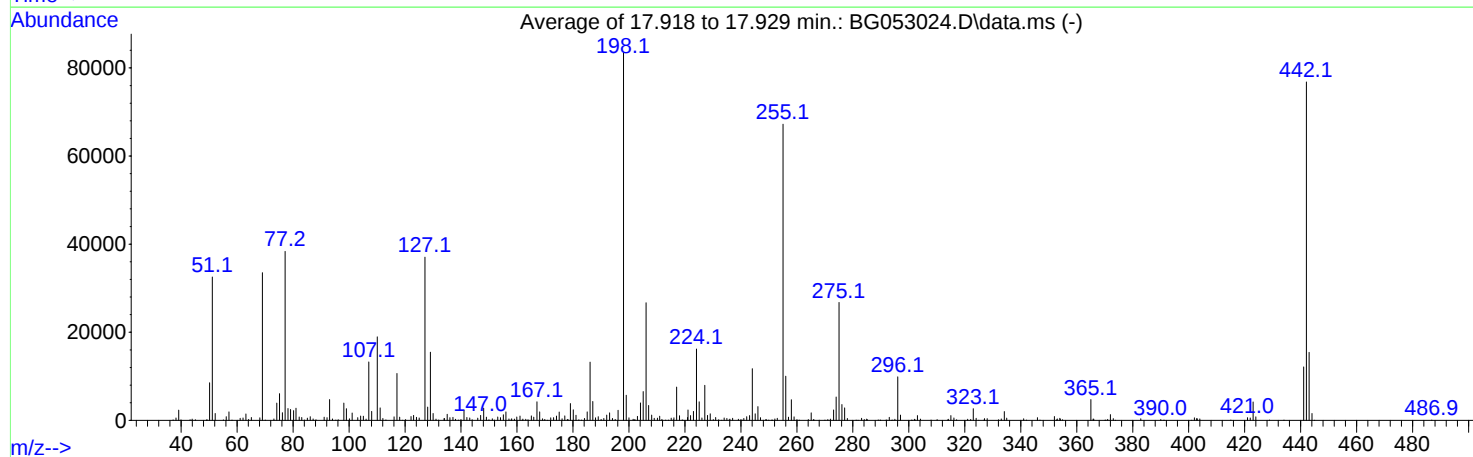


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
 Data File : BG053024.D
 Acq On : 5 Apr 2022 9:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 06 14:35:39 2022

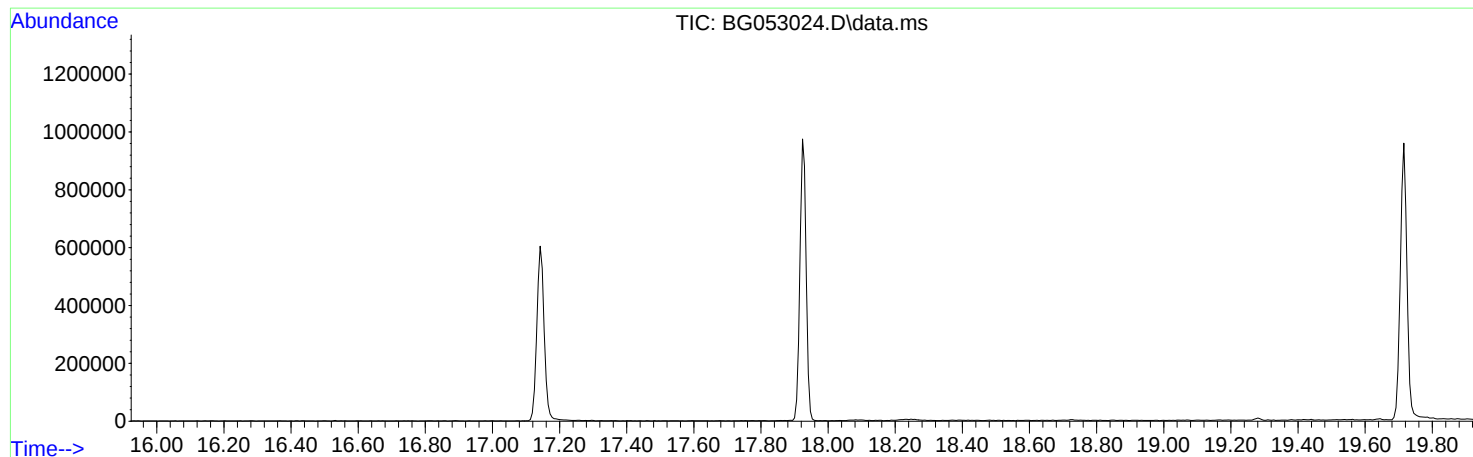




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	32563	PASS
68	69	0.00	2	1.8	589	PASS
69	198	0.00	100	40.2	33544	PASS
70	69	0.00	2	0.3	89	PASS
127	198	10	80	44.4	37053	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83507	PASS
199	198	5	9	6.9	5721	PASS
275	198	10	60	32.0	26757	PASS
365	198	1	100	5.7	4739	PASS
441	198	0.01	100	14.5	12137	PASS
442	442	50	100	100.0	76835	PASS
443	442	15	24	20.1	15426	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
Data File : BG053024.D
Acq On : 5 Apr 2022 9:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 05 14:35:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 14:24:42 2022
Response via : Initial Calibration

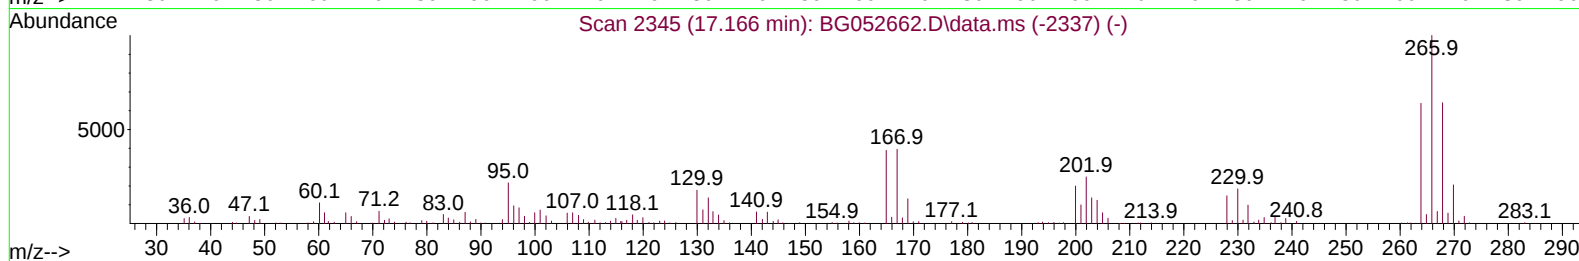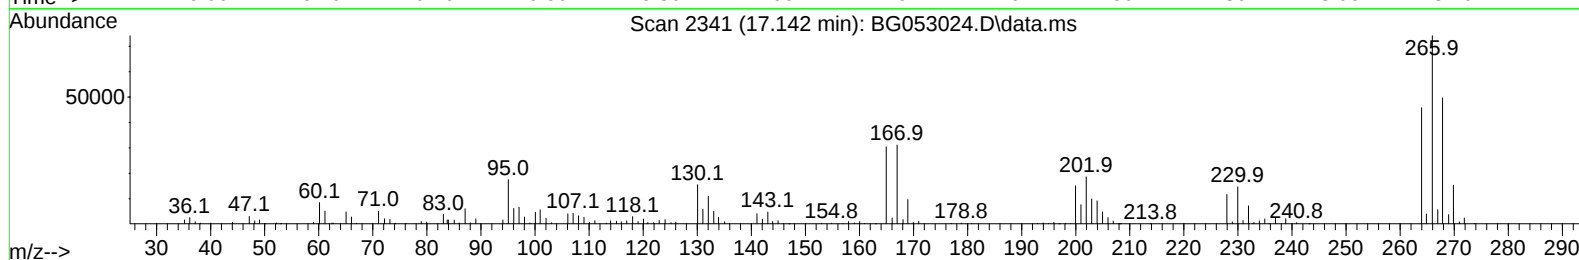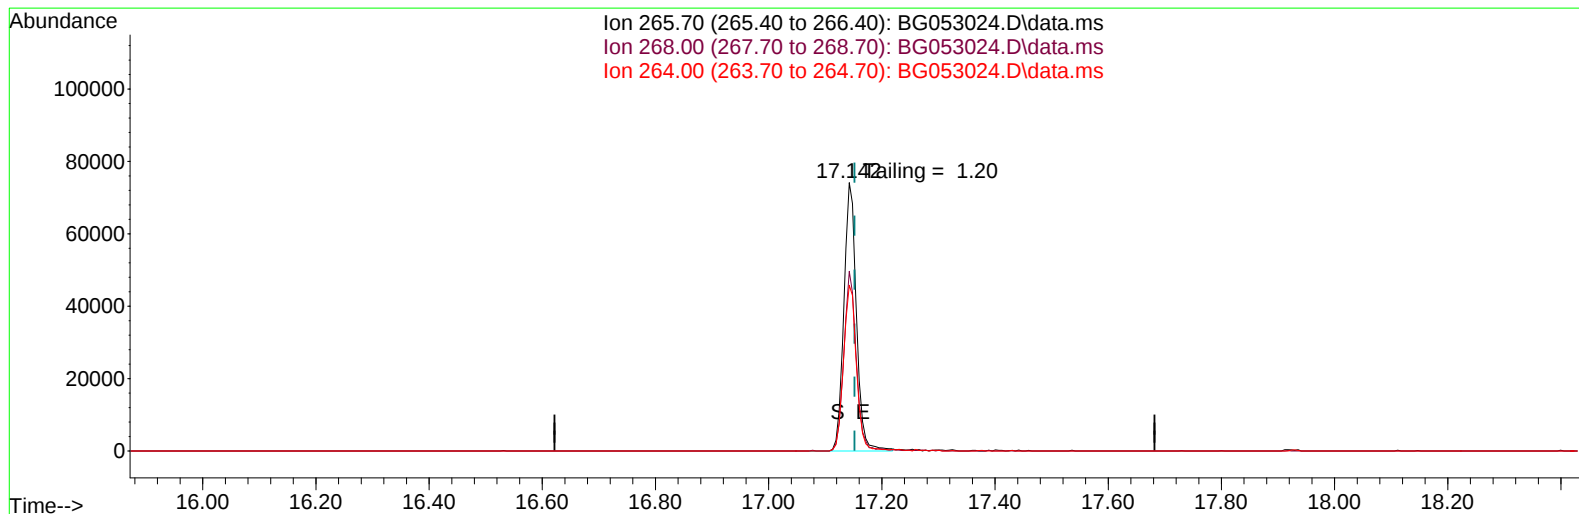

TIC: BG053024.D\data.ms

(70) Pentachlorophenol (C)

17.142min (-0.009) 18785.40 ng




response 114780

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	66.95
264.00	56.60	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
 Data File : BG053024.D
 Acq On : 5 Apr 2022 9:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 05 14:35:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 14:24:42 2022
 Response via : Initial Calibration

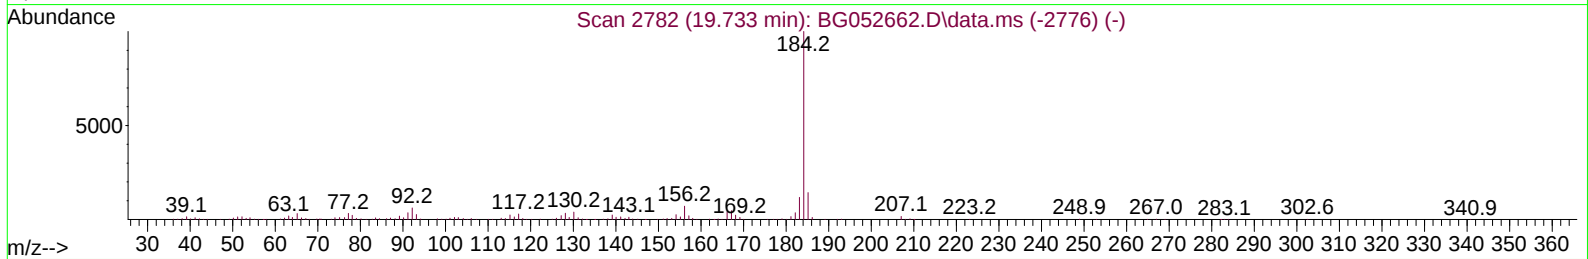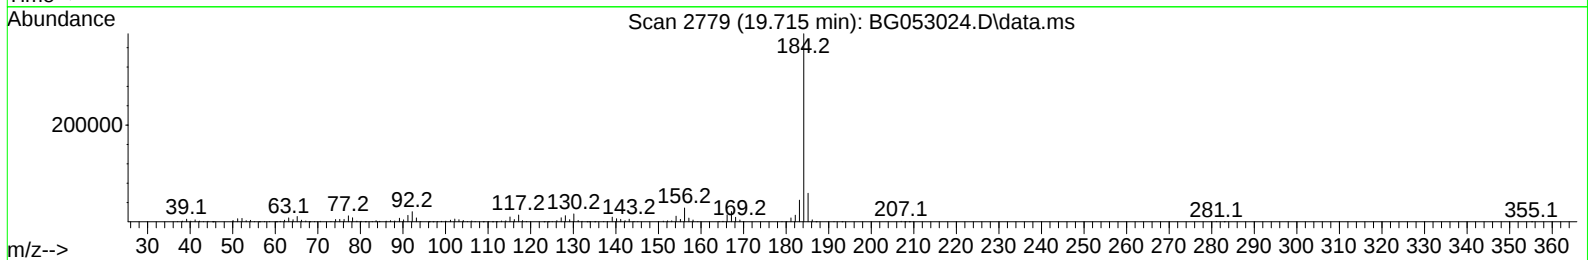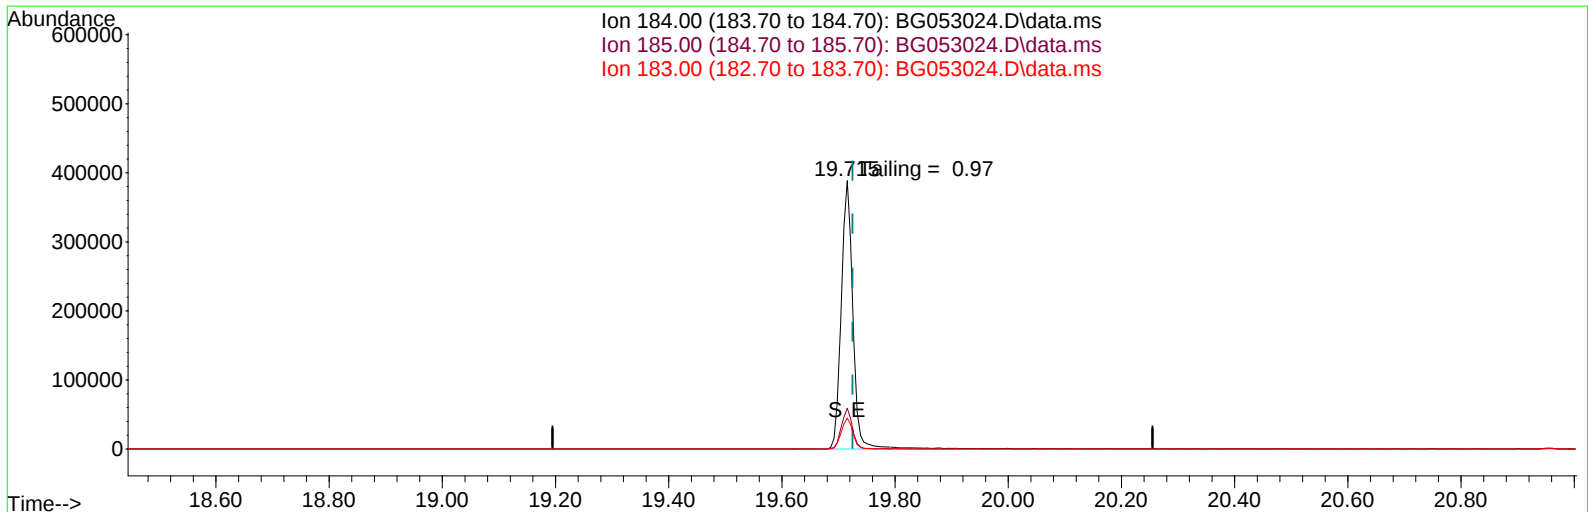

TIC: BG053024.D\data.ms

(77) Benzidine

19.715min (-0.009) 0.00 ng

response 549814

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.22
183.00	11.80	11.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/5/2022	BNA_G	BG053024.D
Compound Name	Response	Retention Time
DDT	335707	20.95
DDD	6367	20.58
DDE	118	20
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6485	342192	1.90

Instrument :
BNA_G
ClientSampleId :
DFTPP