


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
 Data File : BG053033.D
 Acq On : 5 Apr 2022 15:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 06 14:35:39 2022

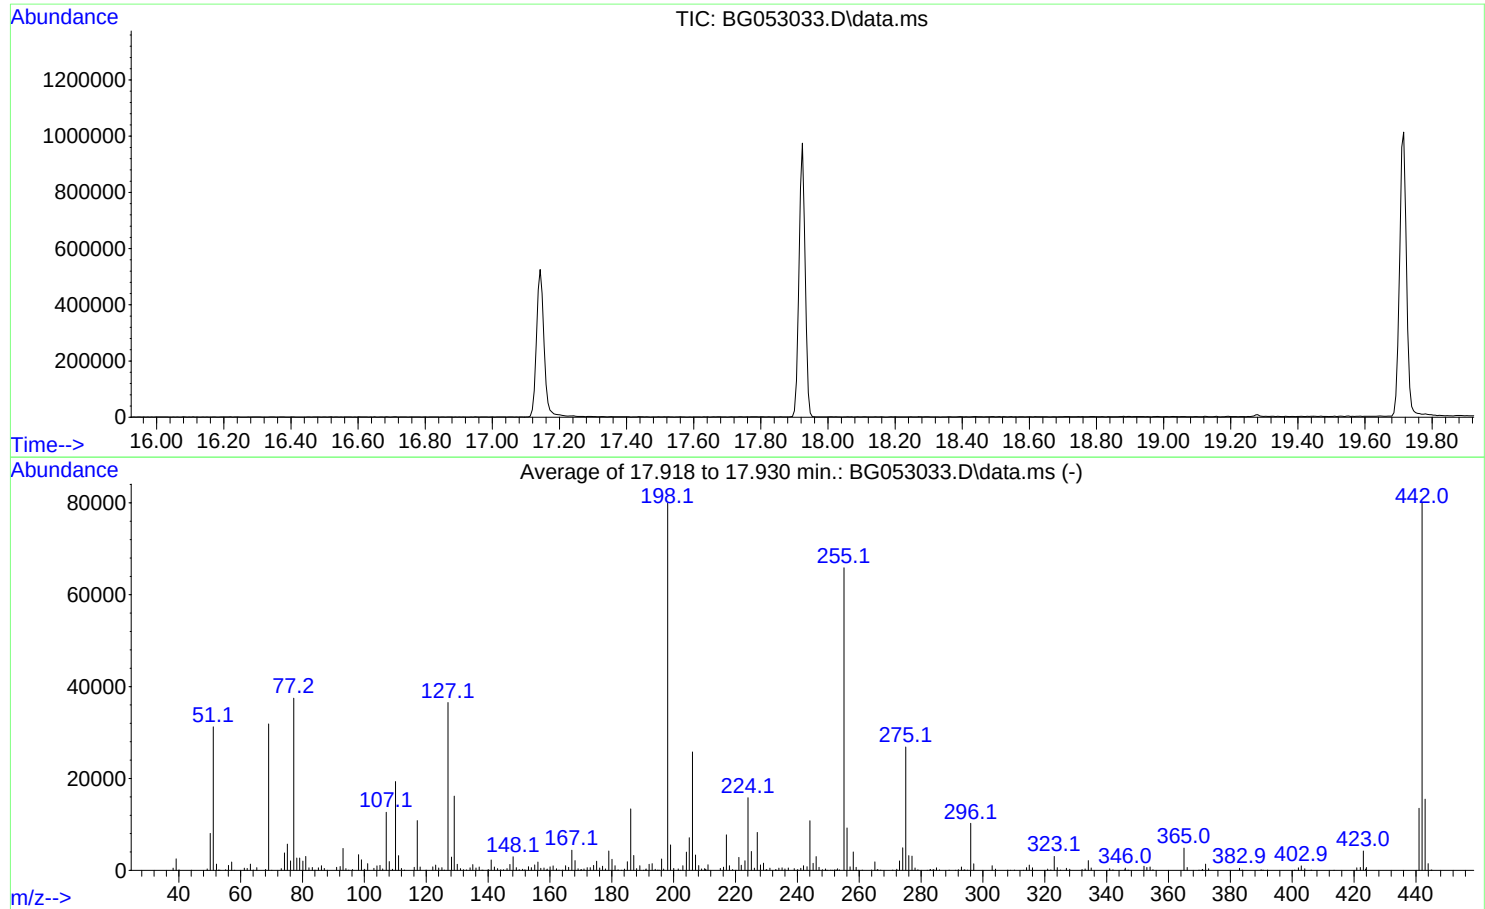




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	31229	PASS
68	69	0.00	2	0.6	204	PASS
69	198	0.00	100	39.9	31864	PASS
70	69	0.00	2	0.2	53	PASS
127	198	10	80	45.8	36557	PASS
197	198	0.00	2	0.4	282	PASS
198	198	100	100	100.0	79888	PASS
199	198	5	9	7.0	5555	PASS
275	198	10	60	33.6	26875	PASS
365	198	1	100	6.1	4859	PASS
441	198	0.01	100	16.9	13532	PASS
442	442	50	100	100.0	80080	PASS
443	442	15	24	19.4	15499	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
Data File : BG053033.D
Acq On : 5 Apr 2022 15:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 05 16:39:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 14:24:42 2022
Response via : Initial Calibration

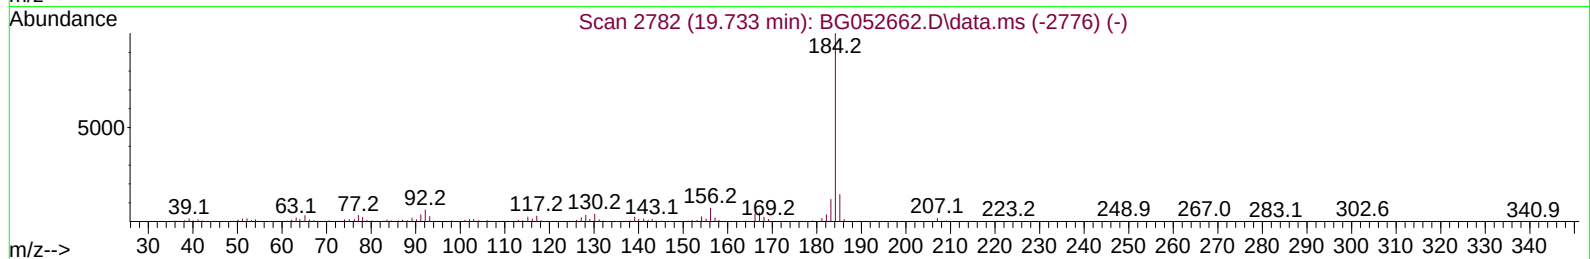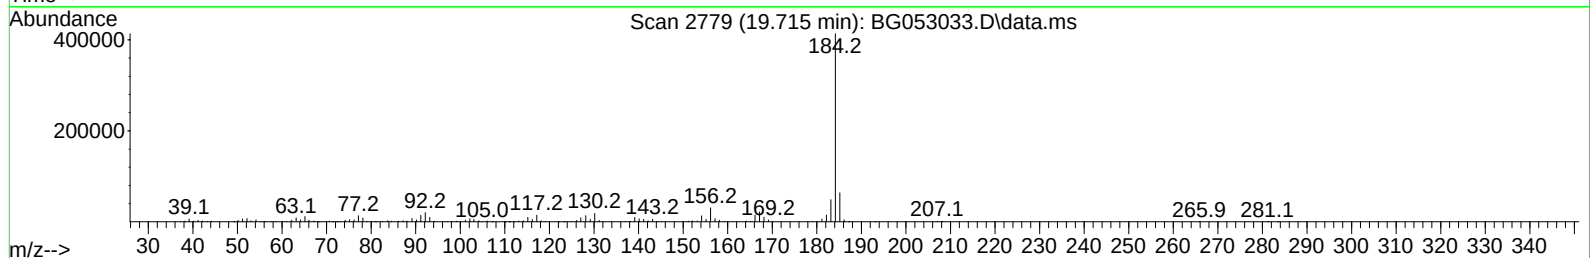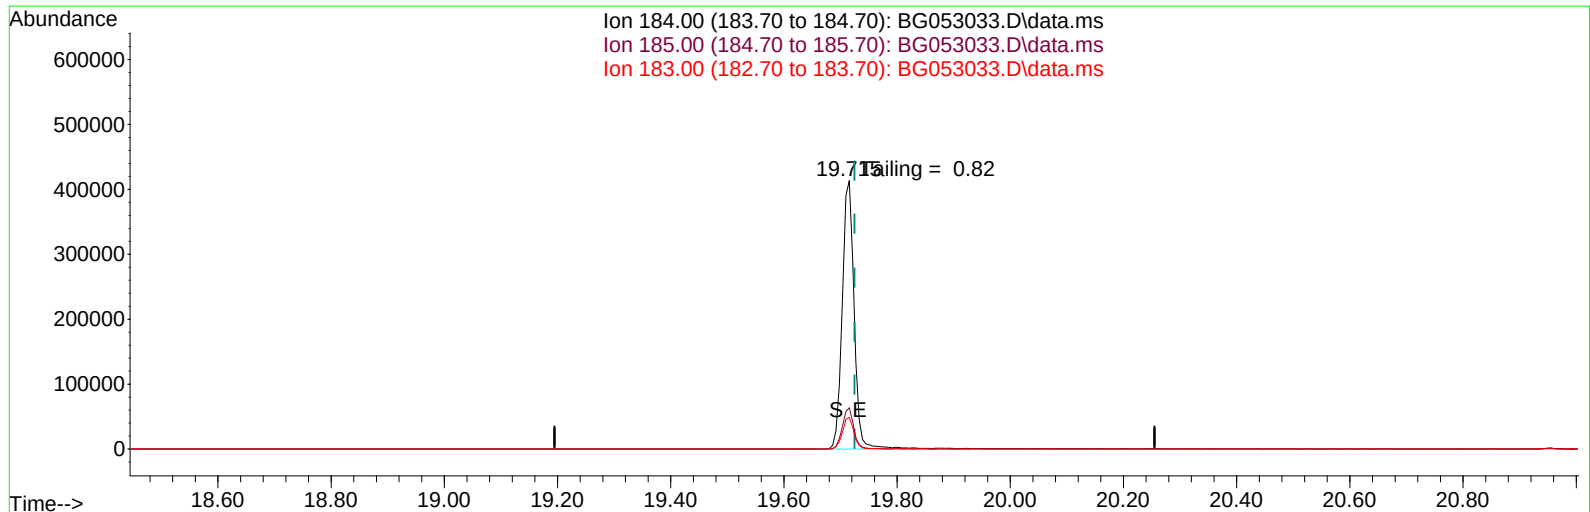

TIC: BG053033.D\data.ms

(77) Benzidine

19.715min (-0.009) 368428.44 ng




response 598658

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	15.42
183.00	11.80	11.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040522\
Data File : BG053033.D
Acq On : 5 Apr 2022 15:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 05 16:39:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 14:24:42 2022
Response via : Initial Calibration

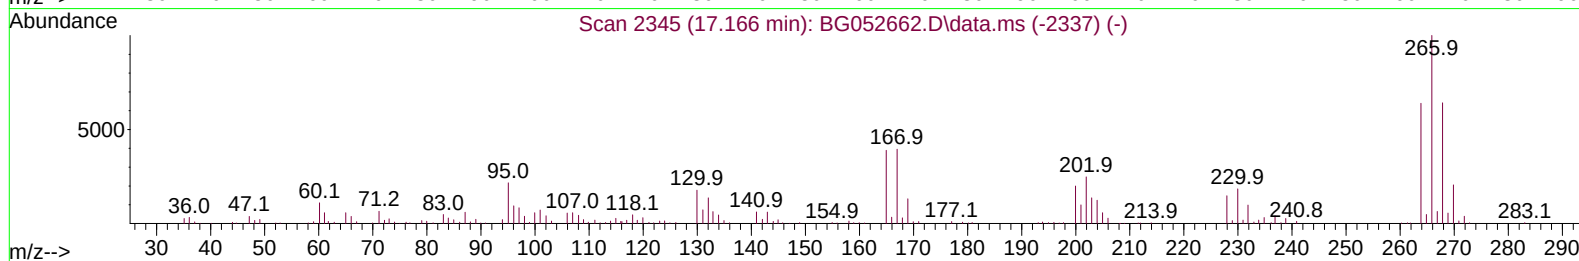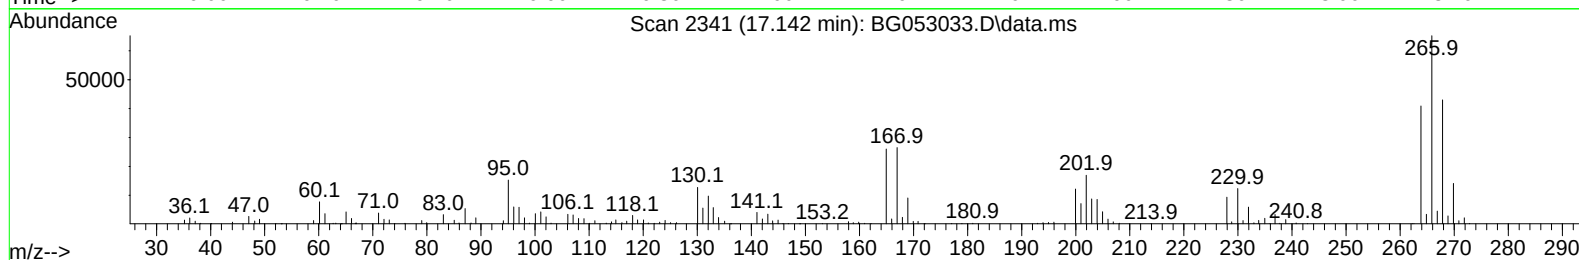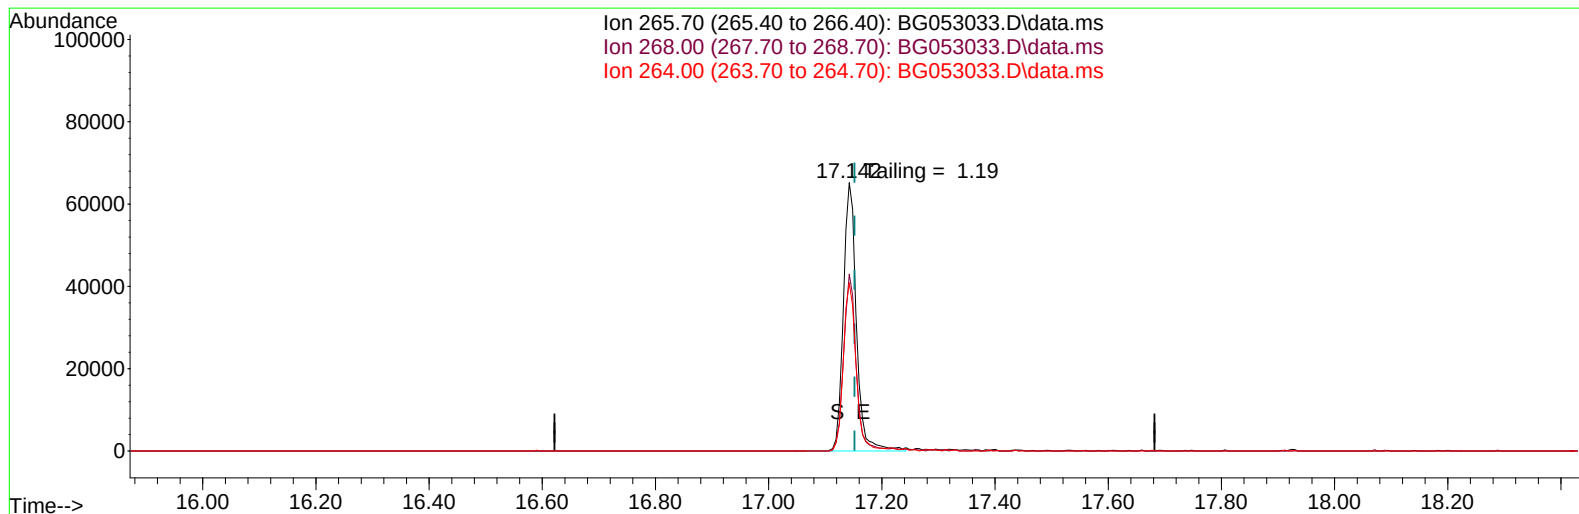

TIC: BG053033.D\data.ms

(70) Pentachlorophenol (C)

17.142min (-0.009) 25512.06 ng

response 104809

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	65.92
264.00	56.60	62.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/5/2022	BNA_G	<u>BG053033.D</u>
Compound Name	Response	Retention Time
DDT	350902	20.95
DDD	8253	20.5
DDE	574	20
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8827	359729	2.45

Instrument :
BNA_G
ClientSampleId :
DFTPP