
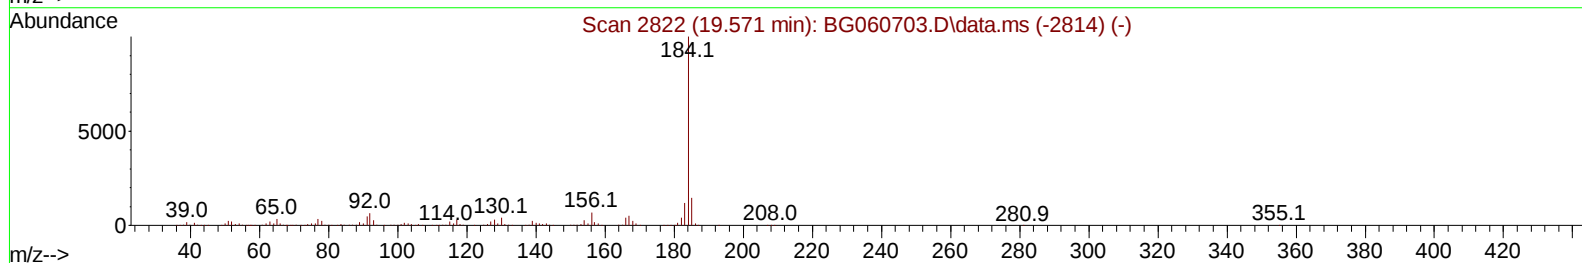
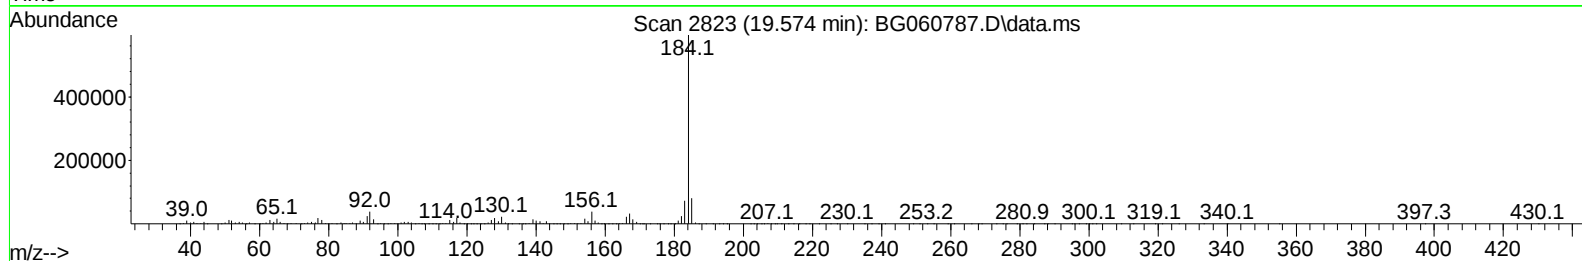


Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	61.30
264.00	64.70	63.20
0.00	0.00	0.00

Quant Time: Apr 05 10:40:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

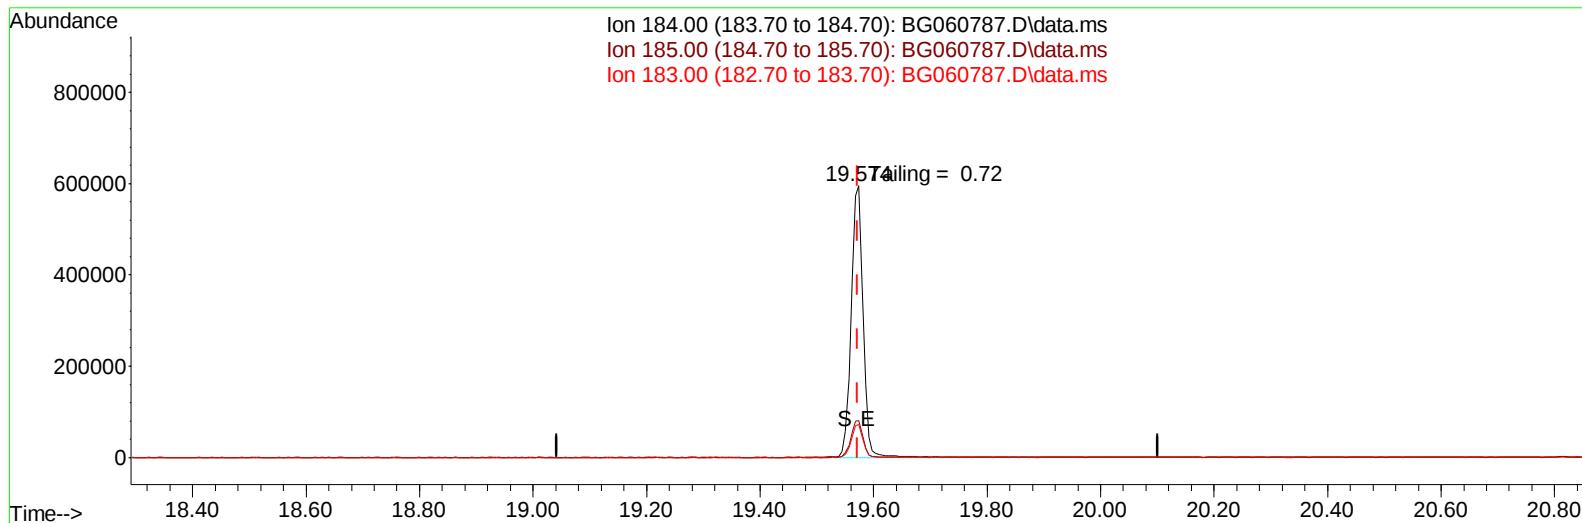

TIC: BG060787.D\data.ms

(77) Benzidine

19.574min (+ 0.003) 86077.11 ng

response **870373**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.49
183.00	11.90	12.21
0.00	0.00	0.00